

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
 Data File : PP044558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 13:07
 Operator : YP\AJ
 Sample : N1645-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:58:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.908	3.164	40768860	35333520	19.676	20.197
2) SA Decachlor...	10.041	8.527	27236637	31093421	19.789	20.270
Target Compounds						
11) L3 AR-1232-1	4.307	3.559	1237565	1061070	26.968	25.534
12) L3 AR-1232-2	4.869	4.326	616136	1089198	27.379	31.538
13) L3 AR-1232-3	5.182	4.511	963211	564215	22.261	30.241 #
14) L3 AR-1232-4	5.356	4.601	489936	510401	24.402	30.954 #
15) L3 AR-1232-5	5.455	4.783	369667	519010	24.366	28.670



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
Data File : PP044558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 13:07
Operator : YP\AJ
Sample : N1645-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:58:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

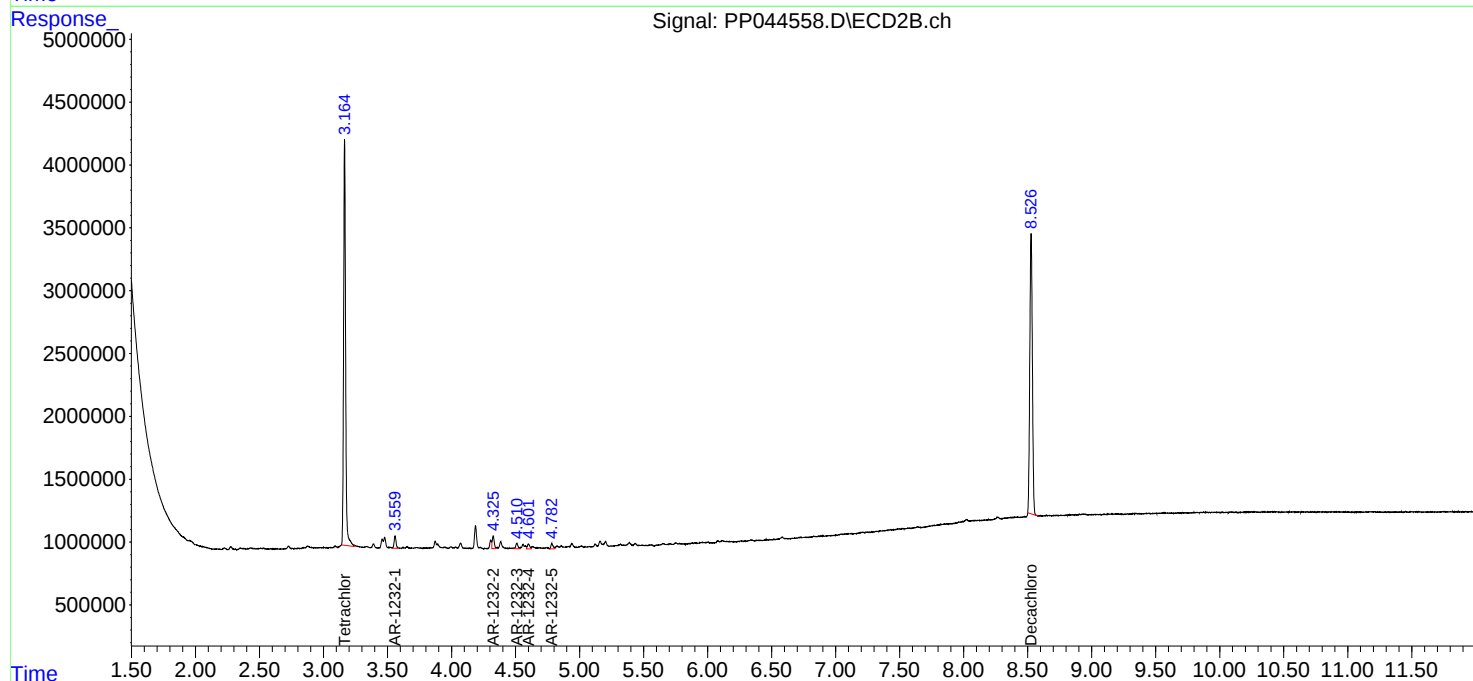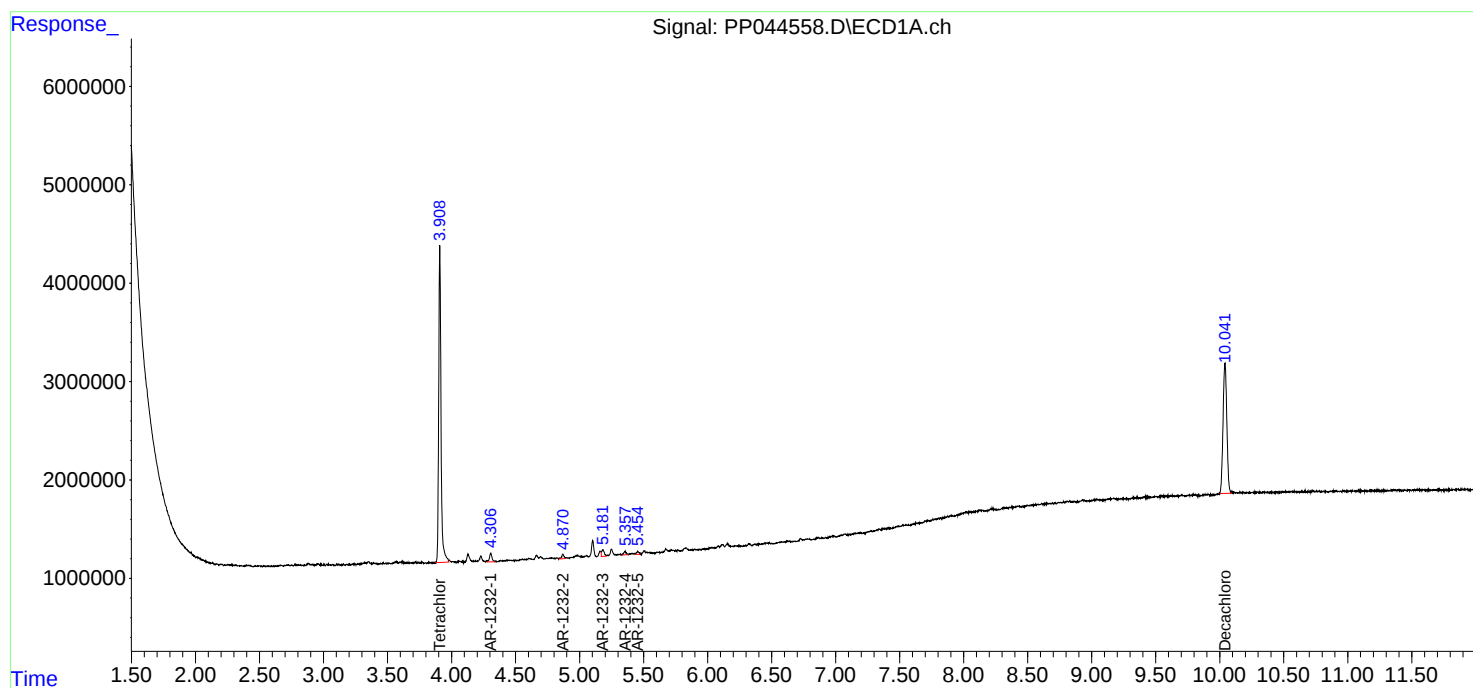


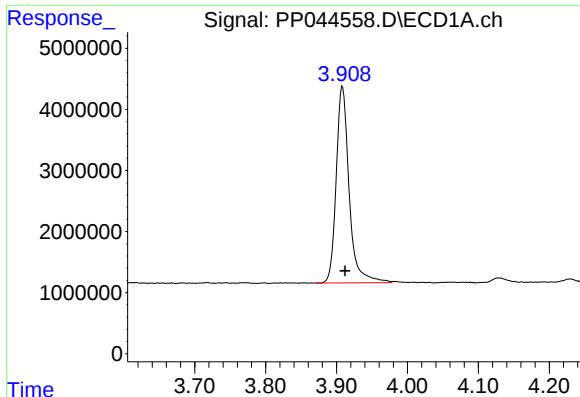

#1 Tetrachloro-m-xylene


R.T.: 3.908 min
Delta R.T.: -0.004 min
Response: 40768860
Conc: 19.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2022

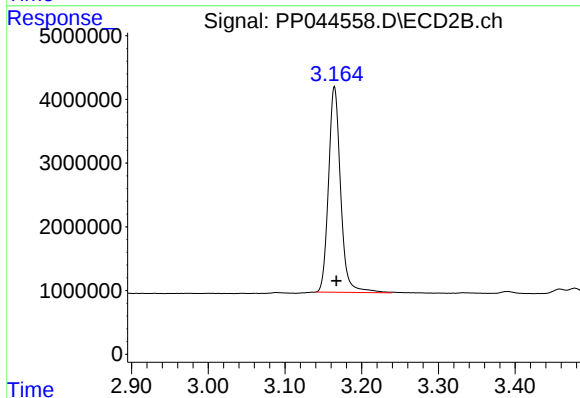


#1 Tetrachloro-m-xylene

R.T.: 3.164 min
Delta R.T.: -0.002 min
Response: 35333520
Conc: 20.20 ng/ml

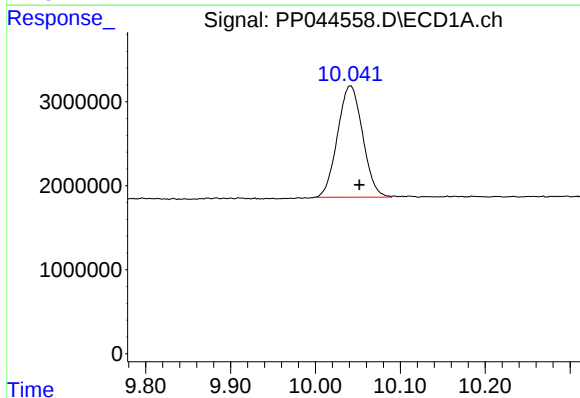


#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.010 min
Response: 27236637
Conc: 19.79 ng/ml

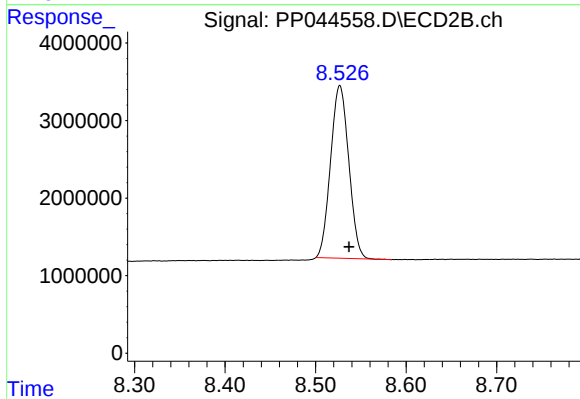

#2 Decachlorobiphenyl


R.T.: 8.527 min
Delta R.T.: -0.010 min
Response: 31093421
Conc: 20.27 ng/ml

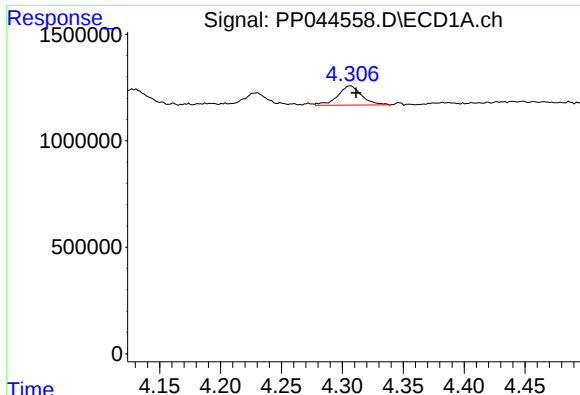

#11 AR-1232-1


R.T.: 4.307 min
Delta R.T.: -0.005 min
Response: 1237565
Conc: 26.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2022

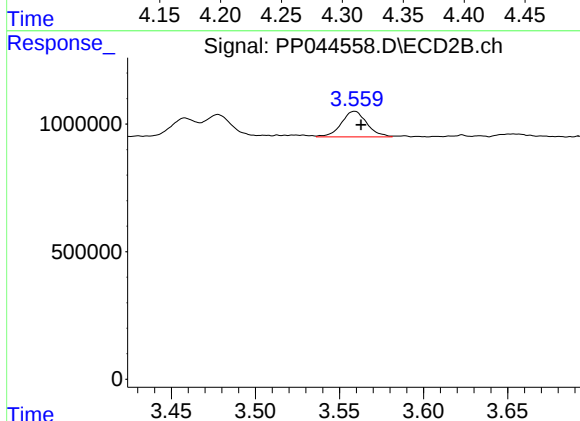


#11 AR-1232-1

R.T.: 3.559 min
Delta R.T.: -0.004 min
Response: 1061070
Conc: 25.53 ng/ml

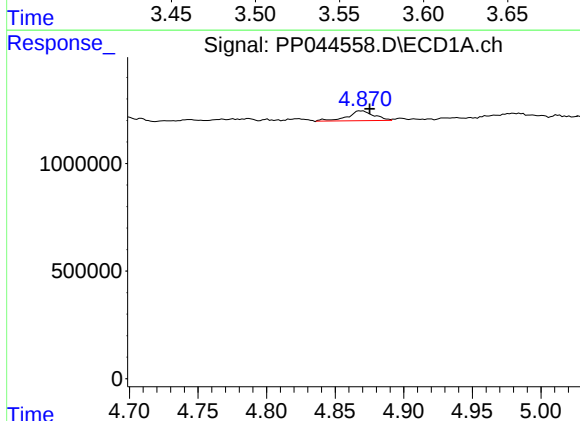


#12 AR-1232-2

R.T.: 4.869 min
Delta R.T.: -0.006 min
Response: 616136
Conc: 27.38 ng/ml

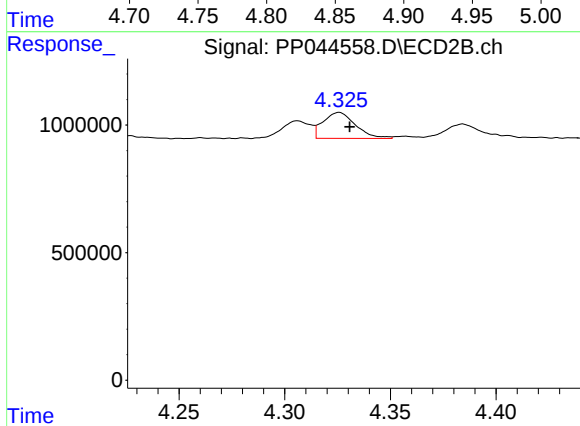

#12 AR-1232-2


R.T.: 4.326 min
Delta R.T.: -0.005 min
Response: 1089198
Conc: 31.54 ng/ml

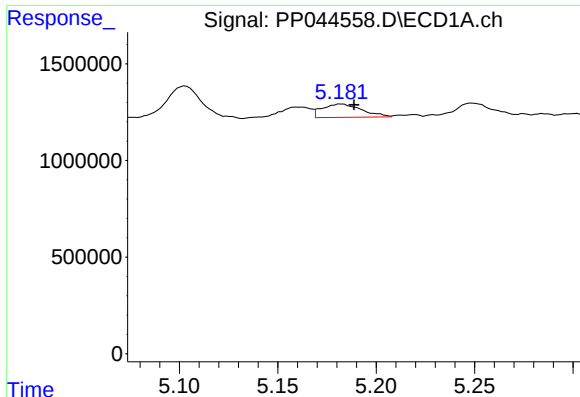

#13 AR-1232-3


R.T.: 5.182 min
Delta R.T.: -0.006 min
Response: 963211
Conc: 22.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2022

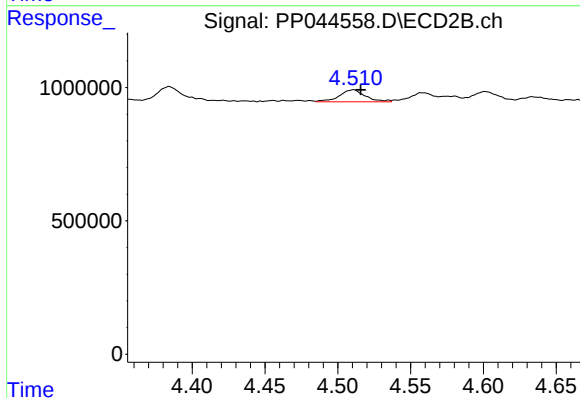


#13 AR-1232-3

R.T.: 4.511 min
Delta R.T.: -0.005 min
Response: 564215
Conc: 30.24 ng/ml

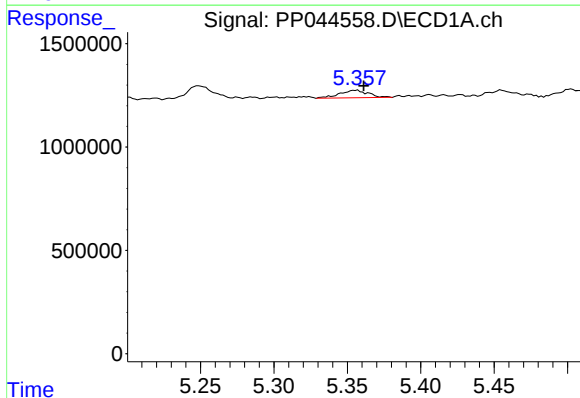


#14 AR-1232-4

R.T.: 5.356 min
Delta R.T.: -0.005 min
Response: 489936
Conc: 24.40 ng/ml

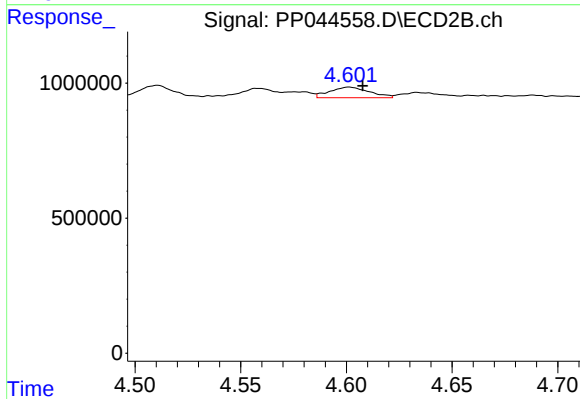

#14 AR-1232-4


R.T.: 4.601 min
Delta R.T.: -0.006 min
Response: 510401
Conc: 30.95 ng/ml

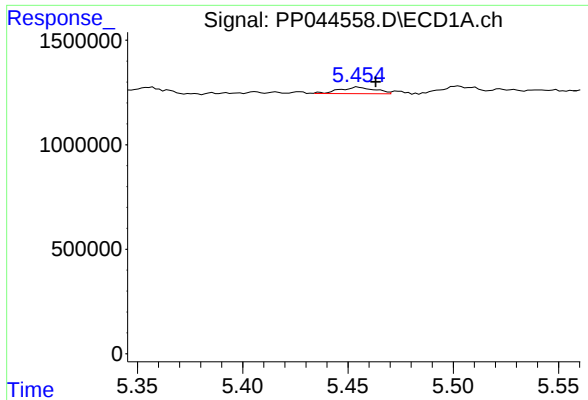

#15 AR-1232-5

R.T.: 5.455 min
Delta R.T.: -0.008 min
Response: 369667
Conc: 24.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2022

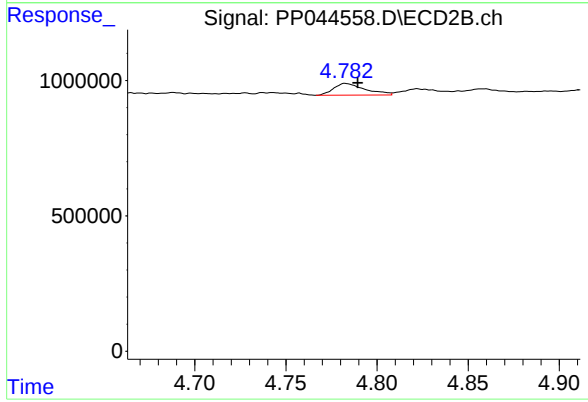

#15 AR-1232-5

R.T.: 4.783 min
Delta R.T.: -0.007 min
Response: 519010
Conc: 28.67 ng/ml