

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
 Data File : PP044604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2022 02:46
 Operator : YP\AJ
 Sample : N1893-10
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2022
 Supervised By :Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 12:12:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.907	3.164	17776079	22695584	8.579m	12.973m#
2) SA Decachlor...	10.041	8.525	9196275	11287452	6.682	7.358
Target Compounds						
16) L4 AR-1242-1	5.159	4.306	74845289	62619634	1375.007	1365.534
17) L4 AR-1242-2	5.182	4.324	98303586	76803746	1234.415	1215.332
18) L4 AR-1242-3	5.250	4.509	25086995	33576628	531.245	940.035 #
19) L4 AR-1242-4	5.354	4.600	39516079	33976081	1020.985	982.084
20) L4 AR-1242-5	6.154	5.159	24636763	23166205	577.854	548.469

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
Data File : PP044604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2022 02:46
Operator : YP\AJ
Sample : N1893-10
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 12:12:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

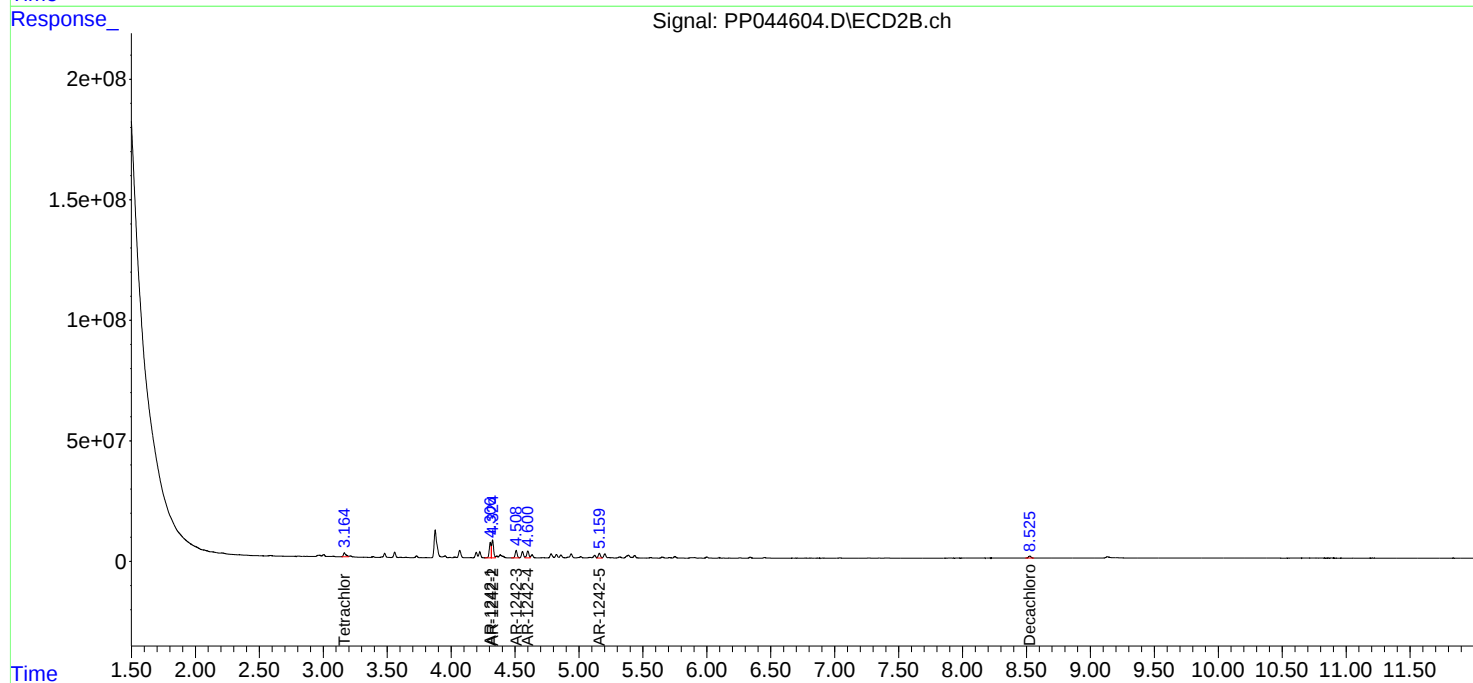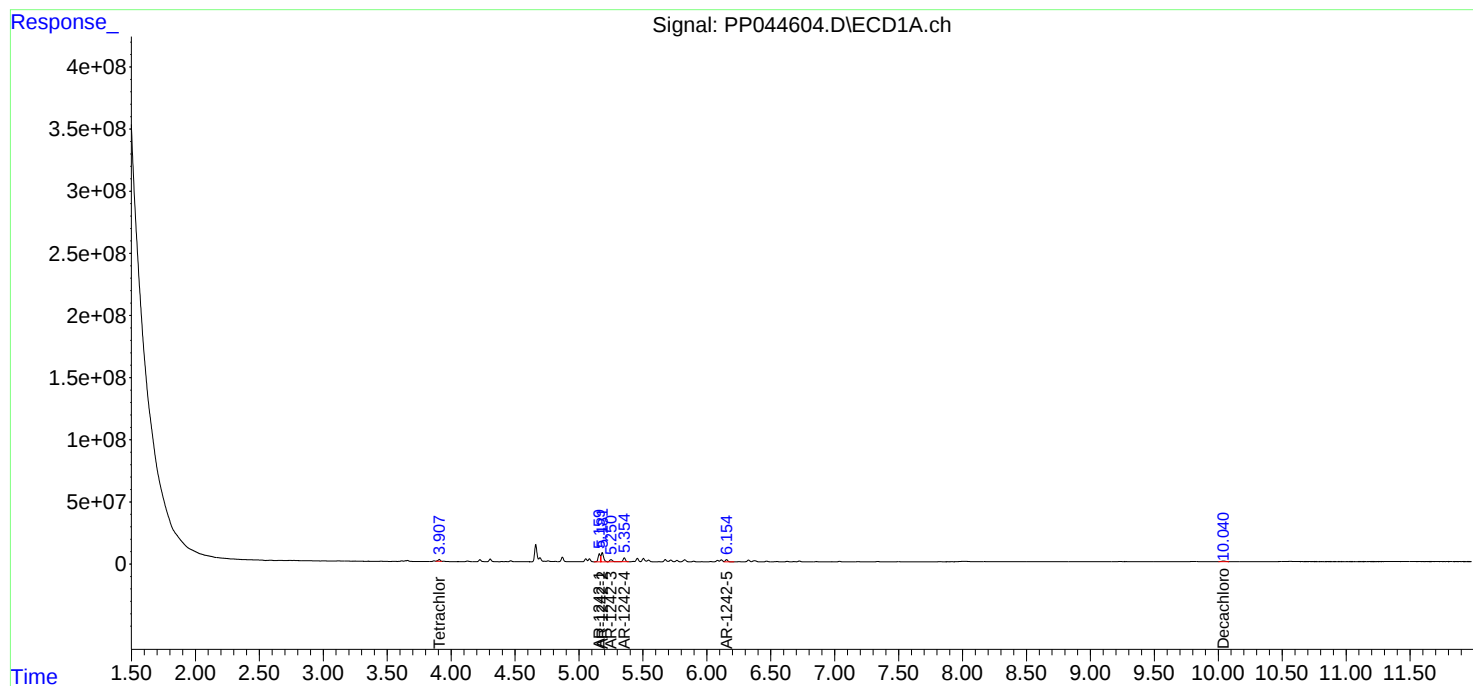

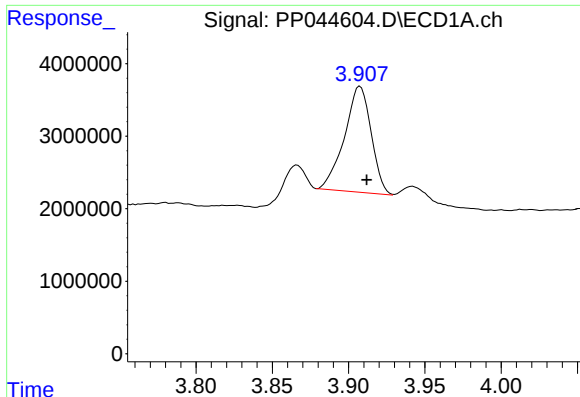


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: -0.005 min
Response: 17776079
Conc: 8.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

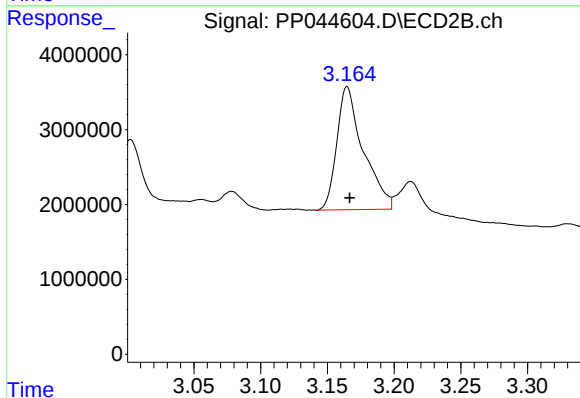


#1 Tetrachloro-m-xylene

R.T.: 3.164 min
Delta R.T.: -0.002 min
Response: 22695584
Conc: 12.97 ng/ml m

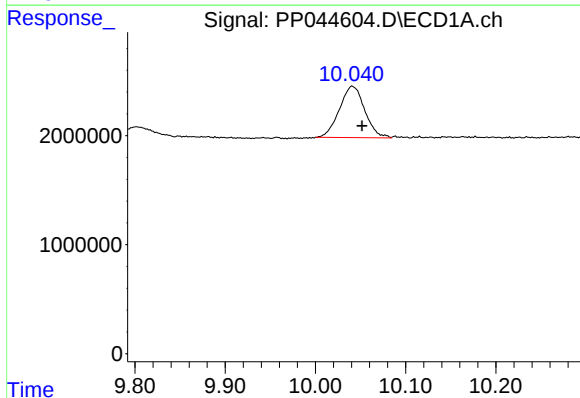


#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.011 min
Response: 9196275
Conc: 6.68 ng/ml

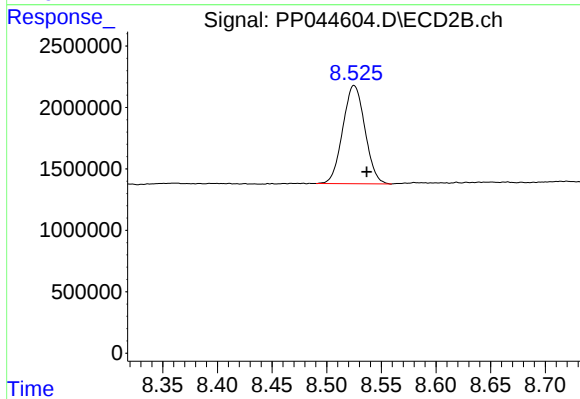

#2 Decachlorobiphenyl

R.T.: 8.525 min
Delta R.T.: -0.012 min
Response: 11287452
Conc: 7.36 ng/ml

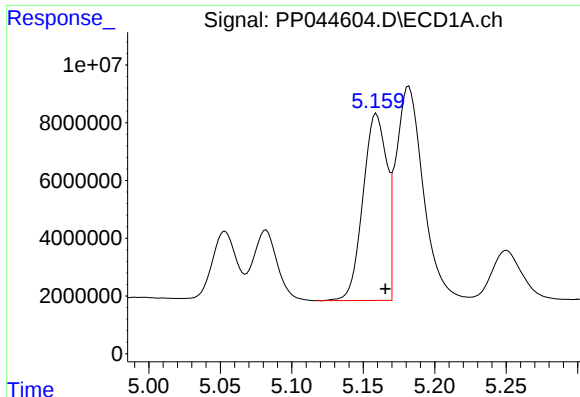


#16 AR-1242-1

R.T.: 5.159 min
Delta R.T.: -0.006 min
Response: 74845289
Conc: 1375.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

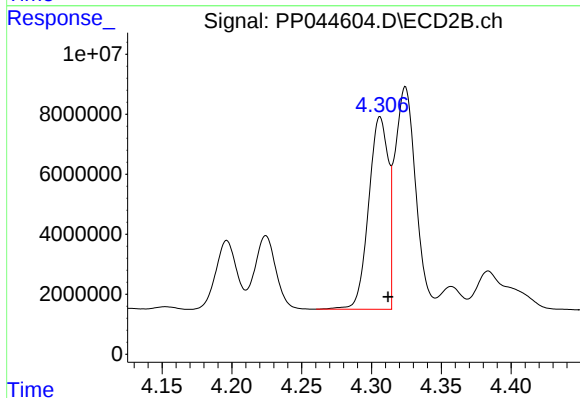


#16 AR-1242-1

R.T.: 4.306 min
Delta R.T.: -0.006 min
Response: 62619634
Conc: 1365.53 ng/ml

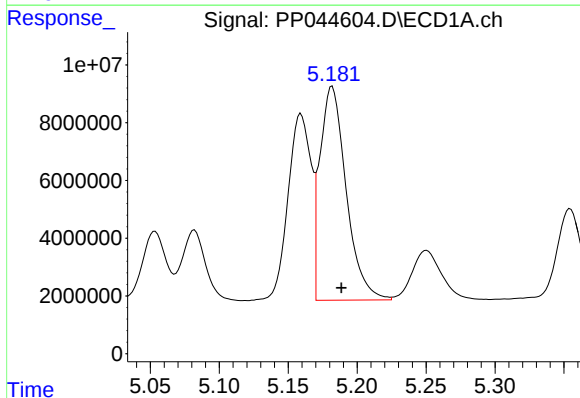


#17 AR-1242-2

R.T.: 5.182 min
Delta R.T.: -0.007 min
Response: 98303586
Conc: 1234.42 ng/ml

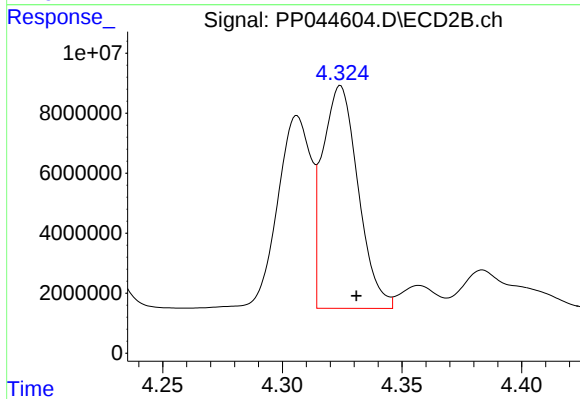

#17 AR-1242-2

R.T.: 4.324 min
Delta R.T.: -0.007 min
Response: 76803746
Conc: 1215.33 ng/ml

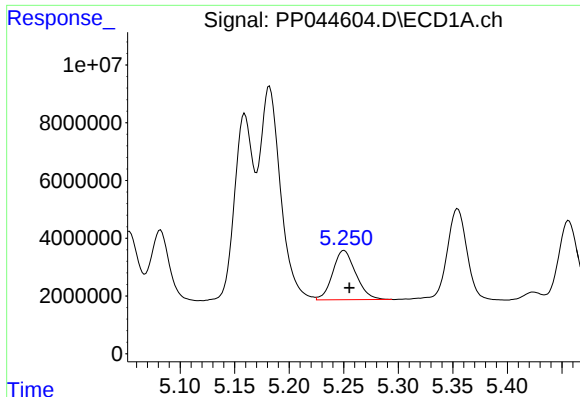


#18 AR-1242-3

R.T.: 5.250 min
Delta R.T.: -0.005 min
Response: 25086995
Conc: 531.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

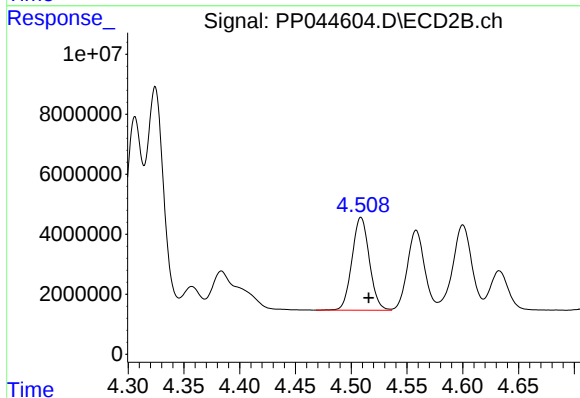


#18 AR-1242-3

R.T.: 4.509 min
Delta R.T.: -0.007 min
Response: 33576628
Conc: 940.04 ng/ml

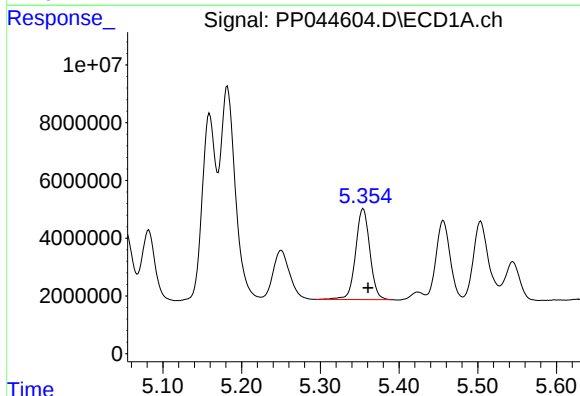


#19 AR-1242-4

R.T.: 5.354 min
Delta R.T.: -0.006 min
Response: 39516079
Conc: 1020.98 ng/ml

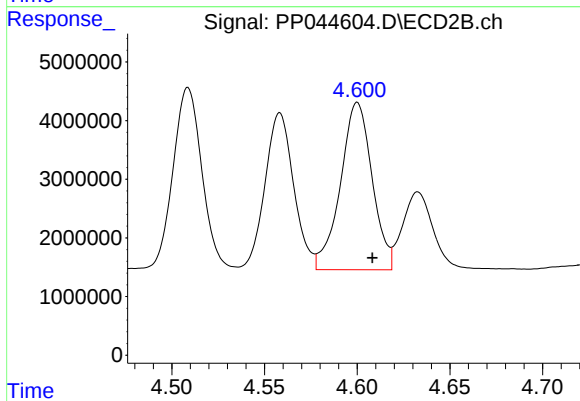

#19 AR-1242-4

R.T.: 4.600 min
Delta R.T.: -0.008 min
Response: 33976081
Conc: 982.08 ng/ml

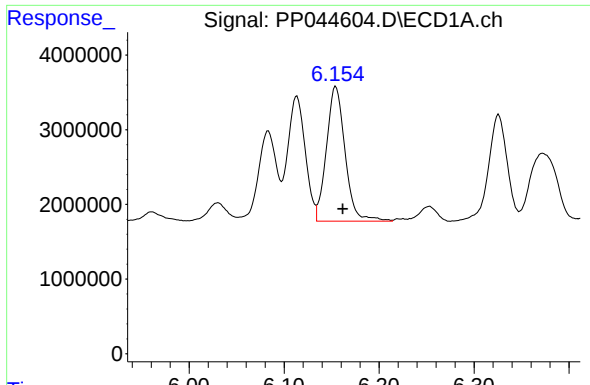


#20 AR-1242-5

R.T.: 6.154 min
Delta R.T.: -0.007 min
Response: 24636763
Conc: 577.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

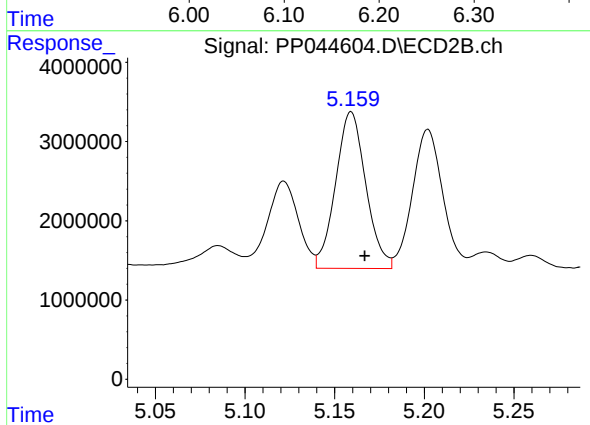

#20 AR-1242-5

R.T.: 5.159 min
Delta R.T.: -0.008 min
Response: 23166205
Conc: 548.47 ng/ml