

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
 Data File : PP044621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2022 08:03
 Operator : YP\AJ
 Sample : N1892-06 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-21A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2022
 Supervised By :Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:24:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.908	3.164	3290710	3346584	1.588	1.913
2) SA Decachlor...	10.043	8.528	3855338	3310360	2.801	2.158
Target Compounds						
41) L9 AR-1268-1	8.501	7.348	6530952	5781504	33.437	25.421
42) L9 AR-1268-2	8.600	7.420	8213433	8527072	45.092	41.624
43) L9 AR-1268-3	8.837	7.640	1769217	1877108	11.463	10.739
44) L9 AR-1268-4	9.280	7.962	3589699	4197878	57.373	51.731
45) L9 AR-1268-5	9.704	8.267	7966559	7877682	16.967	14.615

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031122\
Data File : PP044621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2022 08:03
Operator : YP\AJ
Sample : N1892-06 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-2022-21A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:24:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

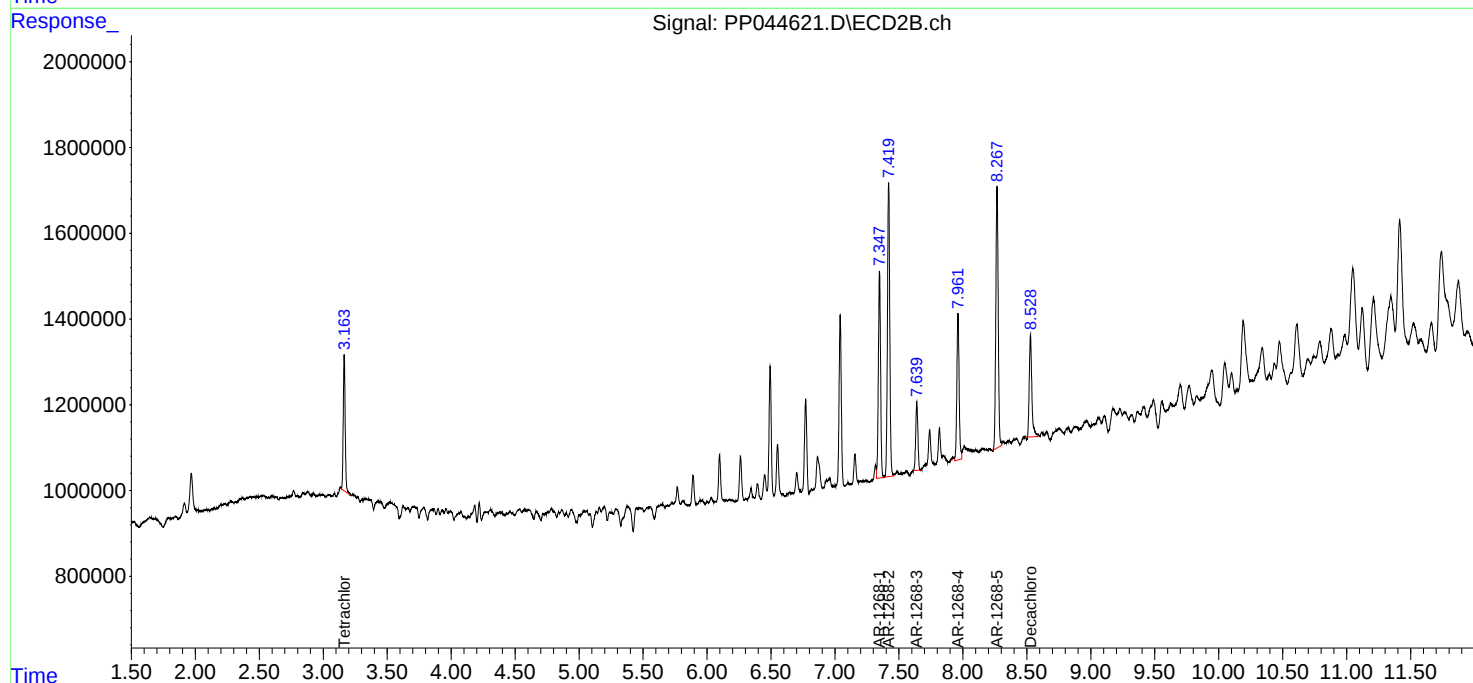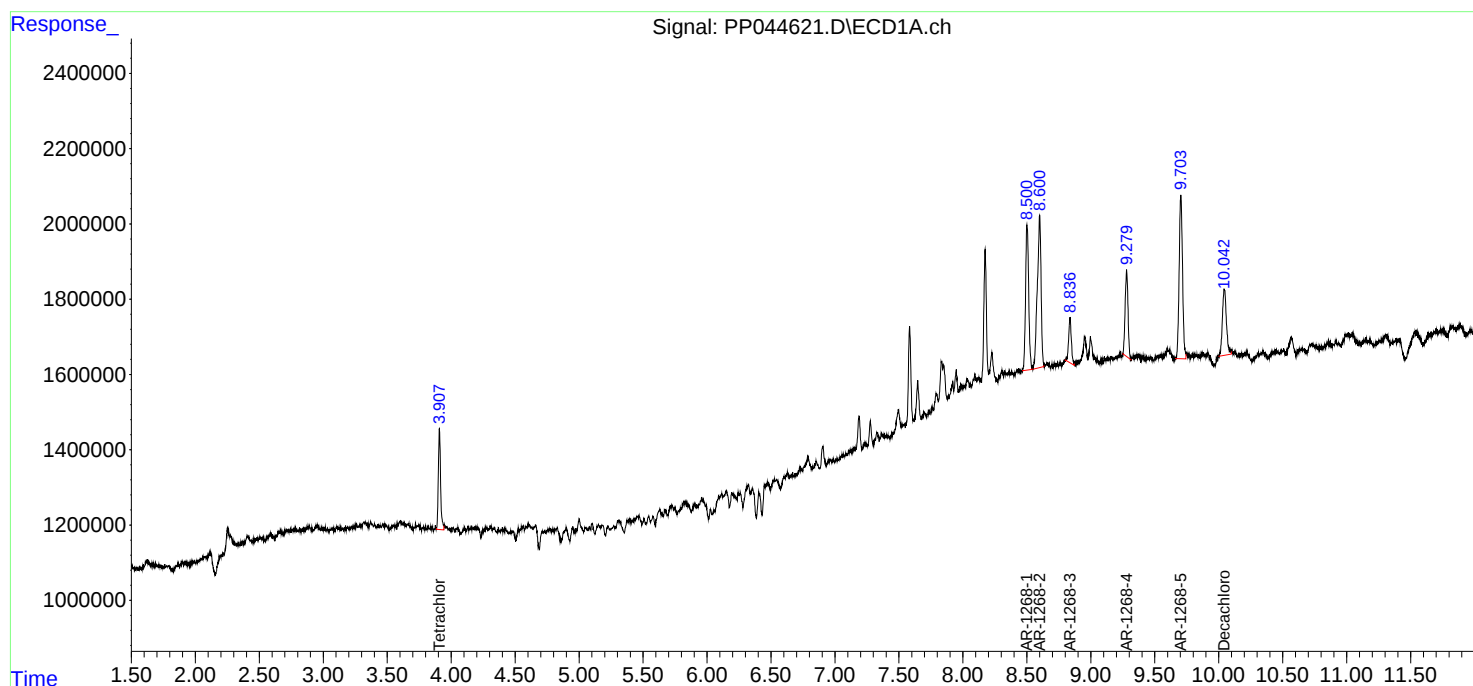

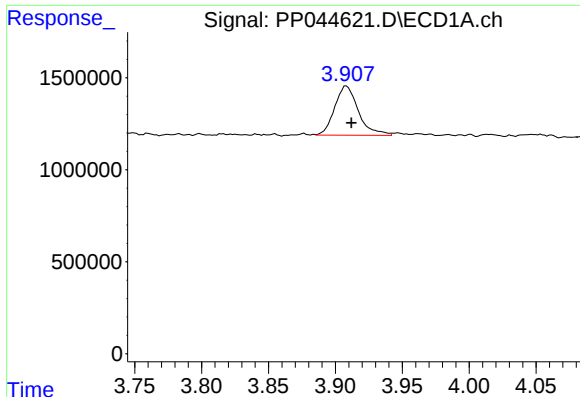


#1 Tetrachloro-m-xylene

R.T.: 3.908 min
Delta R.T.: -0.004 min
Response: 3290710
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-21A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

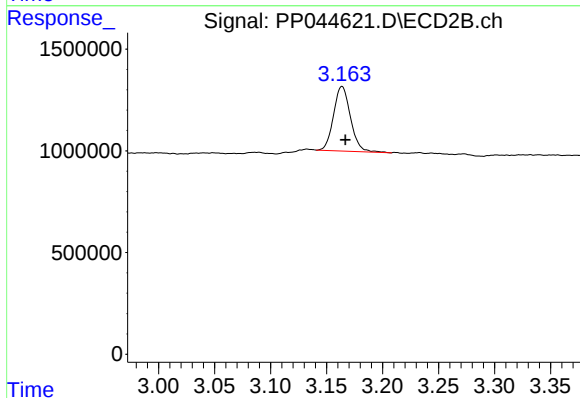


#1 Tetrachloro-m-xylene

R.T.: 3.164 min
Delta R.T.: -0.003 min
Response: 3346584
Conc: 1.91 ng/ml

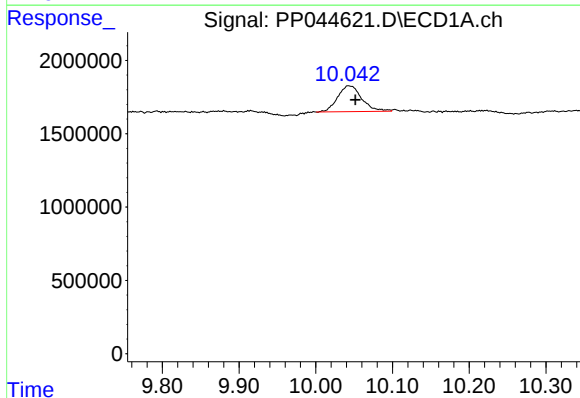


#2 Decachlorobiphenyl

R.T.: 10.043 min
Delta R.T.: -0.009 min
Response: 3855338
Conc: 2.80 ng/ml

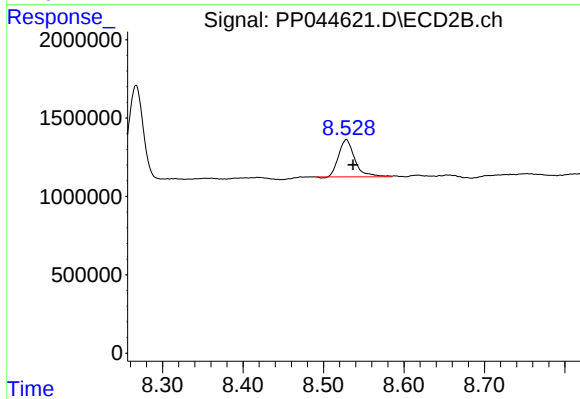

#2 Decachlorobiphenyl

R.T.: 8.528 min
Delta R.T.: -0.008 min
Response: 3310360
Conc: 2.16 ng/ml

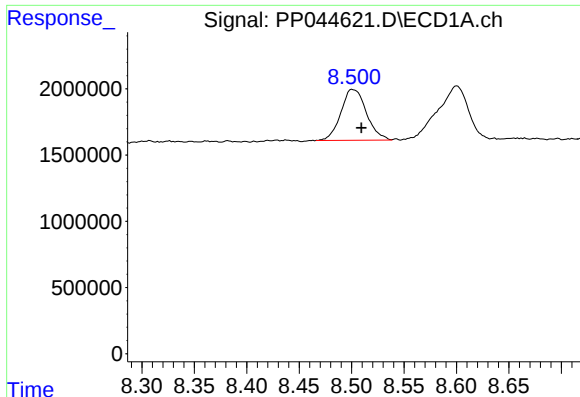


#41 AR-1268-1

R.T.: 8.501 min
Delta R.T.: -0.008 min
Response: 6530952
Conc: 33.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-21A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

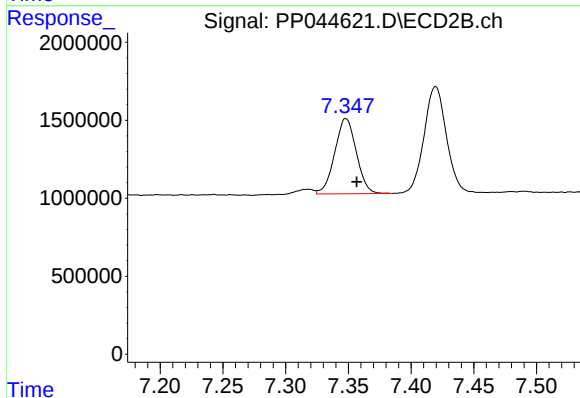


#41 AR-1268-1

R.T.: 7.348 min
Delta R.T.: -0.009 min
Response: 5781504
Conc: 25.42 ng/ml

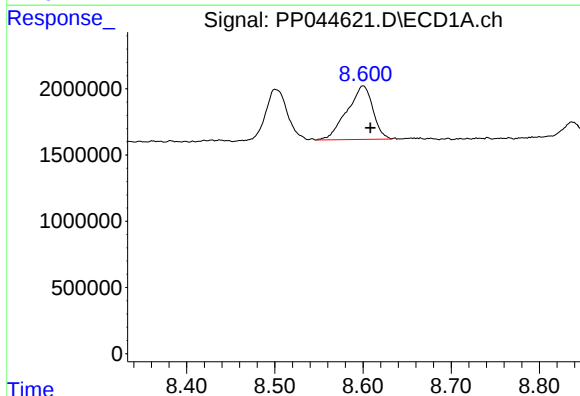


#42 AR-1268-2

R.T.: 8.600 min
Delta R.T.: -0.008 min
Response: 8213433
Conc: 45.09 ng/ml

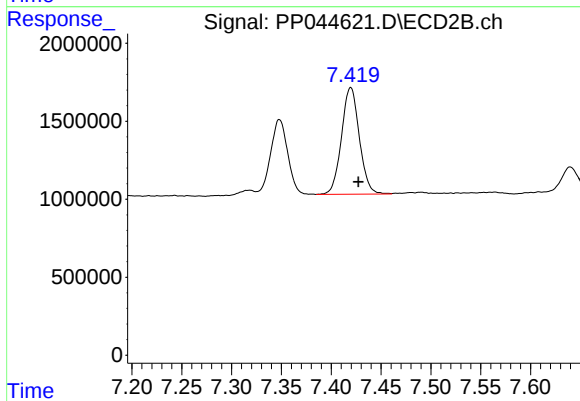

#42 AR-1268-2

R.T.: 7.420 min
Delta R.T.: -0.008 min
Response: 8527072
Conc: 41.62 ng/ml

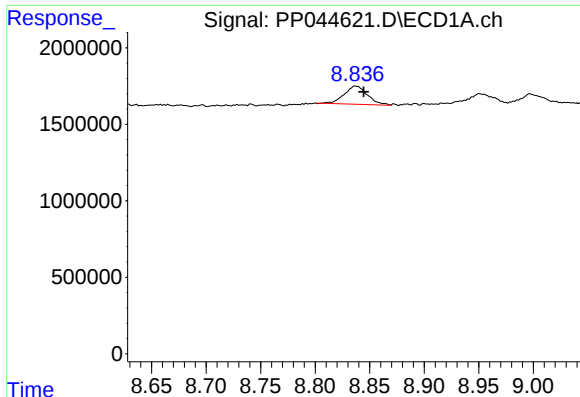


#43 AR-1268-3

R.T.: 8.837 min
Delta R.T.: -0.007 min
Response: 1769217
Conc: 11.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-21A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

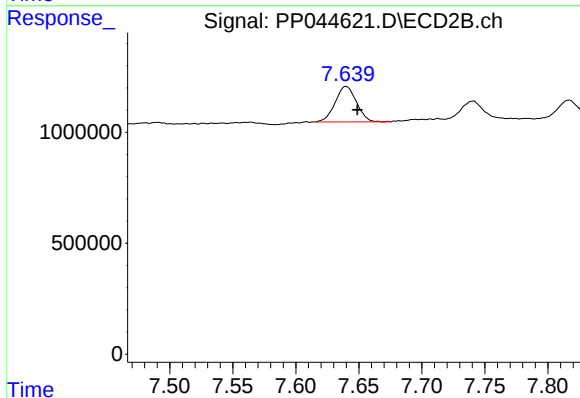


#43 AR-1268-3

R.T.: 7.640 min
Delta R.T.: -0.009 min
Response: 1877108
Conc: 10.74 ng/ml

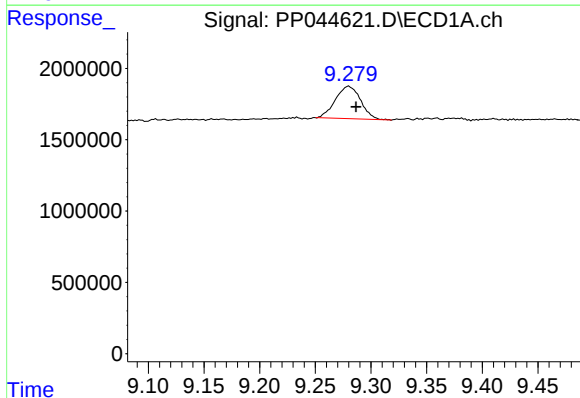


#44 AR-1268-4

R.T.: 9.280 min
Delta R.T.: -0.007 min
Response: 3589699
Conc: 57.37 ng/ml

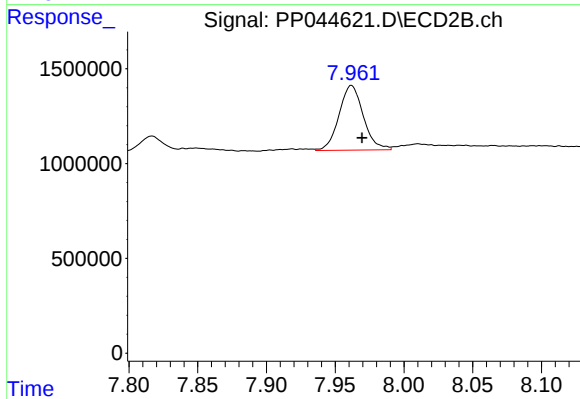

#44 AR-1268-4

R.T.: 7.962 min
Delta R.T.: -0.008 min
Response: 4197878
Conc: 51.73 ng/ml

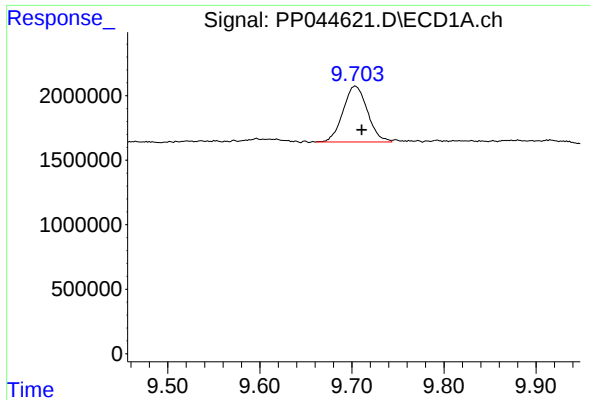


#45 AR-1268-5

R.T.: 9.704 min
Delta R.T.: -0.007 min
Response: 7966559
Conc: 16.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-21A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2022
Supervised By :Ankita Jodhani 03/14/2022

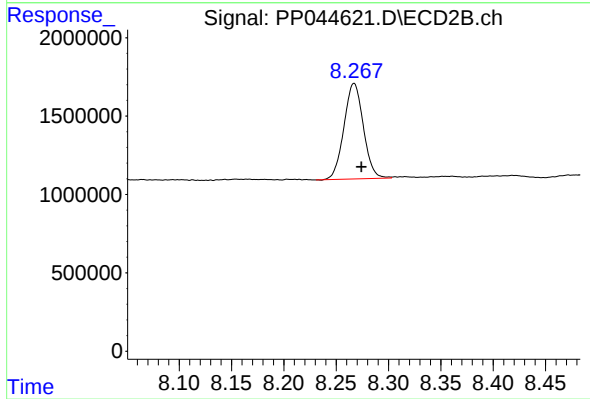

#45 AR-1268-5

R.T.: 8.267 min
Delta R.T.: -0.007 min
Response: 7877682
Conc: 14.62 ng/ml