

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 9:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 12:22:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.860	4.265	2082263	949683	24.065	23.376
2)	SA Decachlor...	10.790	9.593	2003456	637806	23.722	23.901
Target Compounds							
9)	L2 AR-1221-2	5.206	0.000	16044	0	22.832	N.D. #
30)	L6 AR-1254-5	8.411	0.000	18454	0	4.688	N.D. #
35)	L7 AR-1260-5	9.028	0.000	63623	0	8.224	N.D. #
37)	L8 AR-1262-2	9.028	0.000	63623	0	7.361	N.D. #
39)	L8 AR-1262-4	9.429	0.000	2559	0	0.516	N.D. #
42)	L9 AR-1268-2	9.429	0.000	2559	0	0.253	N.D. #
43)	L9 AR-1268-3	9.643	0.000	16643	0	1.874	N.D. #
45)	L9 AR-1268-5	10.474	0.000	20377	0	0.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 9:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 12:22:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

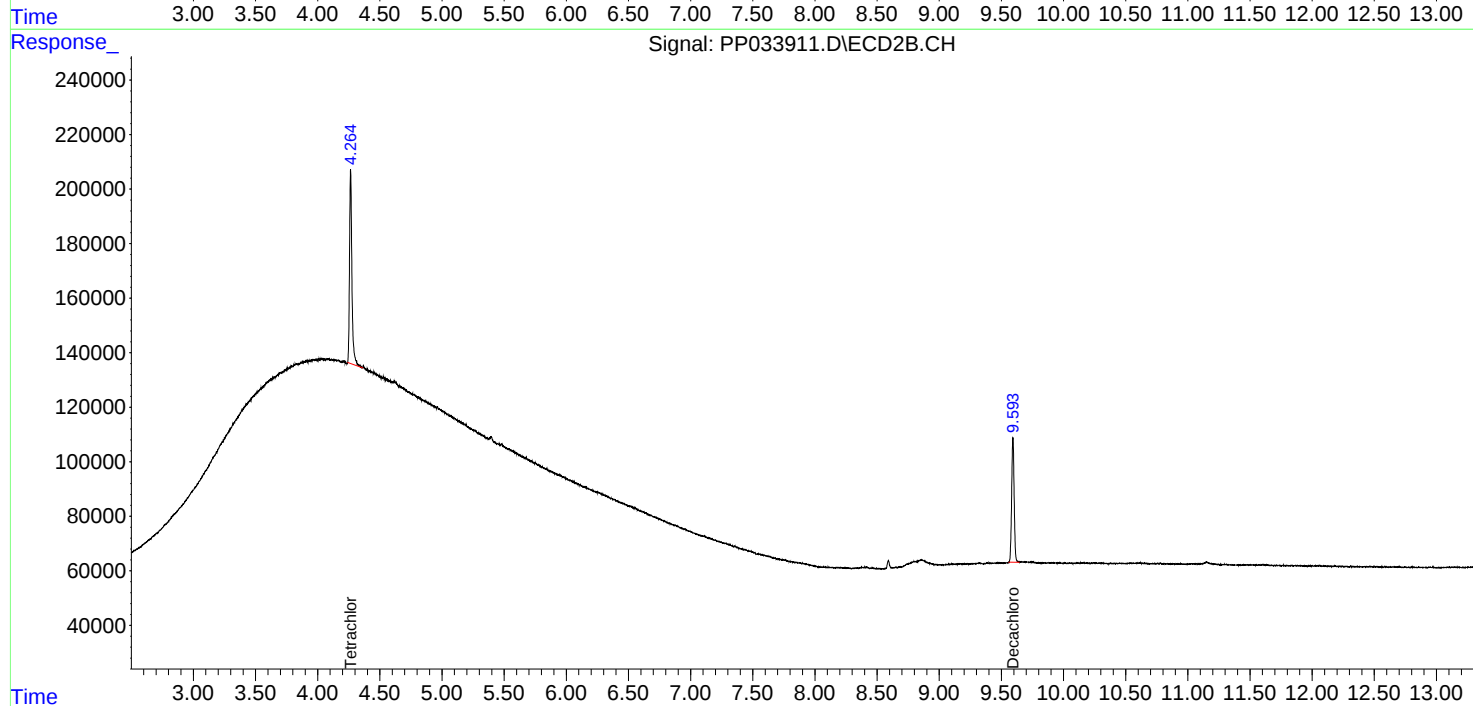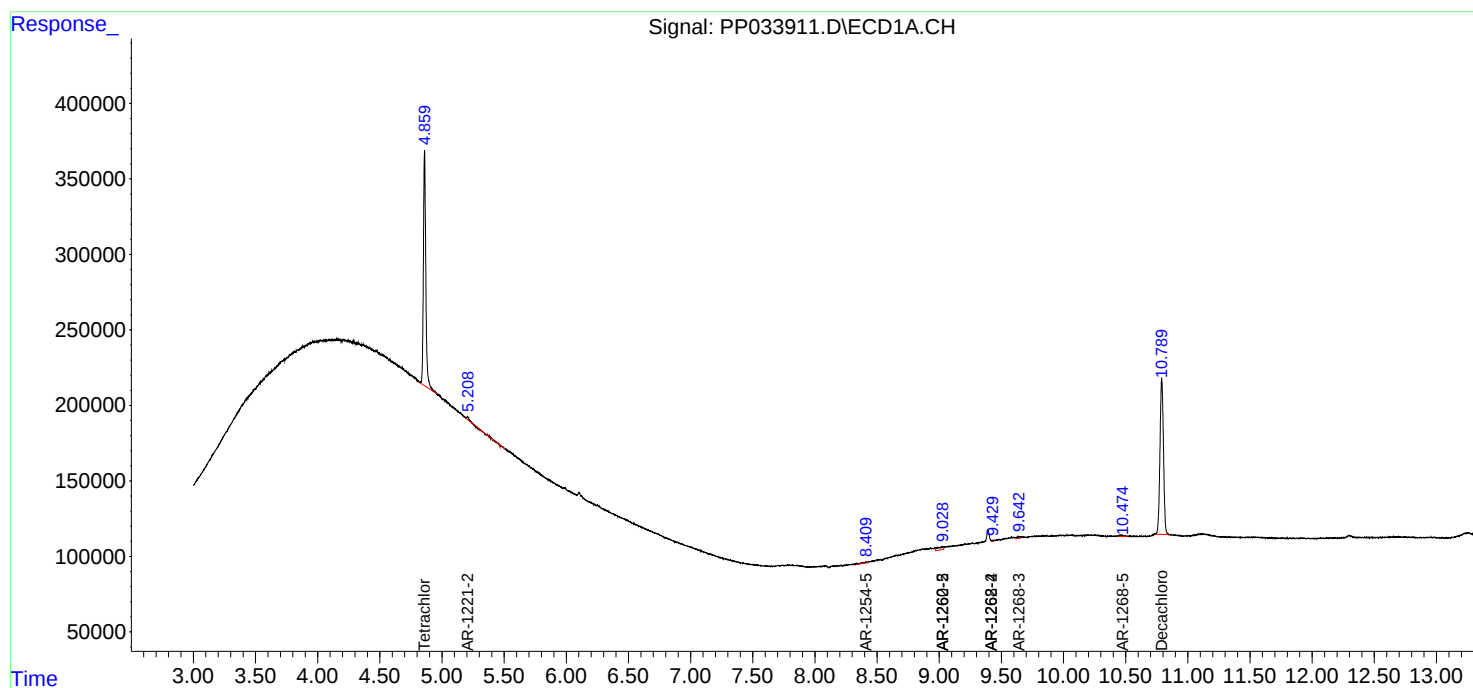


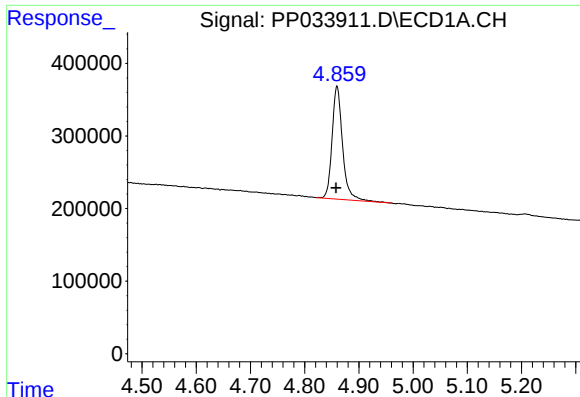

#1 Tetrachloro-m-xylene


R.T.: 4.860 min
Delta R.T.: 0.002 min
Response: 2082263
Conc: 24.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

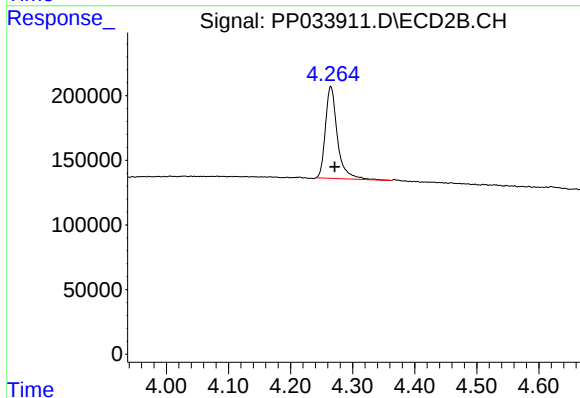


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 949683
Conc: 23.38 ng/ml

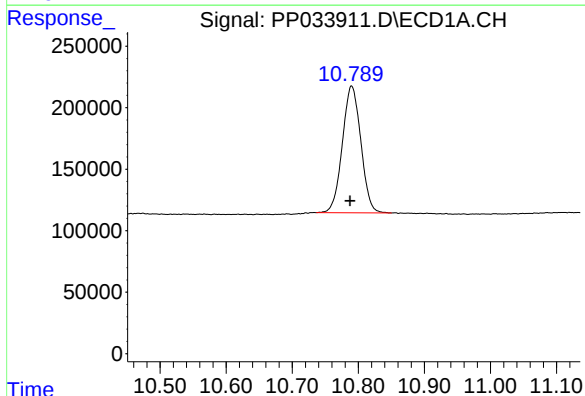


#2 Decachlorobiphenyl

R.T.: 10.790 min
Delta R.T.: 0.002 min
Response: 2003456
Conc: 23.72 ng/ml

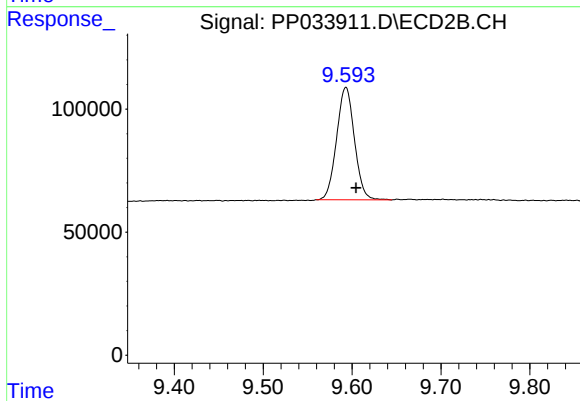

#2 Decachlorobiphenyl


R.T.: 9.593 min
Delta R.T.: -0.011 min
Response: 637806
Conc: 23.90 ng/ml

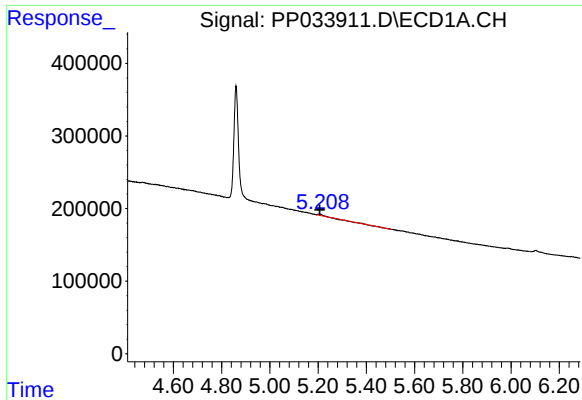

#9 AR-1221-2


R.T.: 5.206 min
Delta R.T.: 0.000 min
Response: 16044
Conc: 22.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

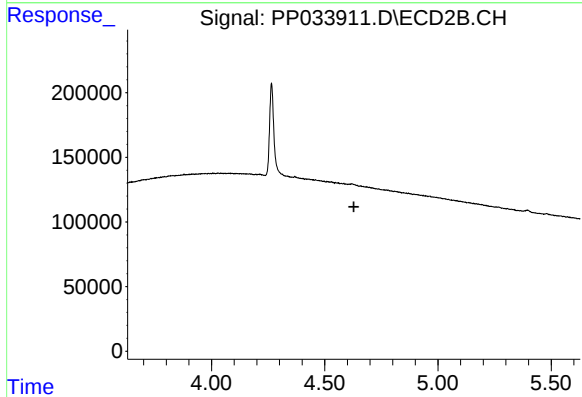


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

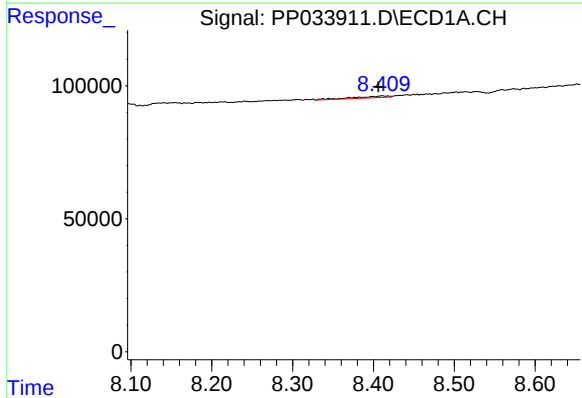


#30 AR-1254-5

R.T.: 8.411 min
Delta R.T.: 0.005 min
Response: 18454
Conc: 4.69 ng/ml

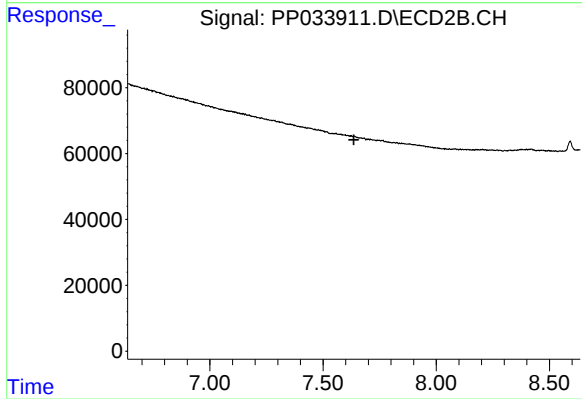

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.636 min
Response: 0
Conc: N.D.

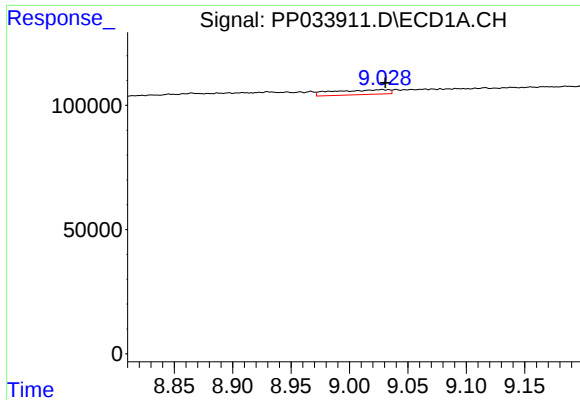

#35 AR-1260-5


R.T.: 9.028 min
Delta R.T.: -0.003 min
Response: 63623
Conc: 8.22 ng/ml

Instrument :
ECD_P
ClientSampleId :

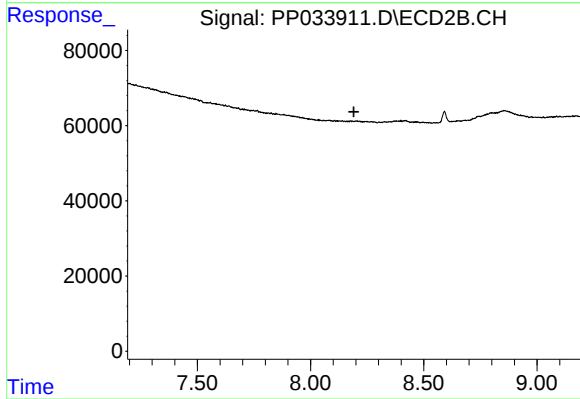


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

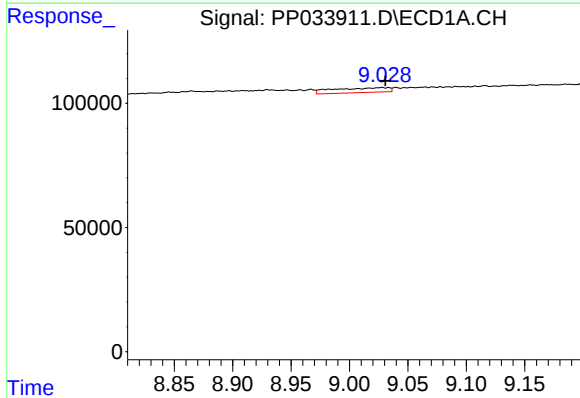


#37 AR-1262-2

R.T.: 9.028 min
Delta R.T.: -0.003 min
Response: 63623
Conc: 7.36 ng/ml

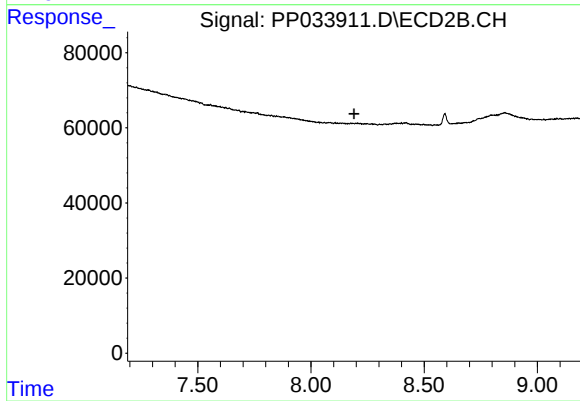

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

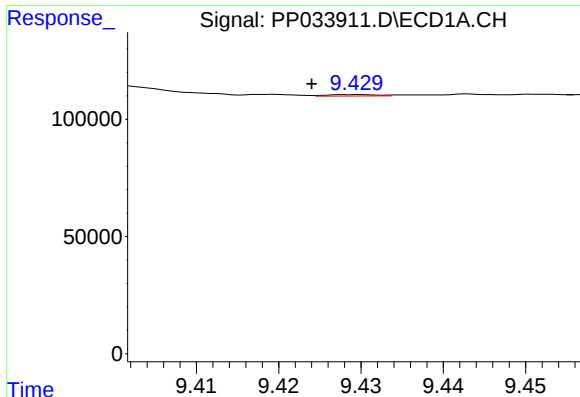

#39 AR-1262-4


R.T.: 9.429 min
Delta R.T.: 0.005 min
Response: 2559
Conc: 0.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

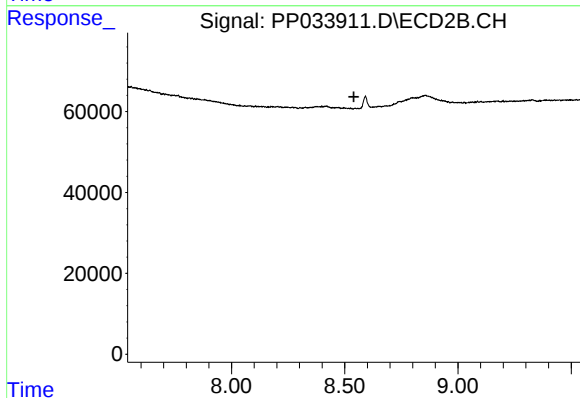


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

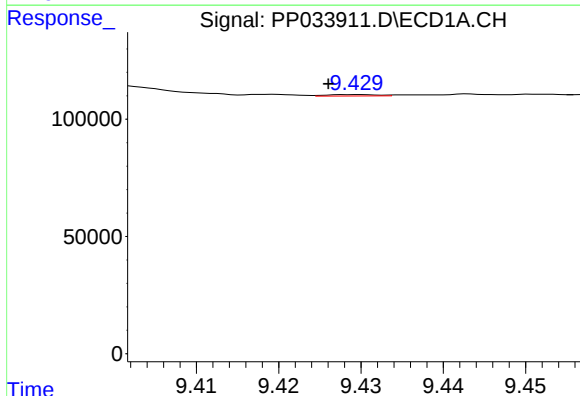


#42 AR-1268-2

R.T.: 9.429 min
Delta R.T.: 0.003 min
Response: 2559
Conc: 0.25 ng/ml

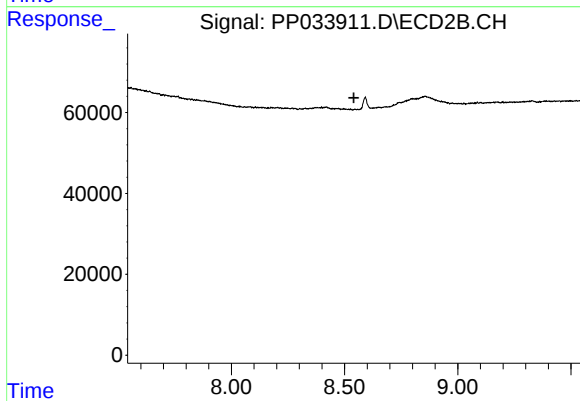

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

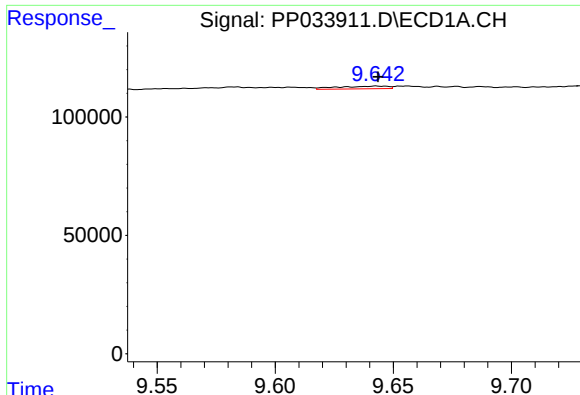

#43 AR-1268-3


R.T.: 9.643 min
Delta R.T.: 0.000 min
Response: 16643
Conc: 1.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

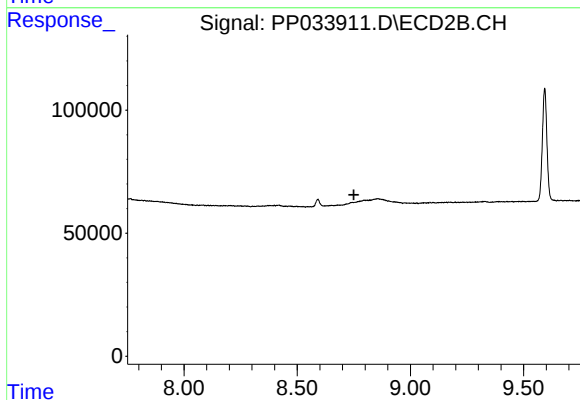


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

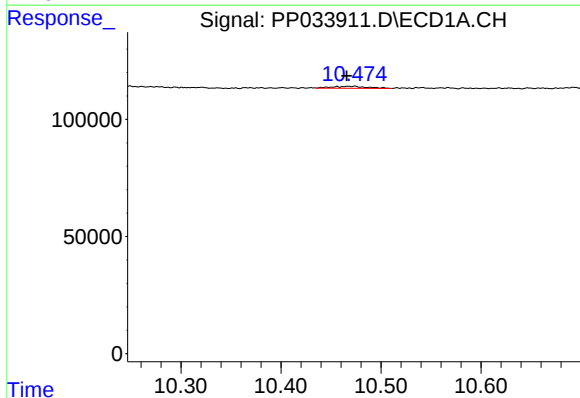

#45 AR-1268-5

R.T.: 10.474 min
Delta R.T.: 0.008 min
Response: 20377
Conc: 0.69 ng/ml

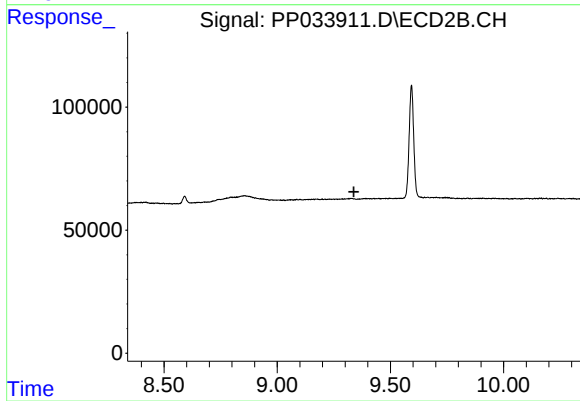

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.338 min
Response: 0
Conc: N.D.