

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033930.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 17:38
 Operator : DD\AJ
 Sample : PB135130BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 02:51:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.858	4.269	1790190	847452	20.690	20.860
2) SA Decachlor...	10.790	9.595	1878746	573825	22.246	21.503
Target Compounds						
9) L2 AR-1221-2	5.206	0.000	31357	0	44.625	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033930.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 17:38
Operator : DD\AJ
Sample : PB135130BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 02:51:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

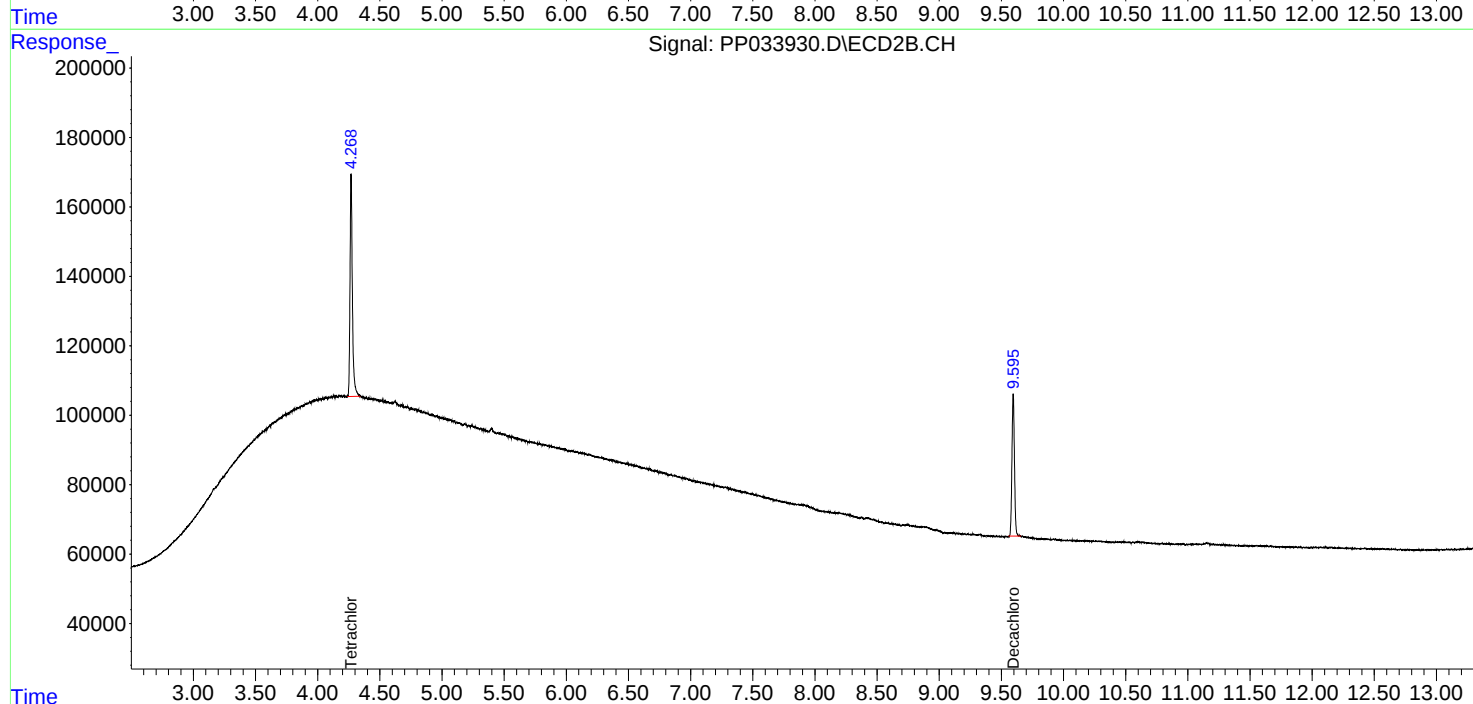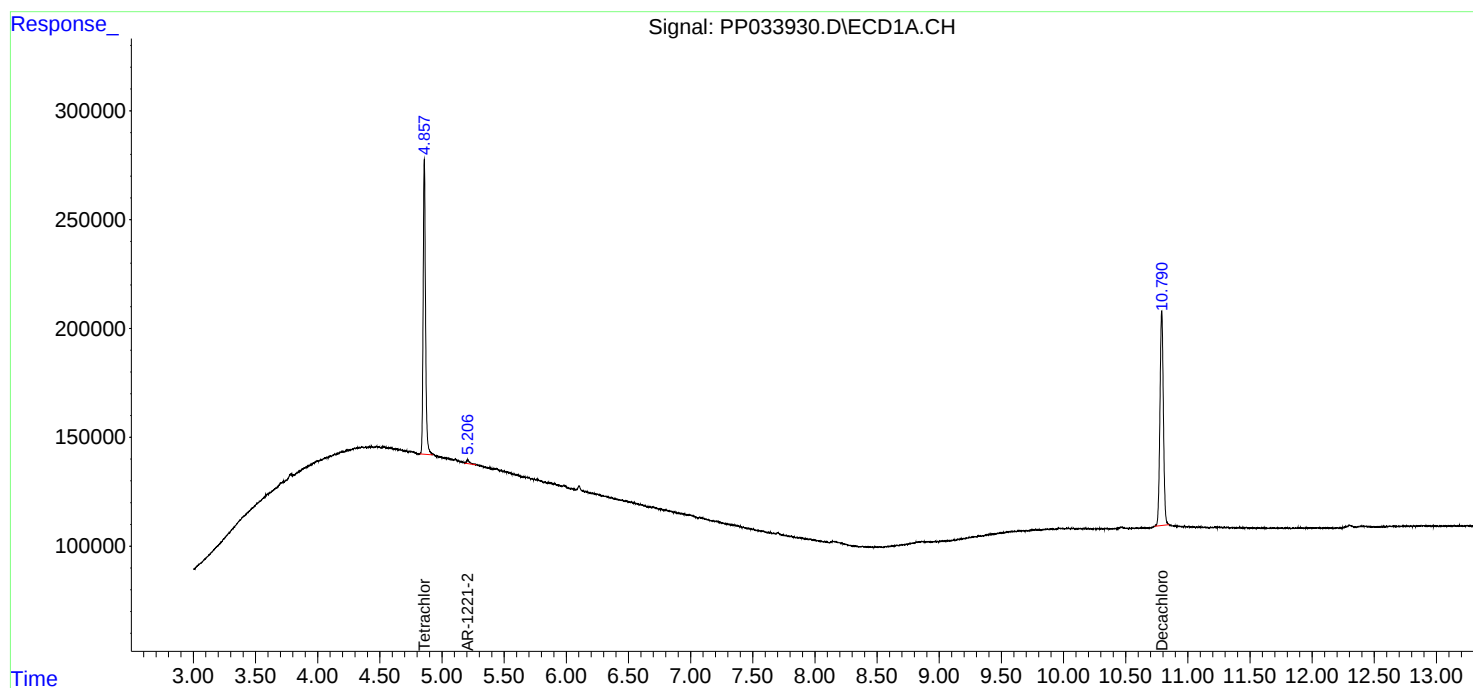


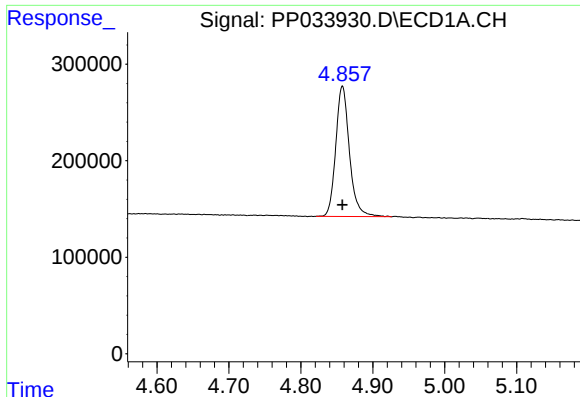

#1 Tetrachloro-m-xylene


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 1790190
Conc: 20.69 ng/ml

Instrument :
ECD_P
ClientSampleId :

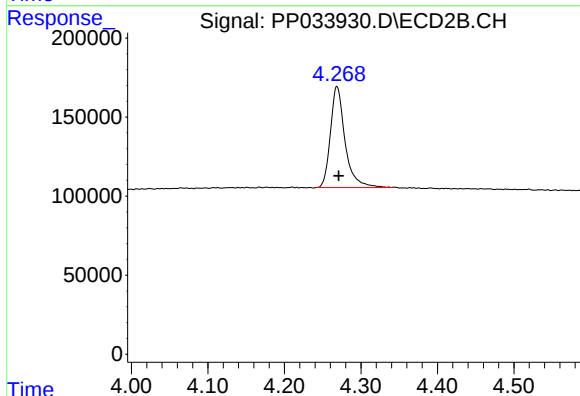


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.002 min
Response: 847452
Conc: 20.86 ng/ml

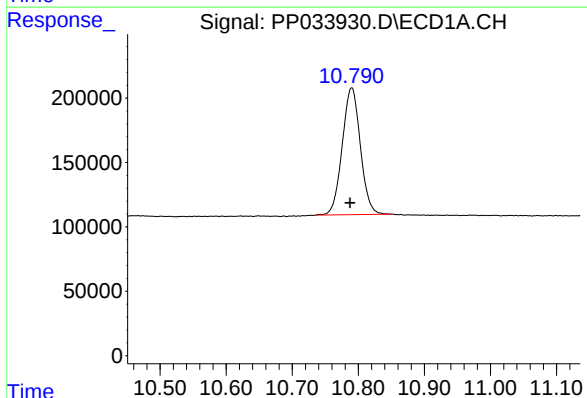


#2 Decachlorobiphenyl

R.T.: 10.790 min
Delta R.T.: 0.002 min
Response: 1878746
Conc: 22.25 ng/ml

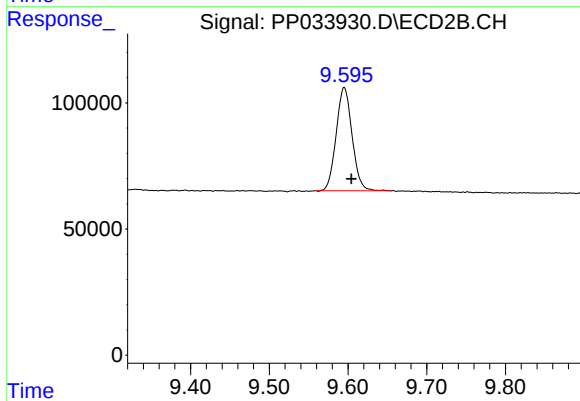

#2 Decachlorobiphenyl


R.T.: 9.595 min
Delta R.T.: -0.009 min
Response: 573825
Conc: 21.50 ng/ml

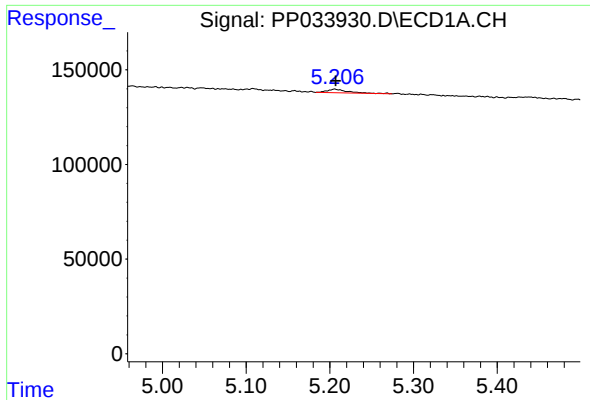

#9 AR-1221-2

R.T.: 5.206 min
Delta R.T.: -0.001 min
Response: 31357
Conc: 44.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

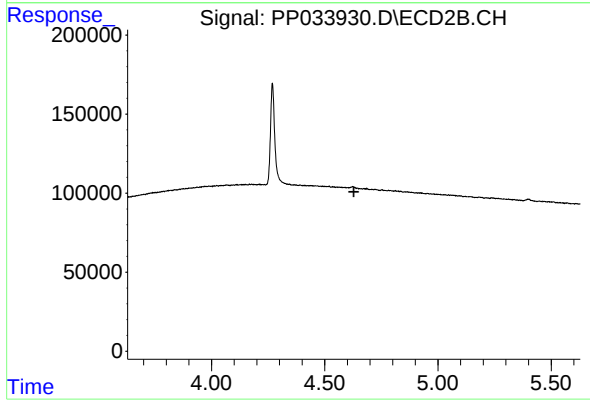

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.