

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033968.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 5:45
 Operator : DD\AJ
 Sample : M1652-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:36:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.854	4.265	1918851	915708	22.177	22.540
2)	SA Decachlor...	10.783	9.589	1474222	504340	17.456	18.900
Target Compounds							
8)	L2 AR-1221-1	5.102	0.000	74001	0	80.192	N.D. #
30)	L6 AR-1254-5	8.411	7.635	91221	46705	23.175	24.797
34)	L7 AR-1260-4	8.685f	0.000	36910	0	9.965	N.D. #
36)	L8 AR-1262-1	0.000	7.635	0	46705	N.D.	43.936 #
38)	L8 AR-1262-3	0.000	8.498f	0	51241	N.D.	35.880 #
39)	L8 AR-1262-4	9.409	0.000	33614	0	6.782	N.D. #
41)	L9 AR-1268-1	0.000	8.498f	0	51241	N.D.	13.397 #
42)	L9 AR-1268-2	9.409f	0.000	33614	0	3.326	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033968.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 5:45
Operator : DD\AJ
Sample : M1652-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:36:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

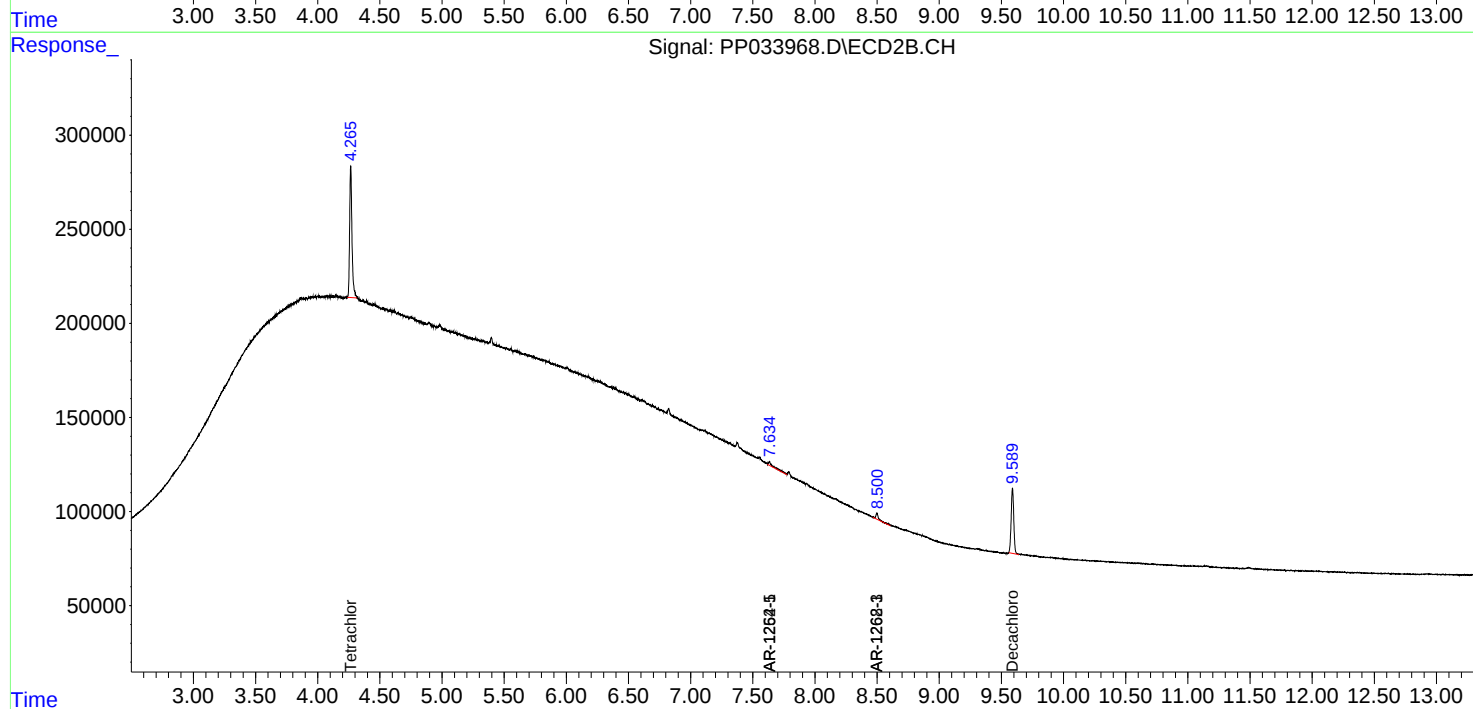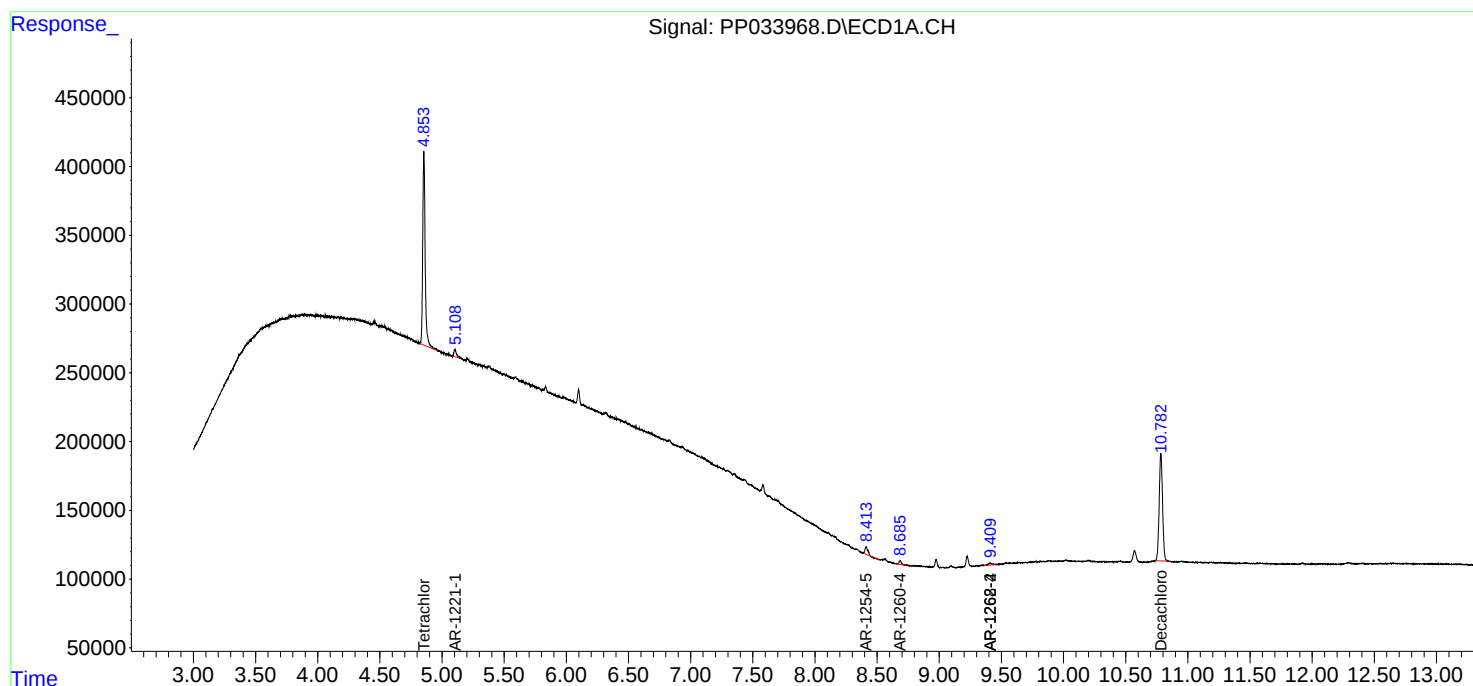


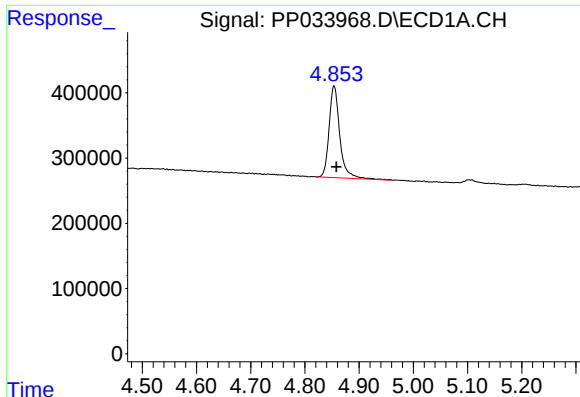

#1 Tetrachloro-m-xylene


R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 1918851
Conc: 22.18 ng/ml

Instrument :
ECD_P
ClientSampleId :

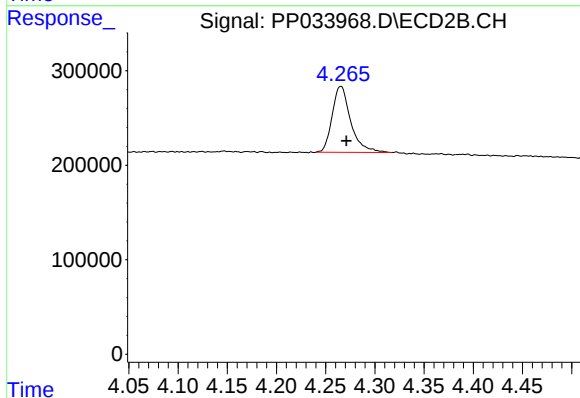


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 915708
Conc: 22.54 ng/ml

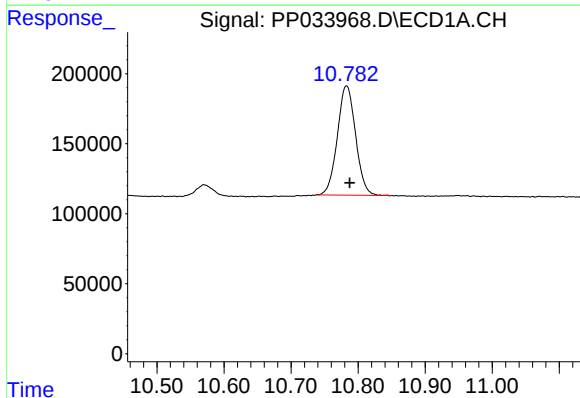


#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: -0.005 min
Response: 1474222
Conc: 17.46 ng/ml

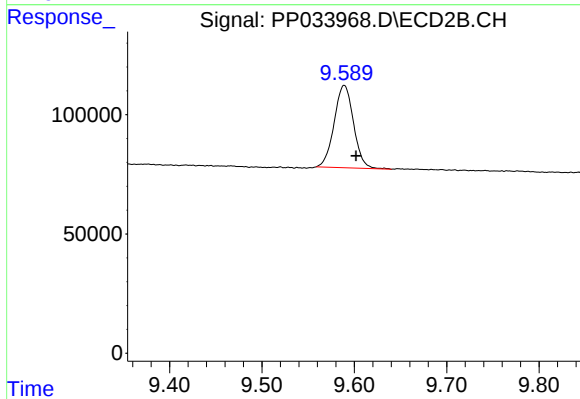

#2 Decachlorobiphenyl


R.T.: 9.589 min
Delta R.T.: -0.013 min
Response: 504340
Conc: 18.90 ng/ml

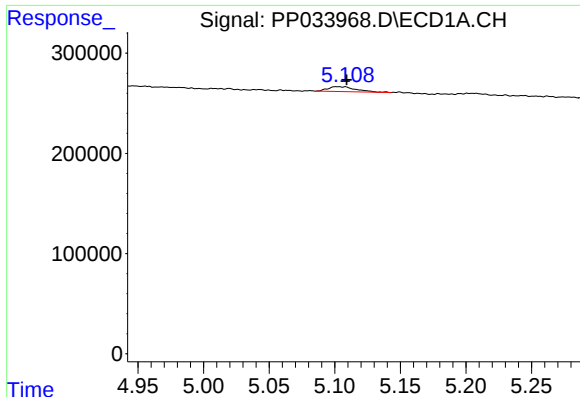

#8 AR-1221-1


R.T.: 5.102 min
Delta R.T.: -0.007 min
Response: 74001
Conc: 80.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

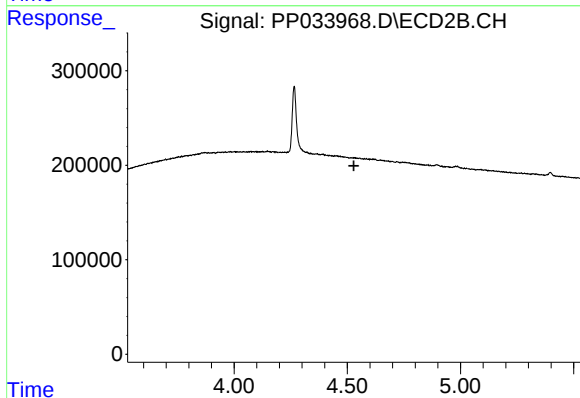


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.529 min
Response: 0
Conc: N.D.

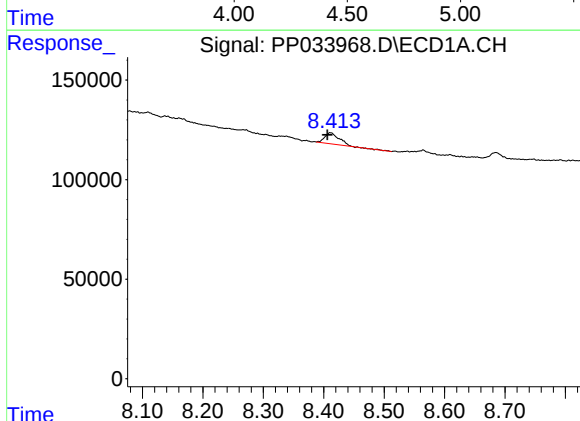


#30 AR-1254-5

R.T.: 8.411 min
Delta R.T.: 0.005 min
Response: 91221
Conc: 23.18 ng/ml

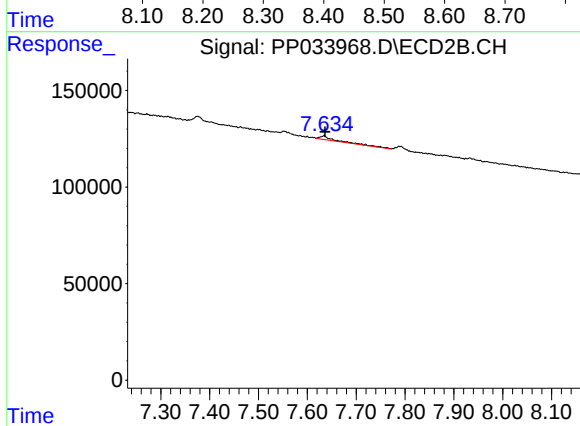

#30 AR-1254-5


R.T.: 7.635 min
Delta R.T.: -0.002 min
Response: 46705
Conc: 24.80 ng/ml

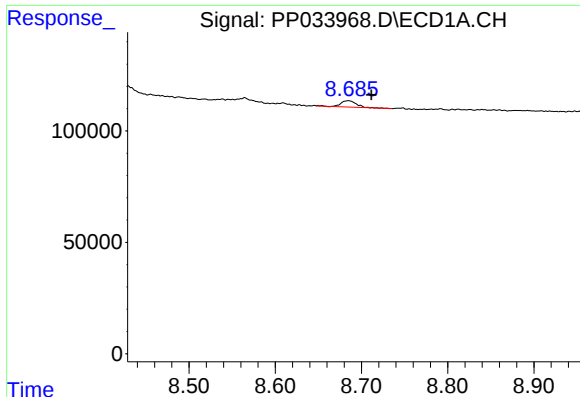

#34 AR-1260-4


R.T.: 8.685 min
Delta R.T.: -0.026 min
Response: 36910
Conc: 9.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

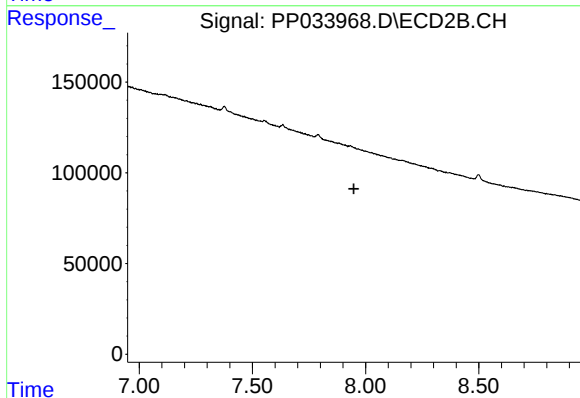


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.948 min
Response: 0
Conc: N.D.

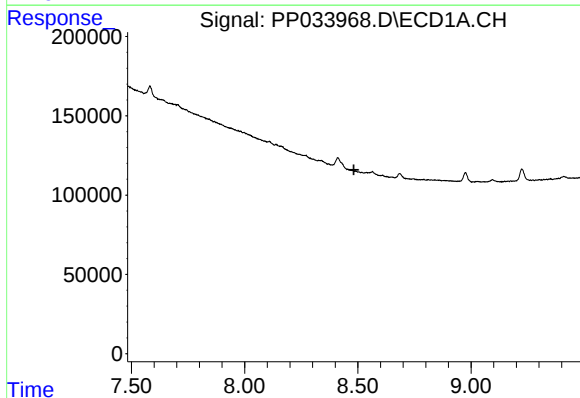


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.483 min
Response: 0
Conc: N.D.

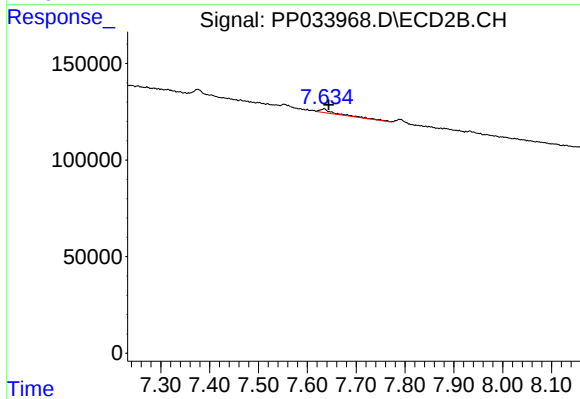

#36 AR-1262-1


R.T.: 7.635 min
Delta R.T.: -0.009 min
Response: 46705
Conc: 43.94 ng/ml

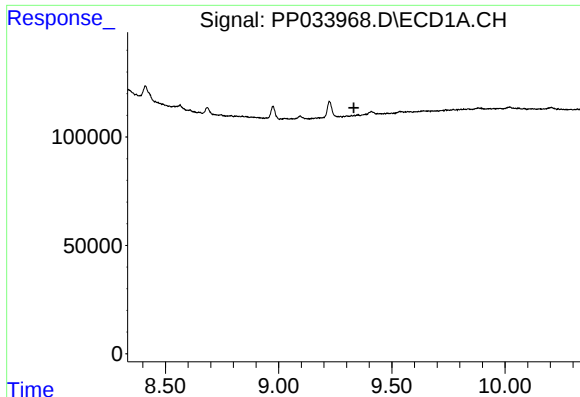

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

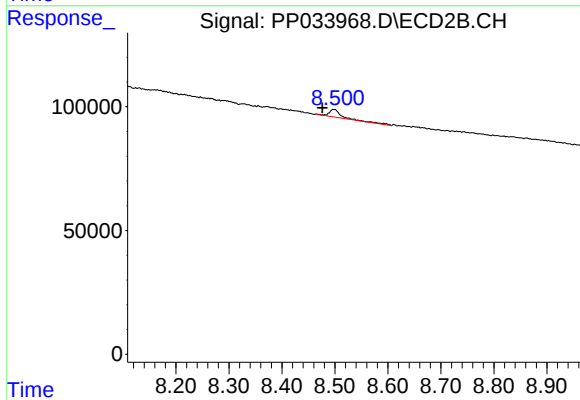


#38 AR-1262-3

R.T.: 8.498 min
Delta R.T.: 0.021 min
Response: 51241
Conc: 35.88 ng/ml

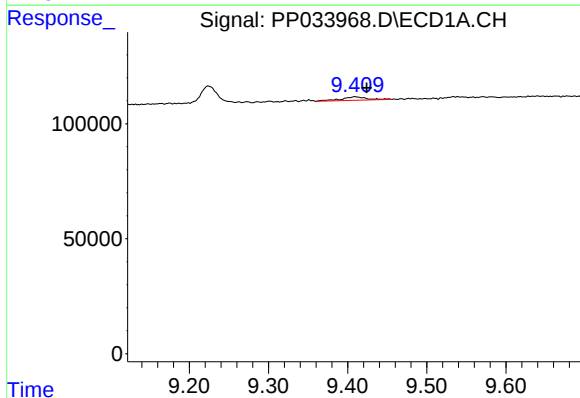


#39 AR-1262-4

R.T.: 9.409 min
Delta R.T.: -0.015 min
Response: 33614
Conc: 6.78 ng/ml

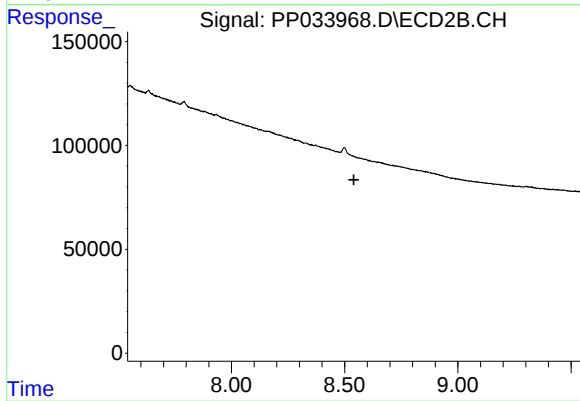

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

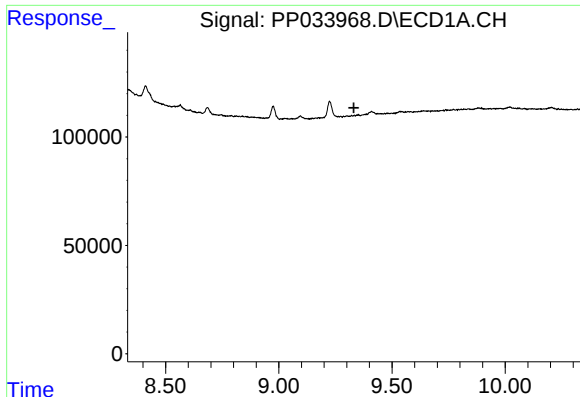

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

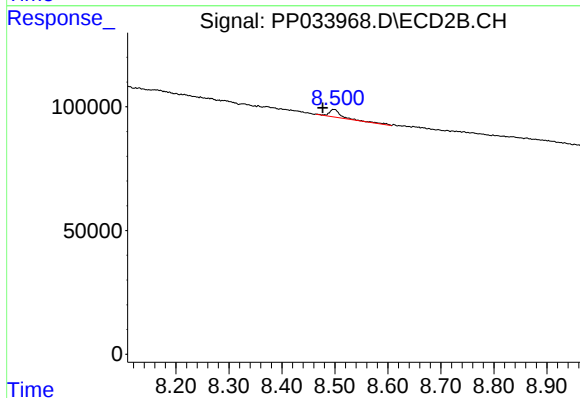


#41 AR-1268-1

R.T.: 8.498 min
Delta R.T.: 0.021 min
Response: 51241
Conc: 13.40 ng/ml

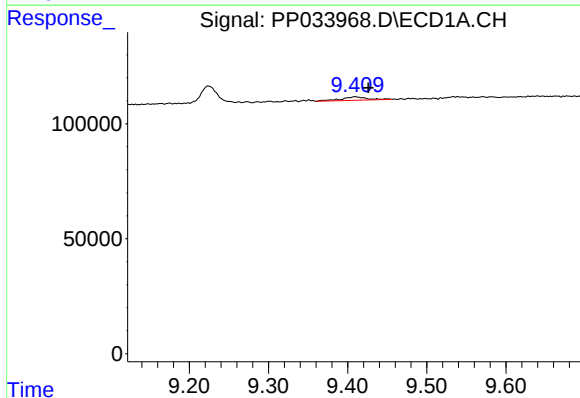

#42 AR-1268-2

R.T.: 9.409 min
Delta R.T.: -0.017 min
Response: 33614
Conc: 3.33 ng/ml

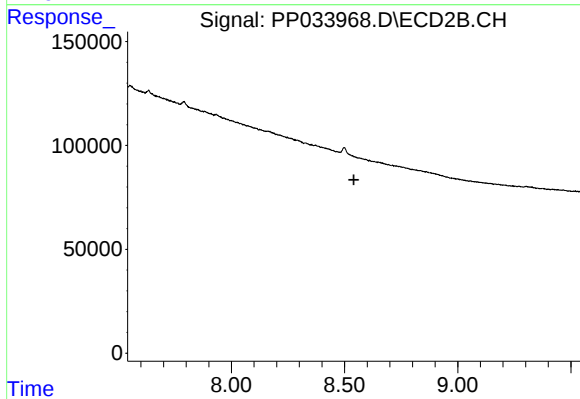

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.