

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033924.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 15:56
 Operator : DD\AJ
 Sample : M1624-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WALLS-3

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:05:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 02:47:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.857	4.269	1274797	597566	14.733	14.709
2) SA Decachlor...	10.789	9.594	3001121	888180	35.536	33.283
Target Compounds						
26) L6 AR-1254-1	7.076	6.396	218768	121944	74.888	74.798
27) L6 AR-1254-2	7.306	6.553	386191	90689	84.931	63.498 #
28) L6 AR-1254-3	7.685	6.975	440771	234247	89.148	102.344
29) L6 AR-1254-4	7.981	7.211	360413	114536	105.076	90.113
30) L6 AR-1254-5	8.409	7.638	759254	266879	192.892m	141.692 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033924.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 15:56
Operator : DD\AJ
Sample : M1624-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WALLS-3


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 02:47:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

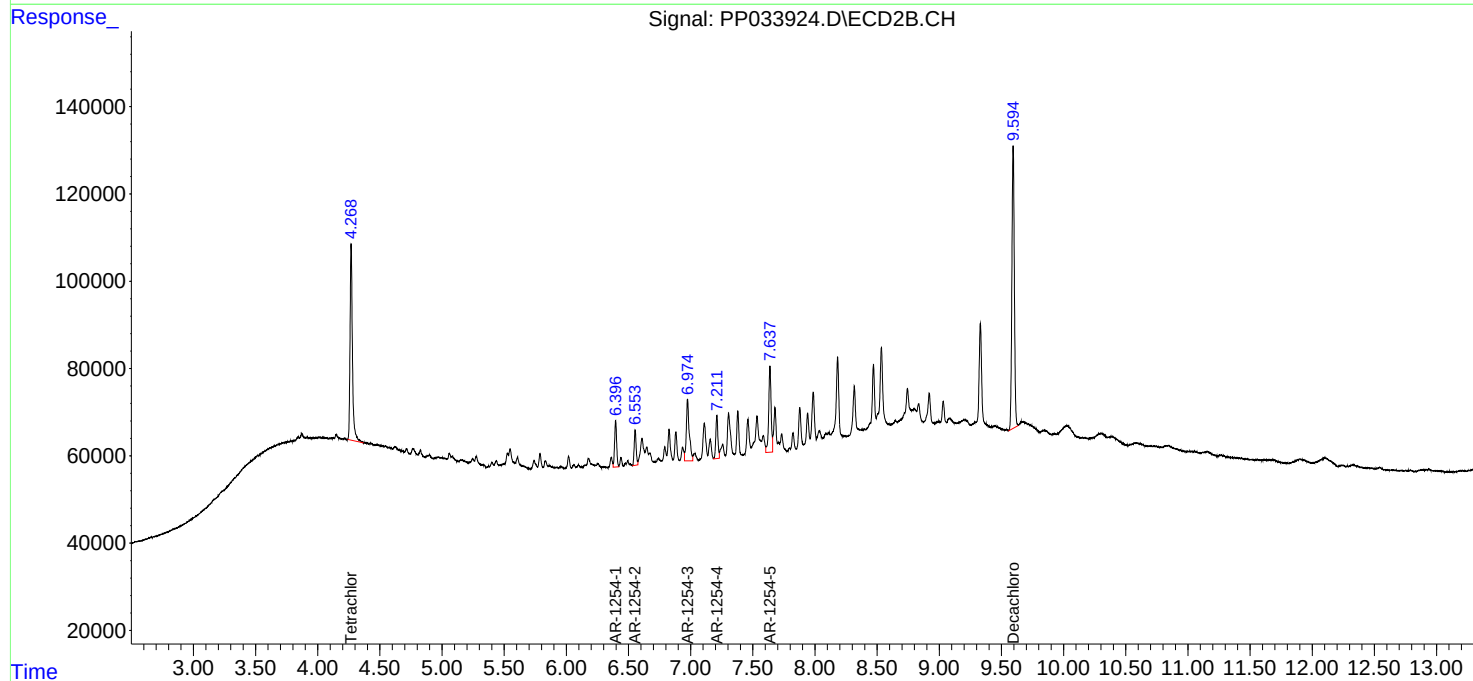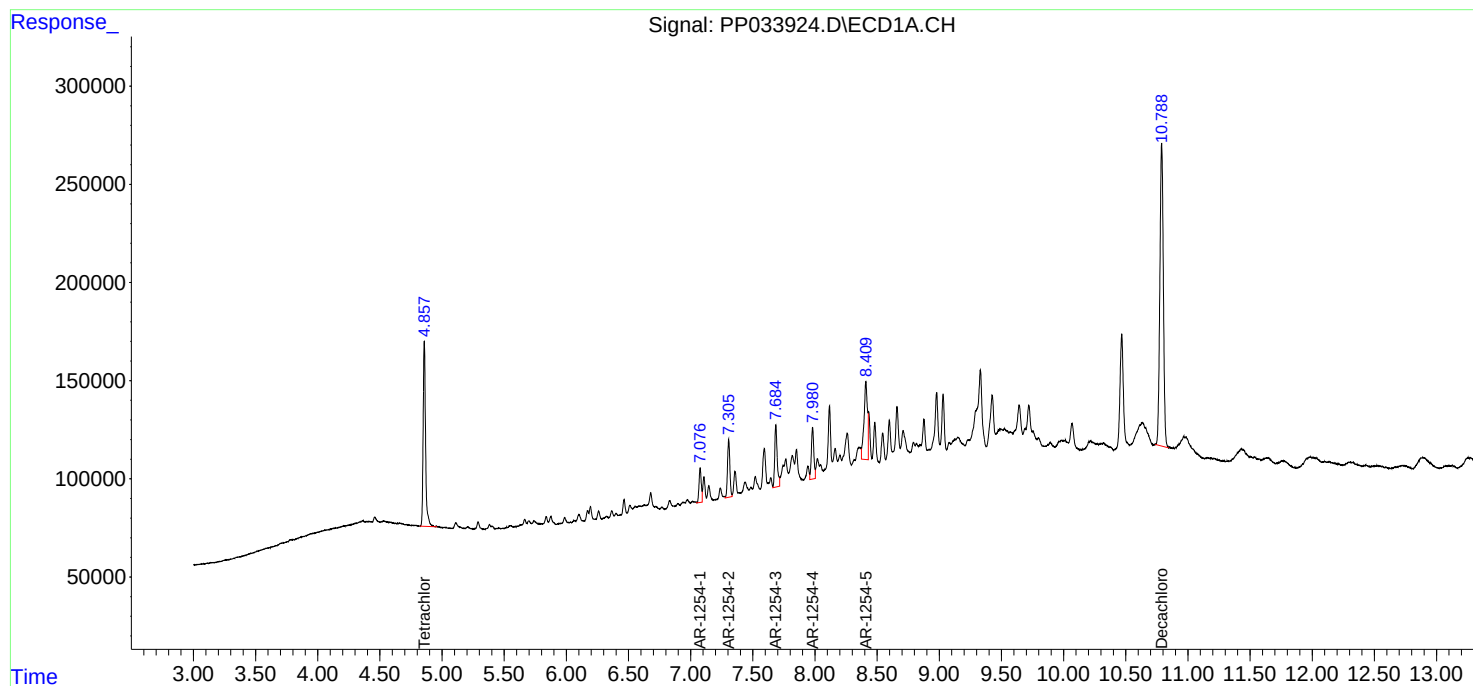

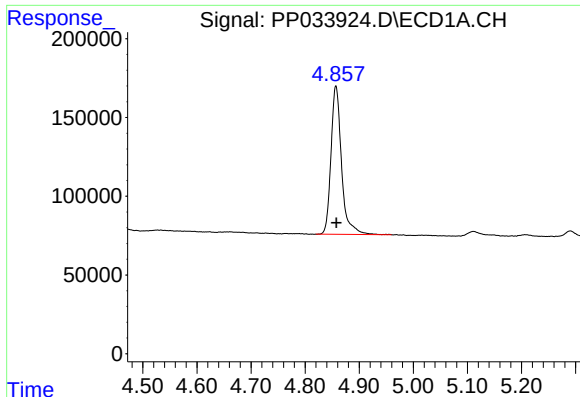


#1 Tetrachloro-m-xylene

R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 1274797
Conc: 14.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
WALLS-3


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:04 PM

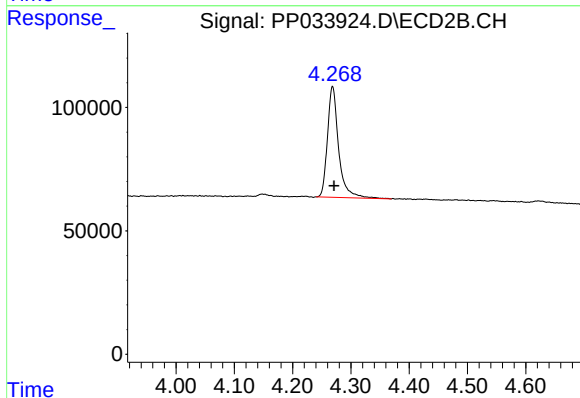


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.003 min
Response: 597566
Conc: 14.71 ng/ml

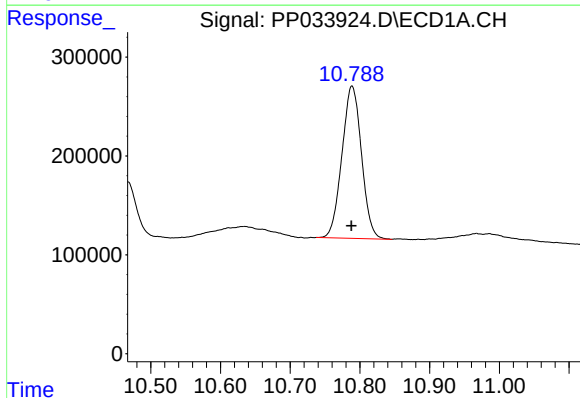


#2 Decachlorobiphenyl

R.T.: 10.789 min
Delta R.T.: 0.000 min
Response: 3001121
Conc: 35.54 ng/ml

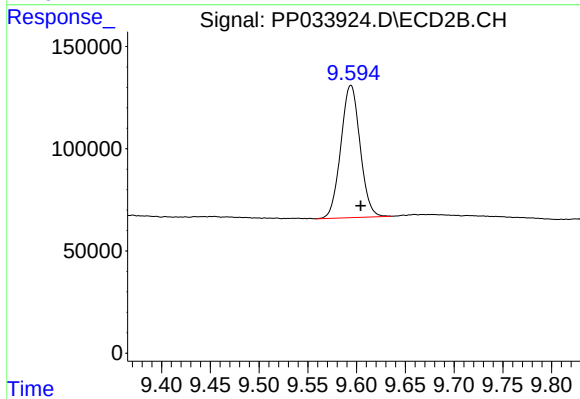

#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: -0.010 min
Response: 888180
Conc: 33.28 ng/ml

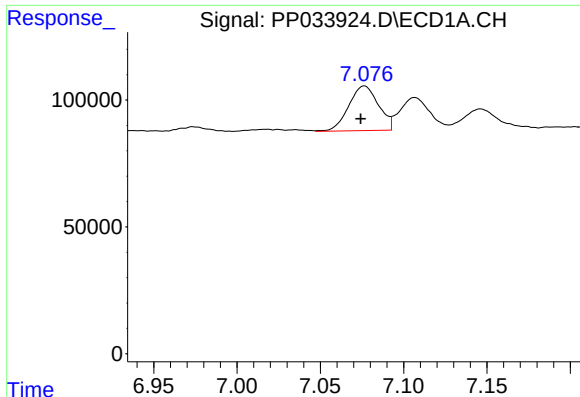


#26 AR-1254-1

R.T.: 7.076 min
Delta R.T.: 0.002 min
Response: 218768
Conc: 74.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
WALLS-3


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:04 PM

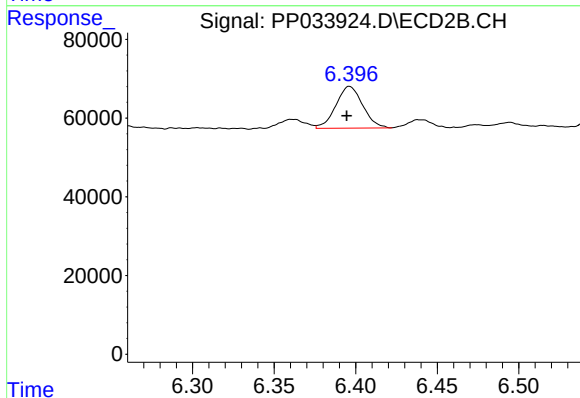


#26 AR-1254-1

R.T.: 6.396 min
Delta R.T.: 0.002 min
Response: 121944
Conc: 74.80 ng/ml

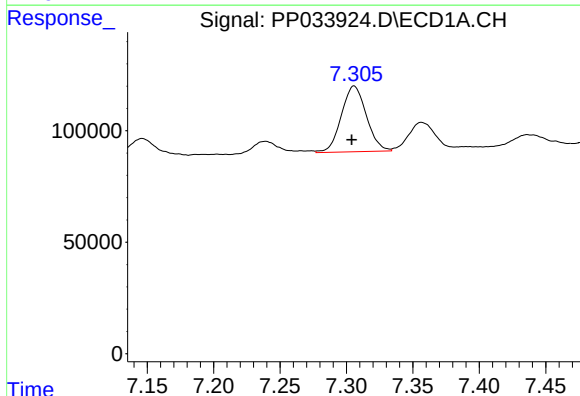


#27 AR-1254-2

R.T.: 7.306 min
Delta R.T.: 0.002 min
Response: 386191
Conc: 84.93 ng/ml

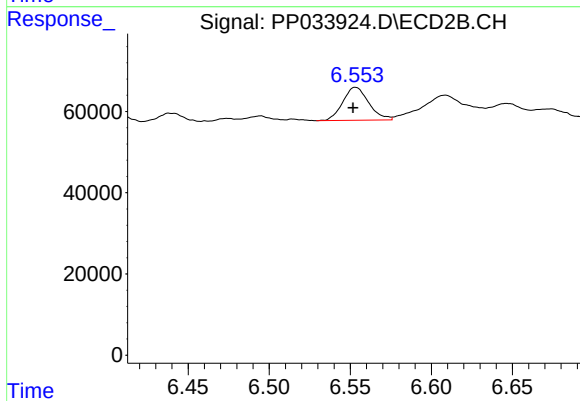

#27 AR-1254-2

R.T.: 6.553 min
Delta R.T.: 0.002 min
Response: 90689
Conc: 63.50 ng/ml

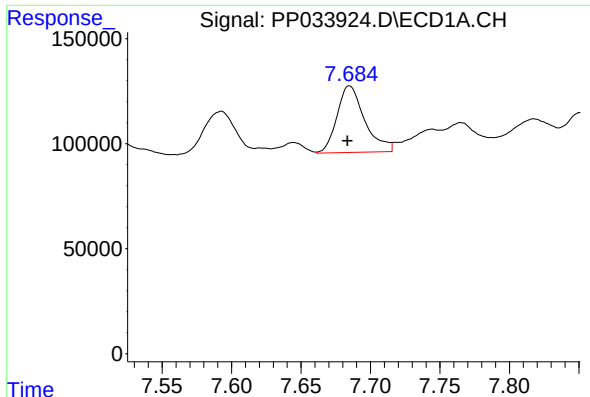


#28 AR-1254-3

R.T.: 7.685 min
Delta R.T.: 0.001 min
Response: 440771
Conc: 89.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
WALLS-3


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:04 PM

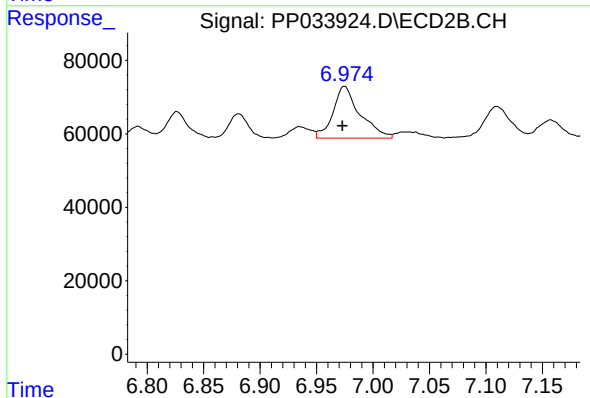


#28 AR-1254-3

R.T.: 6.975 min
Delta R.T.: 0.002 min
Response: 234247
Conc: 102.34 ng/ml

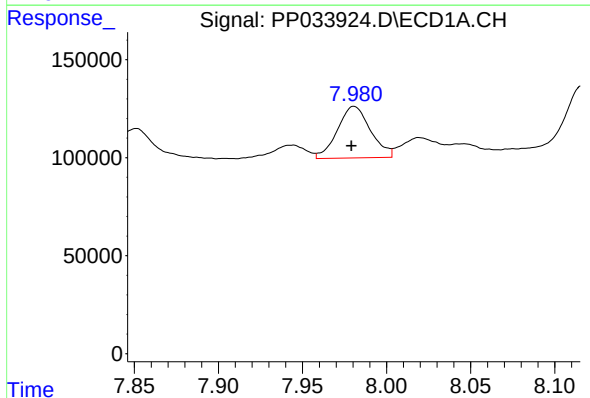


#29 AR-1254-4

R.T.: 7.981 min
Delta R.T.: 0.002 min
Response: 360413
Conc: 105.08 ng/ml

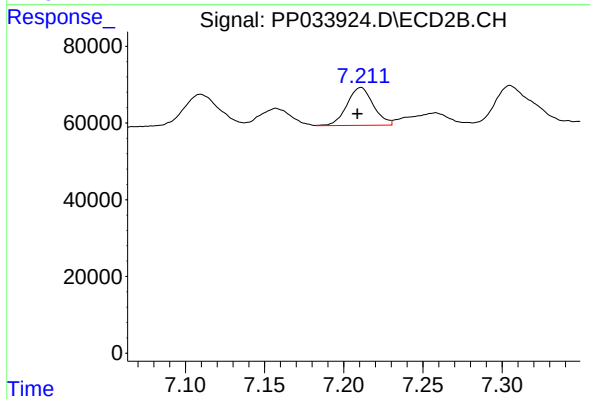

#29 AR-1254-4

R.T.: 7.211 min
Delta R.T.: 0.002 min
Response: 114536
Conc: 90.11 ng/ml

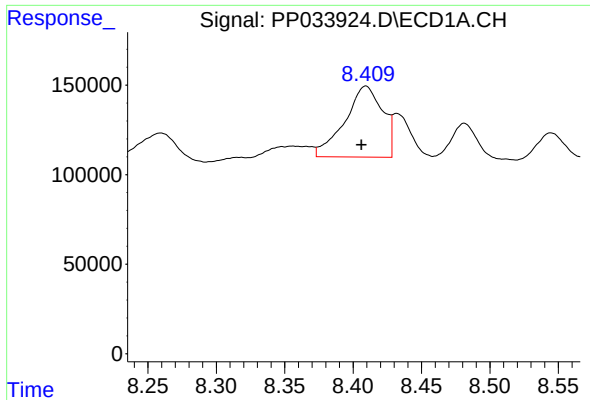


#30 AR-1254-5

R.T.: 8.409 min
Delta R.T.: 0.003 min
Response: 759254
Conc: 192.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
WALLS-3

Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:04 PM

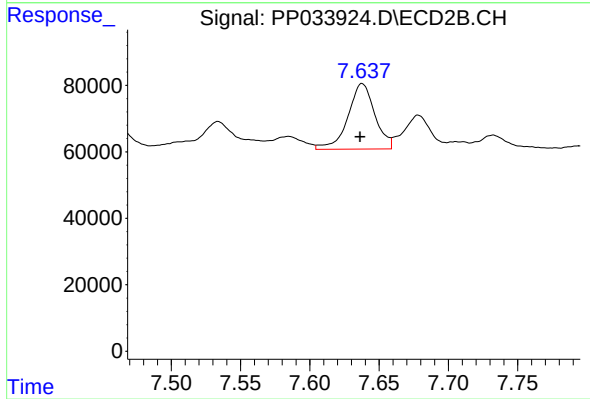

#30 AR-1254-5

R.T.: 7.638 min
Delta R.T.: 0.002 min
Response: 266879
Conc: 141.69 ng/ml