

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033936.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 19:20
 Operator : DD\AJ
 Sample : M1647-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP2-41732:34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 02:54:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.858	4.270	1814671	888273	20.973	21.865
2) SA Decachlor...	10.789	9.594	1448658	447242	17.153	16.760

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 19:20
Operator : DD\AJ
Sample : M1647-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP2-41732:34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 02:54:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

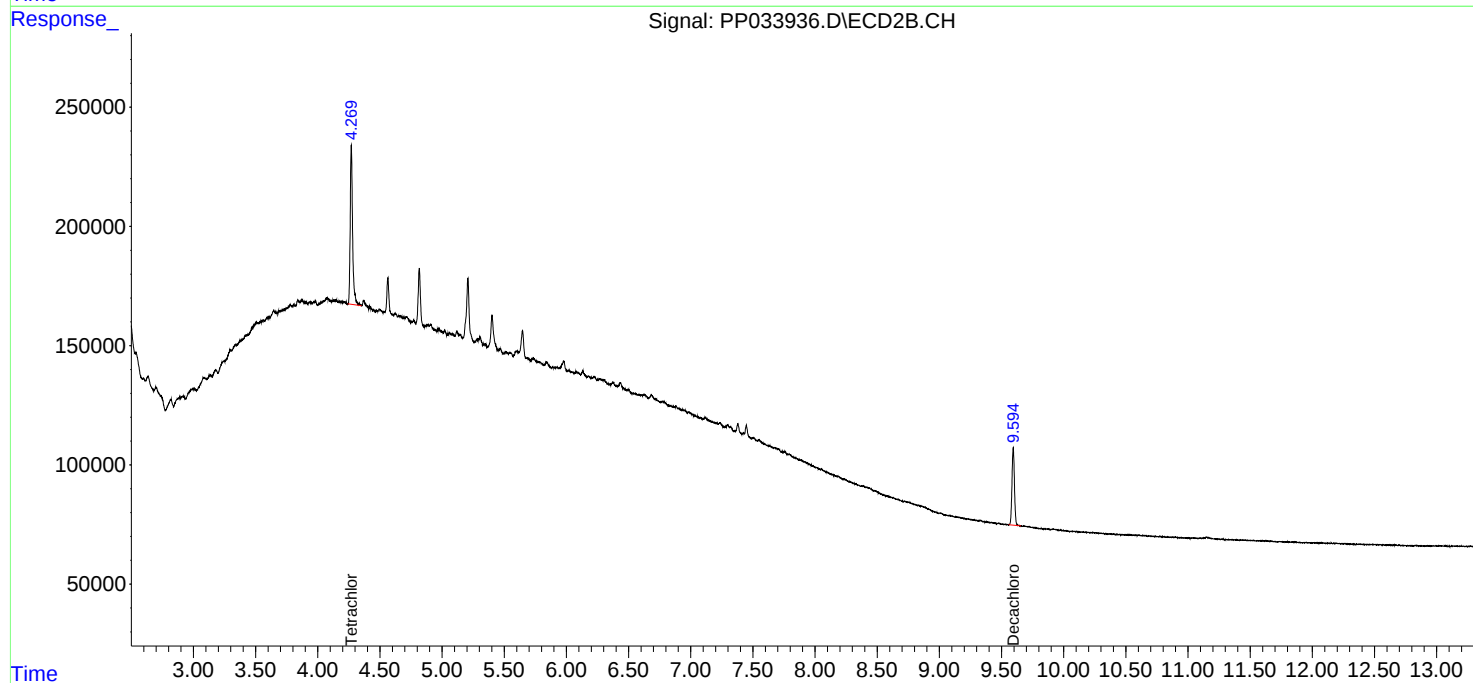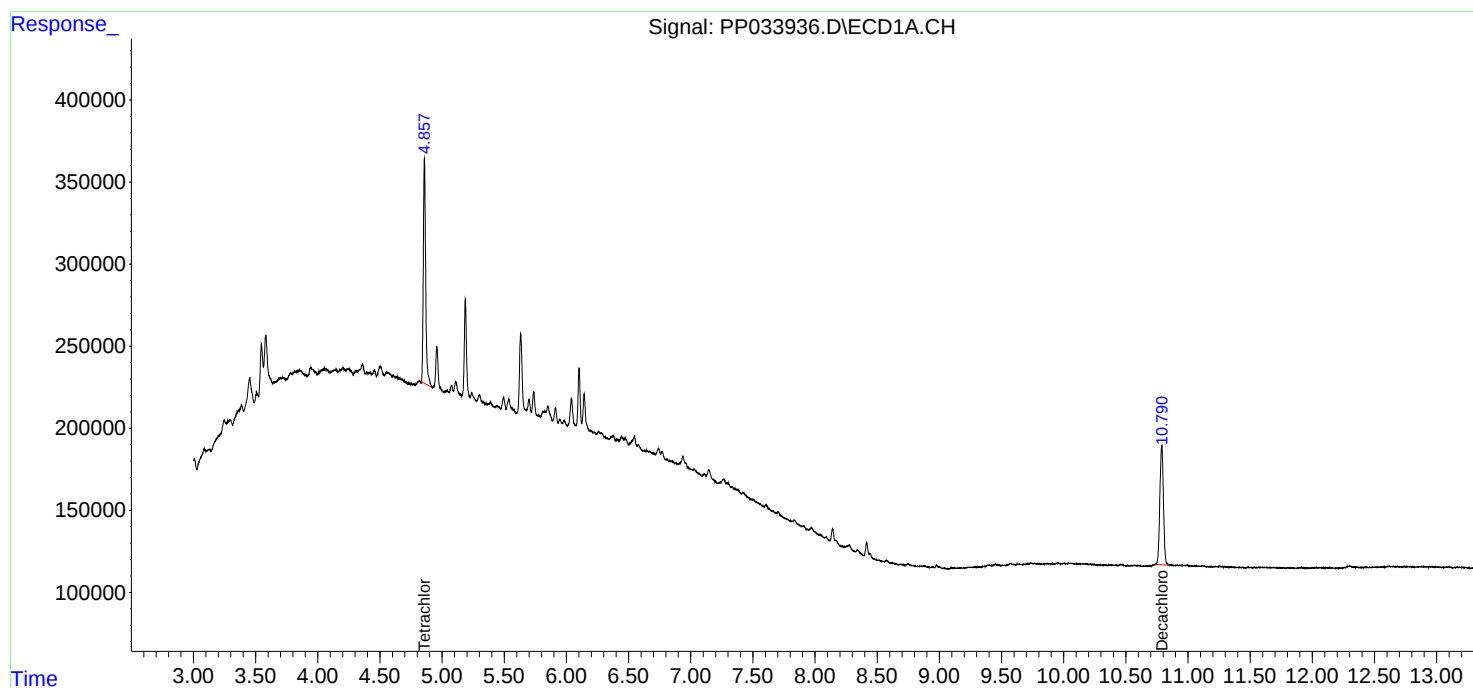


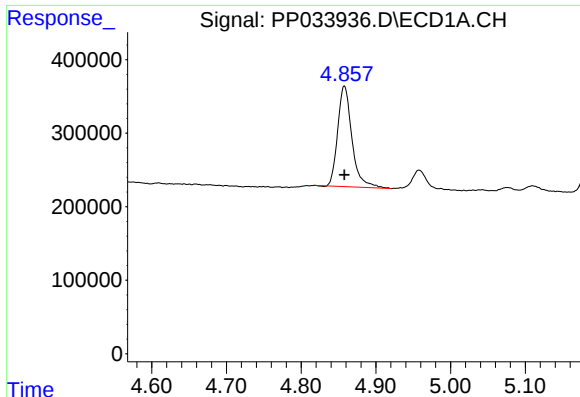

#1 Tetrachloro-m-xylene


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 1814671
Conc: 20.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP2-41732:34

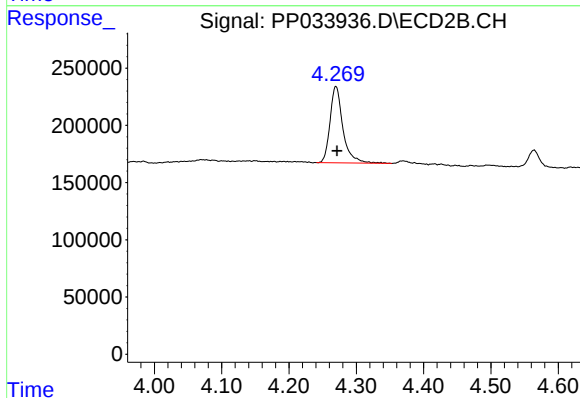


#1 Tetrachloro-m-xylene

R.T.: 4.270 min
Delta R.T.: -0.001 min
Response: 888273
Conc: 21.86 ng/ml

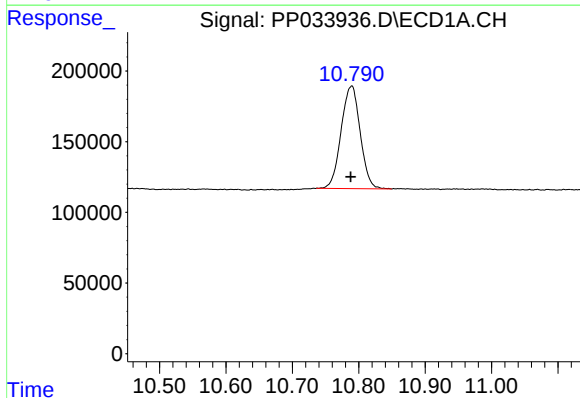

#2 Decachlorobiphenyl

R.T.: 10.789 min
Delta R.T.: 0.002 min
Response: 1448658
Conc: 17.15 ng/ml

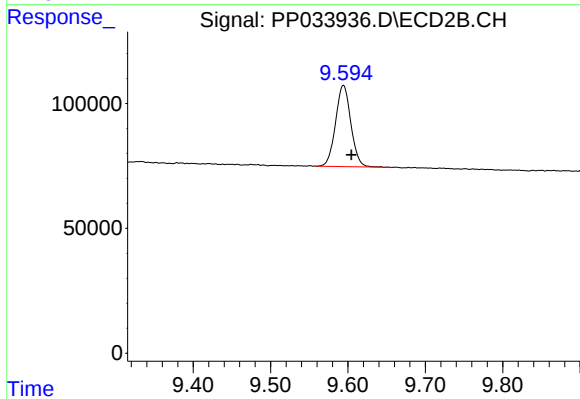

#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: -0.010 min
Response: 447242
Conc: 16.76 ng/ml