

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033965.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 4:54
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:05:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:53:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.855	4.266	4786400	2377402	55.318	58.520
2) SA Decachlor...	10.784	9.591	4568776	1487956	54.098	55.759
Target Compounds						
26) L6 AR-1254-1	7.073	6.394	1659948	915138	568.224	561.324m
27) L6 AR-1254-2	7.302	6.550	2471158	805713	543.458m	564.142m
28) L6 AR-1254-3	7.682	6.971	2686358	1311421	543.331m	572.971m
29) L6 AR-1254-4	7.978	7.207	1888917	713631	550.699	561.461m
30) L6 AR-1254-5	8.405	7.635	2039711	1082378	518.199	574.657

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033965.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 4:54
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:53:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

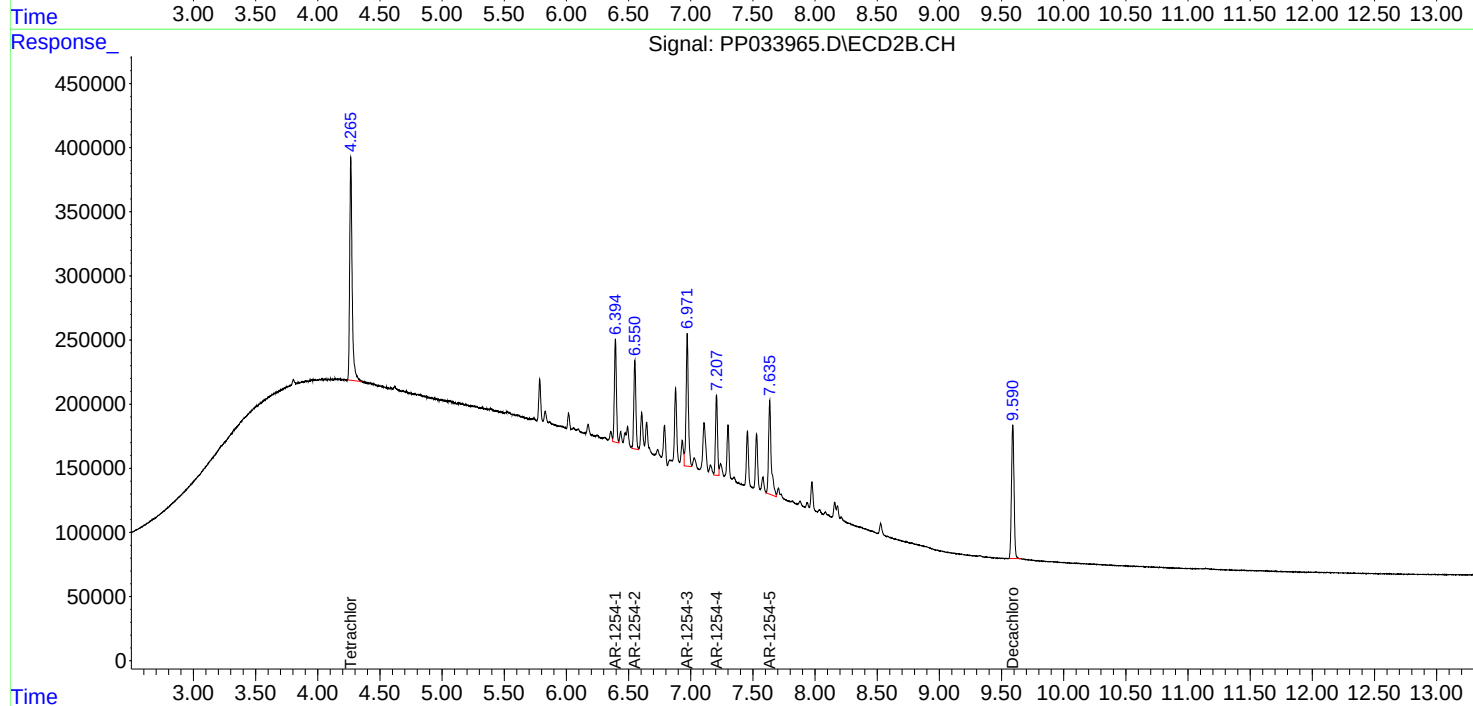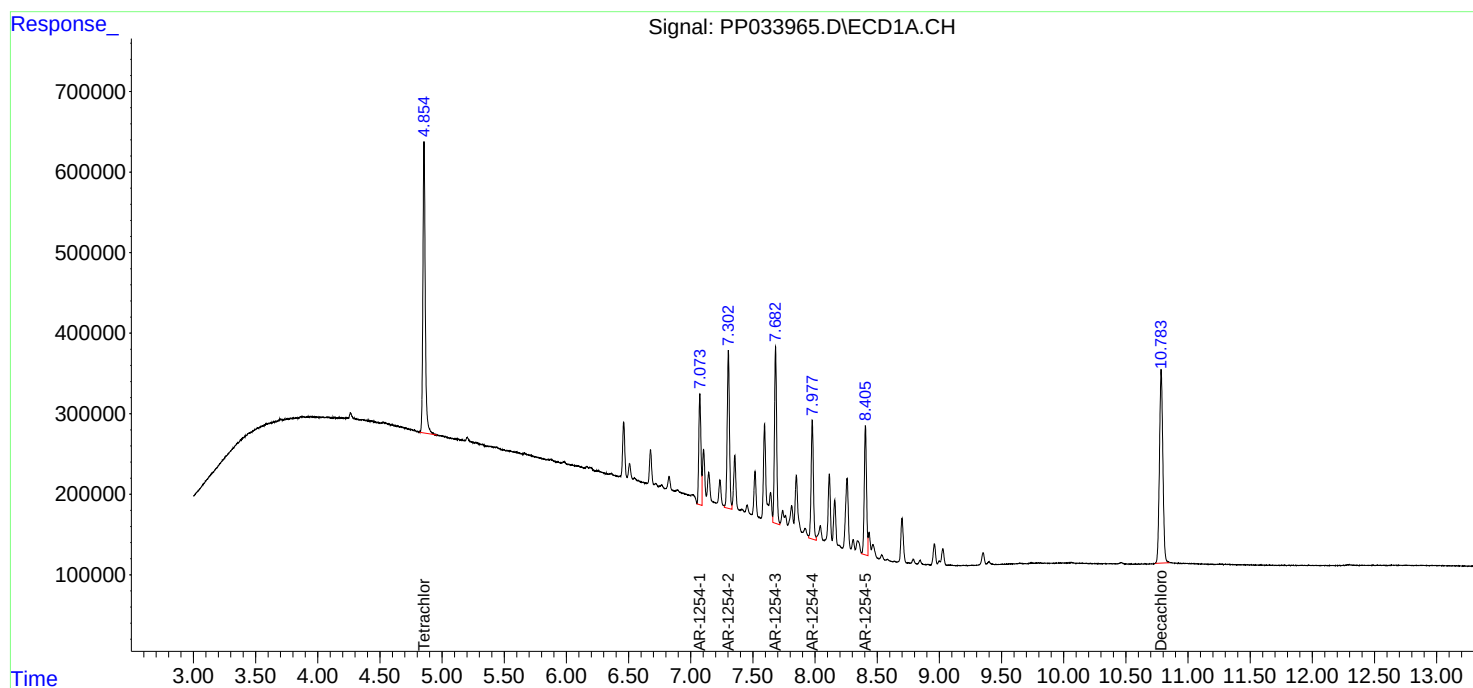

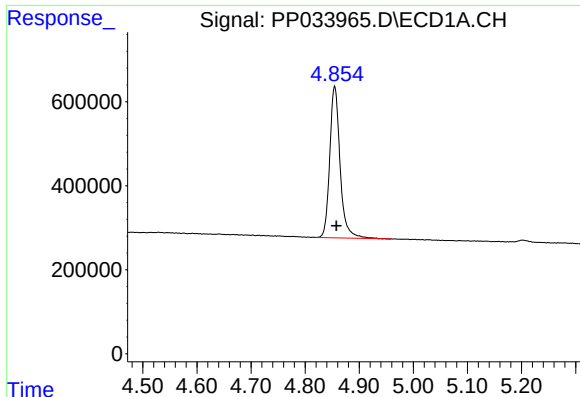


#1 Tetrachloro-m-xylene

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 4786400
Conc: 55.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:21 PM

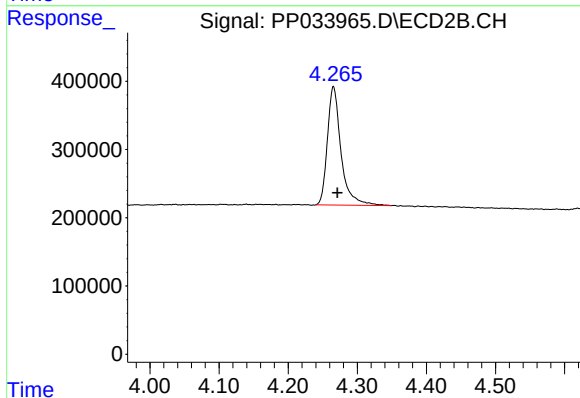


#1 Tetrachloro-m-xylene

R.T.: 4.266 min
Delta R.T.: -0.006 min
Response: 2377402
Conc: 58.52 ng/ml

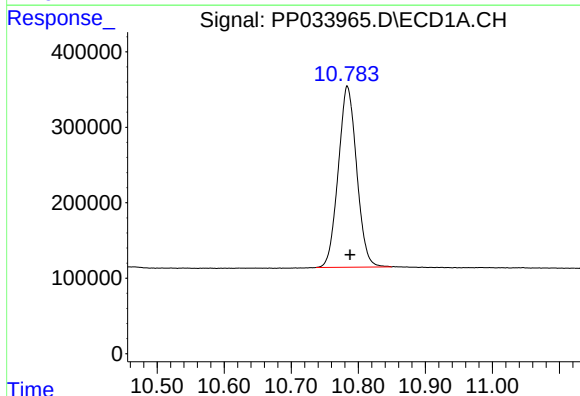


#2 Decachlorobiphenyl

R.T.: 10.784 min
Delta R.T.: -0.004 min
Response: 4568776
Conc: 54.10 ng/ml

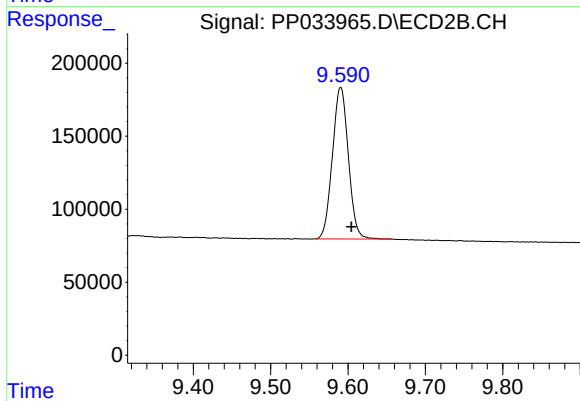

#2 Decachlorobiphenyl

R.T.: 9.591 min
Delta R.T.: -0.014 min
Response: 1487956
Conc: 55.76 ng/ml

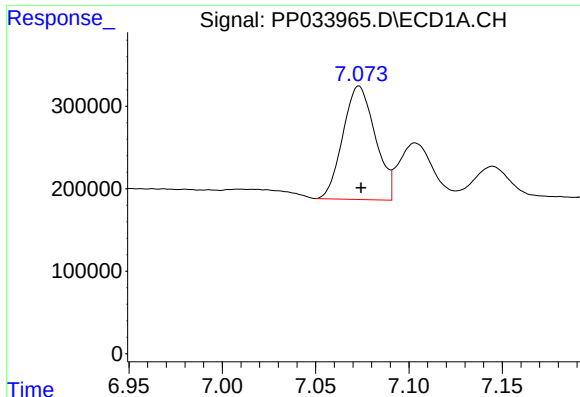


#26 AR-1254-1

R.T.: 7.073 min
Delta R.T.: -0.001 min
Response: 1659948
Conc: 568.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:21 PM

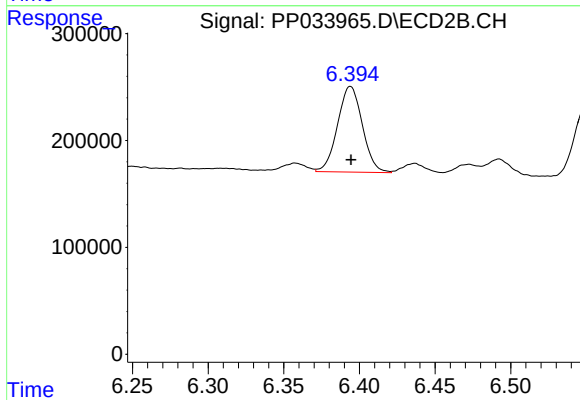


#26 AR-1254-1

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 915138
Conc: 561.32 ng/ml m

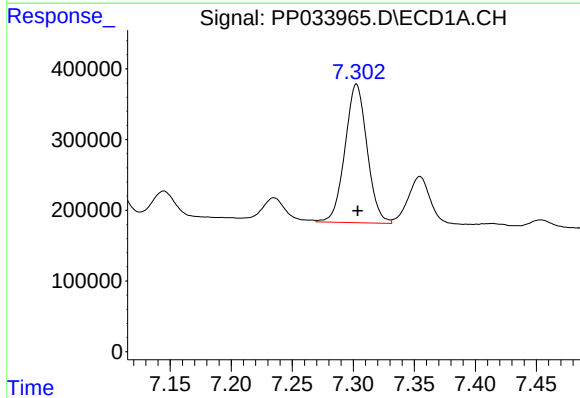


#27 AR-1254-2

R.T.: 7.302 min
Delta R.T.: -0.002 min
Response: 2471158
Conc: 543.46 ng/ml m

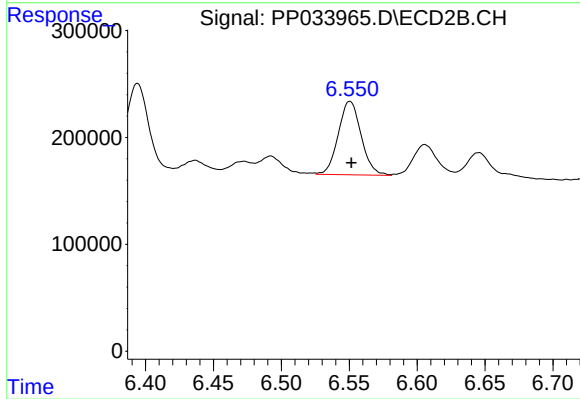

#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.002 min
Response: 805713
Conc: 564.14 ng/ml m

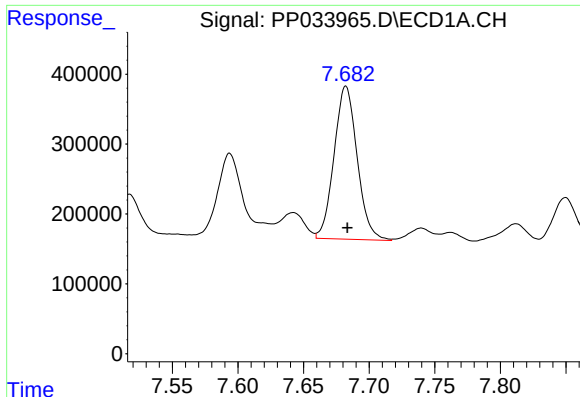


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.002 min
Response: 2686358
Conc: 543.33 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:21 PM

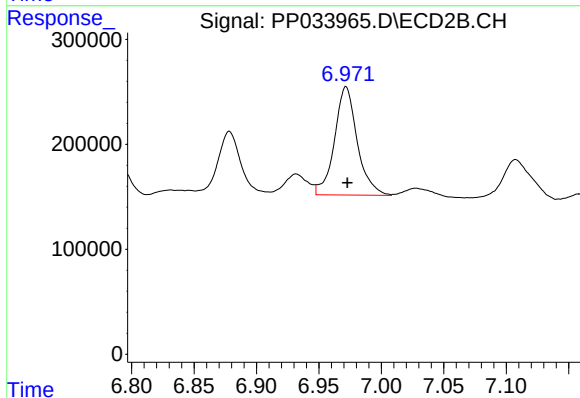


#28 AR-1254-3

R.T.: 6.971 min
Delta R.T.: -0.002 min
Response: 1311421
Conc: 572.97 ng/ml m

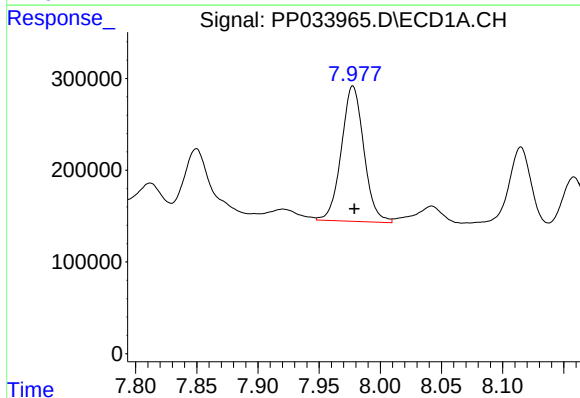


#29 AR-1254-4

R.T.: 7.978 min
Delta R.T.: -0.001 min
Response: 1888917
Conc: 550.70 ng/ml

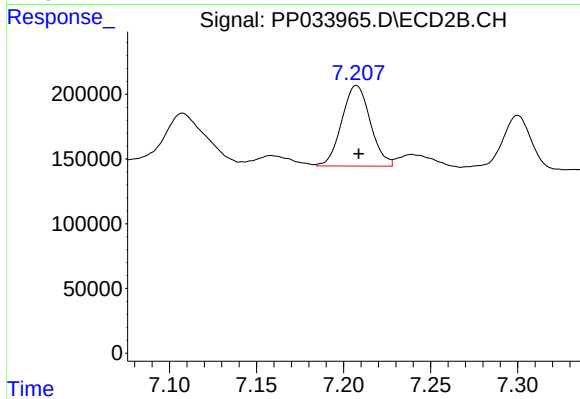

#29 AR-1254-4

R.T.: 7.207 min
Delta R.T.: -0.002 min
Response: 713631
Conc: 561.46 ng/ml m

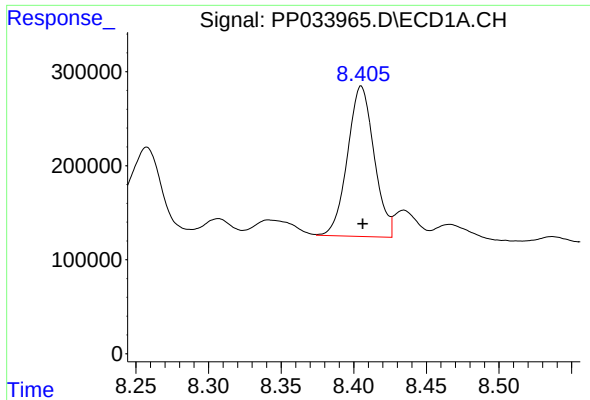


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: 0.000 min
Response: 2039711
Conc: 518.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:21 PM

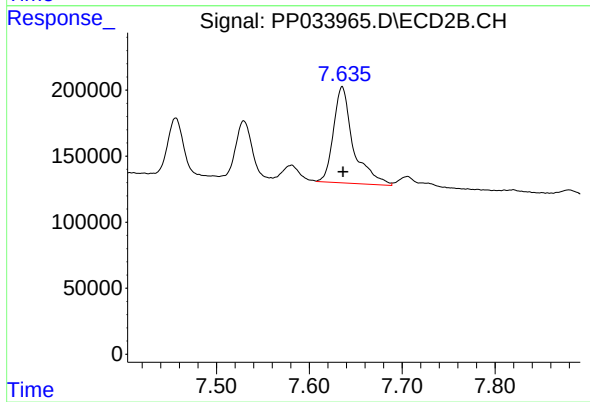

#30 AR-1254-5

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 1082378
Conc: 574.66 ng/ml