

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033973.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 7:09
 Operator : DD\AJ
 Sample : M1660-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-1A

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:05:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:38:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.854	4.265	2324306	1095328	26.863	26.961
2) SA Decachlor...	10.781	9.588	1767067	640841	20.923	24.015m
Target Compounds						
26) L6 AR-1254-1	7.073	6.394	3063878	1547133	1048.809	948.975
27) L6 AR-1254-2	7.301	6.550	7861243	2781612	1728.846	1947.620
28) L6 AR-1254-3	7.682	6.971	13350046	6602844	2700.122	2884.837
29) L6 AR-1254-4	7.977	7.207	9134839	3354766	2663.190	2639.418
30) L6 AR-1254-5	8.405	7.635	24665852	15129747	6266.481	8032.696 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033973.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 7:09
Operator : DD\AJ
Sample : M1660-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-1A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:38:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

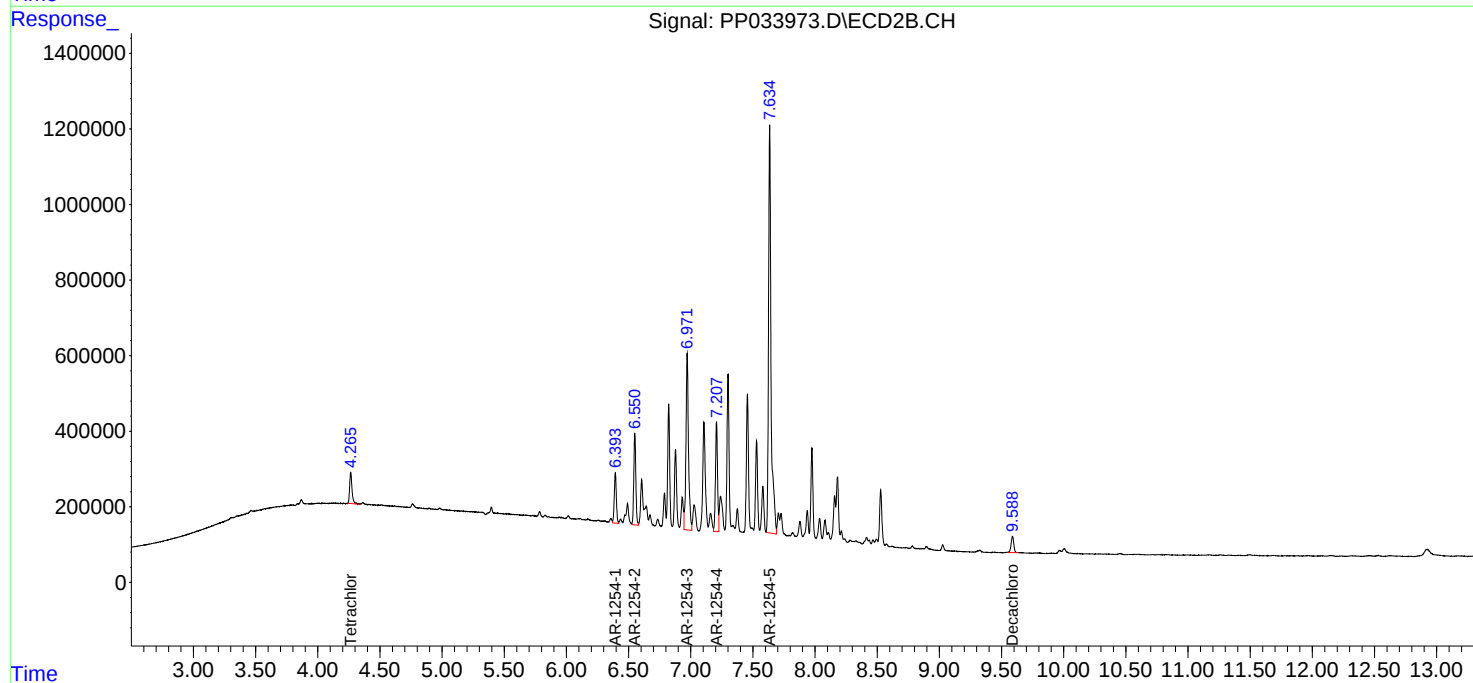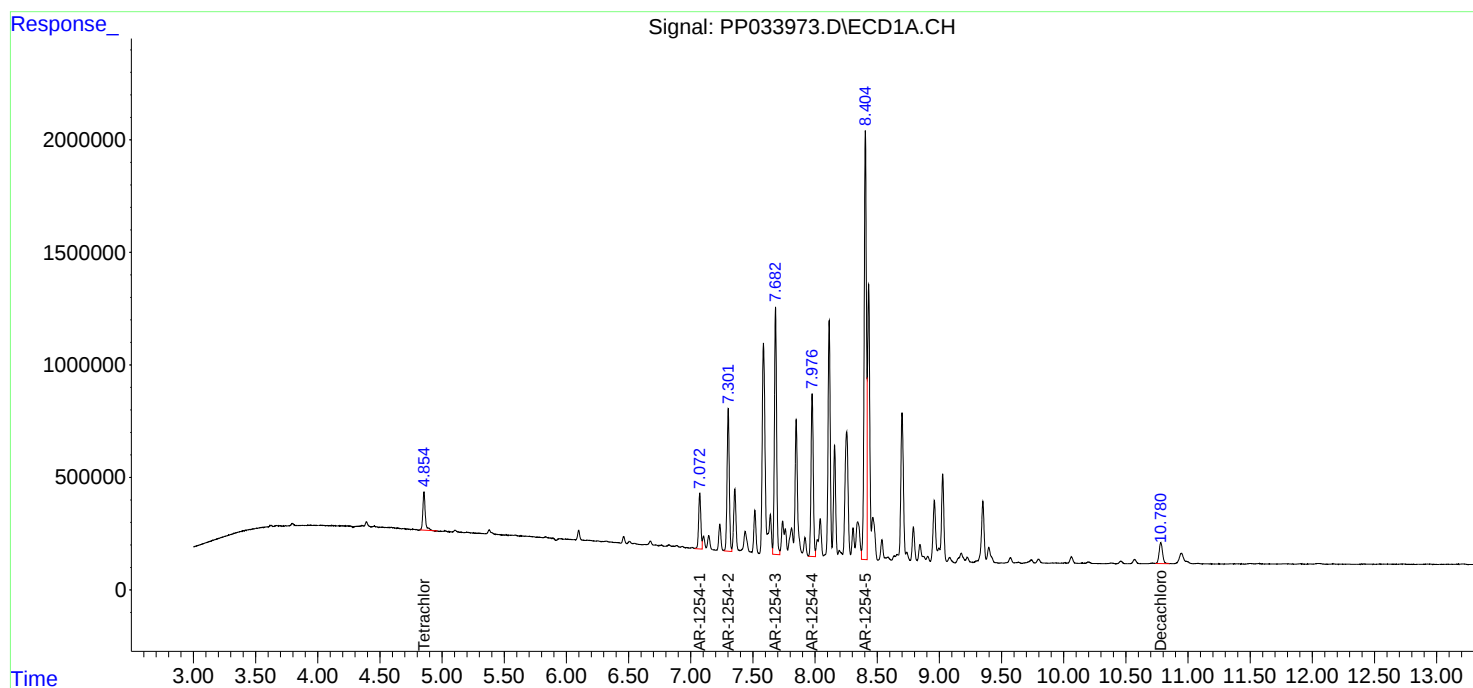

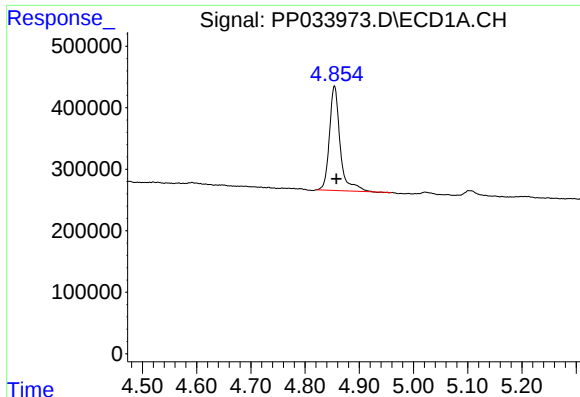


#1 Tetrachloro-m-xylene

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 2324306
Conc: 26.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:24 PM

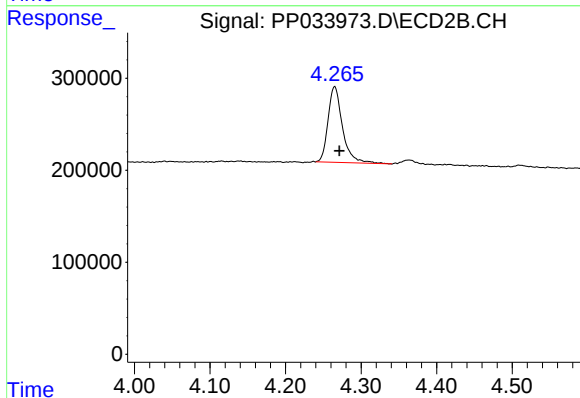


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 1095328
Conc: 26.96 ng/ml

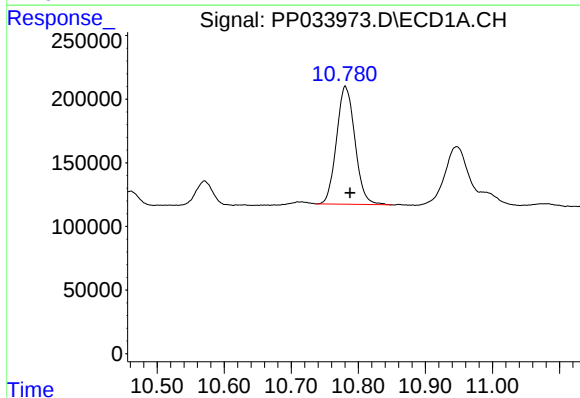


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 1767067
Conc: 20.92 ng/ml

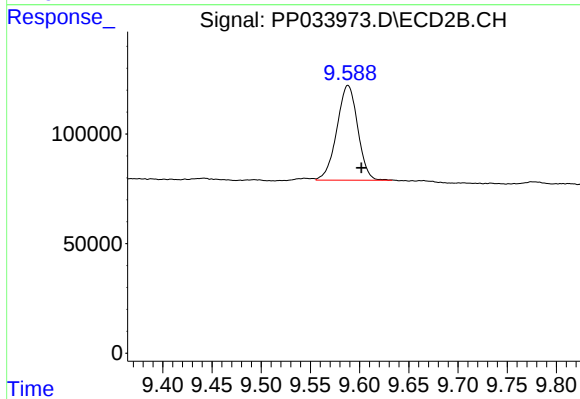

#2 Decachlorobiphenyl

R.T.: 9.588 min
Delta R.T.: -0.014 min
Response: 640841
Conc: 24.01 ng/ml m

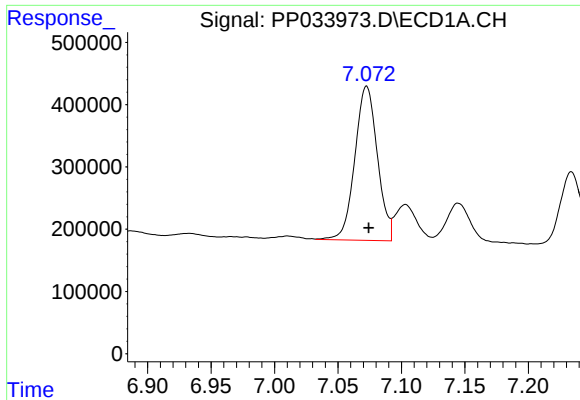


#26 AR-1254-1

R.T.: 7.073 min
Delta R.T.: -0.002 min
Response: 3063878
Conc: 1048.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:24 PM

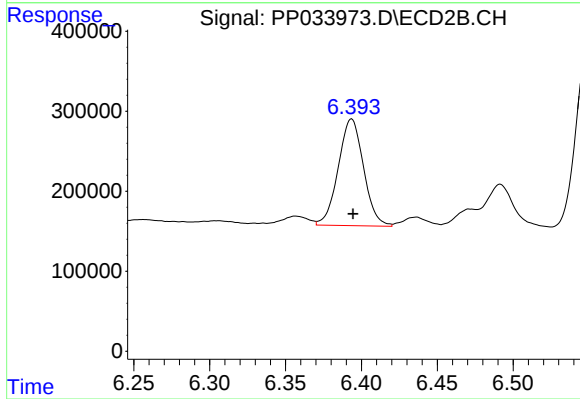


#26 AR-1254-1

R.T.: 6.394 min
Delta R.T.: -0.001 min
Response: 1547133
Conc: 948.97 ng/ml

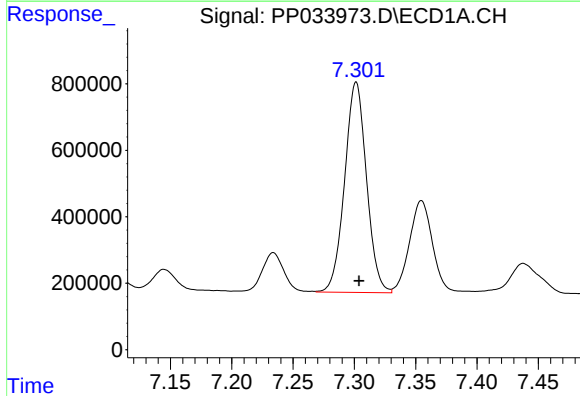


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.002 min
Response: 7861243
Conc: 1728.85 ng/ml

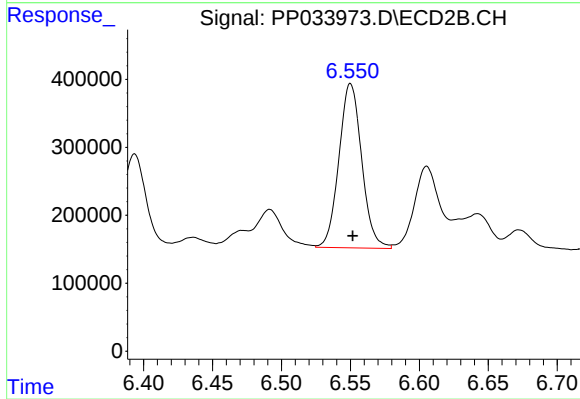

#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.002 min
Response: 2781612
Conc: 1947.62 ng/ml

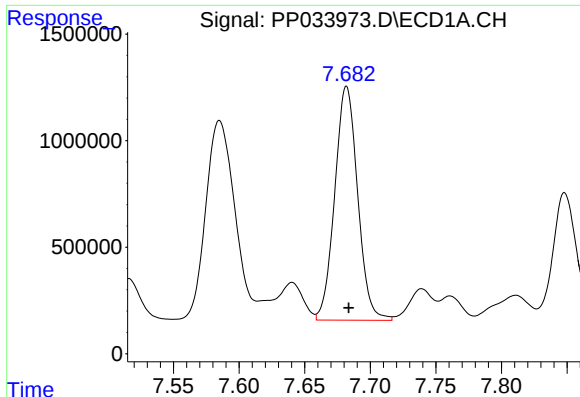


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.002 min
Response: 13350046
Conc: 2700.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:24 PM

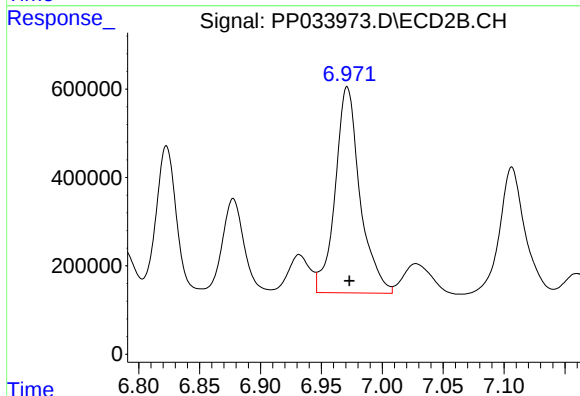


#28 AR-1254-3

R.T.: 6.971 min
Delta R.T.: -0.002 min
Response: 6602844
Conc: 2884.84 ng/ml

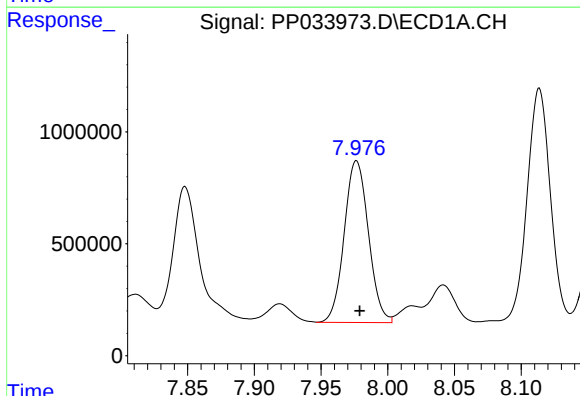


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.002 min
Response: 9134839
Conc: 2663.19 ng/ml

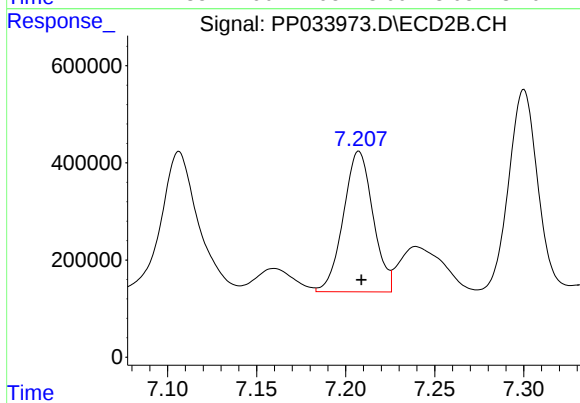

#29 AR-1254-4

R.T.: 7.207 min
Delta R.T.: -0.001 min
Response: 3354766
Conc: 2639.42 ng/ml

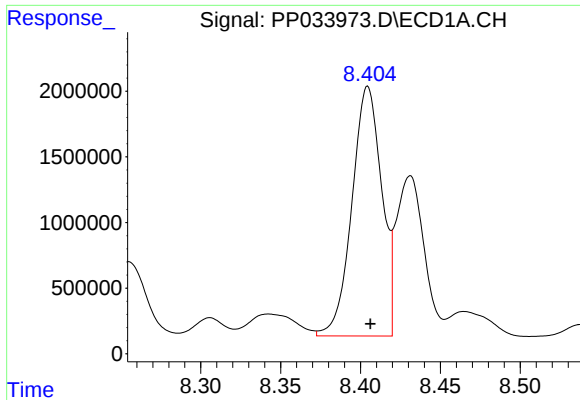


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.002 min
Response: 24665852
Conc: 6266.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-1A

Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:24 PM

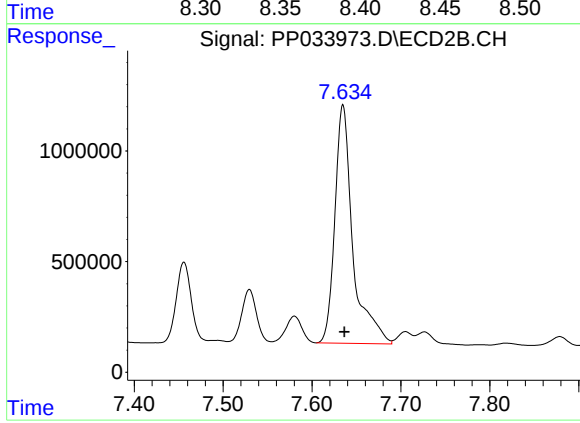

#30 AR-1254-5

R.T.: 7.635 min
Delta R.T.: -0.001 min
Response: 15129747
Conc: 8032.70 ng/ml