

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033978.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 9:07
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:05:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:40:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.264	4808549	2422133	55.574	59.621
2) SA Decachlor...	10.780	9.588	4593645	1480226	54.392	55.470
Target Compounds						
26) L6 AR-1254-1	7.072	6.392	1694264	970594	579.971	595.339m
27) L6 AR-1254-2	7.300	6.548	2496090	834478	548.941m	584.282m
28) L6 AR-1254-3	7.680	6.970	2760724	1340551	558.372m	585.698m
29) L6 AR-1254-4	7.975	7.205	1897455	736319	553.188	579.311m
30) L6 AR-1254-5	8.403	7.634	2048601	1114141	520.457m	591.521

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033978.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 9:07
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
Client Sampled :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:40:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

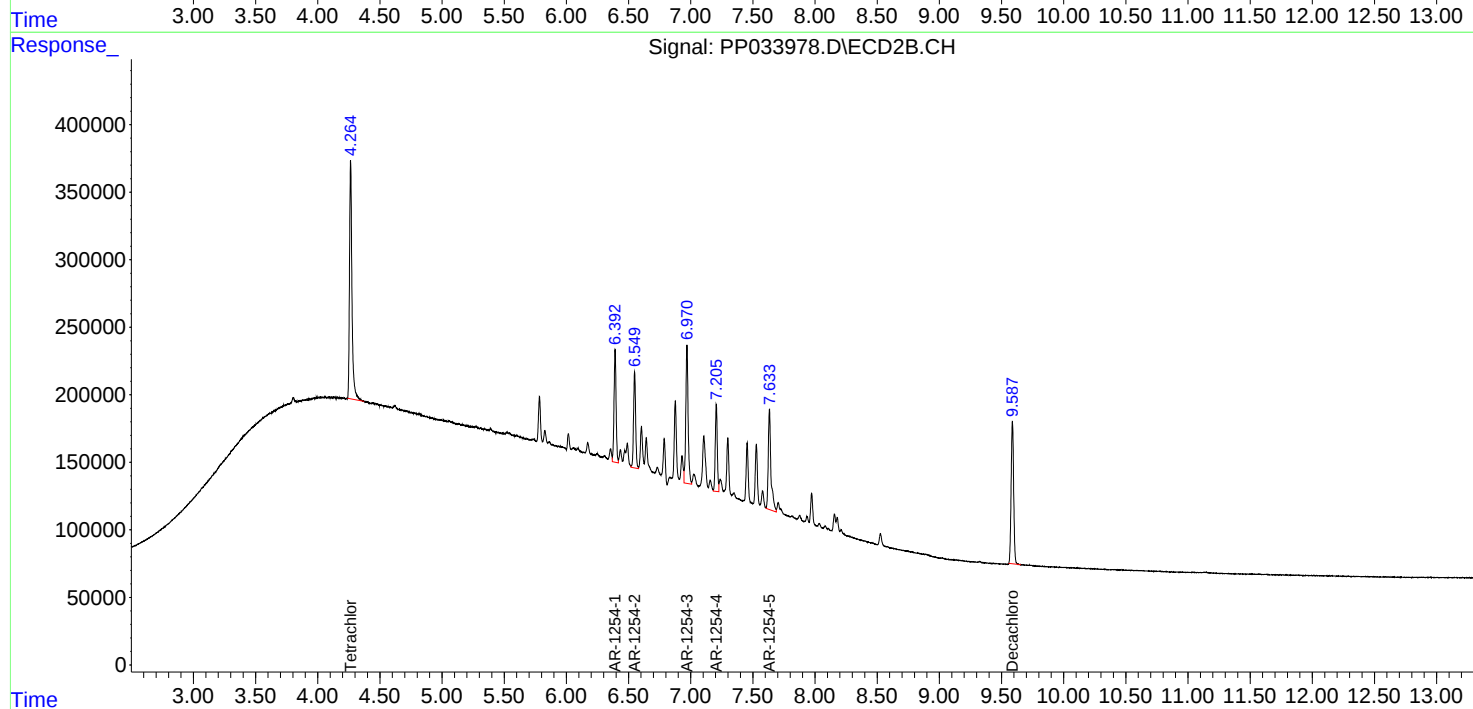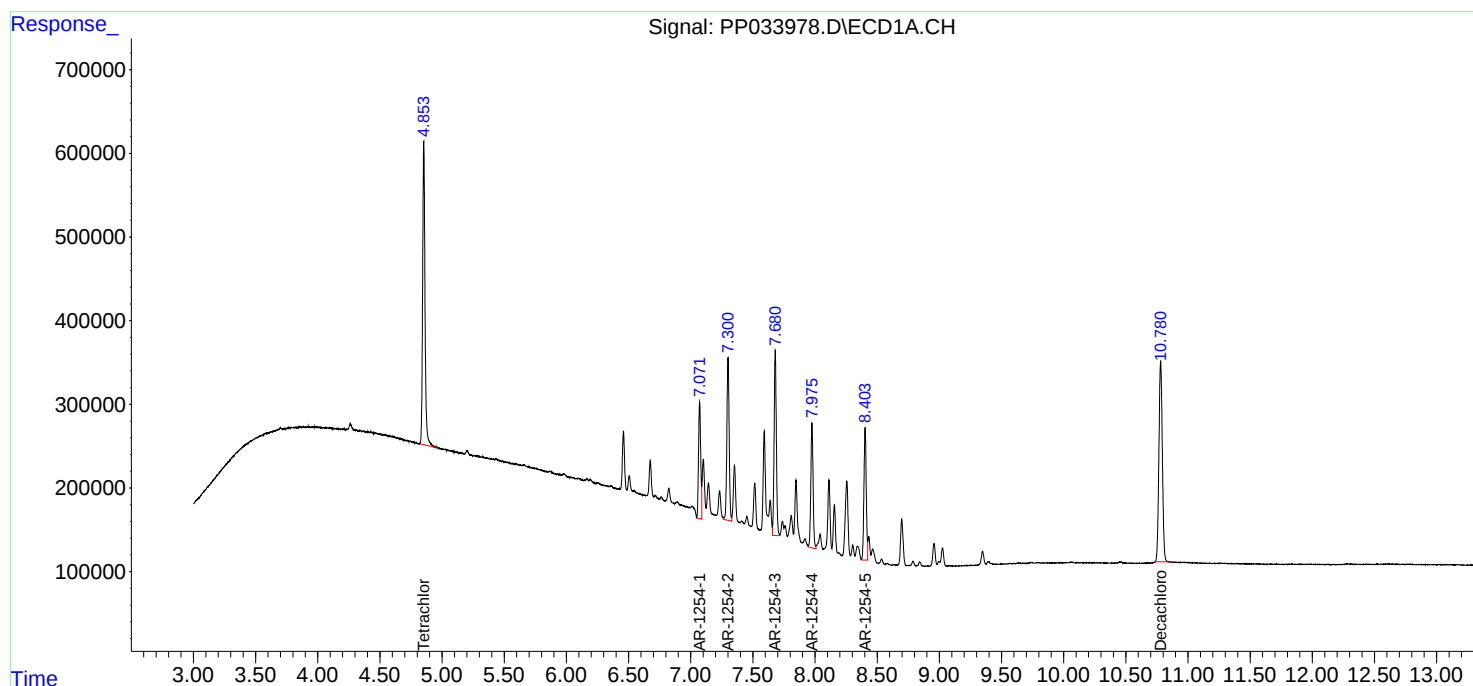

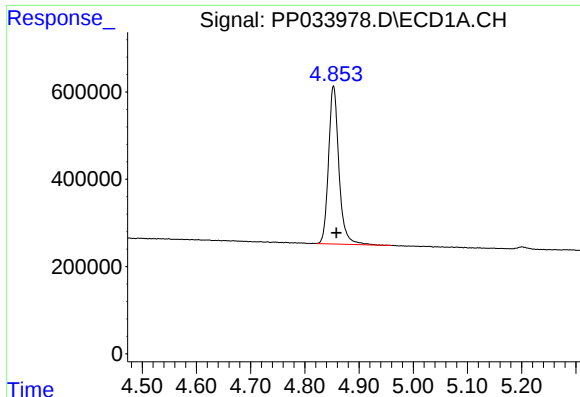


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 4808549
Conc: 55.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:29 PM

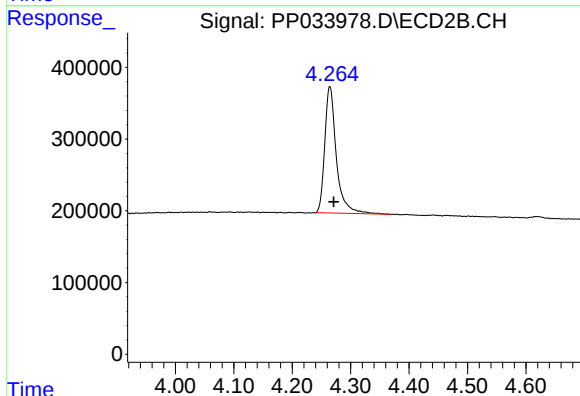


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 2422133
Conc: 59.62 ng/ml

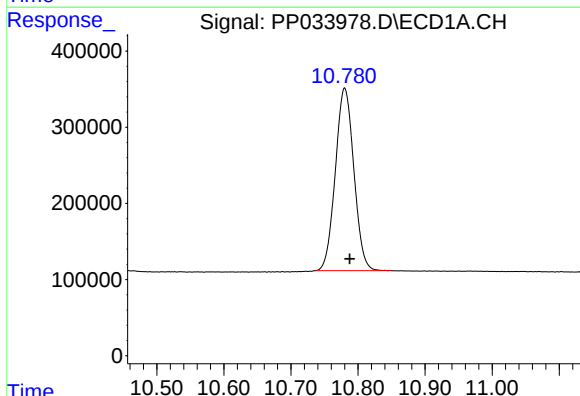


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.008 min
Response: 4593645
Conc: 54.39 ng/ml

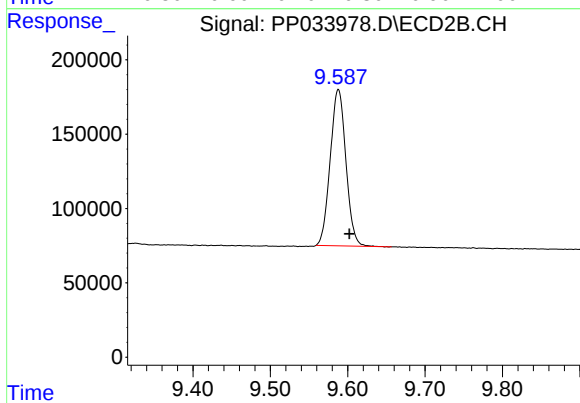

#2 Decachlorobiphenyl

R.T.: 9.588 min
Delta R.T.: -0.014 min
Response: 1480226
Conc: 55.47 ng/ml

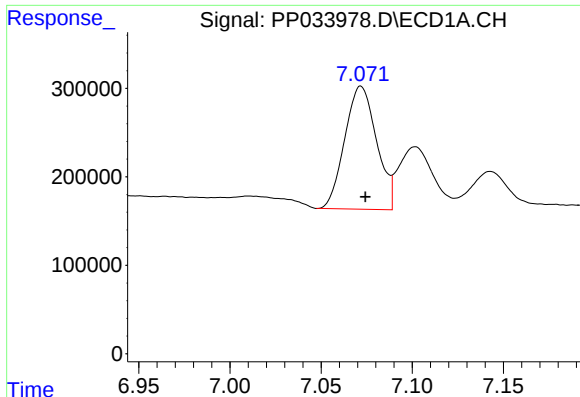


#26 AR-1254-1

R.T.: 7.072 min
Delta R.T.: -0.002 min
Response: 1694264
Conc: 579.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:29 PM

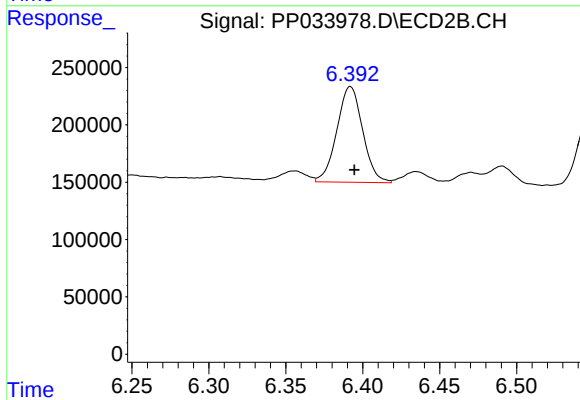


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 970594
Conc: 595.34 ng/ml m

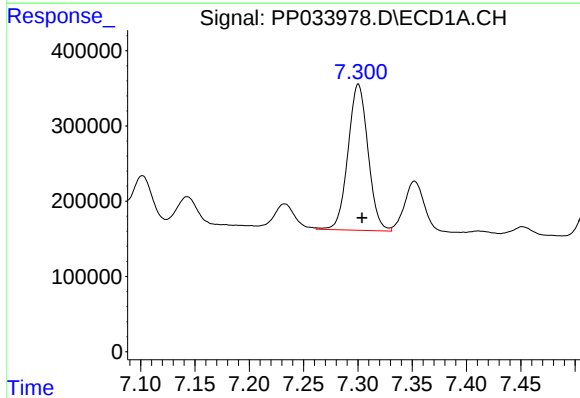


#27 AR-1254-2

R.T.: 7.300 min
Delta R.T.: -0.004 min
Response: 2496090
Conc: 548.94 ng/ml m

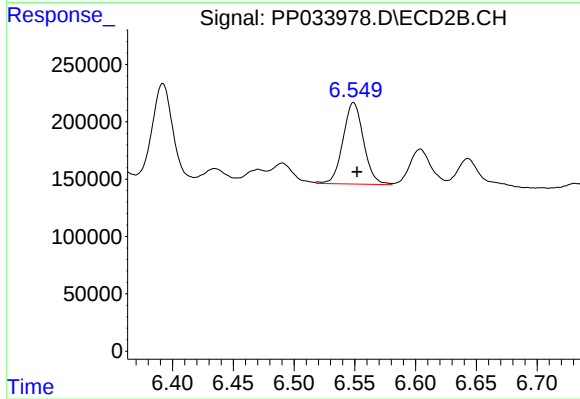

#27 AR-1254-2

R.T.: 6.548 min
Delta R.T.: -0.003 min
Response: 834478
Conc: 584.28 ng/ml m

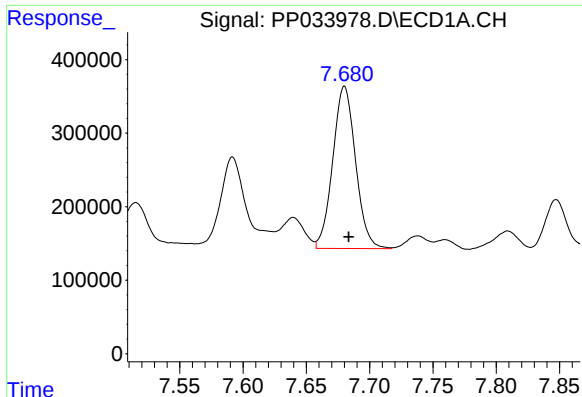


#28 AR-1254-3

R.T.: 7.680 min
Delta R.T.: -0.004 min
Response: 2760724
Conc: 558.37 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:29 PM

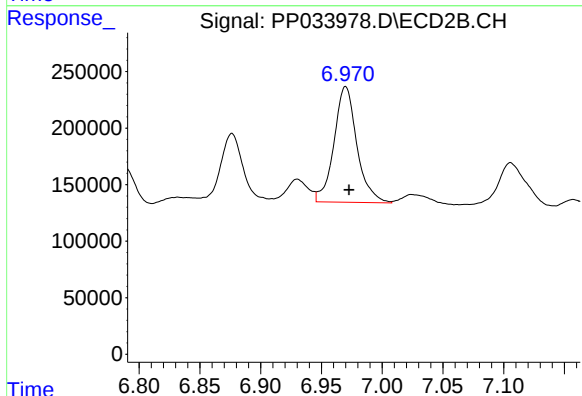


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 1340551
Conc: 585.70 ng/ml m

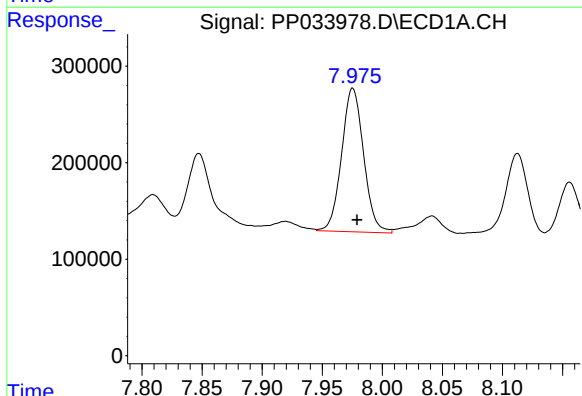


#29 AR-1254-4

R.T.: 7.975 min
Delta R.T.: -0.004 min
Response: 1897455
Conc: 553.19 ng/ml

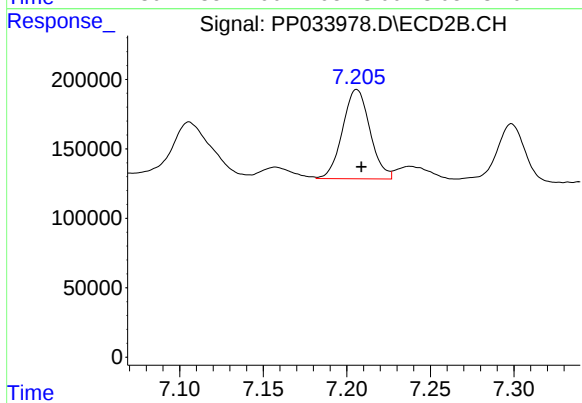

#29 AR-1254-4

R.T.: 7.205 min
Delta R.T.: -0.003 min
Response: 736319
Conc: 579.31 ng/ml m

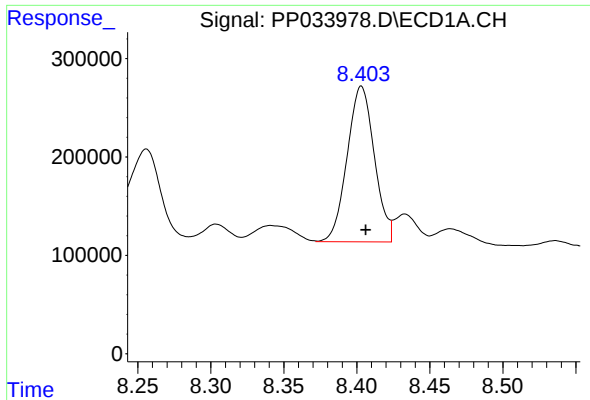


#30 AR-1254-5

R.T.: 8.403 min
Delta R.T.: -0.004 min
Response: 2048601
Conc: 520.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:29 PM

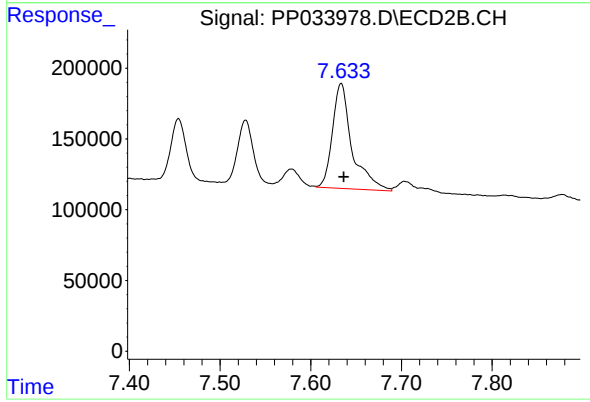

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.003 min
Response: 1114141
Conc: 591.52 ng/ml