

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033981.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 9:57
 Operator : DD\AJ
 Sample : M1660-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-5A

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:05:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 08:02:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.265	1844669	909276	21.319	22.382
2) SA Decachlor...	10.782	9.587	1430696	473407	16.941	17.740
Target Compounds						
26) L6 AR-1254-1	7.069	6.389	24720	36894	8.462	22.630 #
27) L6 AR-1254-2	7.301	6.546	109149	35775	24.004	25.049m
28) L6 AR-1254-3	7.681	6.969	230042	74632	46.527	32.607m#
29) L6 AR-1254-4	7.976	7.204	87151	52946	25.408	41.656m#
30) L6 AR-1254-5	8.405	7.634	394514	235843	100.228	125.214

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 9:57
Operator : DD\AJ
Sample : M1660-14
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-5A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 08:02:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

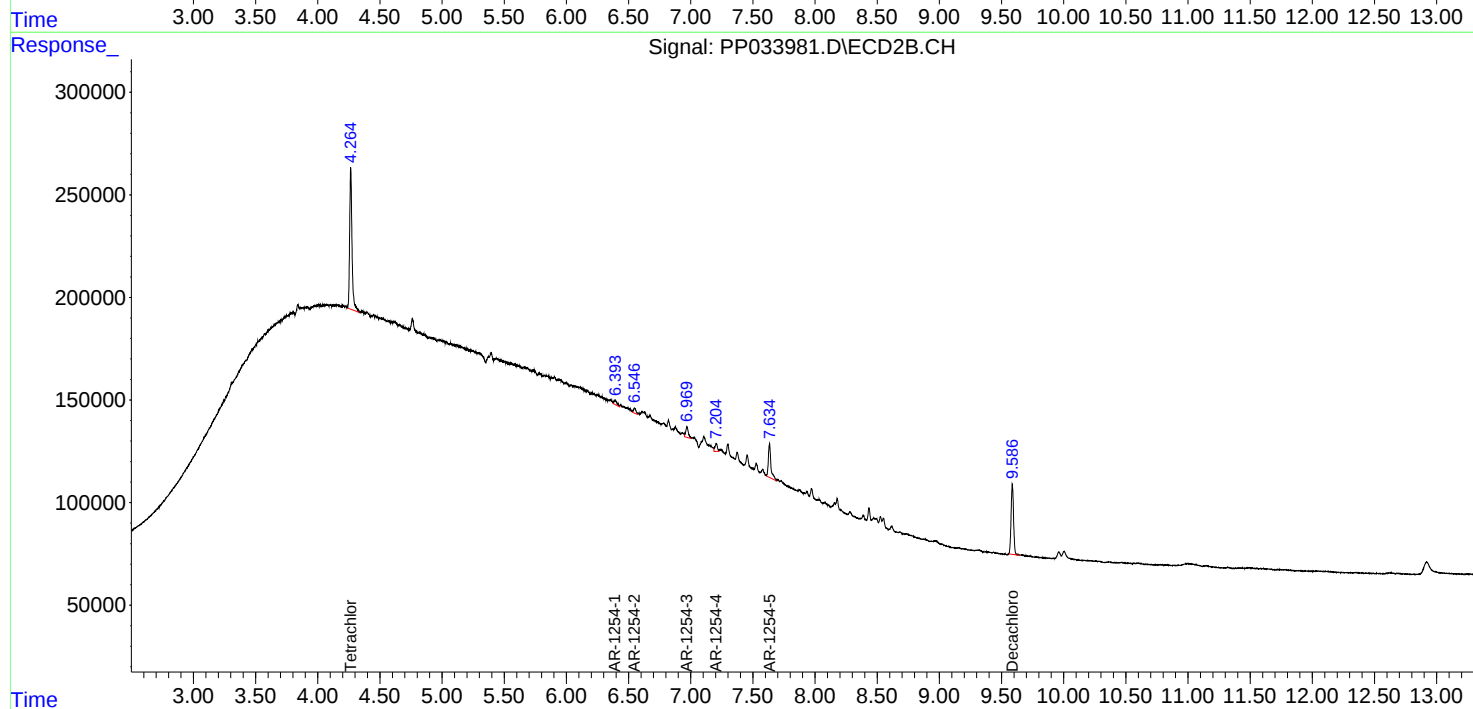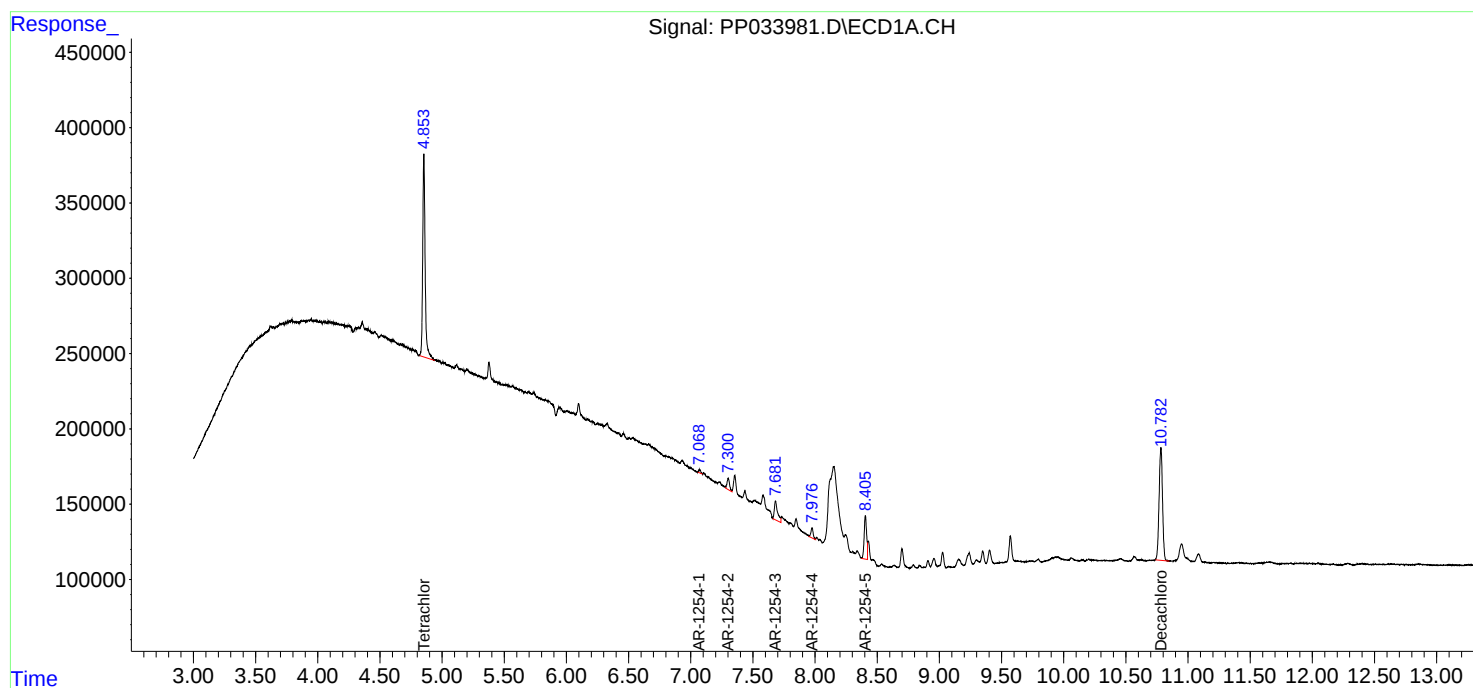

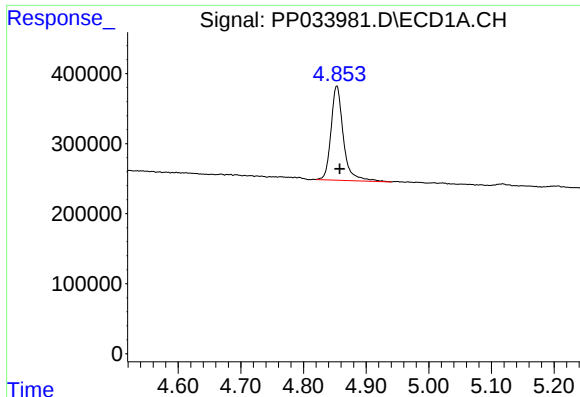


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 1844669
Conc: 21.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-5A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:39 PM

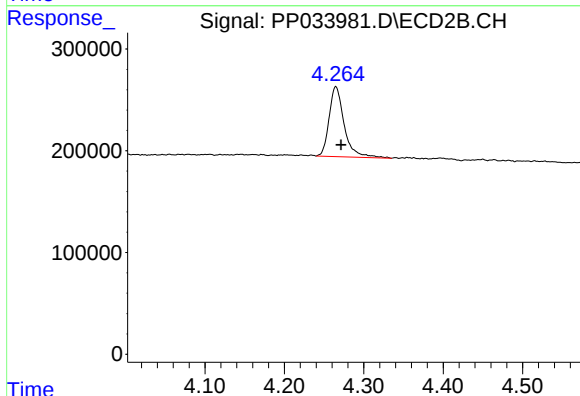


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 909276
Conc: 22.38 ng/ml

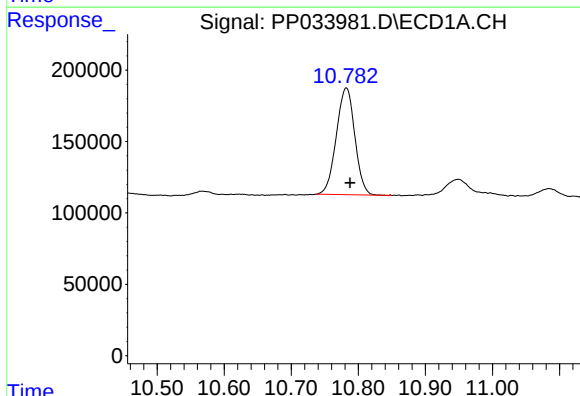


#2 Decachlorobiphenyl

R.T.: 10.782 min
Delta R.T.: -0.006 min
Response: 1430696
Conc: 16.94 ng/ml

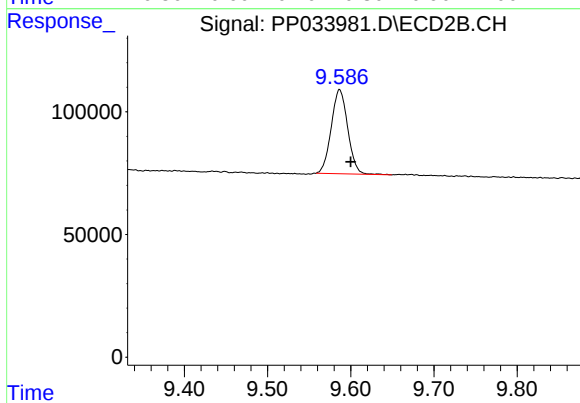

#2 Decachlorobiphenyl

R.T.: 9.587 min
Delta R.T.: -0.013 min
Response: 473407
Conc: 17.74 ng/ml

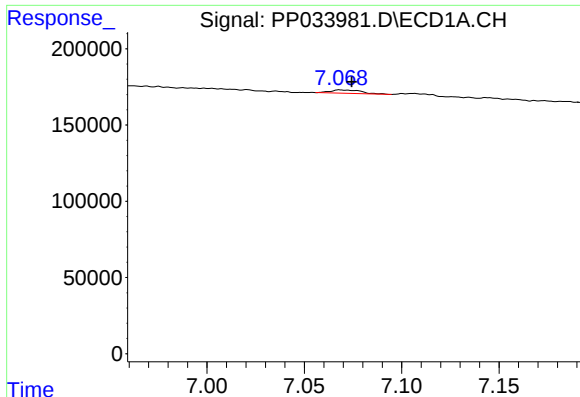


#26 AR-1254-1

R.T.: 7.069 min
Delta R.T.: -0.006 min
Response: 24720
Conc: 8.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-5A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:39 PM

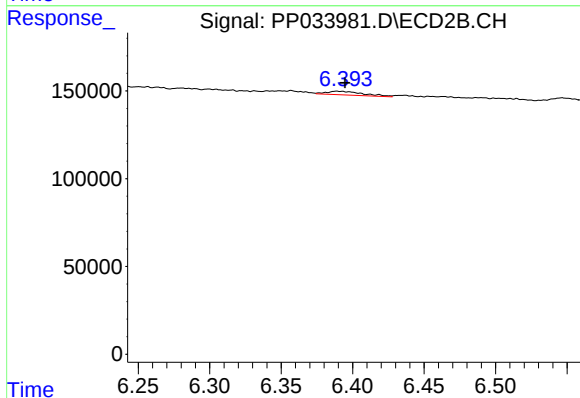


#26 AR-1254-1

R.T.: 6.389 min
Delta R.T.: -0.006 min
Response: 36894
Conc: 22.63 ng/ml

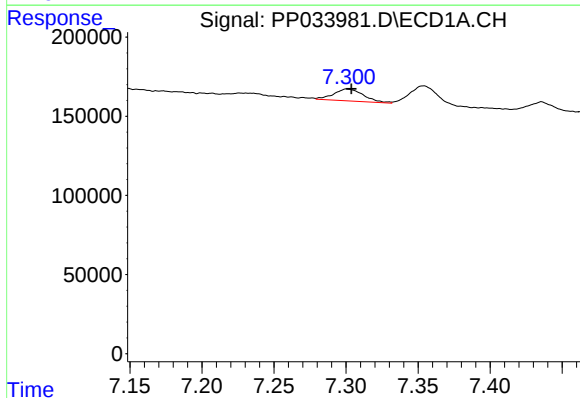


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.003 min
Response: 109149
Conc: 24.00 ng/ml

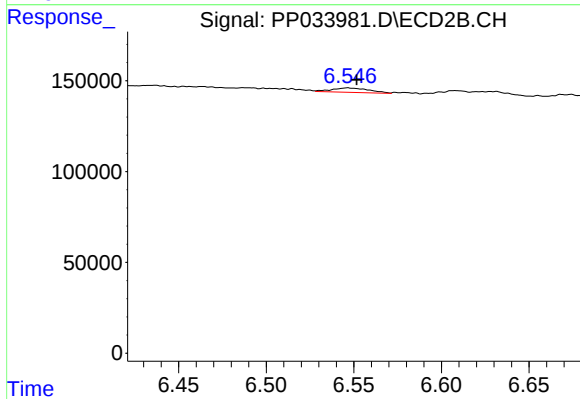

#27 AR-1254-2

R.T.: 6.546 min
Delta R.T.: -0.005 min
Response: 35775
Conc: 25.05 ng/ml m

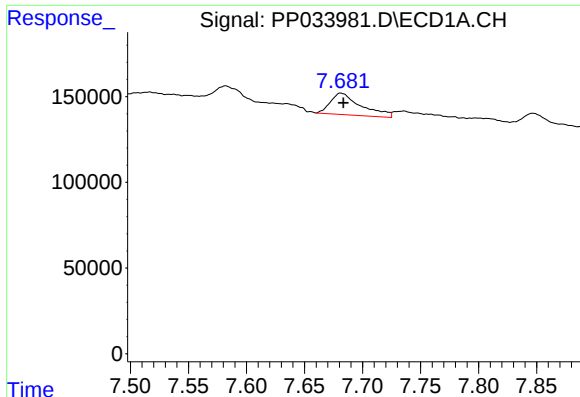


#28 AR-1254-3

R.T.: 7.681 min
Delta R.T.: -0.002 min
Response: 230042
Conc: 46.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-5A


Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:39 PM

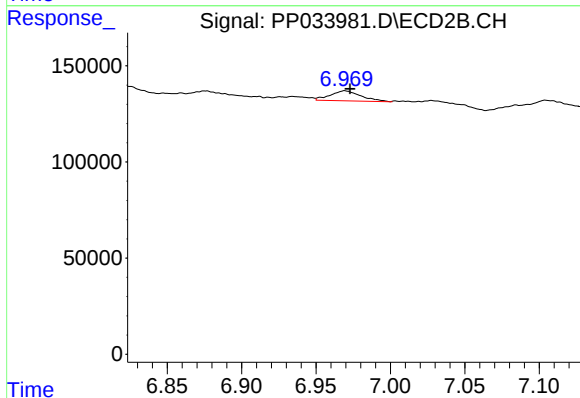


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: -0.004 min
Response: 74632
Conc: 32.61 ng/ml m

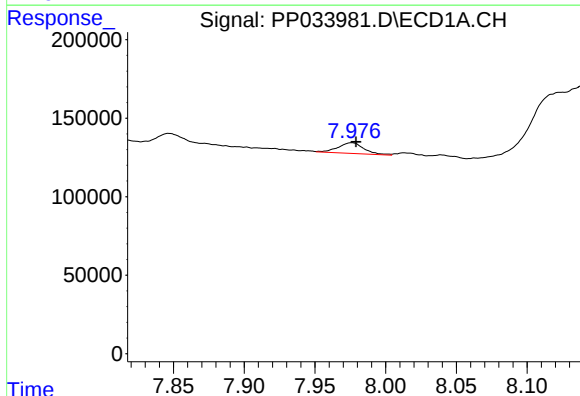


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 87151
Conc: 25.41 ng/ml

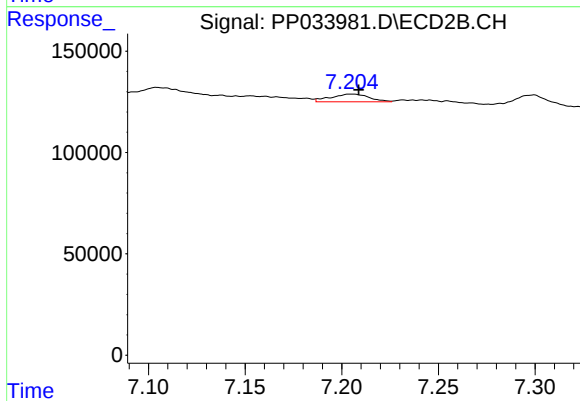

#29 AR-1254-4

R.T.: 7.204 min
Delta R.T.: -0.005 min
Response: 52946
Conc: 41.66 ng/ml m

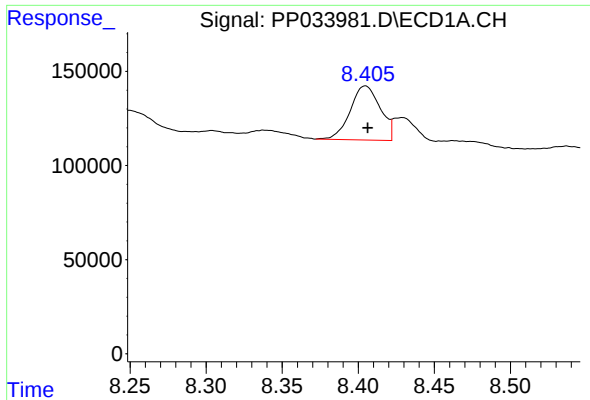


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.002 min
Response: 394514
Conc: 100.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-5A

Manual Integrations
APPROVED

Ankita
3/15/2021 1:05:39 PM

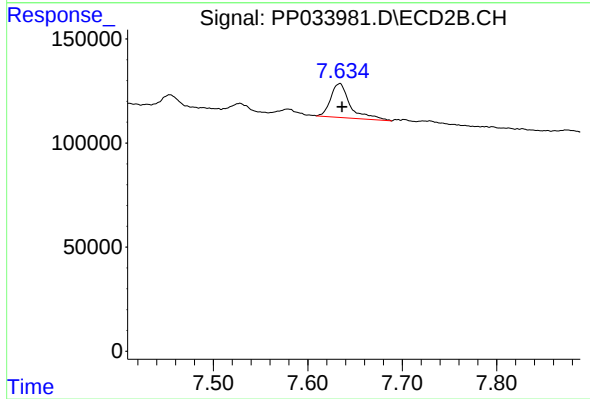

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.002 min
Response: 235843
Conc: 125.21 ng/ml