

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
 Data File : PP033982.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 10:14
 Operator : DD\AJ
 Sample : M1660-17
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-6A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 08:08:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.264	1570702	784499	18.153	19.310
2) SA Decachlor...	10.780	9.586	1242194	408507	14.709	15.308
Target Compounds						
26) L6 AR-1254-1	7.072	6.393	1262540	753985	432.185	462.477
27) L6 AR-1254-2	7.301	6.550	2964453	1214343	651.943	850.254 #
28) L6 AR-1254-3	7.681	6.970	4620094	2459448	934.440	1074.553
29) L6 AR-1254-4	7.977	7.206	3681772	1542711	1073.391	1213.753
30) L6 AR-1254-5	8.404	7.634	8014504	4335728	2036.124	2301.928



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031221\
Data File : PP033982.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 10:14
Operator : DD\AJ
Sample : M1660-17
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
X127-6A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 08:08:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

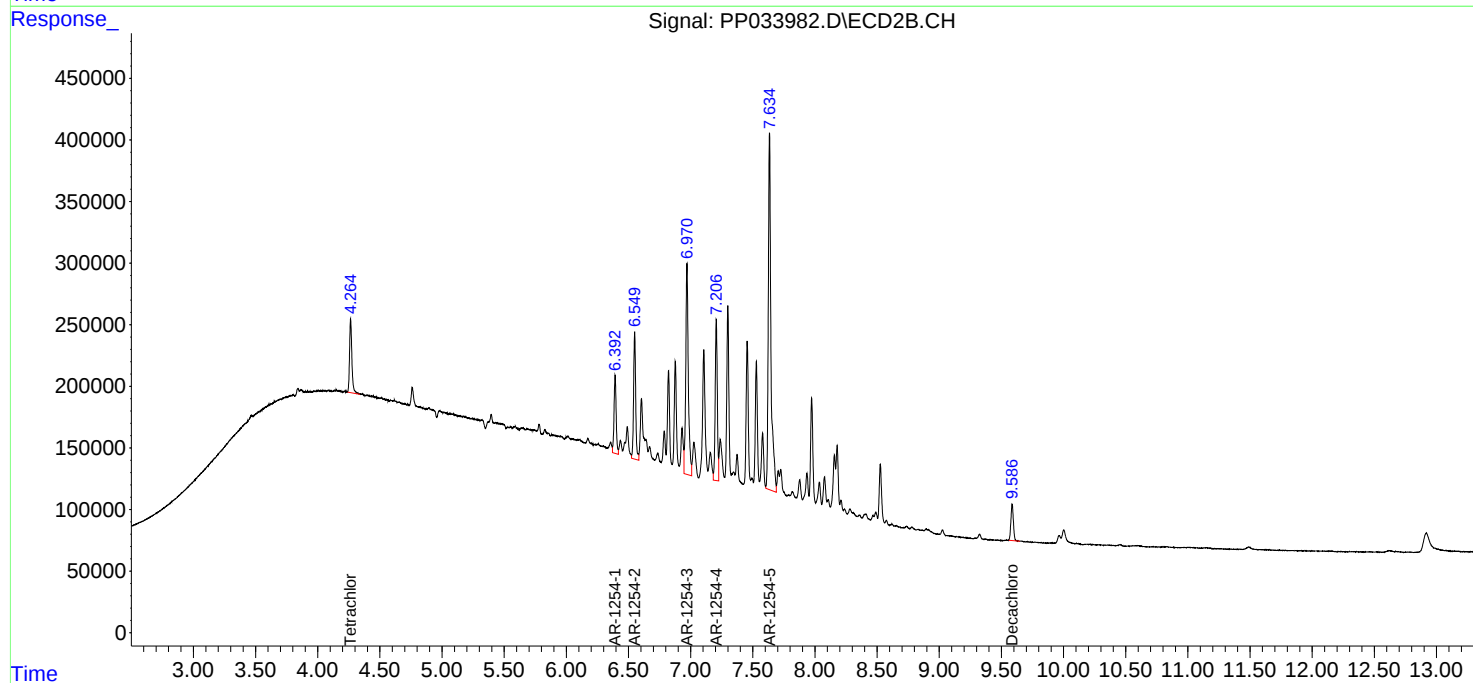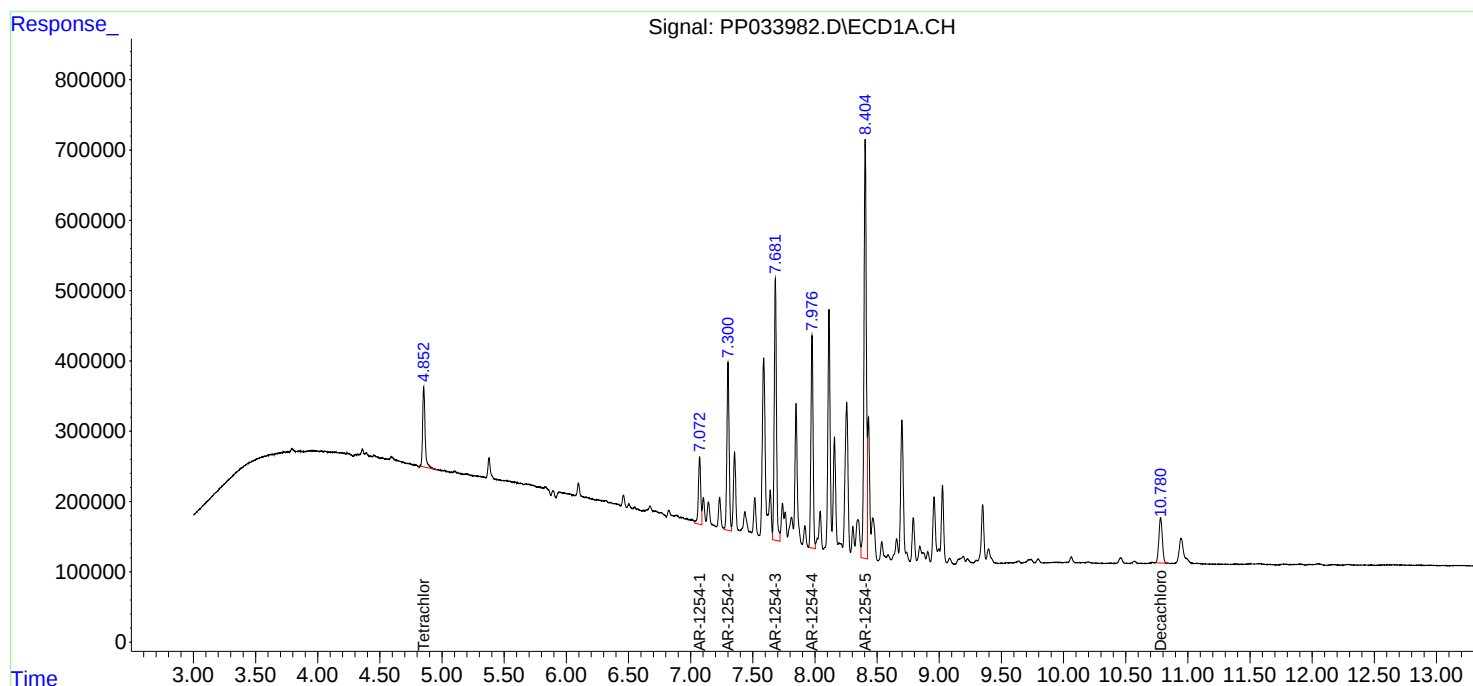


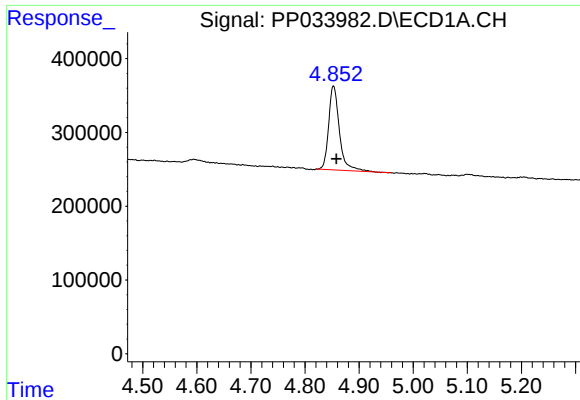

#1 Tetrachloro-m-xylene


R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 1570702
Conc: 18.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6A

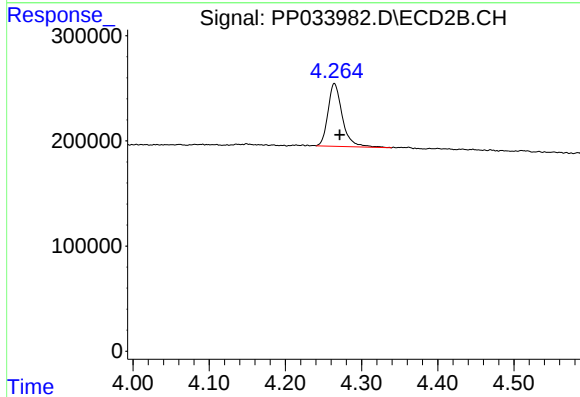


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 784499
Conc: 19.31 ng/ml

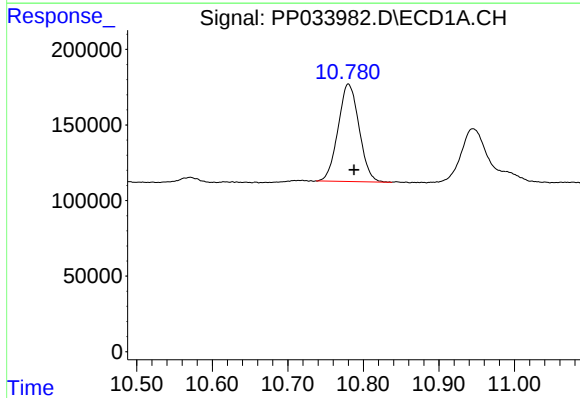


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.008 min
Response: 1242194
Conc: 14.71 ng/ml

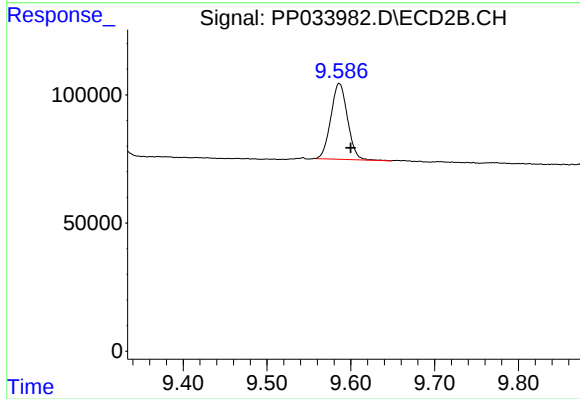

#2 Decachlorobiphenyl


R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 408507
Conc: 15.31 ng/ml

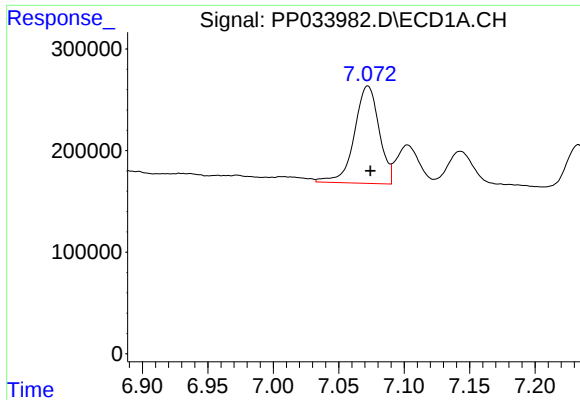

#26 AR-1254-1


R.T.: 7.072 min
Delta R.T.: -0.002 min
Response: 1262540
Conc: 432.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6A

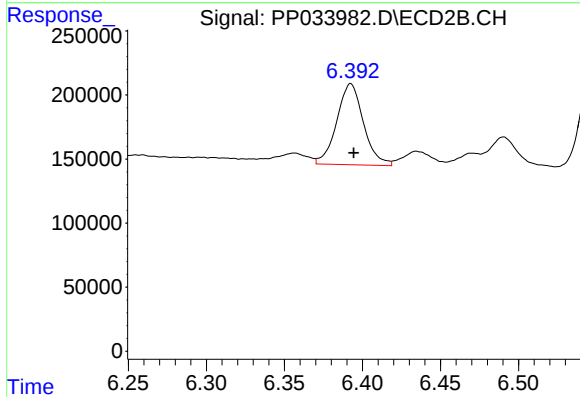


#26 AR-1254-1

R.T.: 6.393 min
Delta R.T.: -0.002 min
Response: 753985
Conc: 462.48 ng/ml

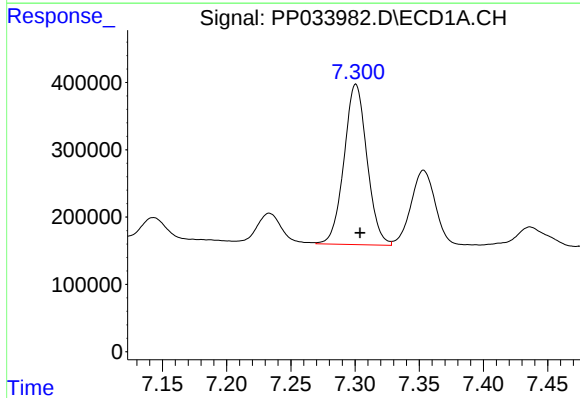


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.003 min
Response: 2964453
Conc: 651.94 ng/ml

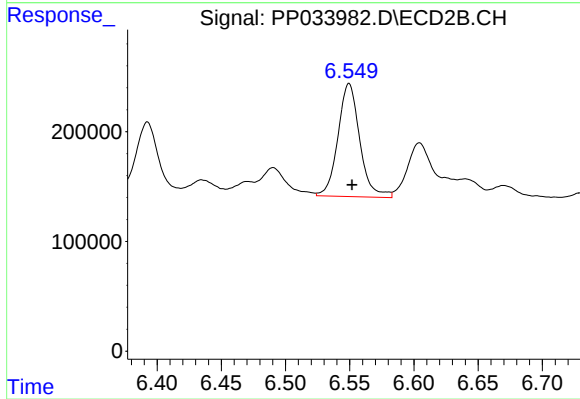

#27 AR-1254-2


R.T.: 6.550 min
Delta R.T.: -0.002 min
Response: 1214343
Conc: 850.25 ng/ml

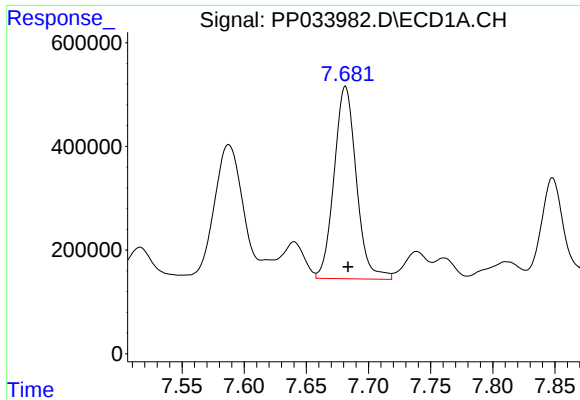

#28 AR-1254-3


R.T.: 7.681 min
Delta R.T.: -0.002 min
Response: 4620094
Conc: 934.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6A

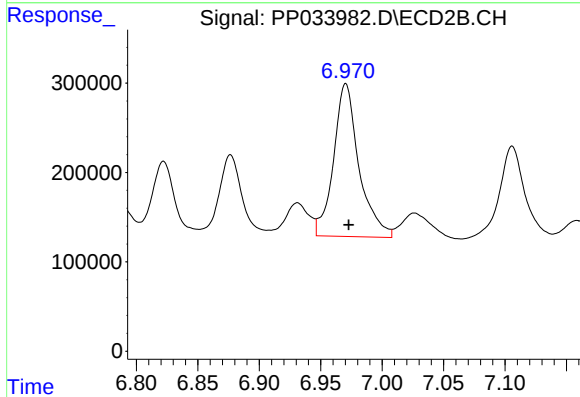


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 2459448
Conc: 1074.55 ng/ml

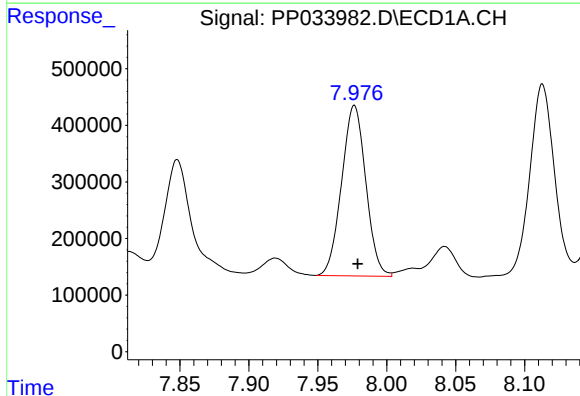


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.002 min
Response: 3681772
Conc: 1073.39 ng/ml

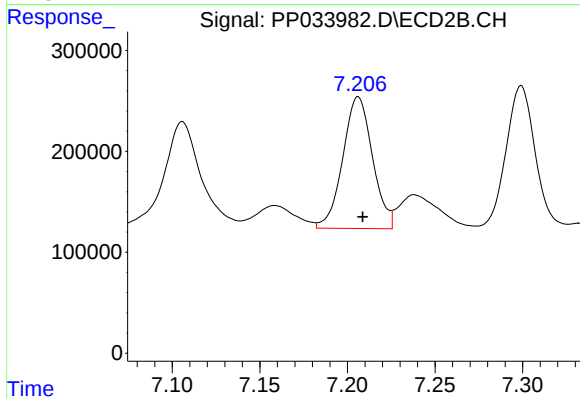

#29 AR-1254-4


R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 1542711
Conc: 1213.75 ng/ml

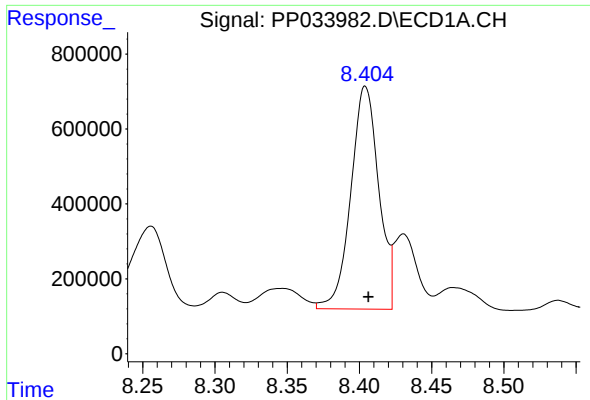

#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 8014504
Conc: 2036.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6A

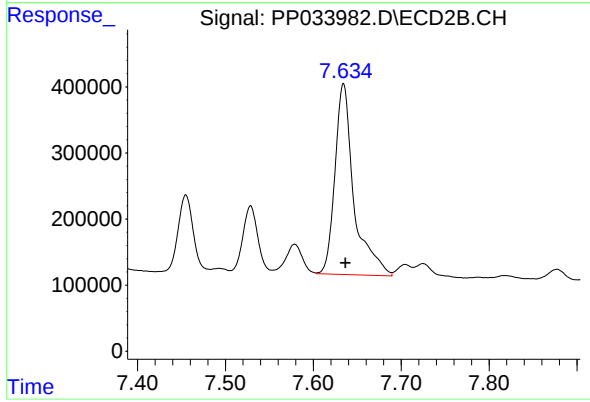

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.002 min
Response: 4335728
Conc: 2301.93 ng/ml