

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
 Data File : PP029267.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2019 9:07
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:55:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.934	12.127	15157440	17813034	504.301	469.351
Target Compounds							
12) T	2,4,5-T	0.000	15.880	0	143267	N.D.	0.865 #
13) T	2,4-DB	16.223	16.447	89385	138923	4.679	6.167 #
15) T	Picloram	17.486	0.000	1073034	0	3.859	N.D. #
16) T	DCPA	18.096	18.050	135323	302864	0.479	1.303 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
Data File : PP029267.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2019 9:07
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:55:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

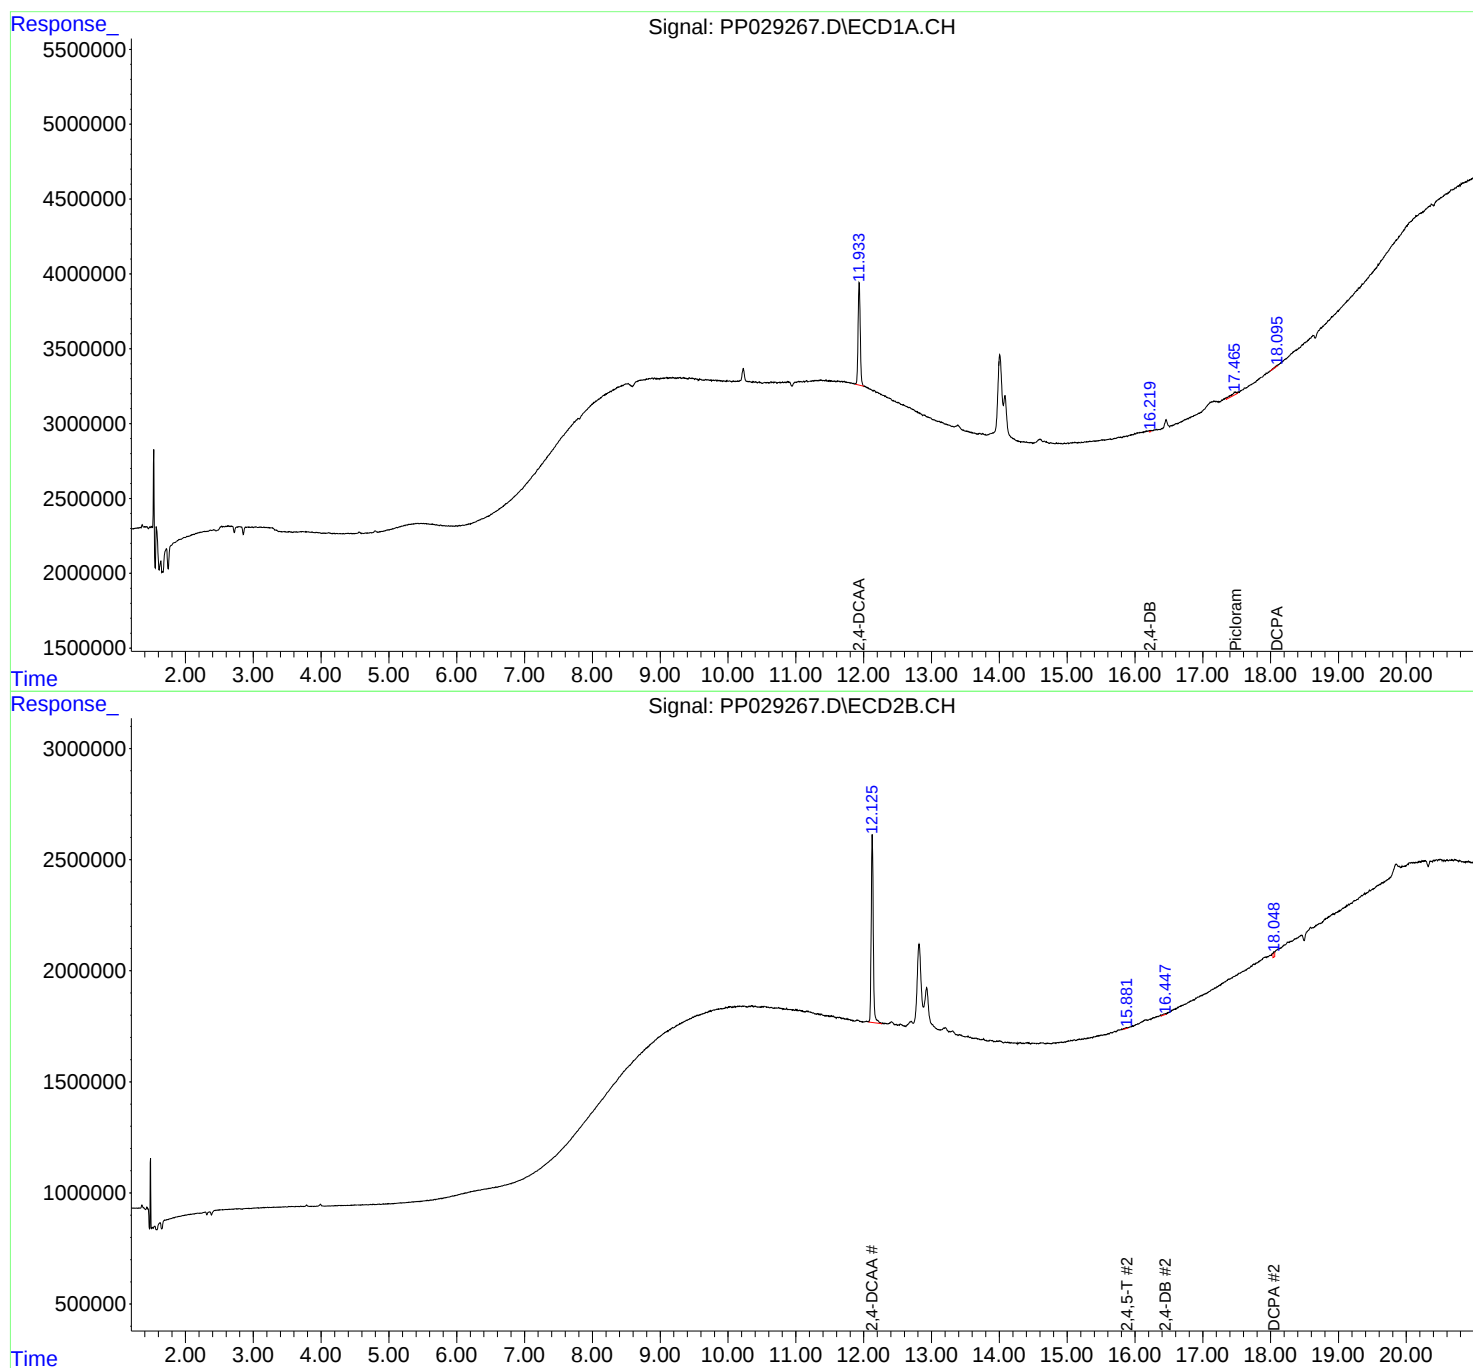


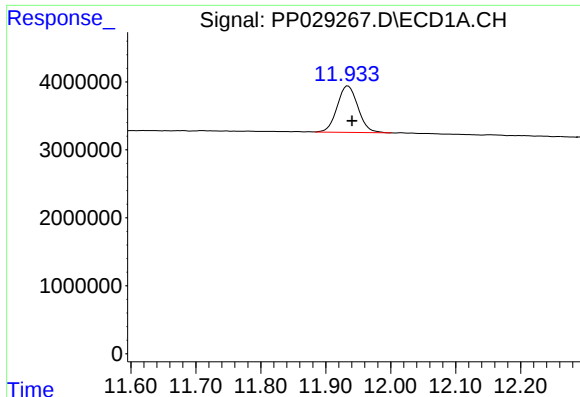

#4 2,4-DCAA


R.T.: 11.934 min
Delta R.T.: -0.006 min
Response: 15157440
Conc: 504.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

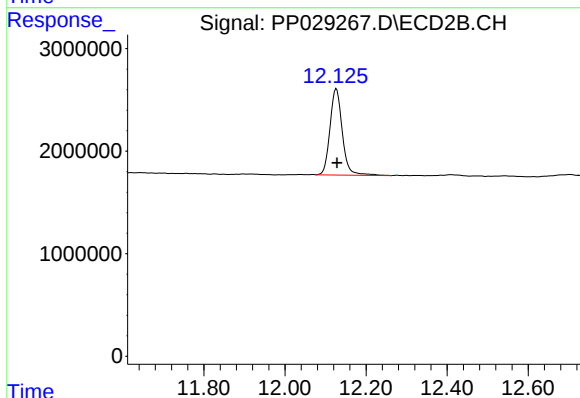


#4 2,4-DCAA

R.T.: 12.127 min
Delta R.T.: -0.002 min
Response: 17813034
Conc: 469.35 ng/ml

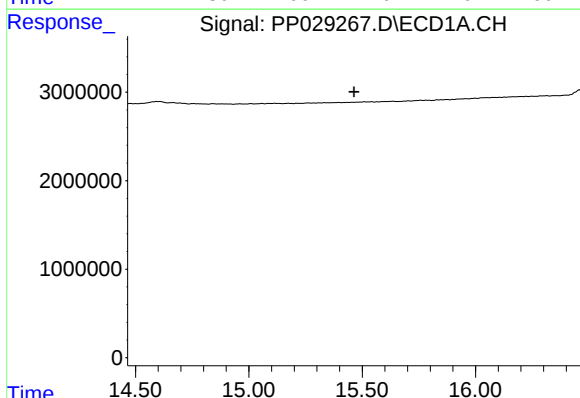


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.464 min
Response: 0
Conc: N.D.

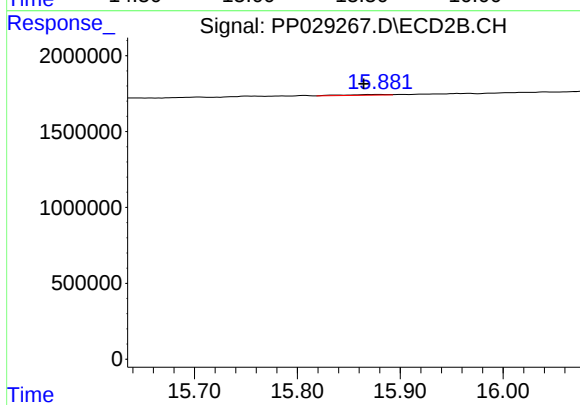

#12 2,4,5-T


R.T.: 15.880 min
Delta R.T.: 0.015 min
Response: 143267
Conc: 0.87 ng/ml

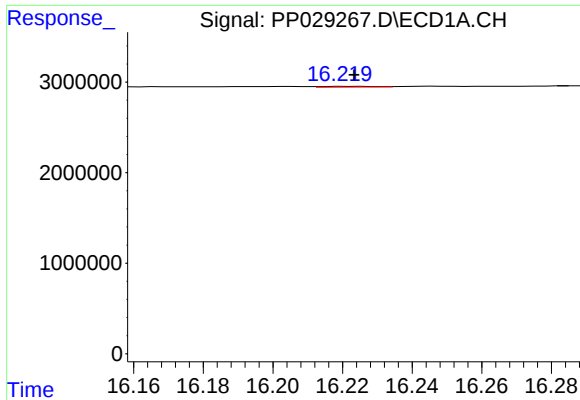

#13 2,4-DB


R.T.: 16.223 min
Delta R.T.: 0.000 min
Response: 89385
Conc: 4.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

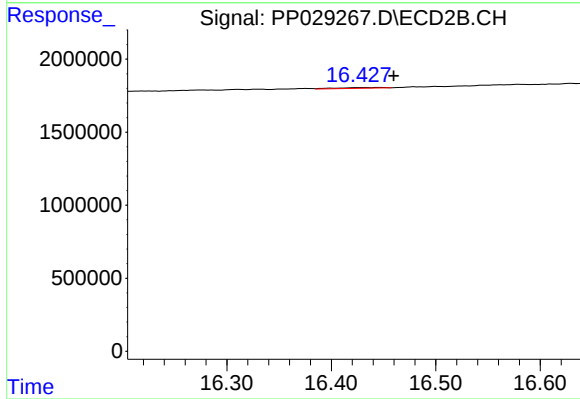


#13 2,4-DB

R.T.: 16.447 min
Delta R.T.: -0.012 min
Response: 138923
Conc: 6.17 ng/ml

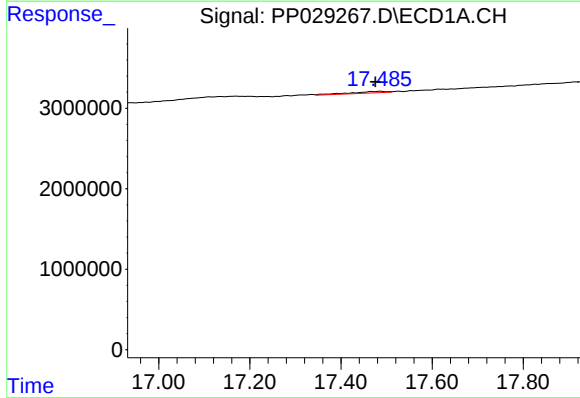


#15 Picloram

R.T.: 17.486 min
Delta R.T.: 0.011 min
Response: 1073034
Conc: 3.86 ng/ml

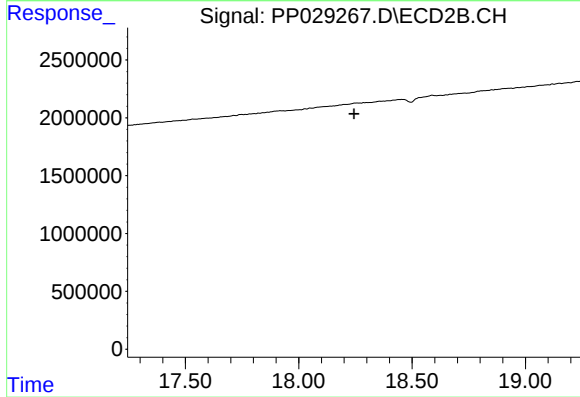

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 18.245 min
Response: 0
Conc: N.D.

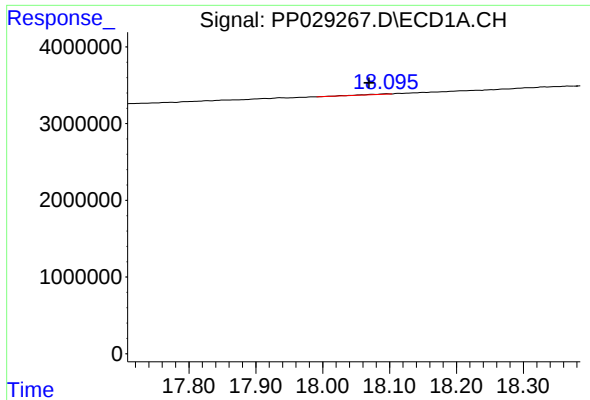

#16 DCPA

R.T.: 18.096 min
Delta R.T.: 0.027 min
Response: 135323
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

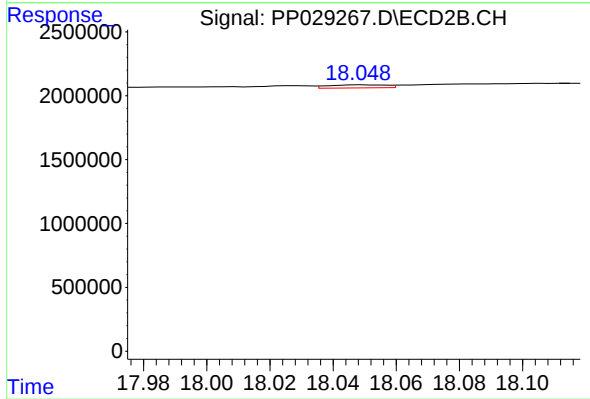

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.069 min
Response: 302864
Conc: 1.30 ng/ml