

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
 Data File : PP029276.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2019 13:43
 Operator : EI\MA
 Sample : K1697-04
 Misc : hexane
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SU-03-031119-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:57:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.932	12.126	16878140	20480387	561.550	539.632
Target Compounds							
3) T	4-Nitroph...	0.000	11.317	0	2909137	N.D.	121.478 #
9) T	2,4-D	13.815	0.000	699509	0	17.841	N.D. #
11) T	2,4,5-TP ...	15.117	0.000	203781	0	0.859	N.D. #
12) T	2,4,5-T	0.000	15.838	0	1954093	N.D.	11.802 #
13) T	2,4-DB	16.223	16.524	758337	2090808	39.699	92.815 #
14) T	DINOSEB	17.686	16.911	91554	3060163	0.629	23.347 #
15) T	Picloram	17.471	0.000	1483791	0	5.336	N.D. #
16) T	DCPA	18.134	0.000	216266	0	0.766	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
Data File : PP029276.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2019 13:43
Operator : EI\MA
Sample : K1697-04
Misc : hexane
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SU-03-031119-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:57:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

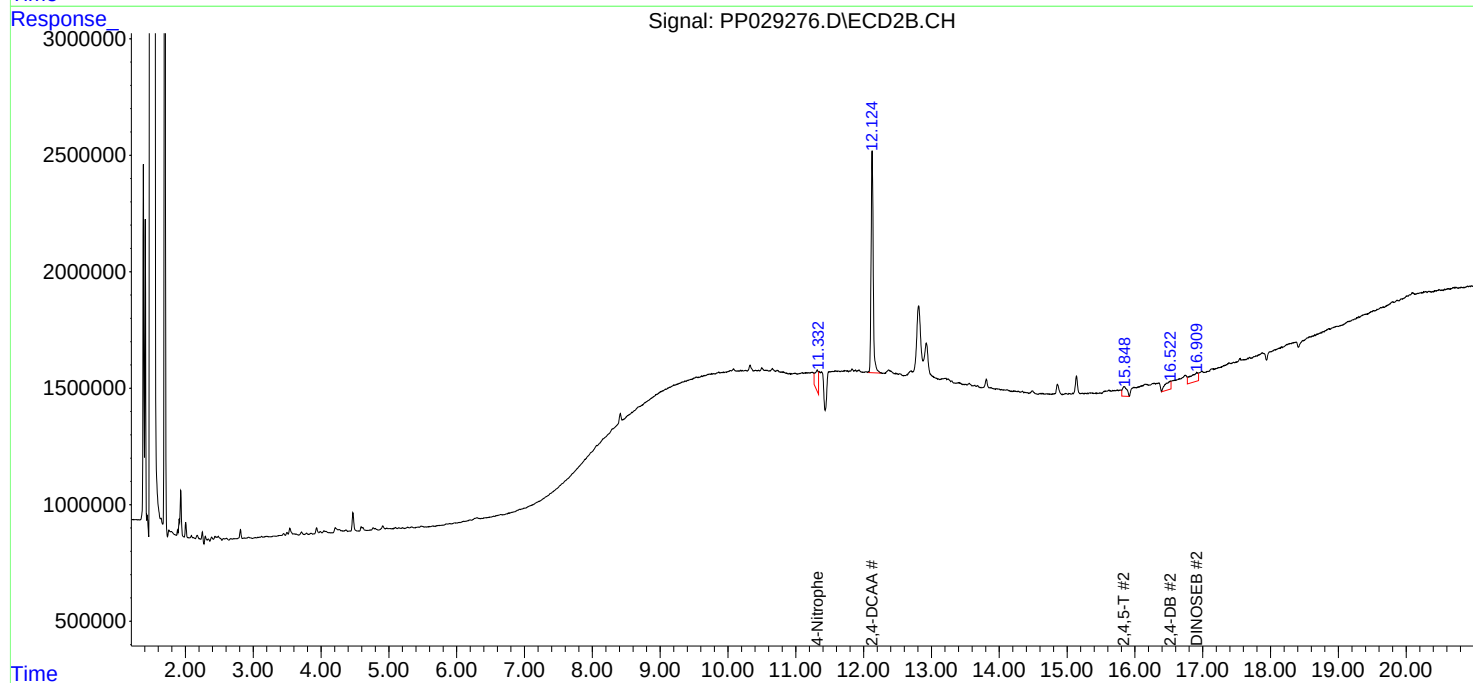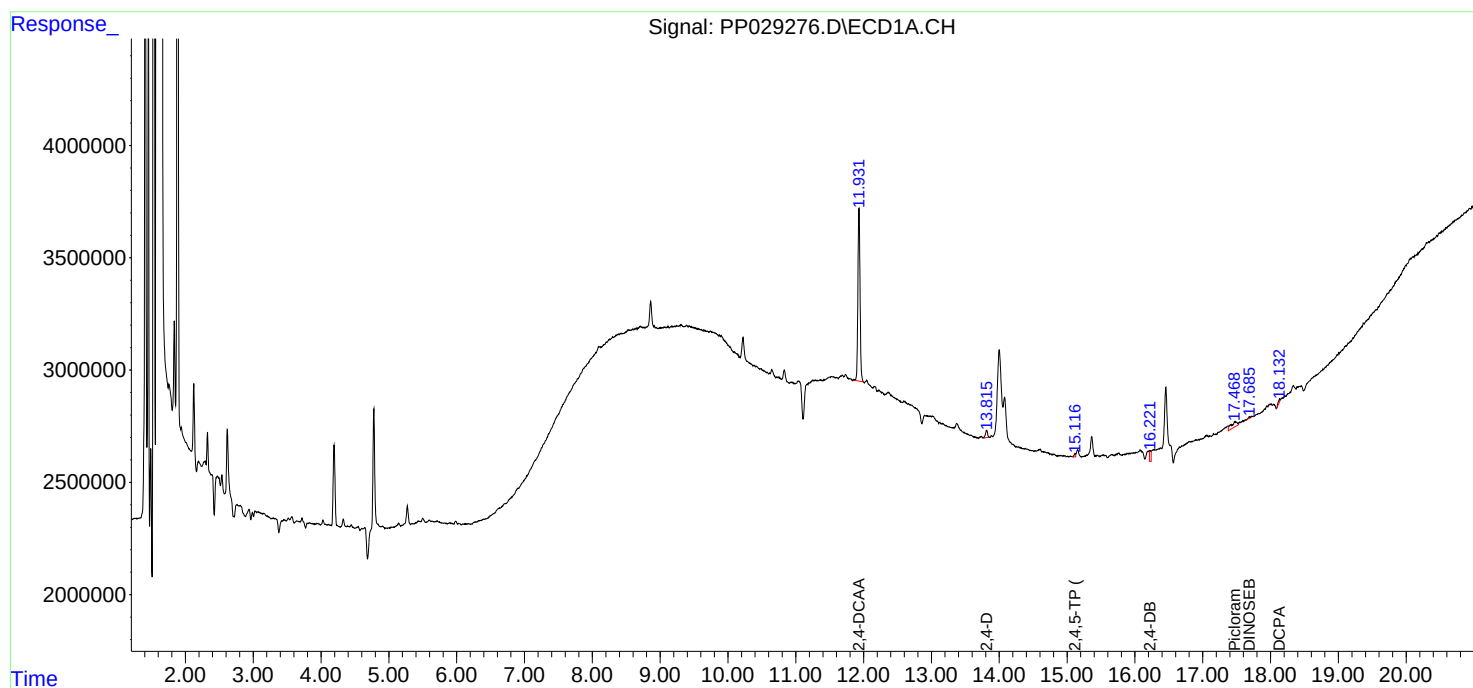


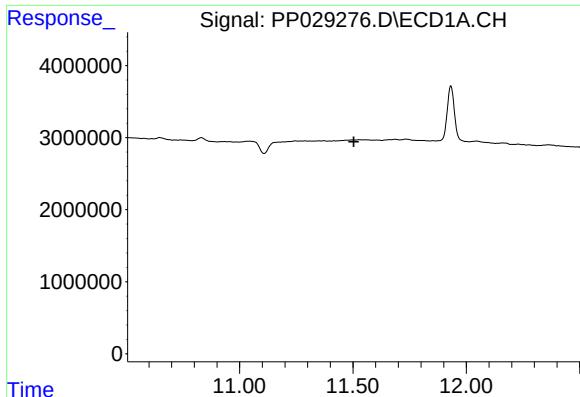

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SU-03-031119-B

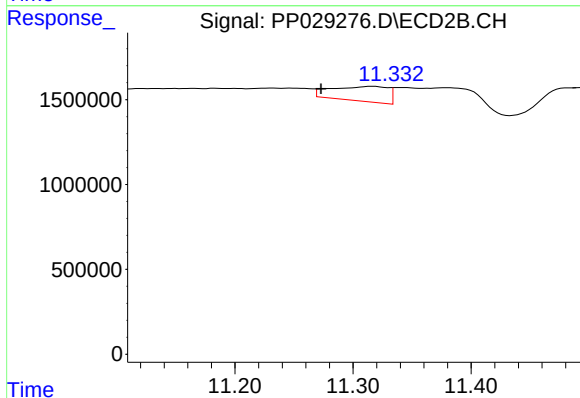


#3 4-Nitrophenol

R.T.: 11.317 min
Delta R.T.: 0.044 min
Response: 2909137
Conc: 121.48 ng/ml

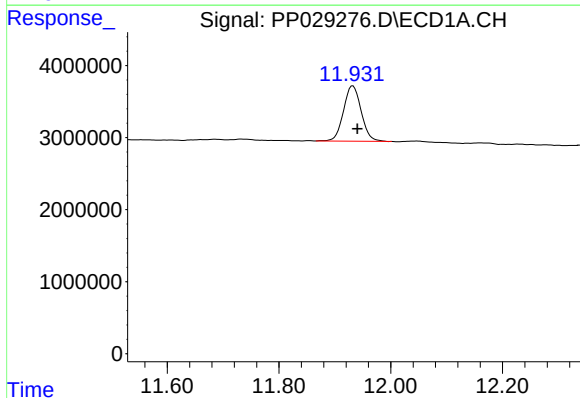


#4 2,4-DCAA

R.T.: 11.932 min
Delta R.T.: -0.008 min
Response: 16878140
Conc: 561.55 ng/ml

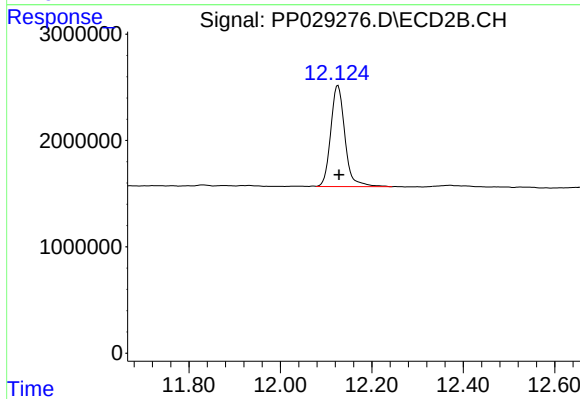

#4 2,4-DCAA


R.T.: 12.126 min
Delta R.T.: -0.003 min
Response: 20480387
Conc: 539.63 ng/ml

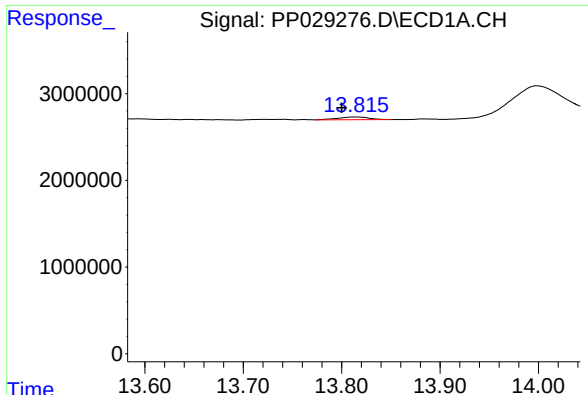

#9 2,4-D


R.T.: 13.815 min
Delta R.T.: 0.014 min
Response: 699509
Conc: 17.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-03-031119-B

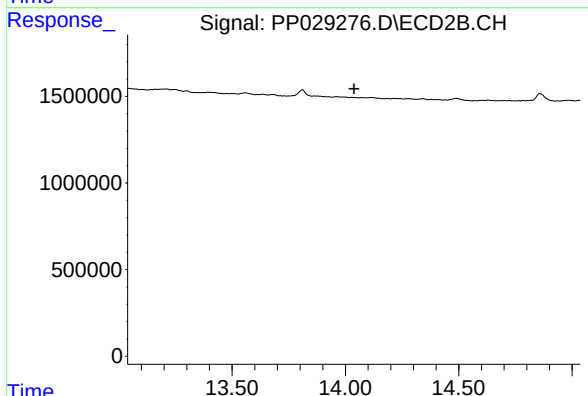


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.038 min
Response: 0
Conc: N.D.

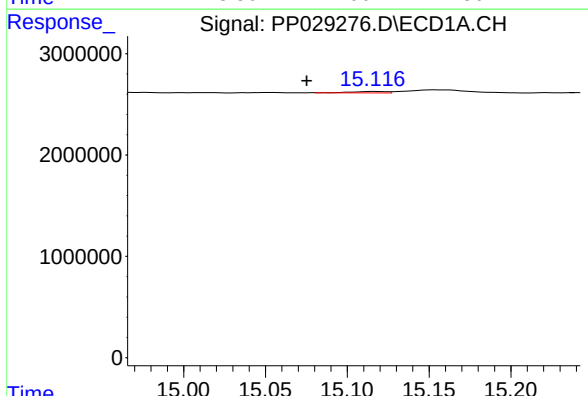


#11 2,4,5-TP (SILVEX)

R.T.: 15.117 min
Delta R.T.: 0.042 min
Response: 203781
Conc: 0.86 ng/ml

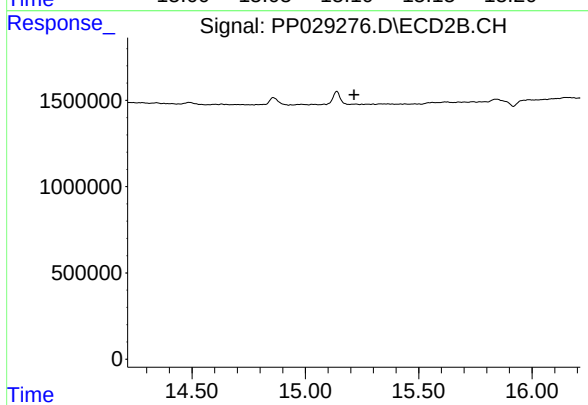

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 15.216 min
Response: 0
Conc: N.D.

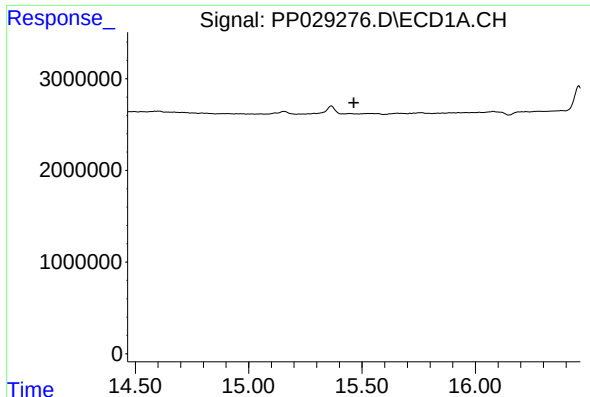

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SU-03-031119-B

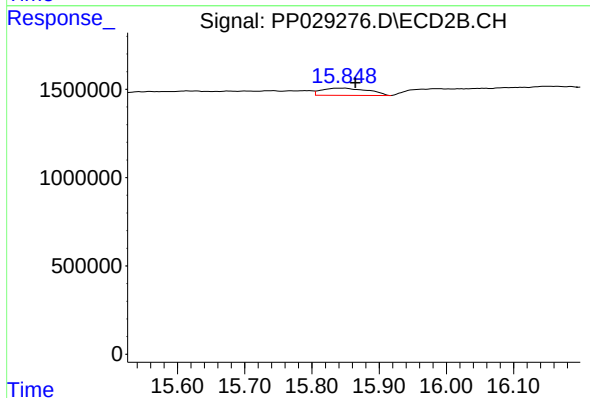


#12 2,4,5-T

R.T.: 15.838 min
Delta R.T.: -0.026 min
Response: 1954093
Conc: 11.80 ng/ml

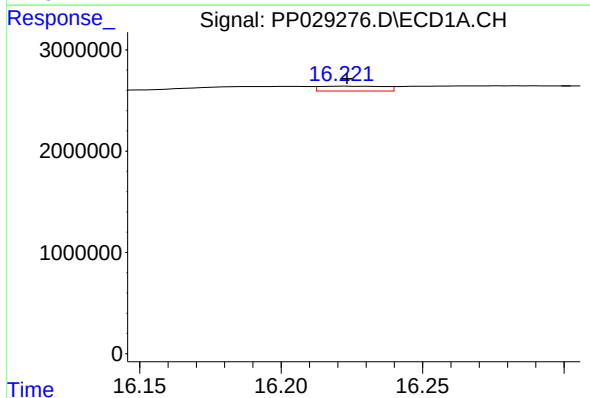


#13 2,4-DB

R.T.: 16.223 min
Delta R.T.: 0.000 min
Response: 758337
Conc: 39.70 ng/ml

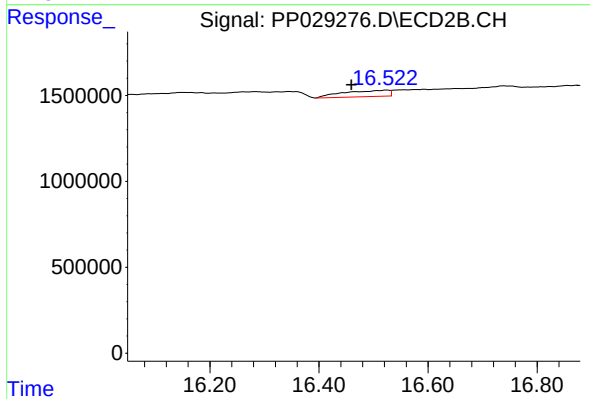

#13 2,4-DB


R.T.: 16.524 min
Delta R.T.: 0.064 min
Response: 2090808
Conc: 92.82 ng/ml

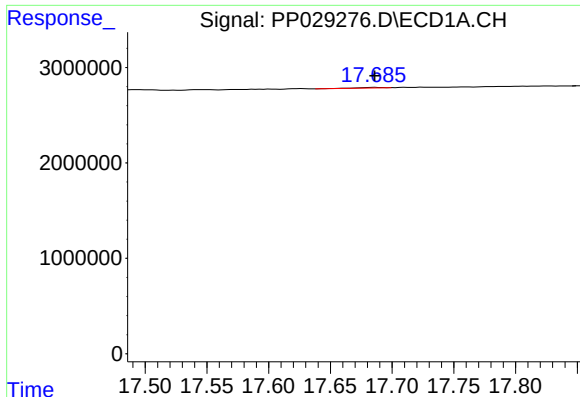

#14 DINOSEB


R.T.: 17.686 min
Delta R.T.: 0.000 min
Response: 91554
Conc: 0.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-03-031119-B

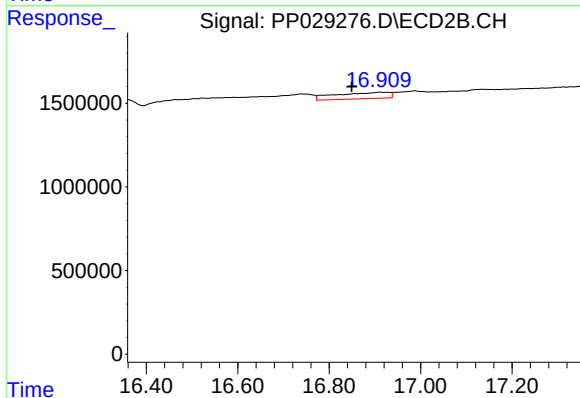


#14 DINOSEB

R.T.: 16.911 min
Delta R.T.: 0.061 min
Response: 3060163
Conc: 23.35 ng/ml

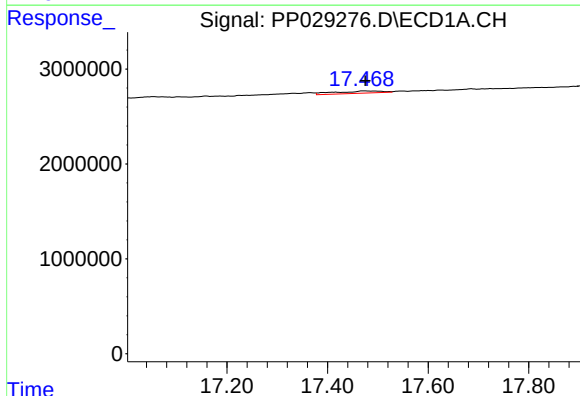


#15 Picloram

R.T.: 17.471 min
Delta R.T.: -0.004 min
Response: 1483791
Conc: 5.34 ng/ml

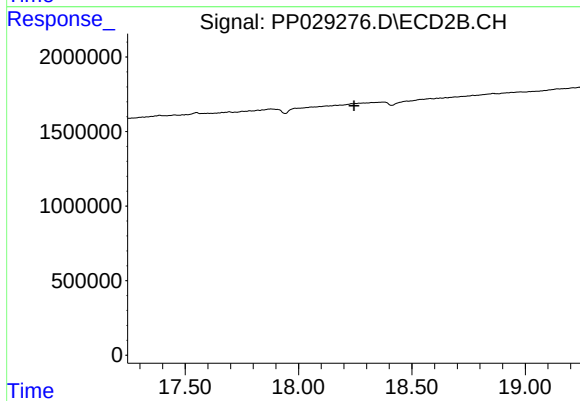

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 18.245 min
Response: 0
Conc: N.D.

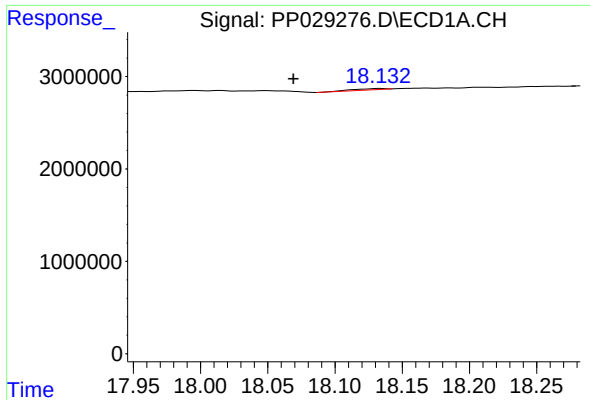

#16 DCPA

R.T.: 18.134 min
Delta R.T.: 0.065 min
Response: 216266
Conc: 0.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-03-031119-B

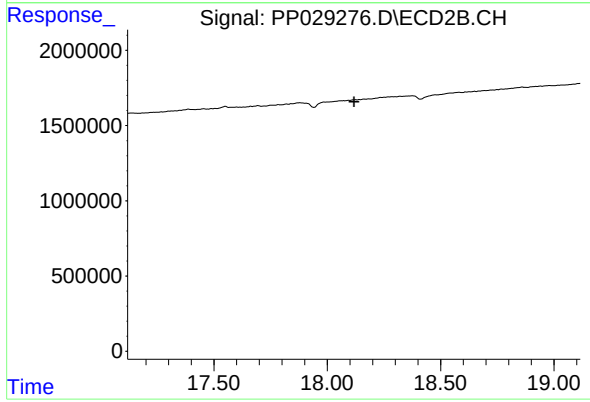

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.118 min
Response: 0
Conc: N.D.