

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
 Data File : PP029282.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2019 16:16
 Operator : EI\MA
 Sample : K1697-08
 Misc : hexane
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SU-04-031119-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:02:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.932	12.126	17940575	21390074	596.898	563.601
Target Compounds							
8) T	DICHLORPROP	13.383	0.000	549146	0	17.797	N.D. #
9) T	2,4-D	13.813	0.000	473758	0	12.083	N.D. #
11) T	2,4,5-TP ...	0.000	15.191	0	3881578	N.D.	19.083 #
12) T	2,4,5-T	0.000	15.846	0	2045938	N.D.	12.357 #
13) T	2,4-DB	16.233	0.000	1318298	0	69.012	N.D. #
14) T	DINOSEB	17.681	0.000	1094297	0	7.514	N.D. #
15) T	Picloram	17.469	18.293	890249	2566994	3.202	11.408 #
16) T	DCPA	0.000	18.136	0	2090372	N.D.	8.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
Data File : PP029282.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2019 16:16
Operator : EI\MA
Sample : K1697-08
Misc : hexane
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:02:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

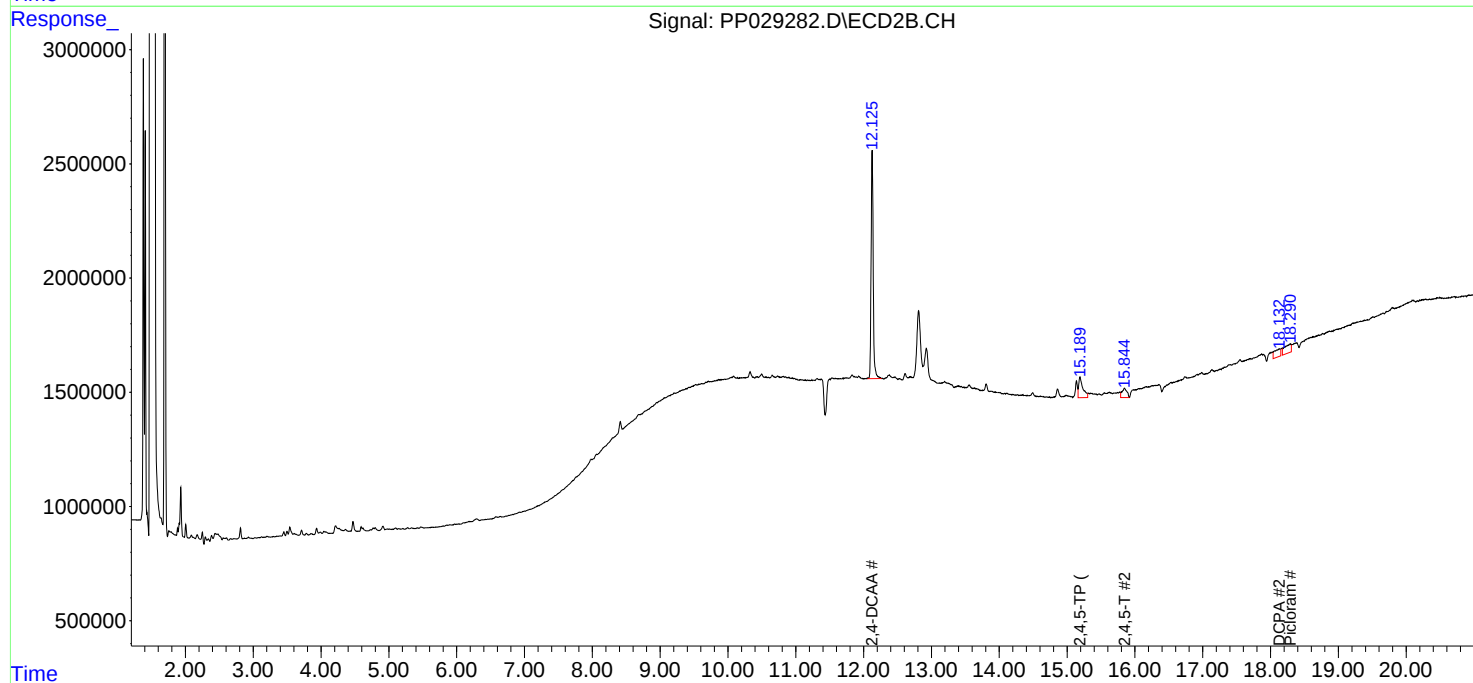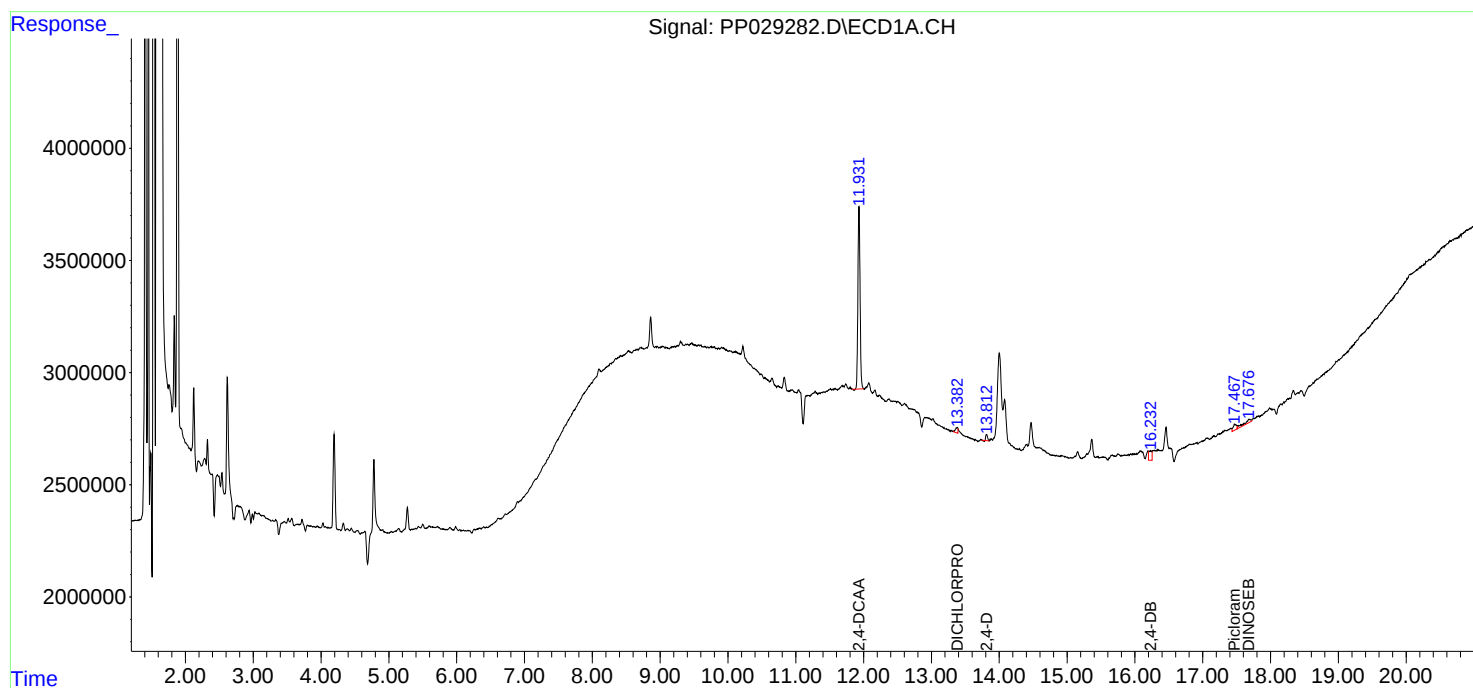


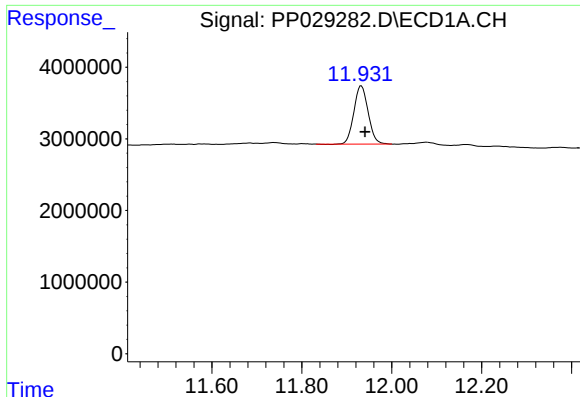

#4 2,4-DCAA


R.T.: 11.932 min
Delta R.T.: -0.008 min
Response: 17940575
Conc: 596.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

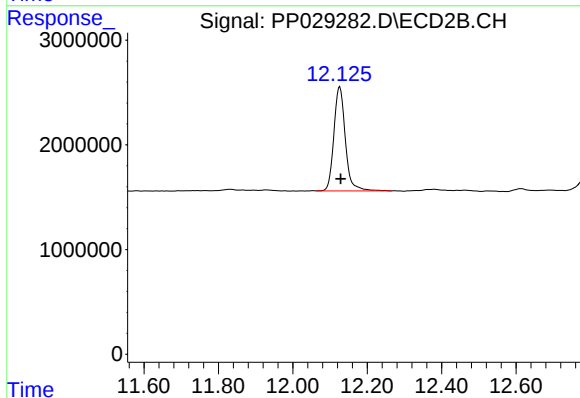


#4 2,4-DCAA

R.T.: 12.126 min
Delta R.T.: -0.002 min
Response: 21390074
Conc: 563.60 ng/ml

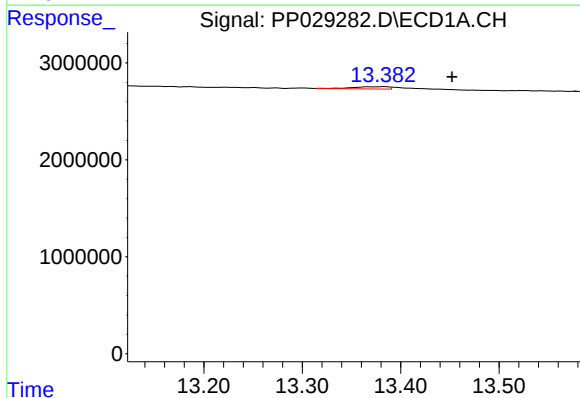


#8 DICHLORPROP

R.T.: 13.383 min
Delta R.T.: -0.069 min
Response: 549146
Conc: 17.80 ng/ml

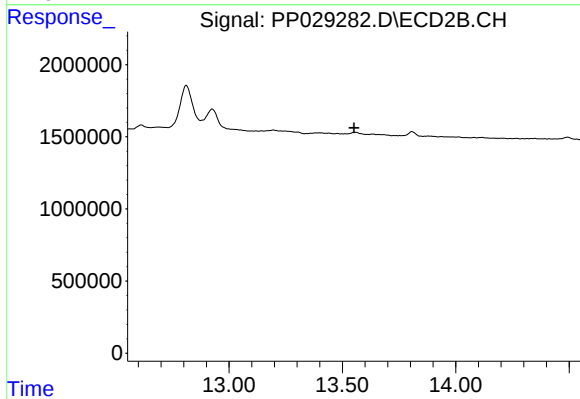

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.552 min
Response: 0
Conc: N.D.

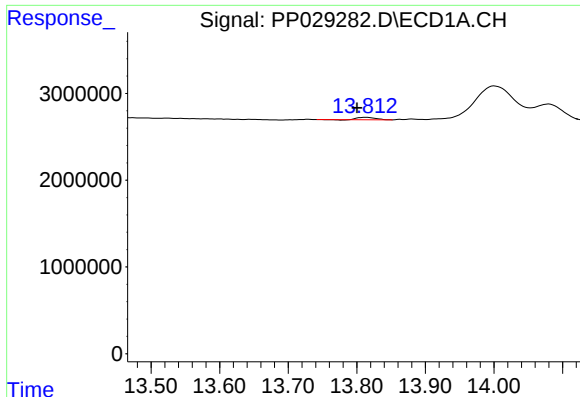

#9 2,4-D


R.T.: 13.813 min
Delta R.T.: 0.013 min
Response: 473758
Conc: 12.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

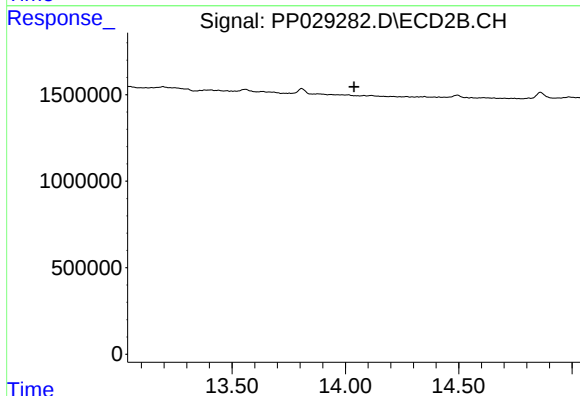


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.038 min
Response: 0
Conc: N.D.

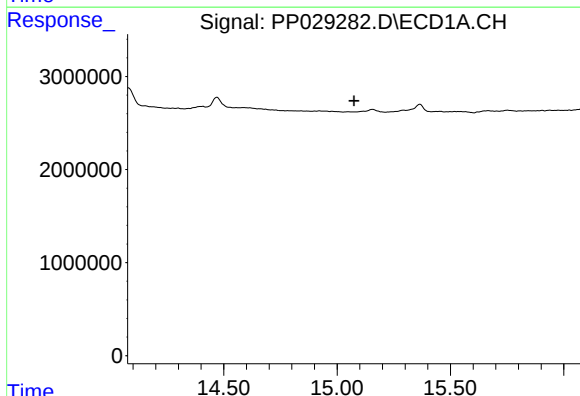


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.075 min
Response: 0
Conc: N.D.

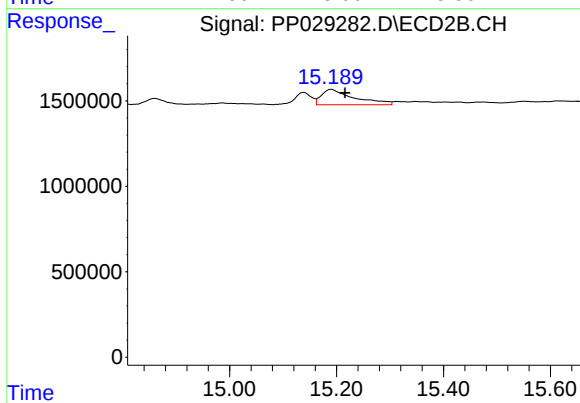

#11 2,4,5-TP (SILVEX)


R.T.: 15.191 min
Delta R.T.: -0.025 min
Response: 3881578
Conc: 19.08 ng/ml

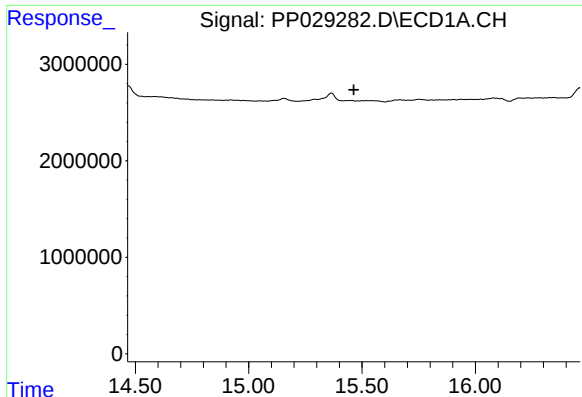

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

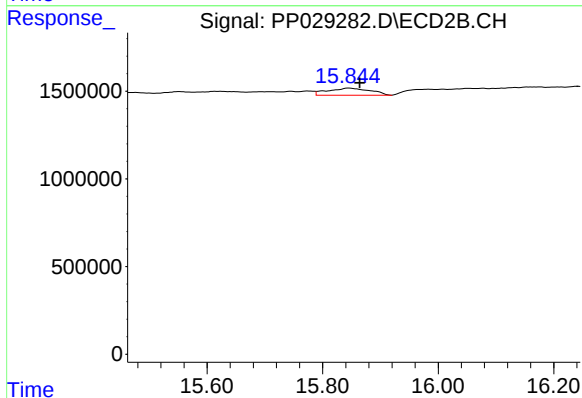


#12 2,4,5-T

R.T.: 15.846 min
Delta R.T.: -0.019 min
Response: 2045938
Conc: 12.36 ng/ml

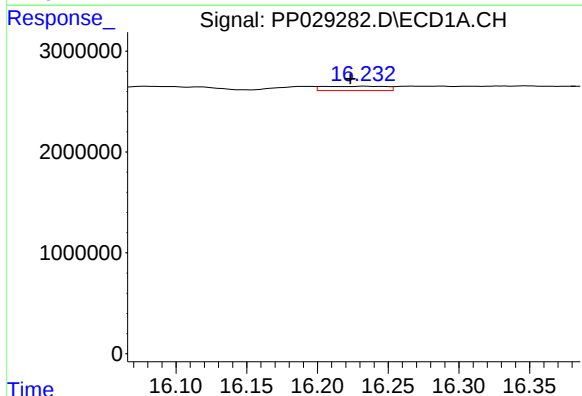


#13 2,4-DB

R.T.: 16.233 min
Delta R.T.: 0.010 min
Response: 1318298
Conc: 69.01 ng/ml

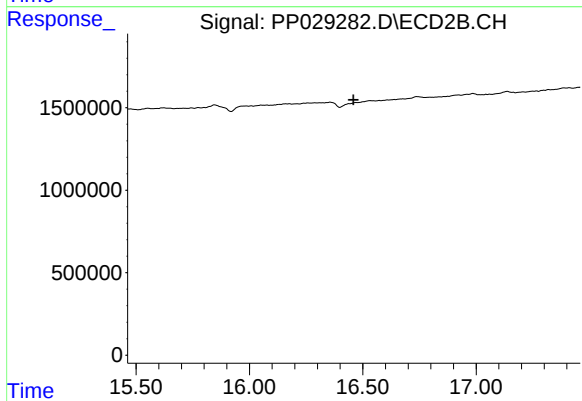

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.460 min
Response: 0
Conc: N.D.

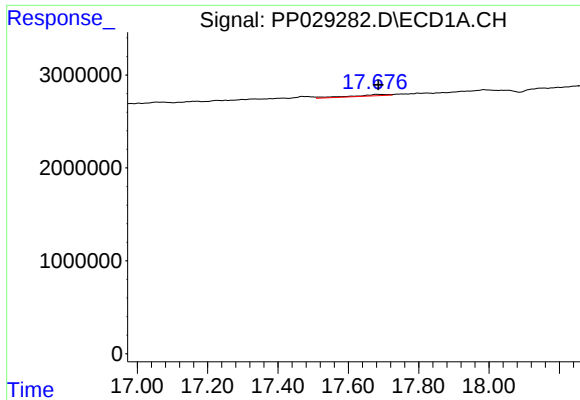

#14 DINOSEB


R.T.: 17.681 min
Delta R.T.: -0.005 min
Response: 1094297
Conc: 7.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

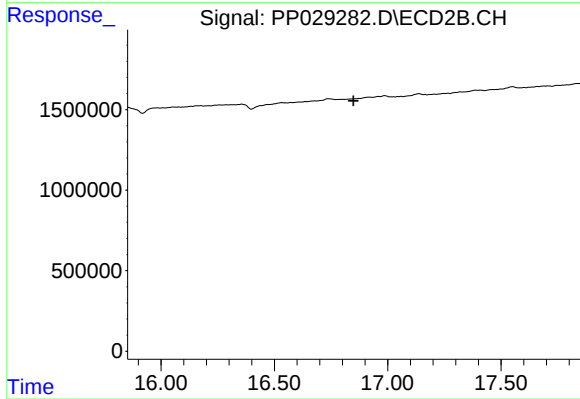


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.849 min
Response: 0
Conc: N.D.

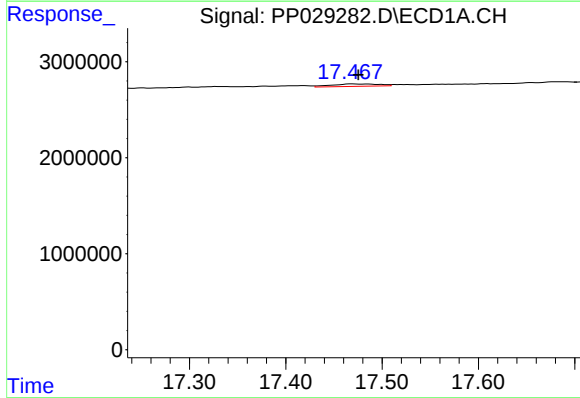


#15 Picloram

R.T.: 17.469 min
Delta R.T.: -0.006 min
Response: 890249
Conc: 3.20 ng/ml

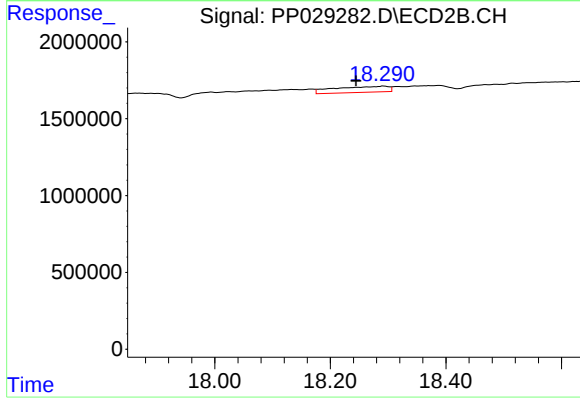

#15 Picloram


R.T.: 18.293 min
Delta R.T.: 0.048 min
Response: 2566994
Conc: 11.41 ng/ml

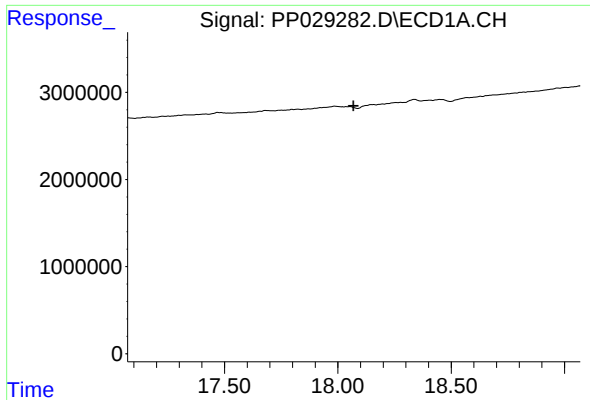

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SU-04-031119-B

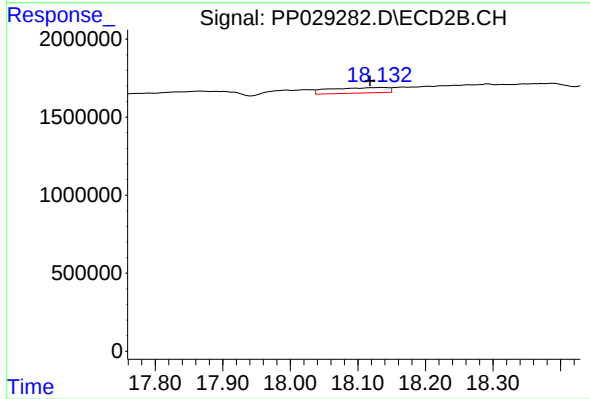

#16 DCPA

R.T.: 18.136 min
Delta R.T.: 0.017 min
Response: 2090372
Conc: 8.99 ng/ml