

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
 Data File : PP029289.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2019 19:14
 Operator : EI\MA
 Sample : K1849-07
 Misc : hexane
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 C135-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:03:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.932	12.126	16578131	23122802	551.568	609.256
Target Compounds							
3) T	4-Nitroph...	0.000	11.314	0	2729107	N.D.	113.961 #
5) T	DICAMBA	12.275	0.000	1302626	0	9.796	N.D. #
9) T	2,4-D	13.794	14.035	4951490	5446129	126.290	120.108
12) T	2,4,5-T	0.000	15.843	0	2267913	N.D.	13.697 #
13) T	2,4-DB	0.000	16.523	0	3003330	N.D.	133.324 #
14) T	DINOSEB	17.678	16.860	975554	325475	6.699	2.483 #
15) T	Picloram	17.469	18.245	5155118	7617527	18.540	33.852 #
16) T	DCPA	0.000	18.132	0	478527	N.D.	2.059 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031319\
Data File : PP029289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2019 19:14
Operator : EI\MA
Sample : K1849-07
Misc : hexane
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
C135-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:03:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

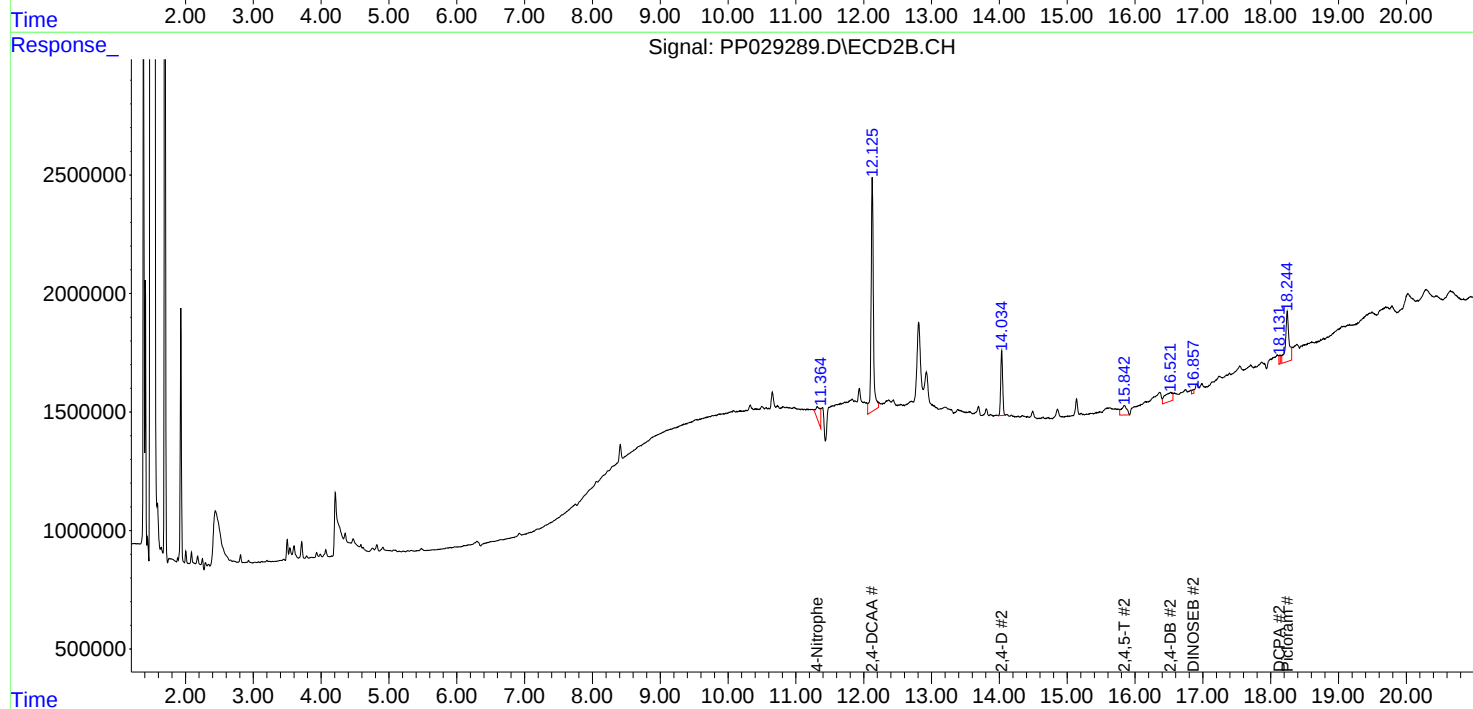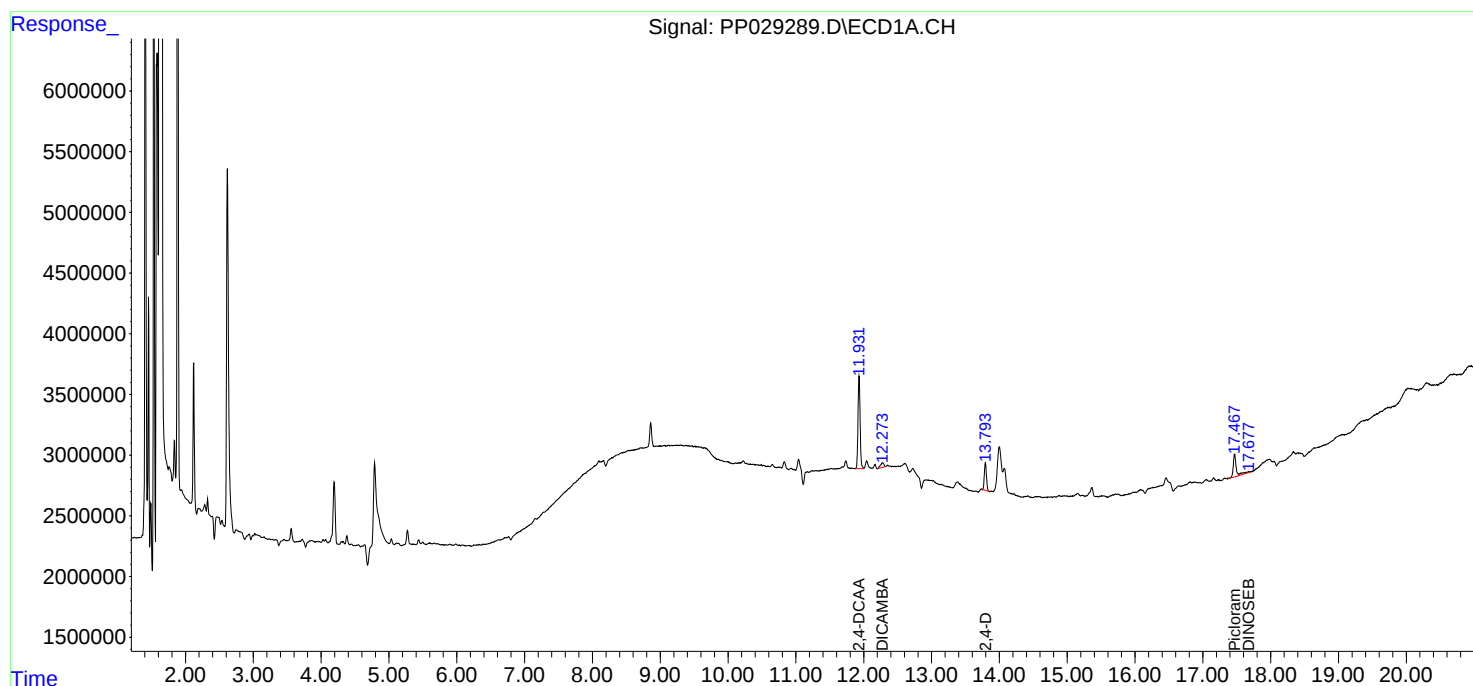


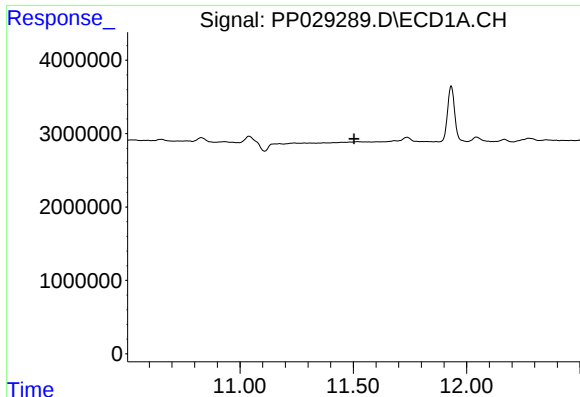

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
C135-CON

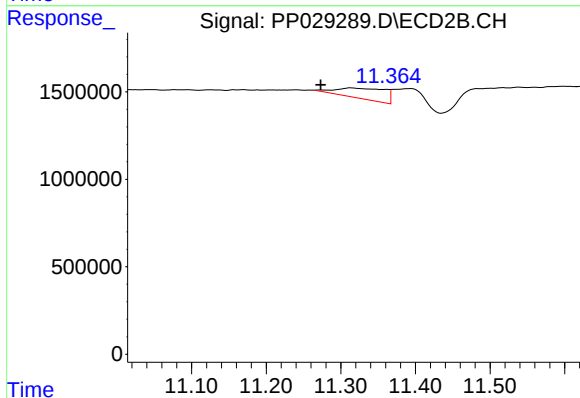


#3 4-Nitrophenol

R.T.: 11.314 min
Delta R.T.: 0.041 min
Response: 2729107
Conc: 113.96 ng/ml

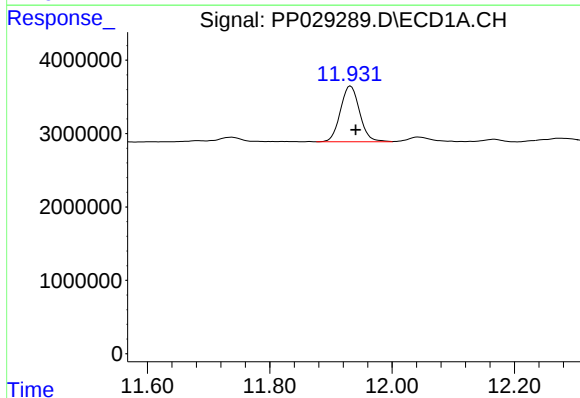


#4 2,4-DCAA

R.T.: 11.932 min
Delta R.T.: -0.008 min
Response: 16578131
Conc: 551.57 ng/ml

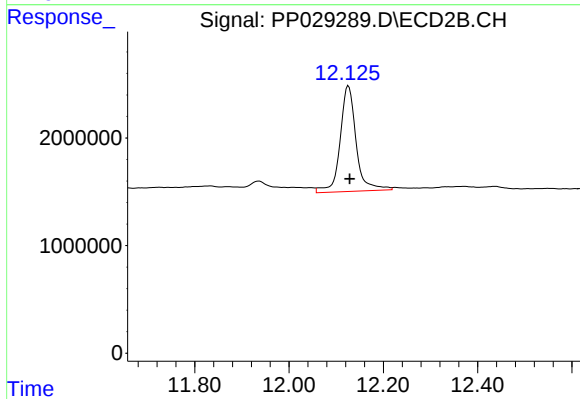

#4 2,4-DCAA


R.T.: 12.126 min
Delta R.T.: -0.003 min
Response: 23122802
Conc: 609.26 ng/ml

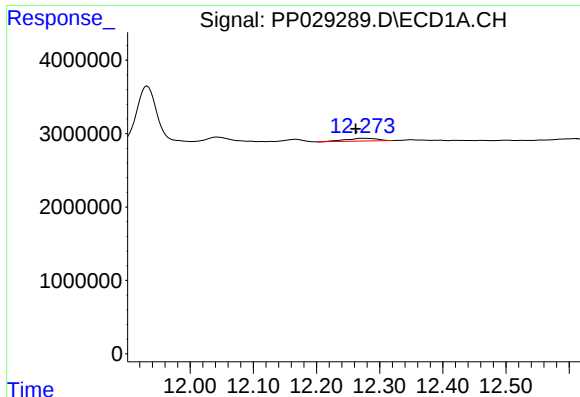

#5 DICAMBA


R.T.: 12.275 min
Delta R.T.: 0.013 min
Response: 1302626
Conc: 9.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
C135-CON

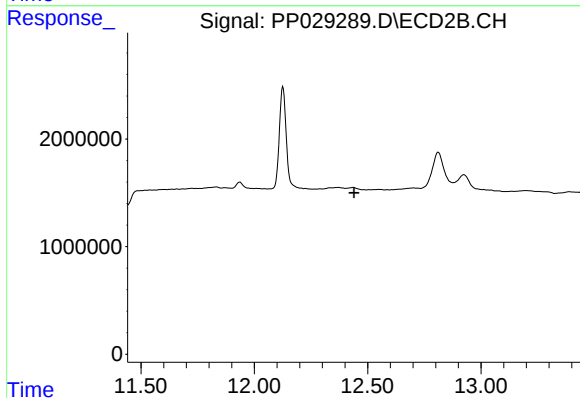


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 12.441 min
Response: 0
Conc: N.D.

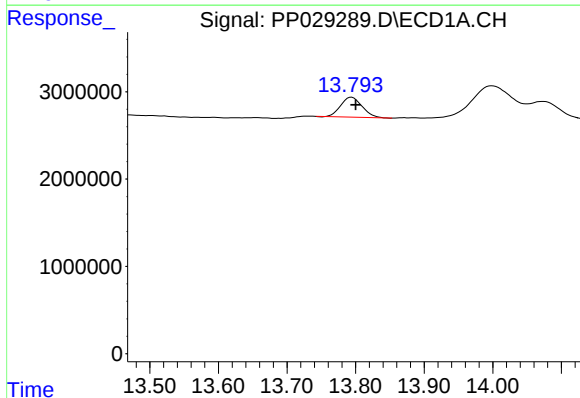


#9 2,4-D

R.T.: 13.794 min
Delta R.T.: -0.006 min
Response: 4951490
Conc: 126.29 ng/ml

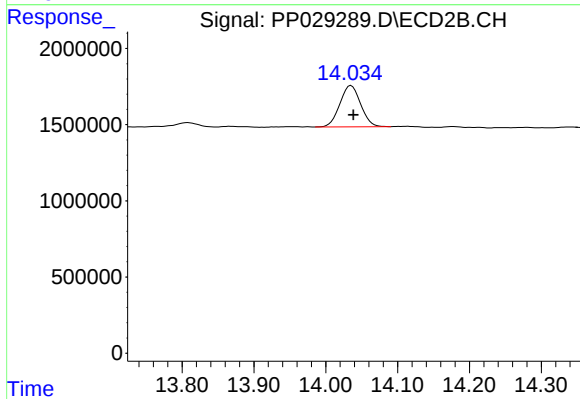

#9 2,4-D


R.T.: 14.035 min
Delta R.T.: -0.003 min
Response: 5446129
Conc: 120.11 ng/ml

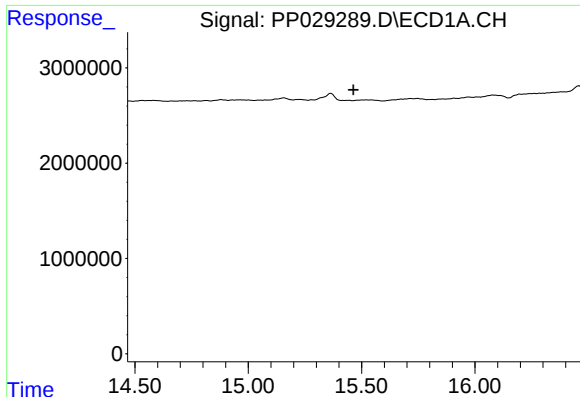

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
C135-CON

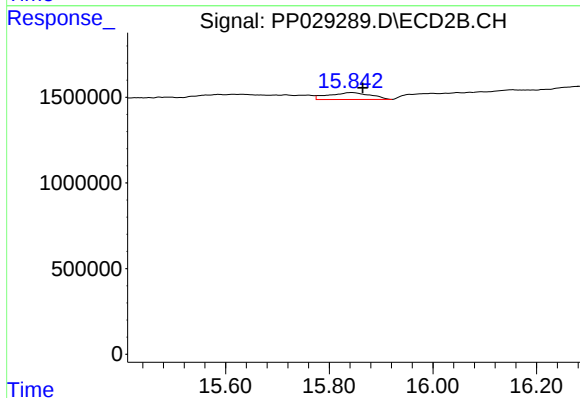


#12 2,4,5-T

R.T.: 15.843 min
Delta R.T.: -0.021 min
Response: 2267913
Conc: 13.70 ng/ml

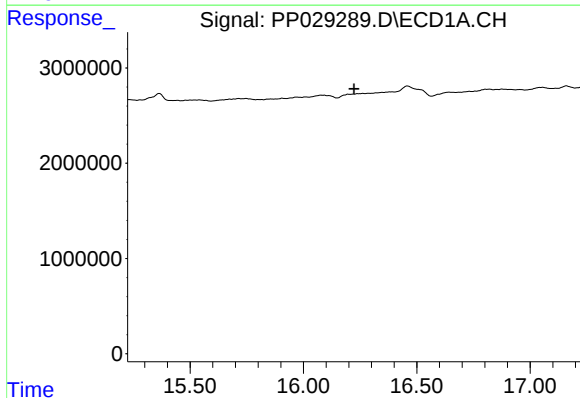


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.223 min
Response: 0
Conc: N.D.

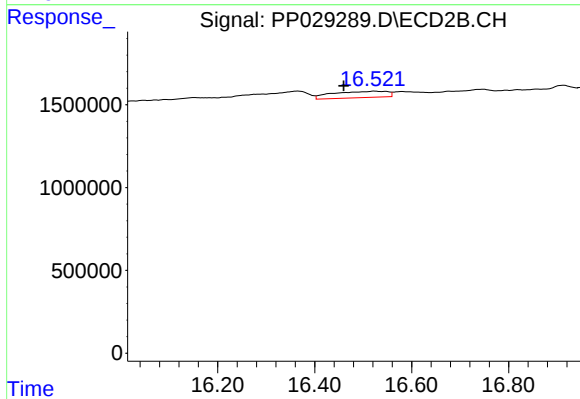

#13 2,4-DB


R.T.: 16.523 min
Delta R.T.: 0.064 min
Response: 3003330
Conc: 133.32 ng/ml

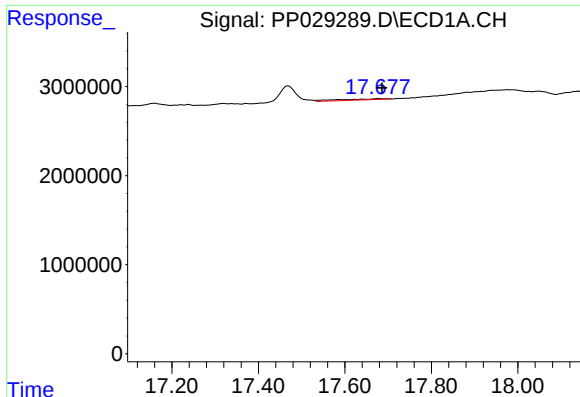

#14 DINOSEB


R.T.: 17.678 min
Delta R.T.: -0.008 min
Response: 975554
Conc: 6.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
C135-CON

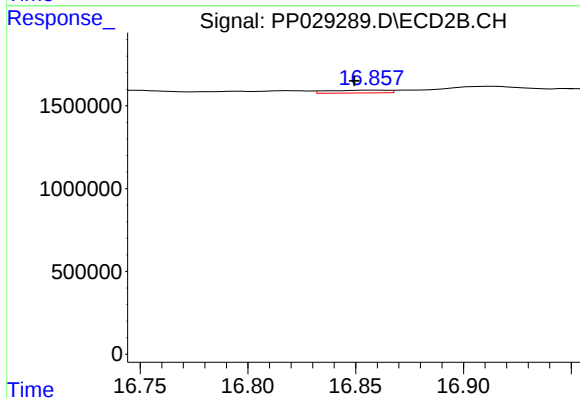


#14 DINOSEB

R.T.: 16.860 min
Delta R.T.: 0.011 min
Response: 325475
Conc: 2.48 ng/ml

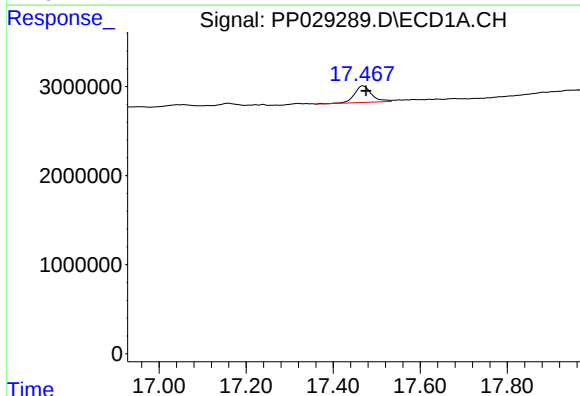


#15 Picloram

R.T.: 17.469 min
Delta R.T.: -0.007 min
Response: 5155118
Conc: 18.54 ng/ml

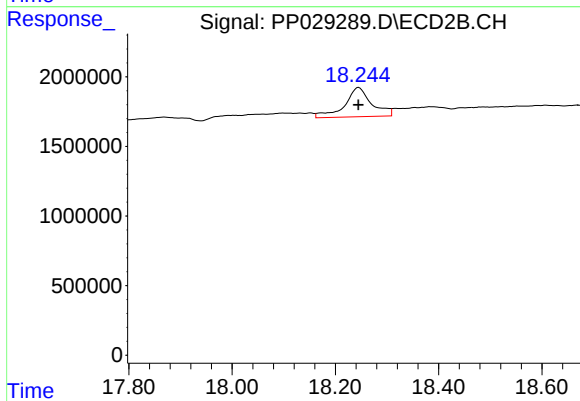

#15 Picloram


R.T.: 18.245 min
Delta R.T.: 0.000 min
Response: 7617527
Conc: 33.85 ng/ml

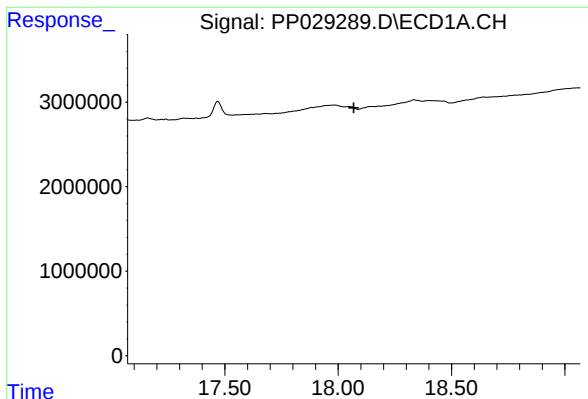

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
C135-CON

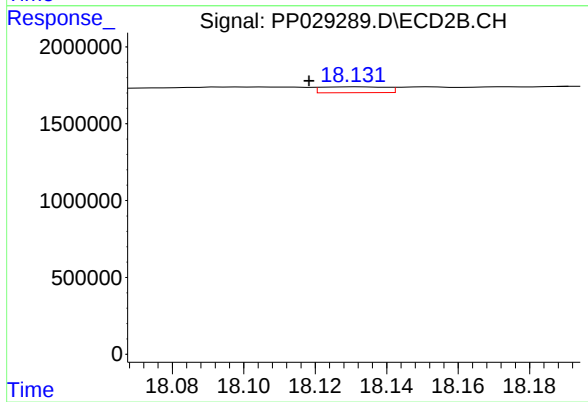

#16 DCPA

R.T.: 18.132 min
Delta R.T.: 0.014 min
Response: 478527
Conc: 2.06 ng/ml