

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
 Data File : PP056451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 19:02
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 21:52:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.316	3.557	26318360	23409656	16.950	16.590
2) SA Decachlor...	10.058	8.554	34954467	19989363	17.597	17.882

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
Data File : PP056451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 19:02
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 21:52:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

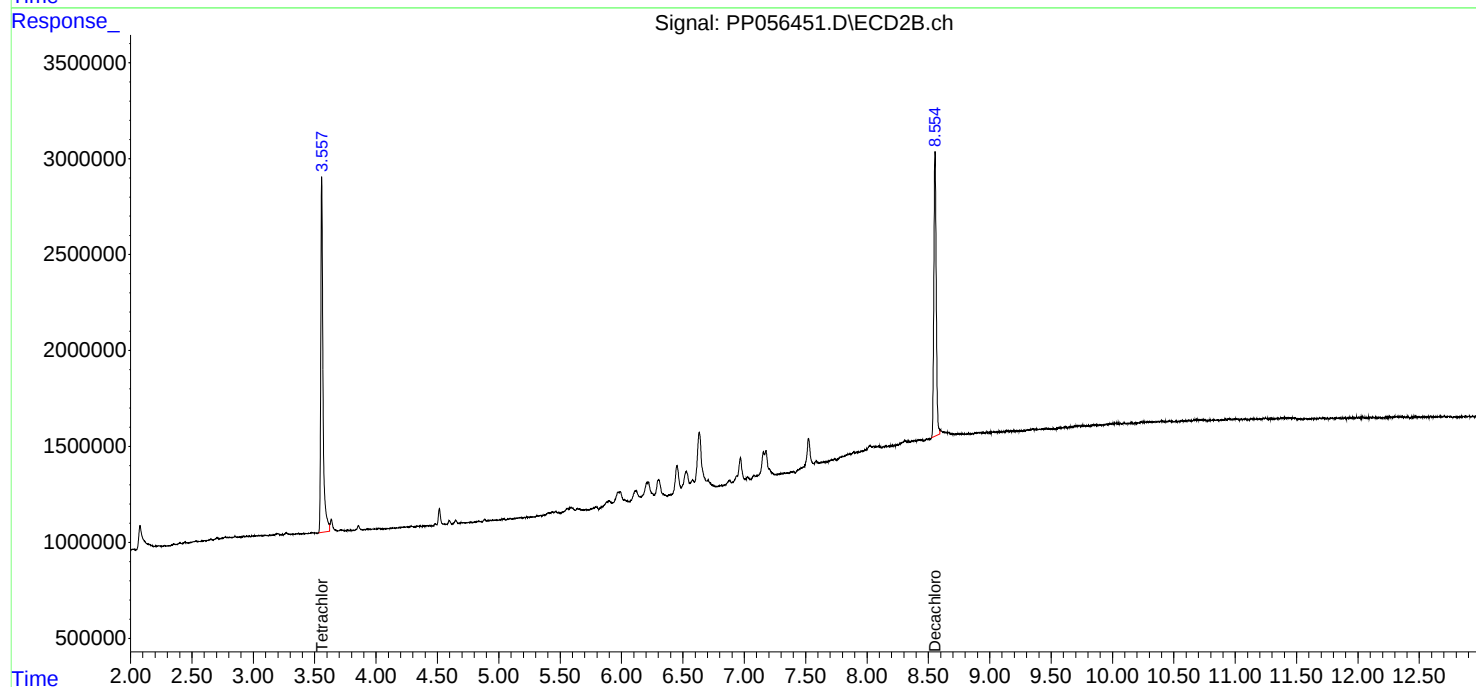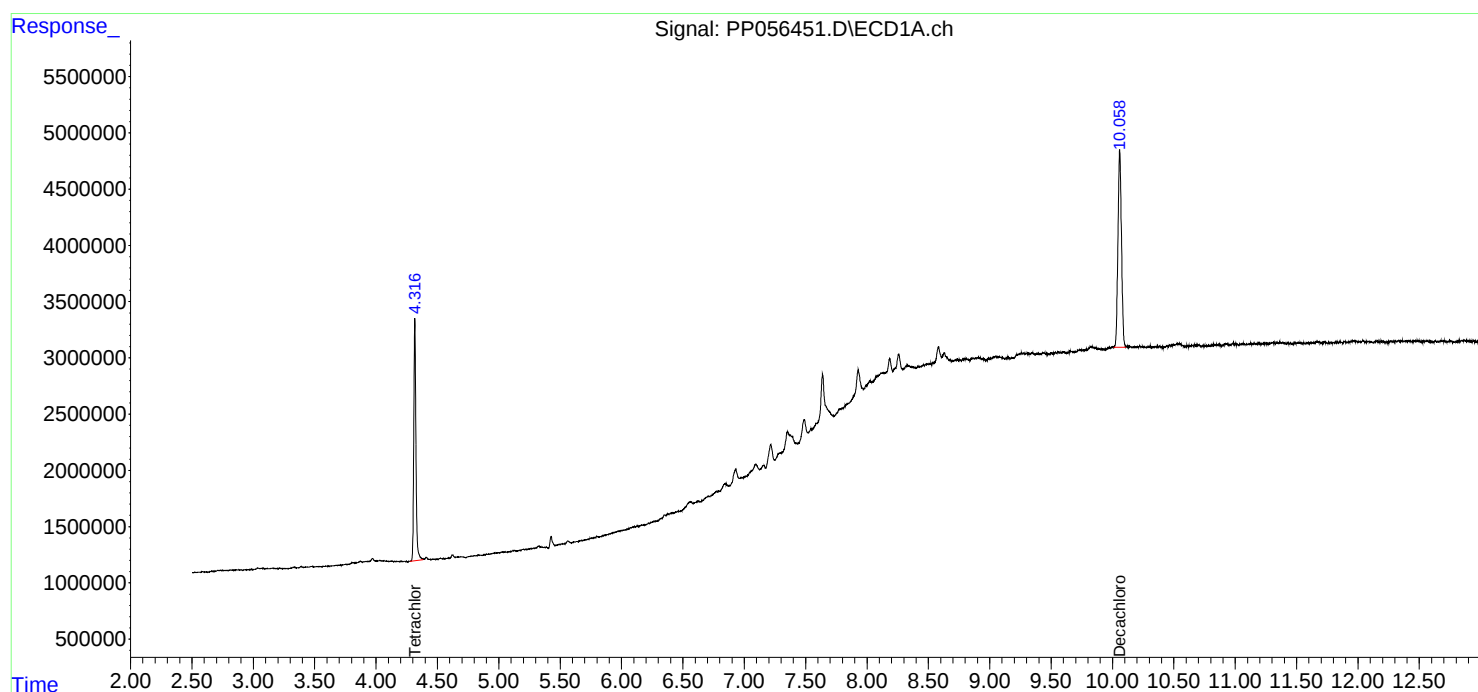


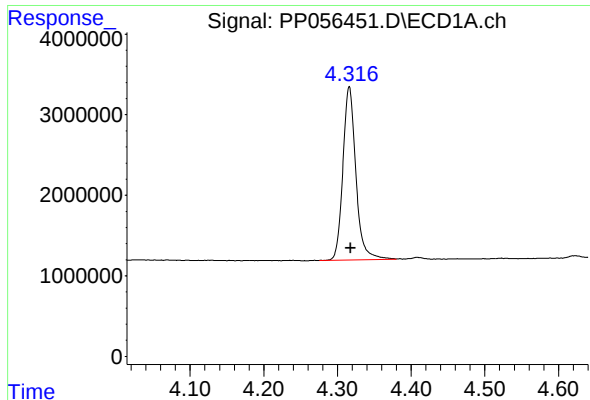

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: -0.002 min
Response: 26318360
Conc: 16.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

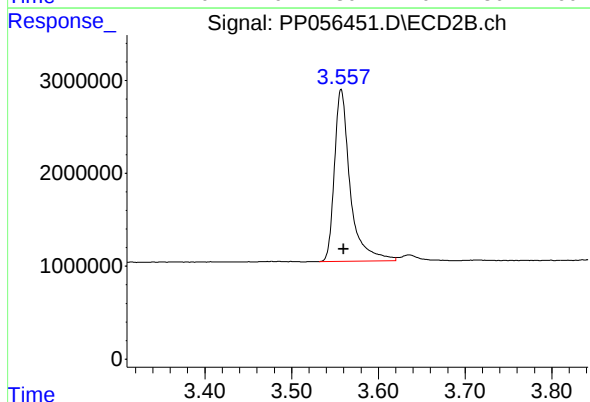


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.003 min
Response: 23409656
Conc: 16.59 ng/ml

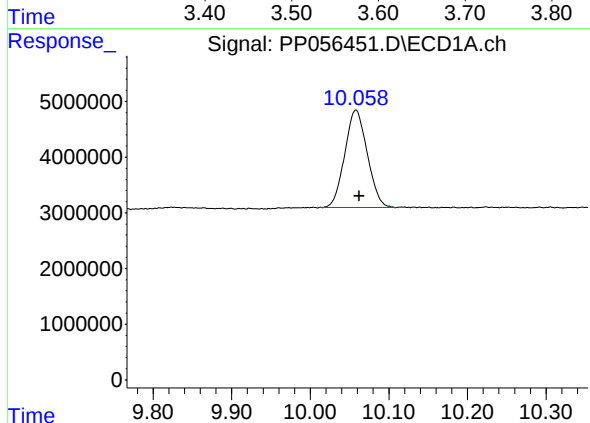

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: -0.004 min
Response: 34954467
Conc: 17.60 ng/ml

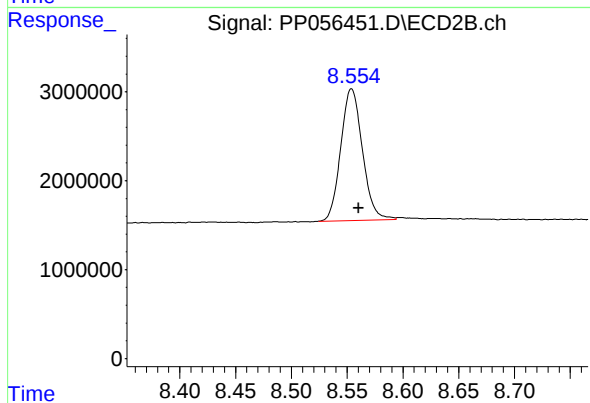

#2 Decachlorobiphenyl

R.T.: 8.554 min
Delta R.T.: -0.007 min
Response: 19989363
Conc: 17.88 ng/ml