

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
 Data File : PP056459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2023 21:14
 Operator : YP\AJ
 Sample : 01878-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 F-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2023
 Supervised By :Ankita Jodhani 03/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 21:57:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.557	37621124	32406677	24.229	22.966
2) SA Decachlor...	10.059	8.555	45187121	26455046	22.749	23.666

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
Data File : PP056459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2023 21:14
Operator : YP\AJ
Sample : 01878-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
F-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2023
Supervised By :Ankita Jodhani 03/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 21:57:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

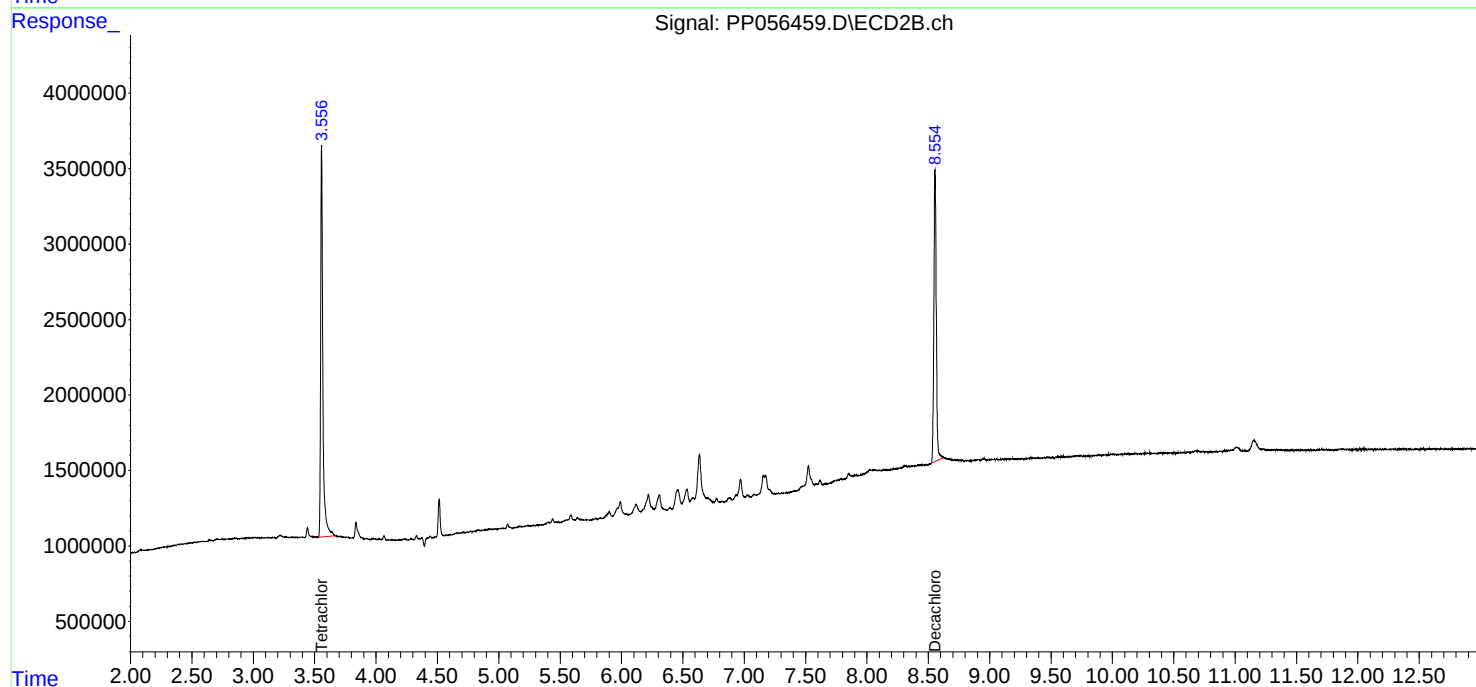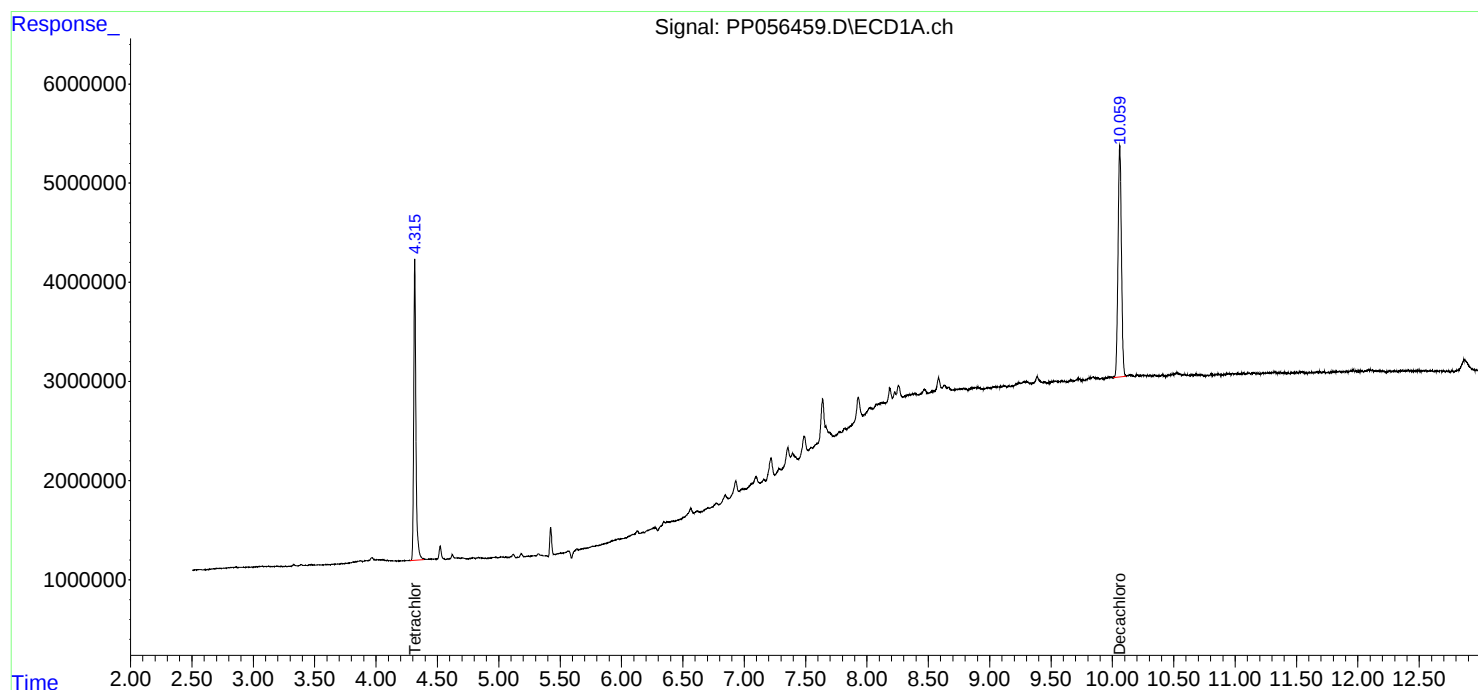

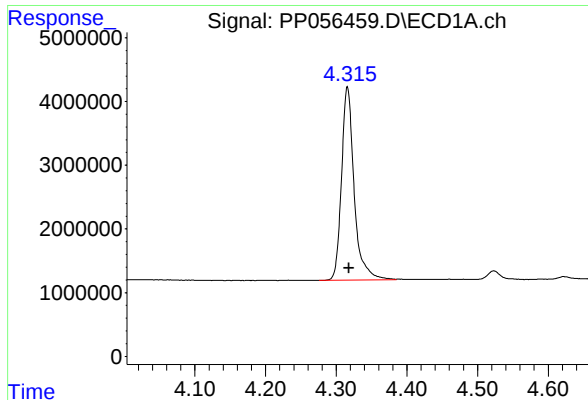


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.002 min
Response: 37621124
Conc: 24.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
F-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2023
Supervised By :Ankita Jodhani 03/14/2023

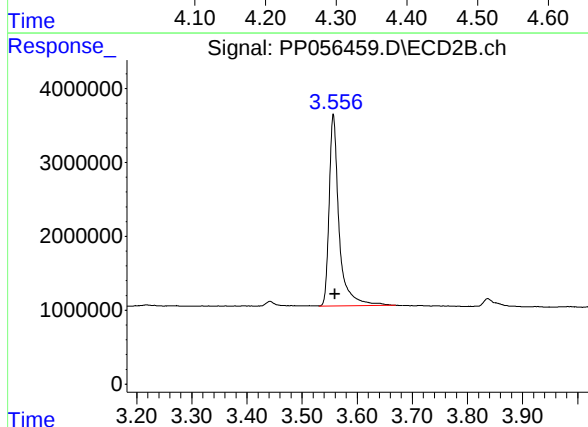


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.003 min
Response: 32406677
Conc: 22.97 ng/ml

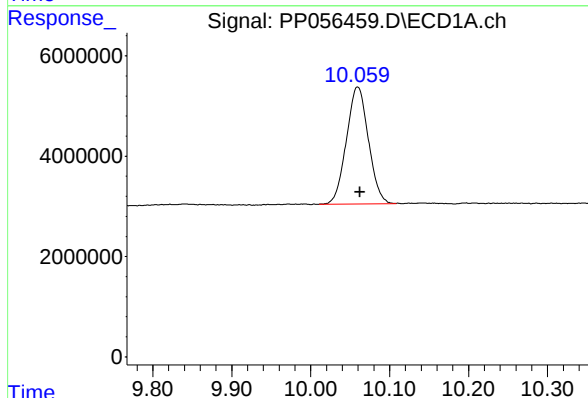

#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.003 min
Response: 45187121
Conc: 22.75 ng/ml

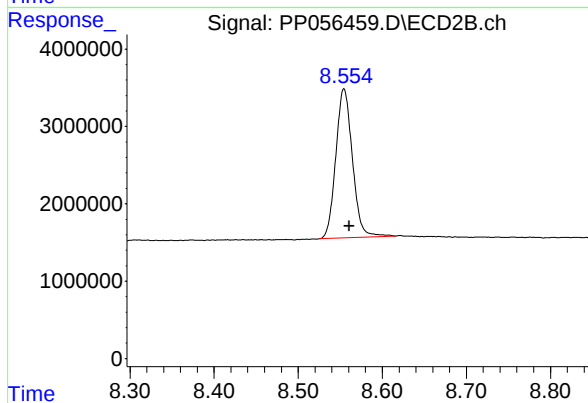

#2 Decachlorobiphenyl

R.T.: 8.555 min
Delta R.T.: -0.006 min
Response: 26455046
Conc: 23.67 ng/ml