

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
 Data File : PP056469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 00:30
 Operator : YP\AJ
 Sample : 01883-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34355

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:48:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.316	3.556	35387679	27685412	22.791	19.620
2) SA Decachlor...	10.061	8.556	45694335	25789303	23.004	23.070

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
Data File : PP056469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 00:30
Operator : YP\AJ
Sample : 01883-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
34355

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:48:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

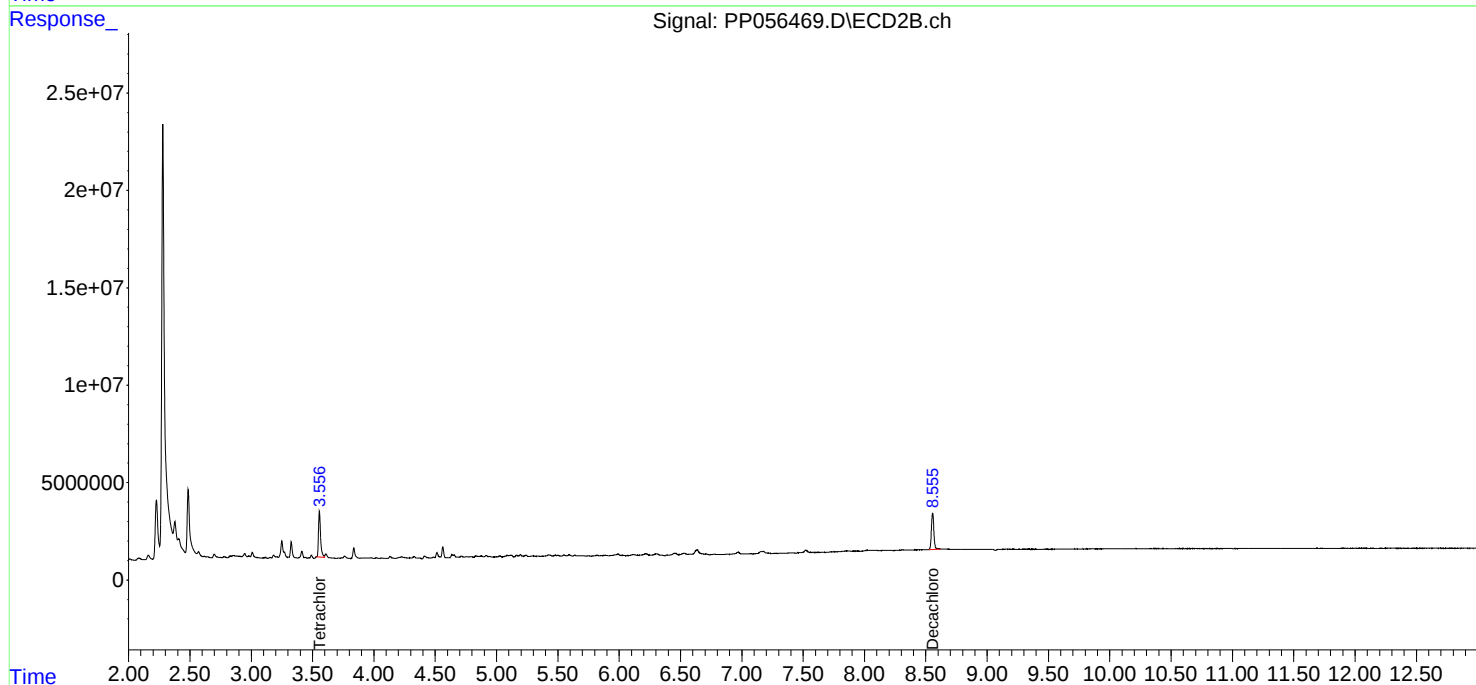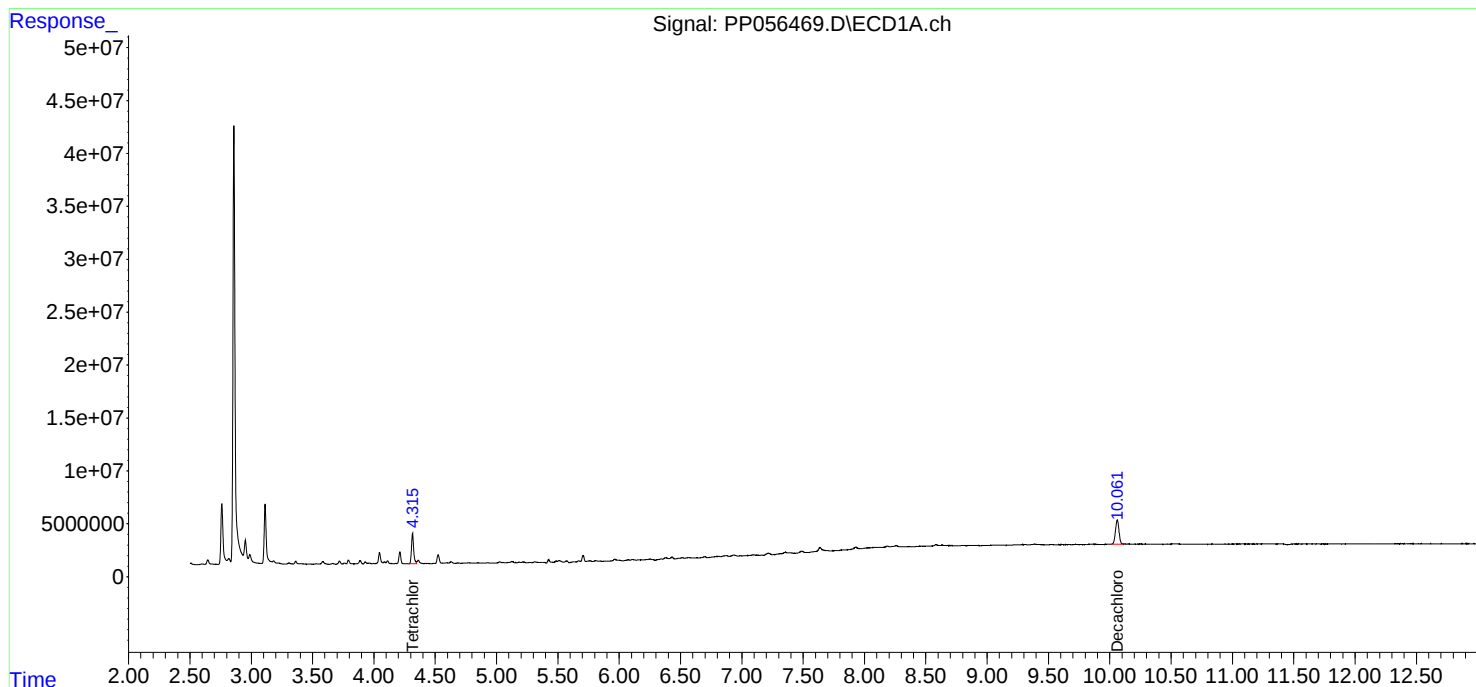


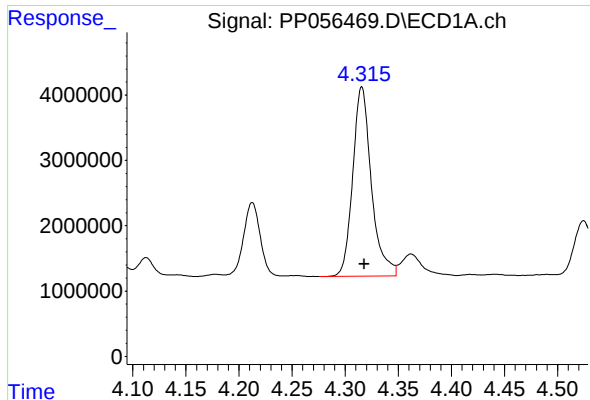

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: -0.002 min
Response: 35387679
Conc: 22.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
34355

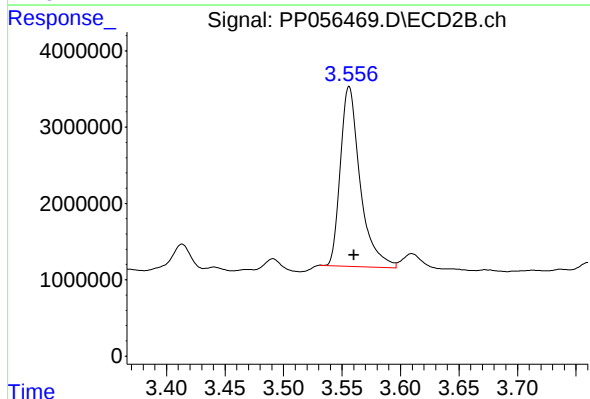


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: -0.004 min
Response: 27685412
Conc: 19.62 ng/ml

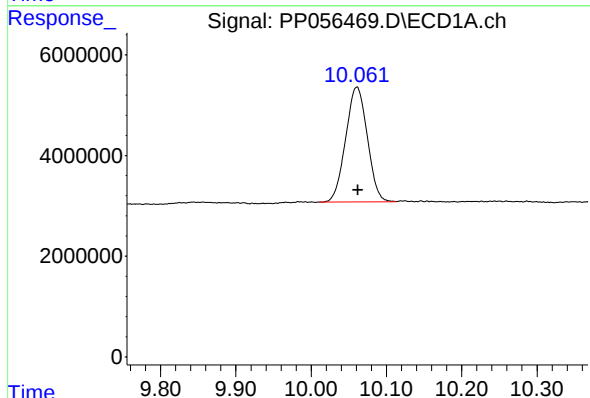

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: -0.002 min
Response: 45694335
Conc: 23.00 ng/ml

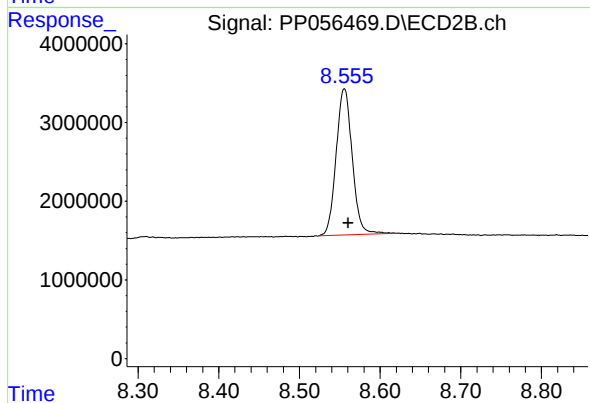

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: -0.005 min
Response: 25789303
Conc: 23.07 ng/ml