

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
 Data File : PP056471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 01:03
 Operator : YP\AJ
 Sample : 01883-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34357

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2023
 Supervised By :Ankita Jodhani 03/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:49:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.558	14399714	9380342	9.274	6.648m#
2) SA Decachlor...	10.070	8.562	2786106	21698292	1.403m	19.411m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031323\
Data File : PP056471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 01:03
Operator : YP\AJ
Sample : 01883-04
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
34357


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2023
Supervised By :Ankita Jodhani 03/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:49:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

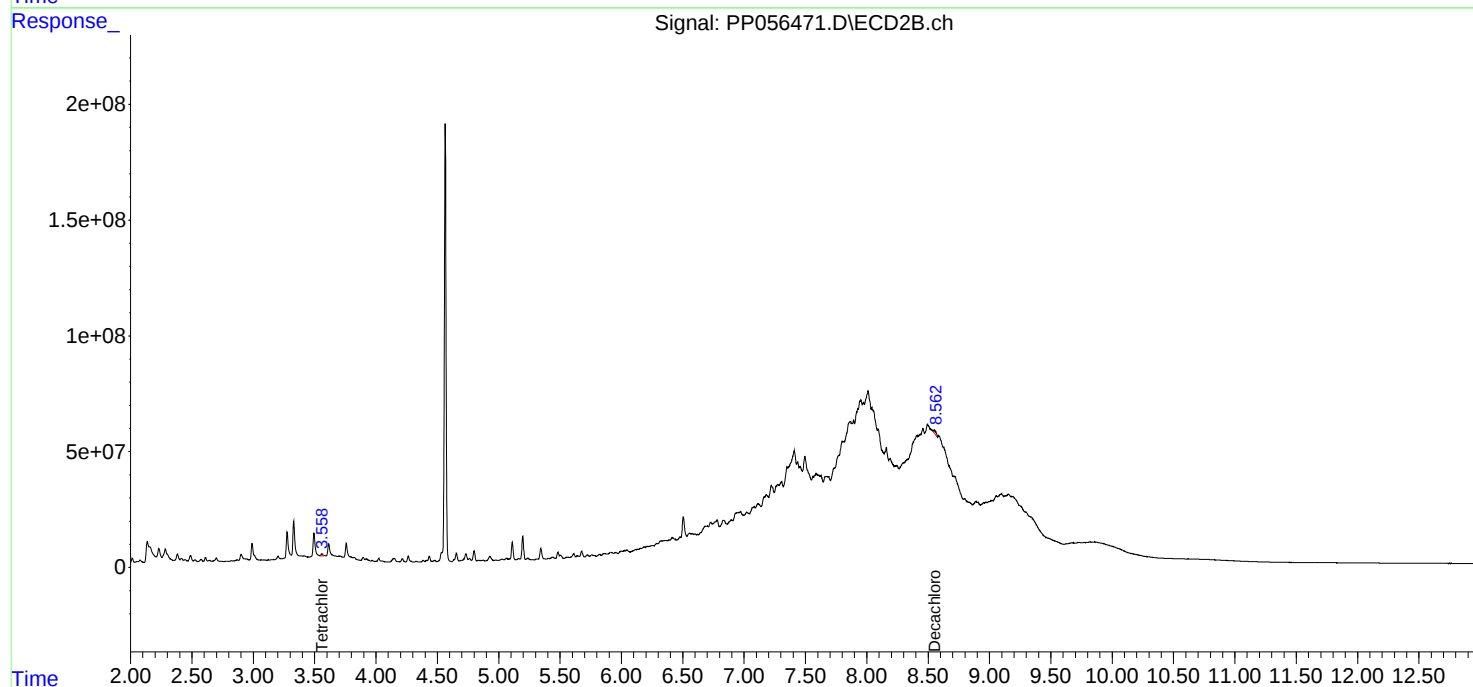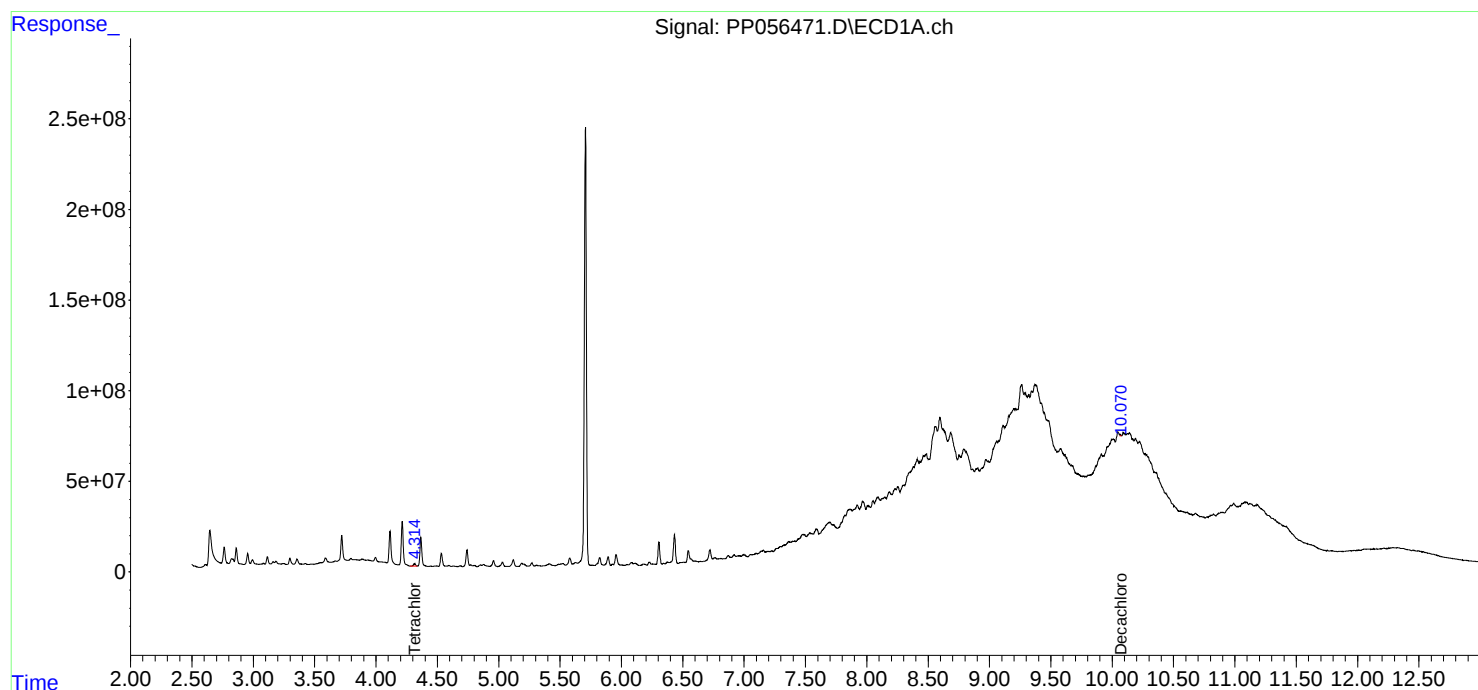

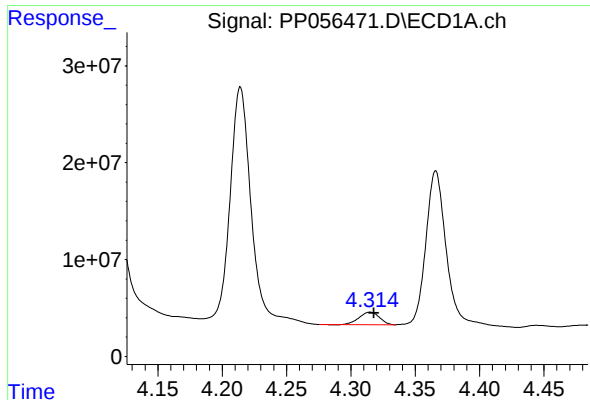


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: -0.003 min
Response: 14399714
Conc: 9.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
34357


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2023
Supervised By :Ankita Jodhani 03/14/2023

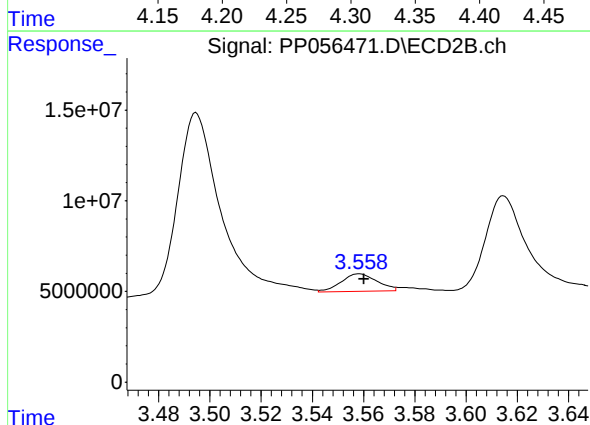


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.002 min
Response: 9380342
Conc: 6.65 ng/ml

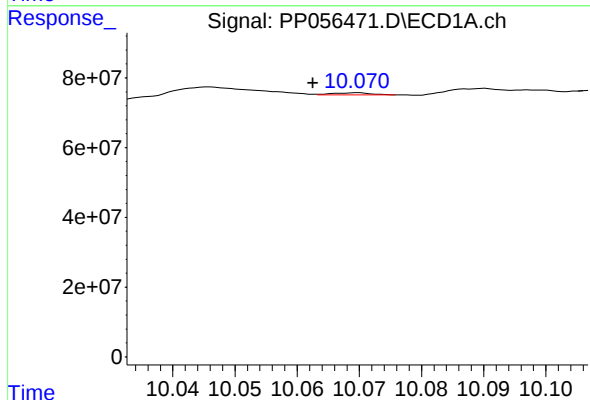

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: 0.007 min
Response: 2786106
Conc: 1.40 ng/ml

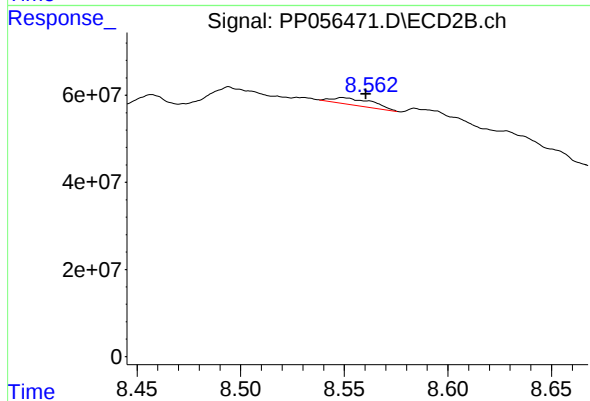

#2 Decachlorobiphenyl

R.T.: 8.562 min
Delta R.T.: 0.001 min
Response: 21698292
Conc: 19.41 ng/ml