

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031325\
 Data File : PP070488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2025 13:49
 Operator : YP\AJ
 Sample : Q1554-19 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC107490LOK-END-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2025
 Supervised By :Ankita Jodhani 03/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 14:14:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.826	2812829	1639536	1.808m	1.636m
2) SA Decachlor...	10.244	8.876	2013971	1916541	1.896m	1.959

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031325\
Data File : PP070488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2025 13:49
Operator : YP\AJ
Sample : Q1554-19 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC107490LOK-END-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2025
Supervised By :Ankita Jodhani 03/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 14:14:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

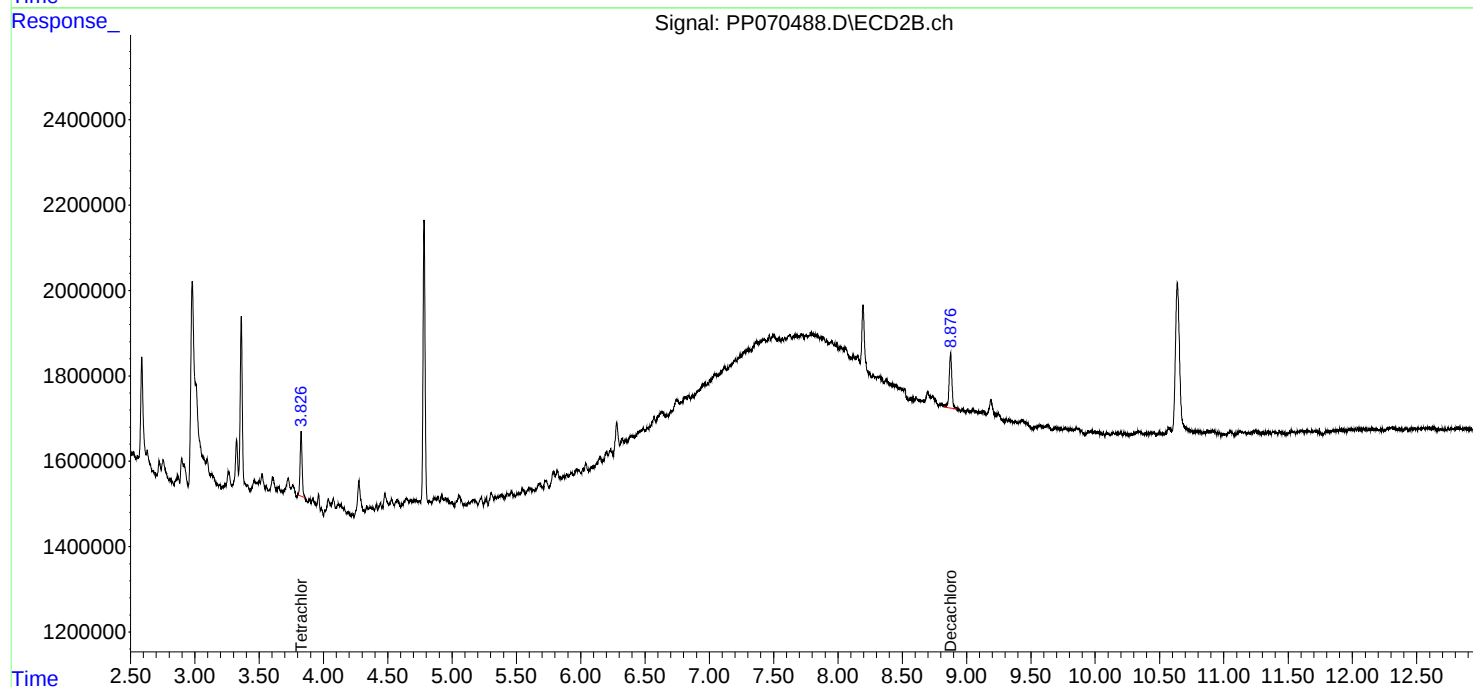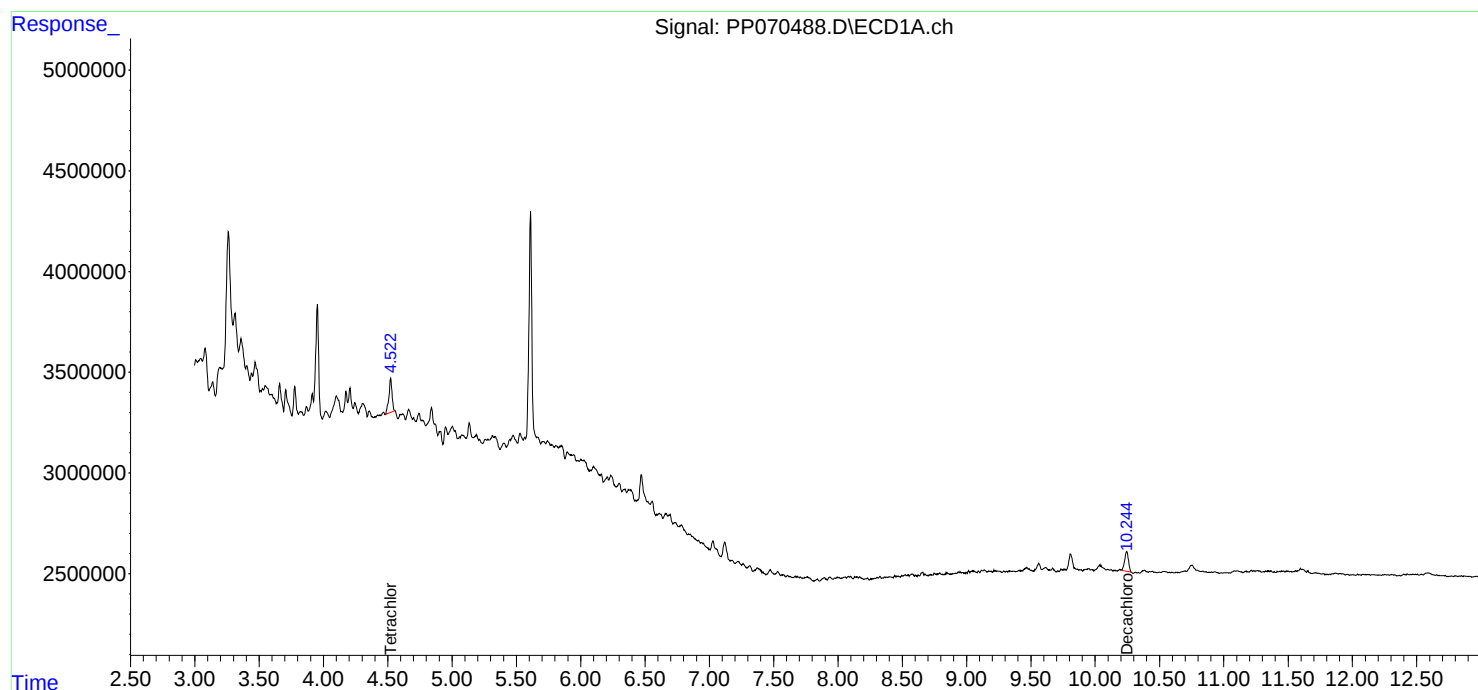

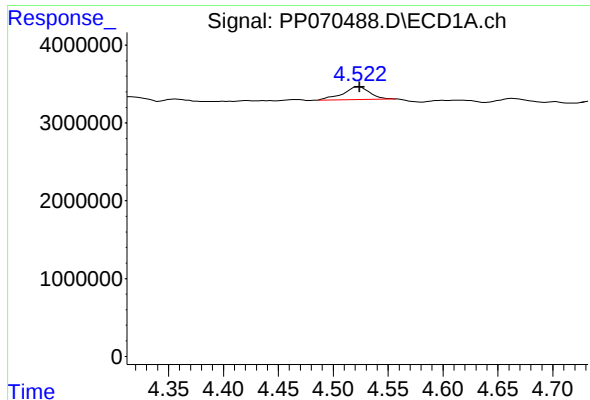


#1 Tetrachloro-m-xylene

R.T.: 4.522 min
Delta R.T.: -0.002 min
Response: 2812829
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC107490LOK-END-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2025
Supervised By :Ankita Jodhani 03/14/2025

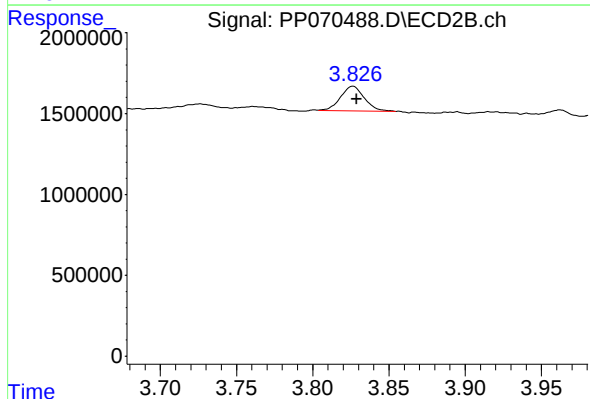


#1 Tetrachloro-m-xylene

R.T.: 3.826 min
Delta R.T.: -0.003 min
Response: 1639536
Conc: 1.64 ng/ml m

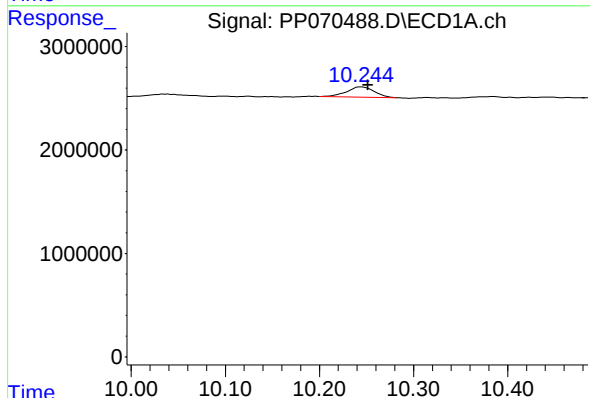

#2 Decachlorobiphenyl

R.T.: 10.244 min
Delta R.T.: -0.007 min
Response: 2013971
Conc: 1.90 ng/ml m

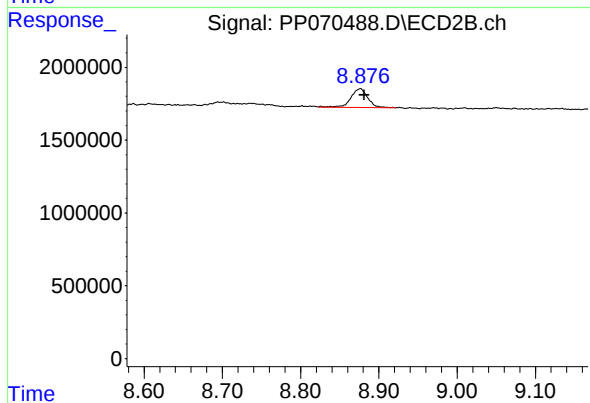

#2 Decachlorobiphenyl

R.T.: 8.876 min
Delta R.T.: -0.005 min
Response: 1916541
Conc: 1.96 ng/ml