

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031419\
 Data File : PP029295.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Mar 2019 11:09
 Operator : EI\MA
 Sample : HEXANE
 Misc : hexane
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 15:28:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	12.469	0	2392529	N.D. 18.692 #
15) T	Picloram	17.480	18.184	4332533	20086305	15.582 89.263 #
16) T	DCPA	0.000	18.184	0	20086305	N.D. 86.431 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031419\
Data File : PP029295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Mar 2019 11:09
Operator : EI\MA
Sample : HEXANE
Misc : hexane
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 15:28:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

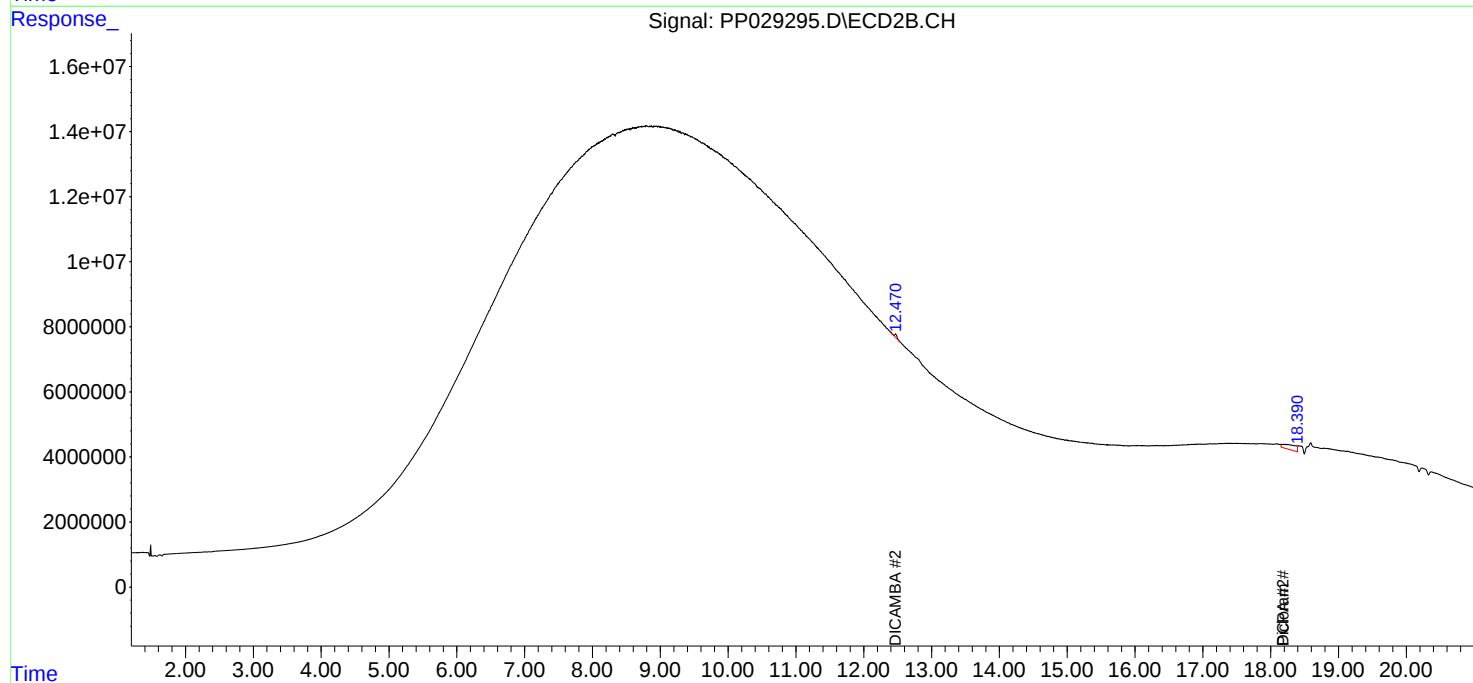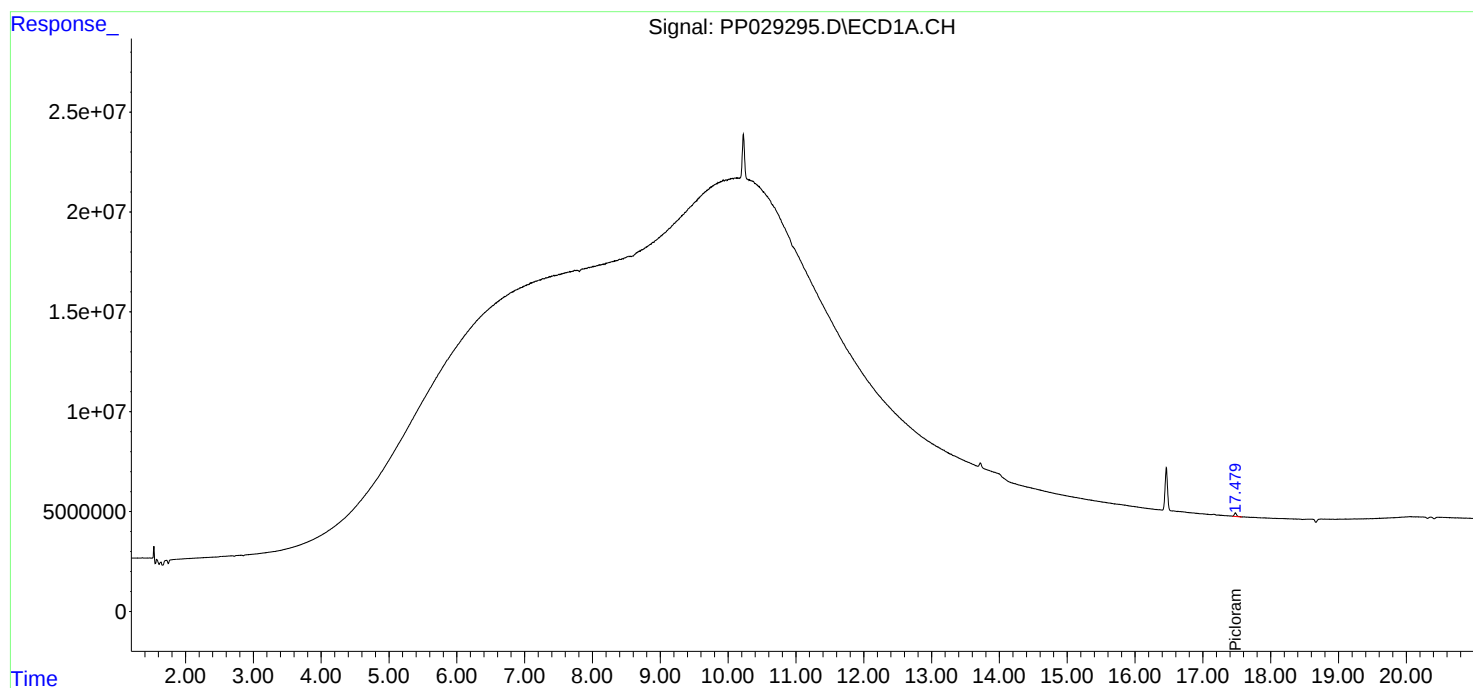


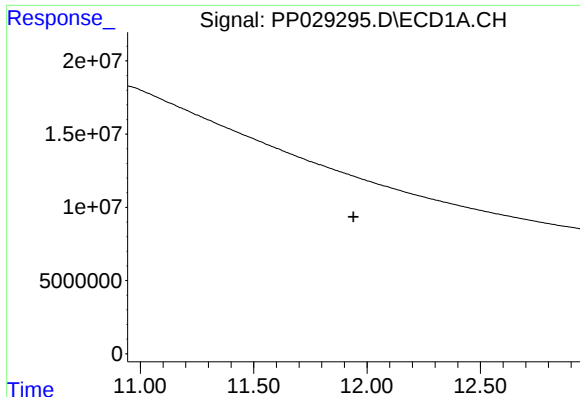

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

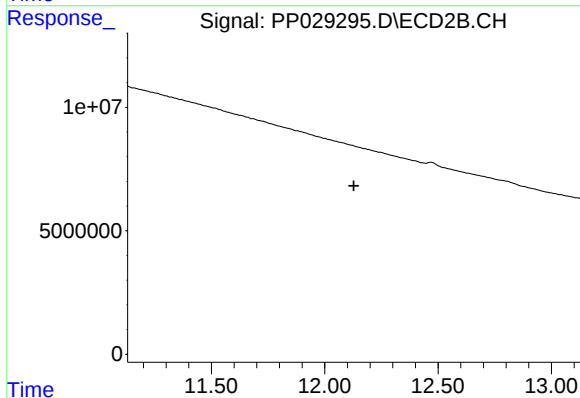


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.129 min
Response: 0
Conc: N.D.

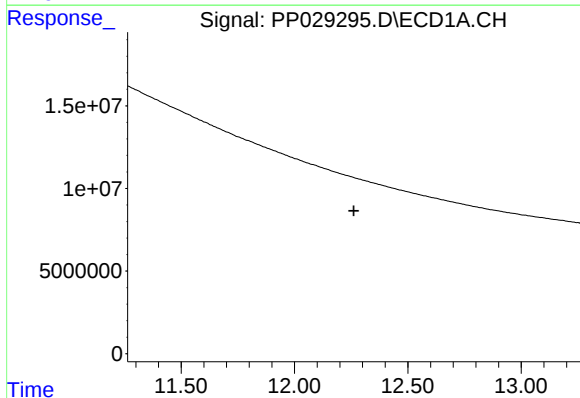


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.262 min
Response: 0
Conc: N.D.

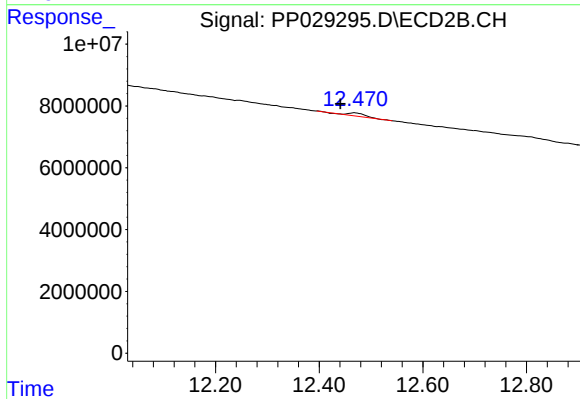

#5 DICAMBA


R.T.: 12.469 min
Delta R.T.: 0.028 min
Response: 2392529
Conc: 18.69 ng/ml

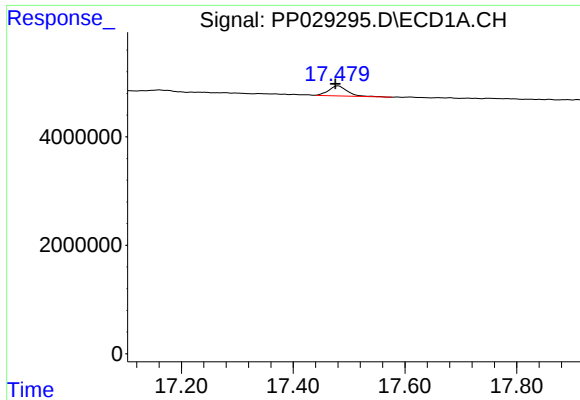

#15 Picloram


R.T.: 17.480 min
Delta R.T.: 0.005 min
Response: 4332533
Conc: 15.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

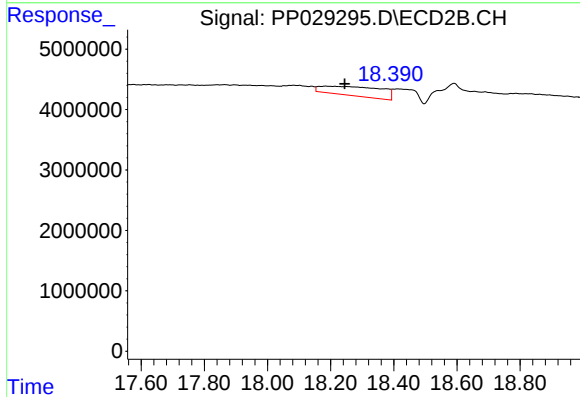


#15 Picloram

R.T.: 18.184 min
Delta R.T.: -0.061 min
Response: 20086305
Conc: 89.26 ng/ml

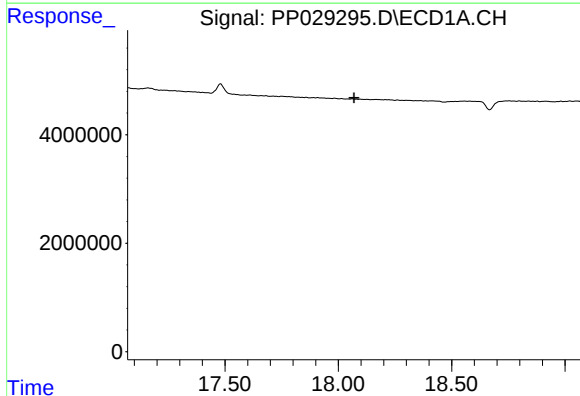

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.069 min
Response: 0
Conc: N.D.

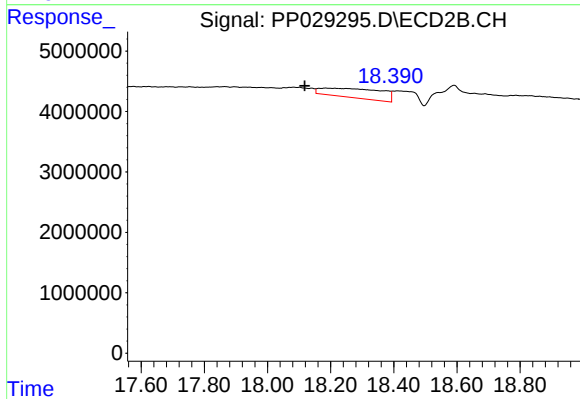

#16 DCPA

R.T.: 18.184 min
Delta R.T.: 0.066 min
Response: 20086305
Conc: 86.43 ng/ml