

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031422\
 Data File : PP044698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 04:21
 Operator : YP\AJ
 Sample : N1905-15
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-14A-1A-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2022
 Supervised By :Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 09:50:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.914	3.193f	31664522	23589720	15.282m	13.484m
2) SA Decachlor...	10.063	8.551	24934838	15003203	18.117	9.781m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031422\
Data File : PP044698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 04:21
Operator : YP\AJ
Sample : N1905-15
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2022
Supervised By :Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 09:50:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

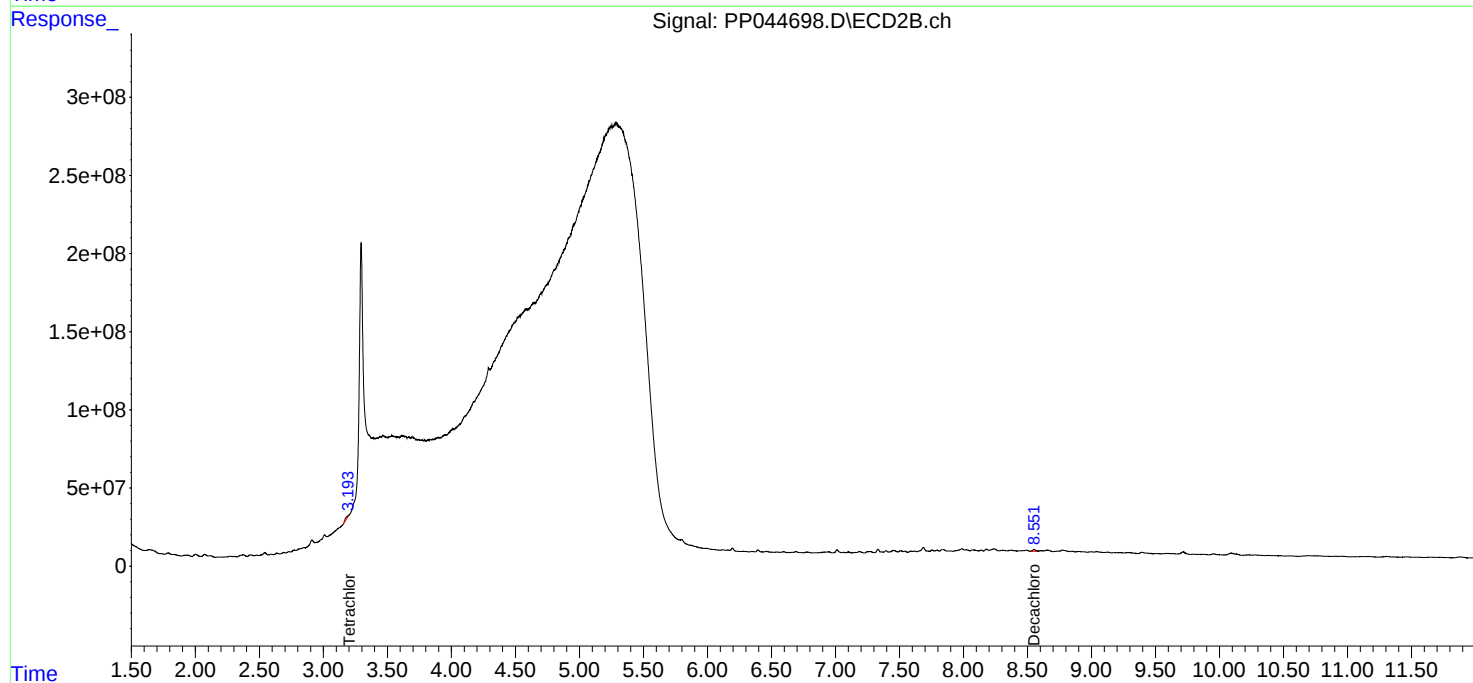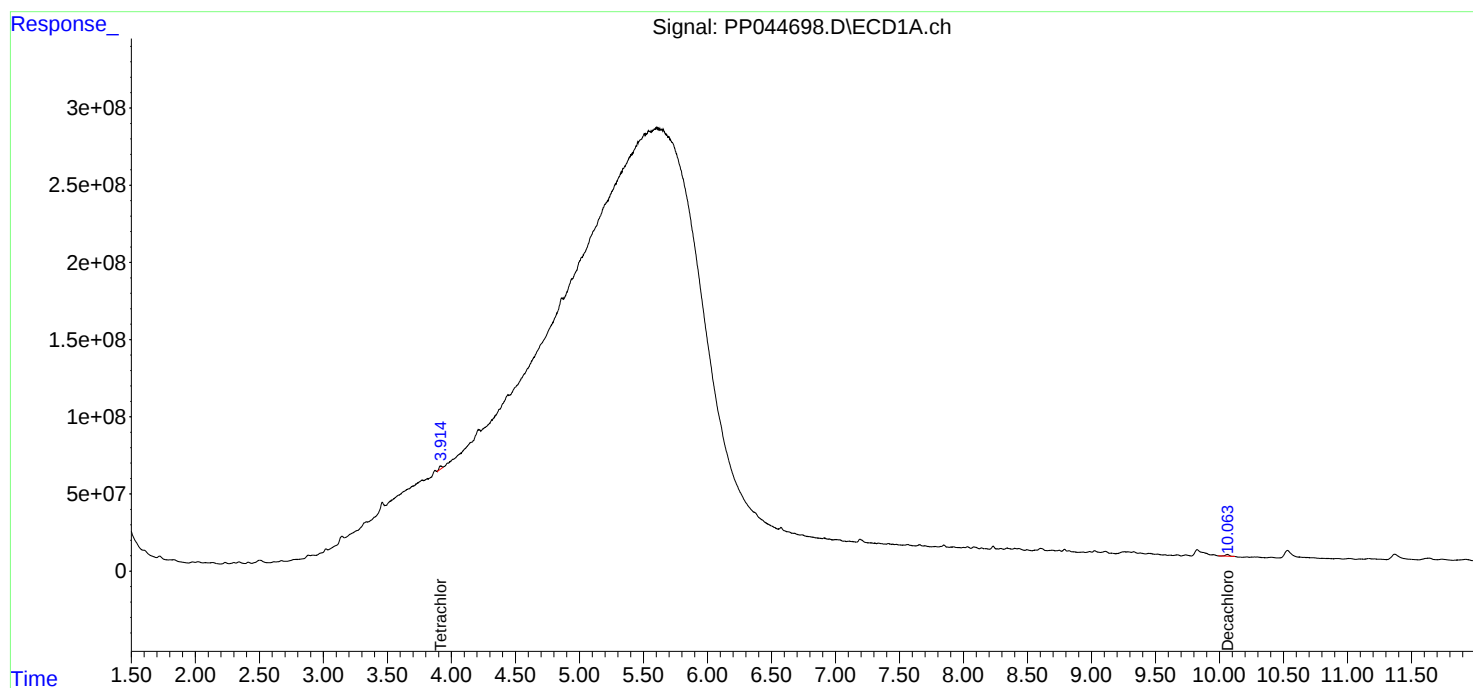

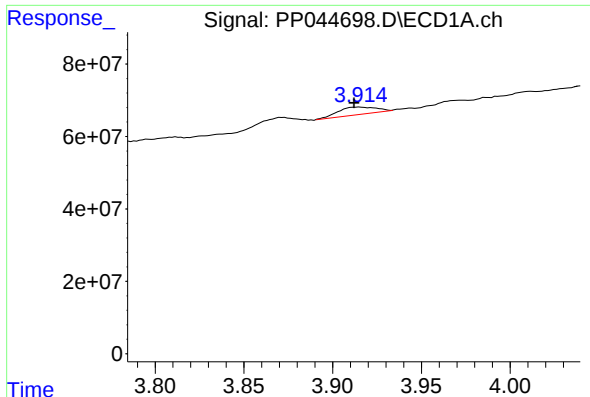


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: 0.002 min
Response: 31664522
Conc: 15.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2022
Supervised By :Ankita Jodhani 03/15/2022

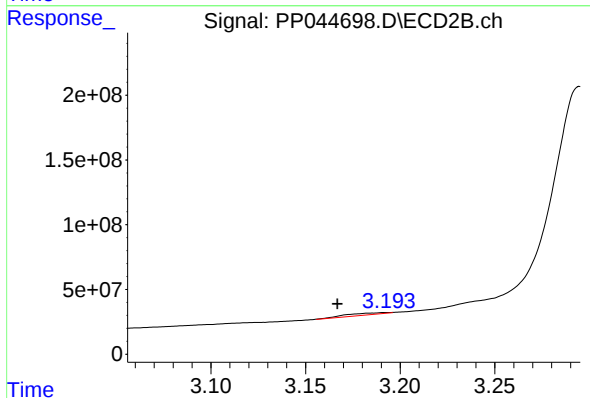


#1 Tetrachloro-m-xylene

R.T.: 3.193 min
Delta R.T.: 0.026 min
Response: 23589720
Conc: 13.48 ng/ml m

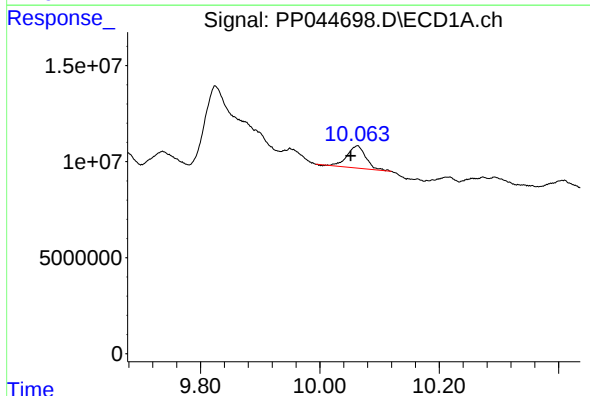

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: 0.012 min
Response: 24934838
Conc: 18.12 ng/ml

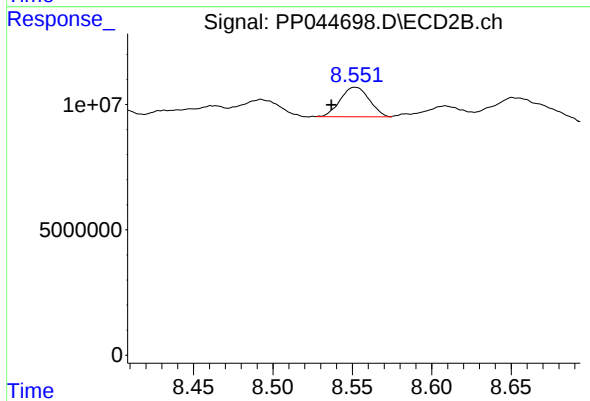

#2 Decachlorobiphenyl

R.T.: 8.551 min
Delta R.T.: 0.014 min
Response: 15003203
Conc: 9.78 ng/ml m