

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031519\
 Data File : PP029318.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2019 11:04
 Operator : EI\MA
 Sample : HEXANE
 Misc : hexane
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:02:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	0.000	10.166	0	454988	N.D. 8.977 #
3) T	4-Nitroph...	0.000	11.258	0	9392963	N.D. 392.226 #
10) T	Pentachlo...	0.000	14.625	0	362410	N.D. 0.704 #
11) T	2,4,5-TP ...	0.000	15.232	0	362754	N.D. 1.783 #
12) T	2,4,5-T	0.000	15.846	0	1663852	N.D. 10.049 #
13) T	2,4-DB	0.000	16.422	0	10313667	N.D. 457.844 #
14) T	DINOSEB	0.000	16.850	0	17478073	N.D. 133.347 #
15) T	Picloram	0.000	18.247	0	56610216	N.D. 251.575 #
16) T	DCPA	0.000	18.129	0	16010197	N.D. 68.892 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031519\
Data File : PP029318.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2019 11:04
Operator : EI\MA
Sample : HEXANE
Misc : hexane
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:02:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

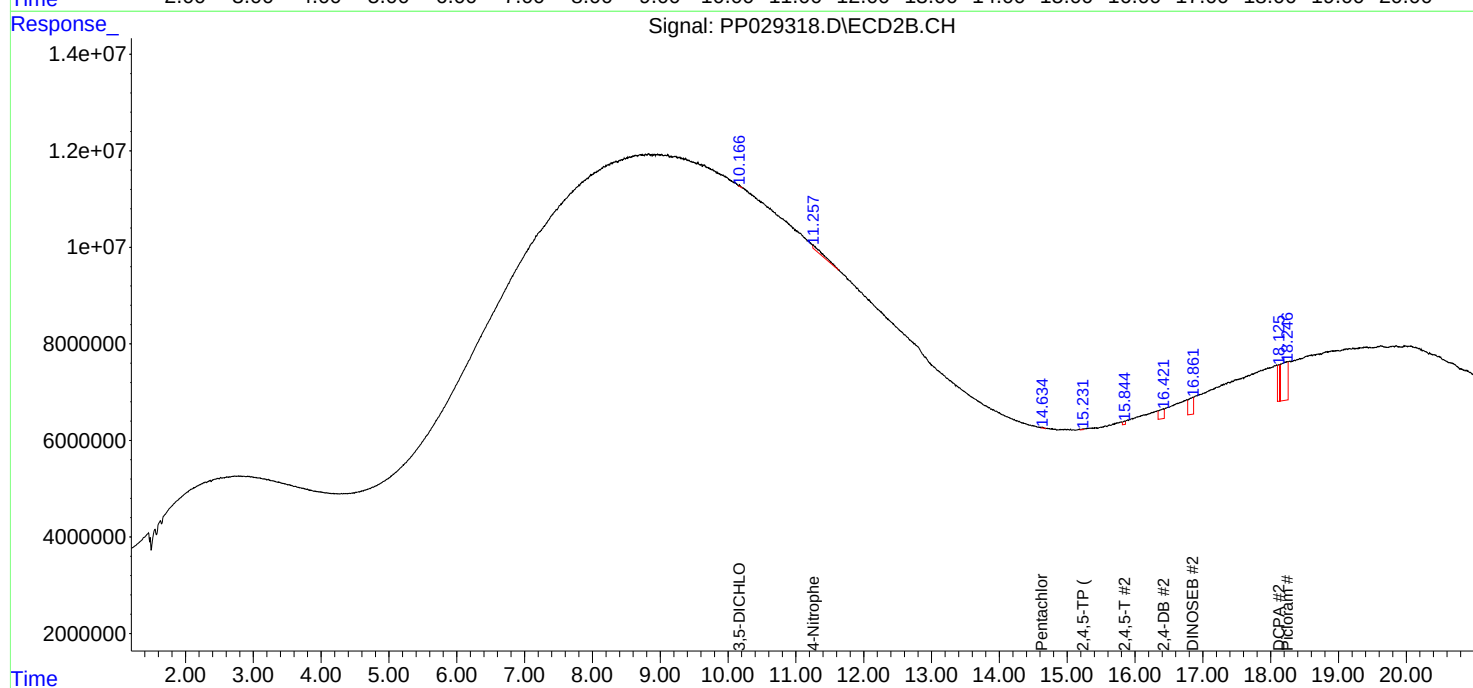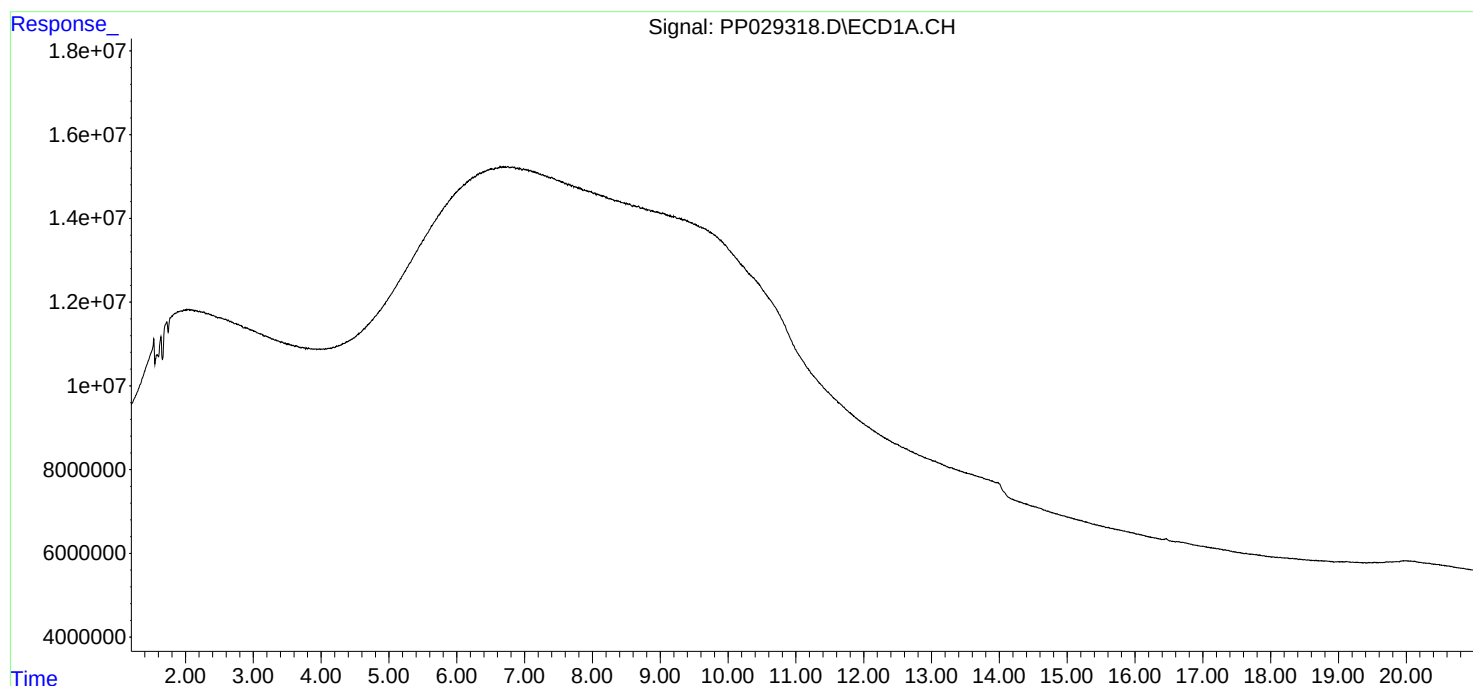


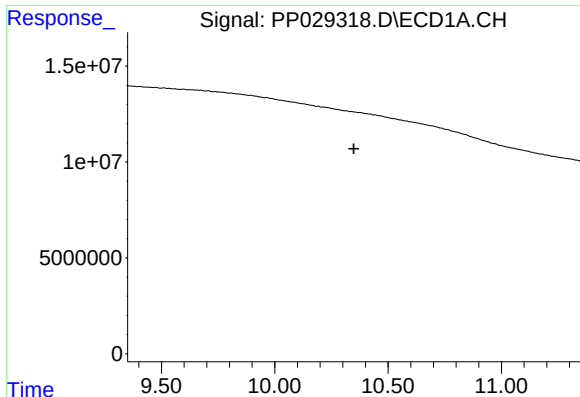

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.348 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

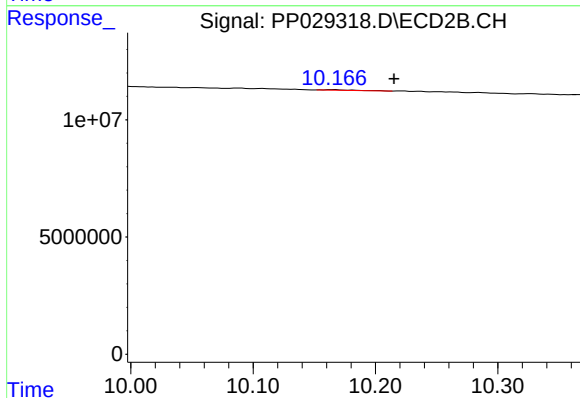


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.166 min
Delta R.T.: -0.049 min
Response: 454988
Conc: 8.98 ng/ml

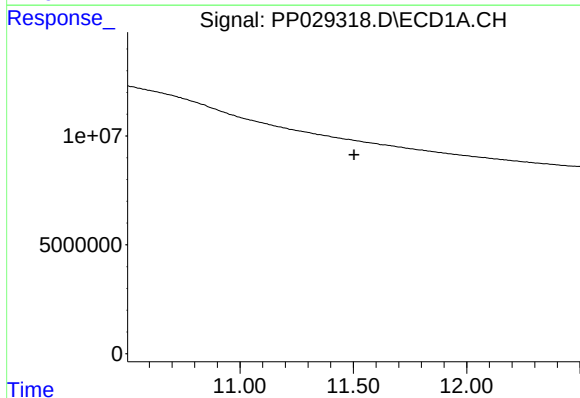


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

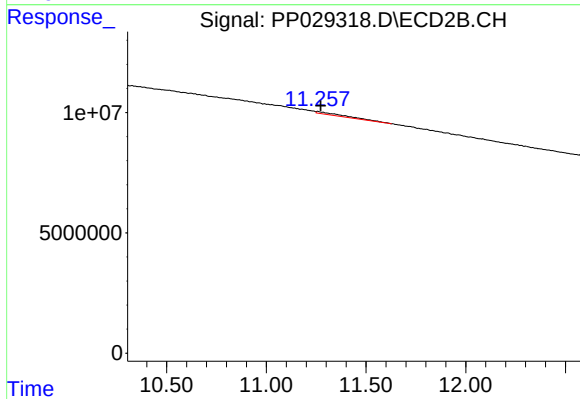

#3 4-Nitrophenol


R.T.: 11.258 min
Delta R.T.: -0.015 min
Response: 9392963
Conc: 392.23 ng/ml

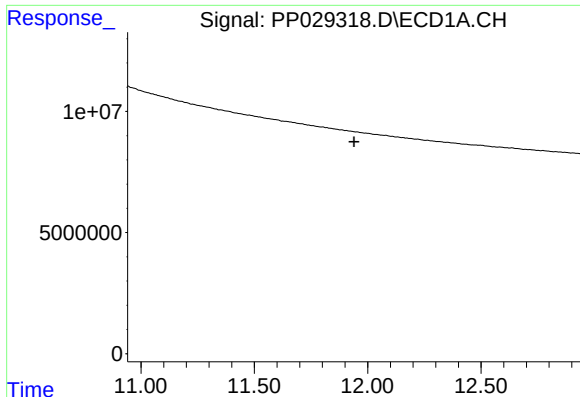

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

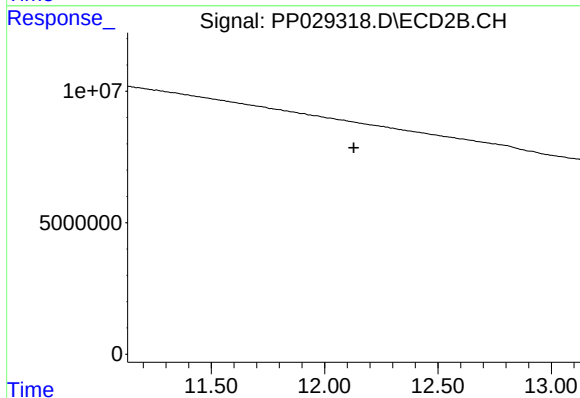


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.129 min
Response: 0
Conc: N.D.

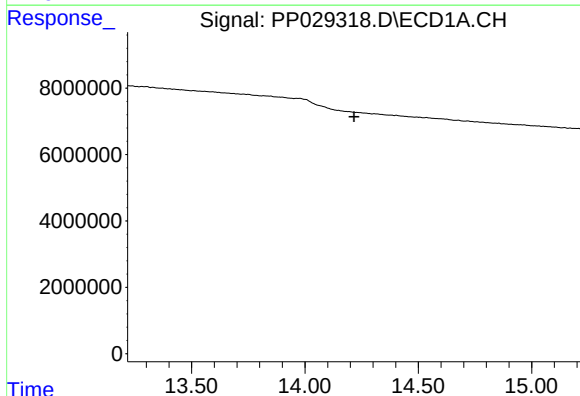


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.216 min
Response: 0
Conc: N.D.

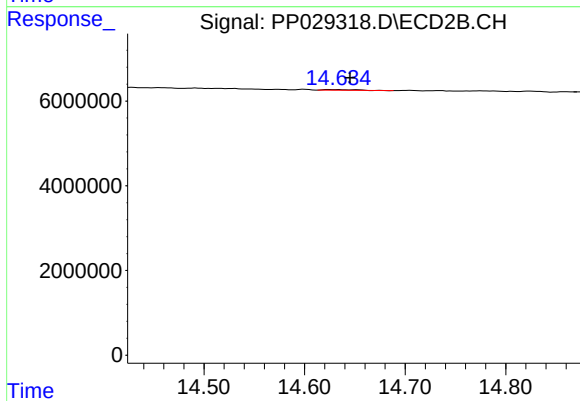

#10 Pentachlorophenol


R.T.: 14.625 min
Delta R.T.: -0.020 min
Response: 362410
Conc: 0.70 ng/ml

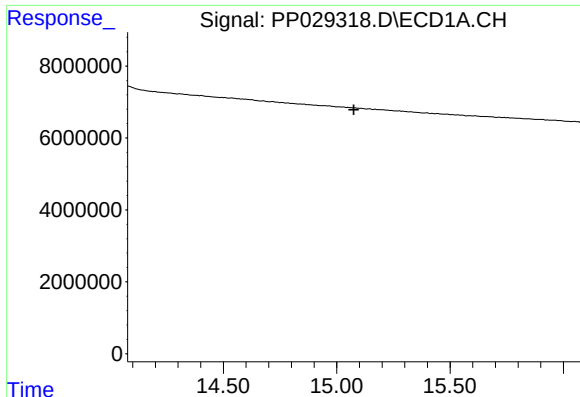

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

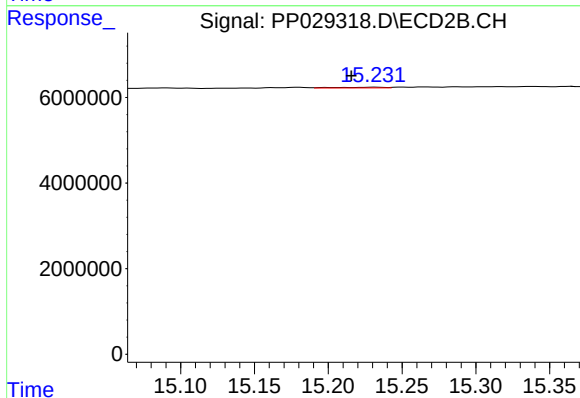


#11 2,4,5-TP (SILVEX)

R.T.: 15.232 min
Delta R.T.: 0.017 min
Response: 362754
Conc: 1.78 ng/ml

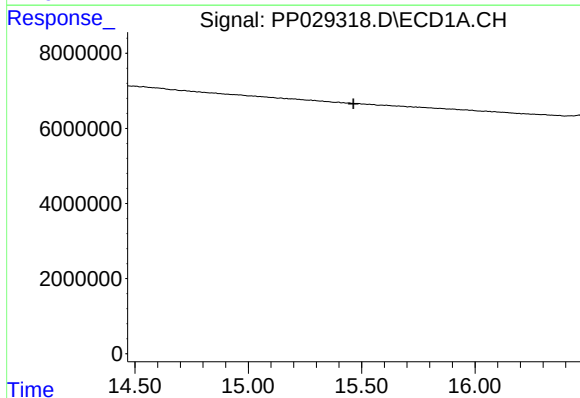


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

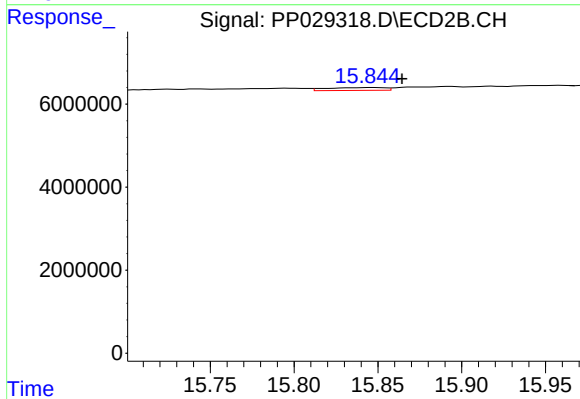

#12 2,4,5-T


R.T.: 15.846 min
Delta R.T.: -0.018 min
Response: 1663852
Conc: 10.05 ng/ml

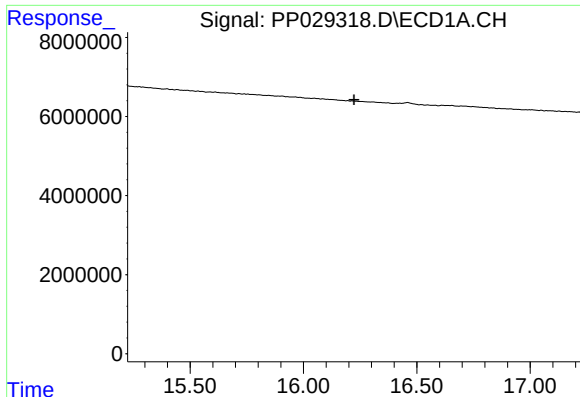

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

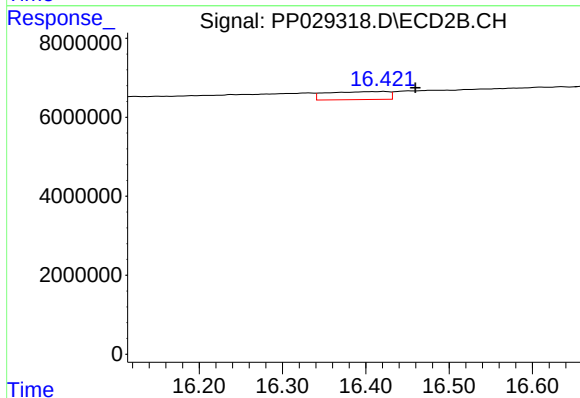


#13 2,4-DB

R.T.: 16.422 min
Delta R.T.: -0.037 min
Response: 10313667
Conc: 457.84 ng/ml

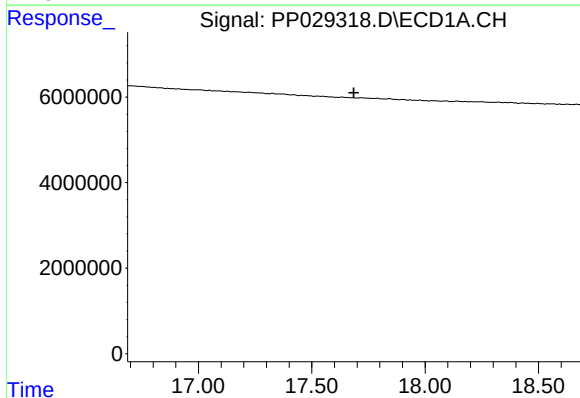


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.686 min
Response: 0
Conc: N.D.

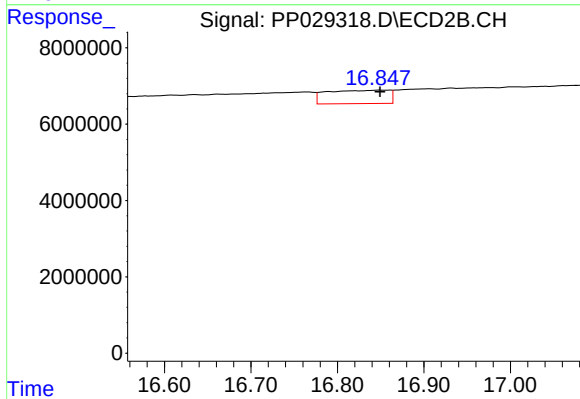

#14 DINOSEB


R.T.: 16.850 min
Delta R.T.: 0.000 min
Response: 17478073
Conc: 133.35 ng/ml

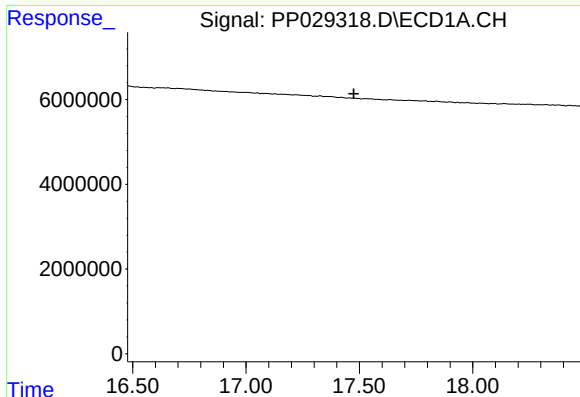

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

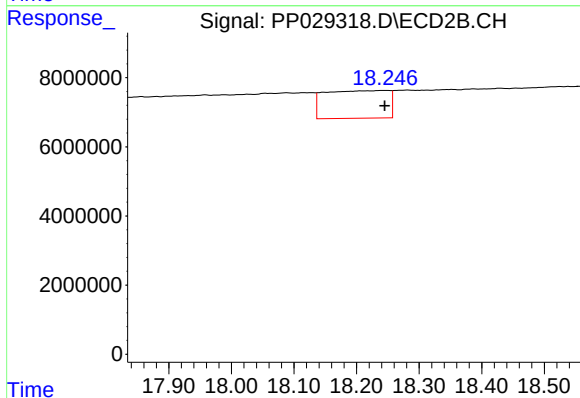


#15 Picloram

R.T.: 18.247 min
Delta R.T.: 0.002 min
Response: 56610216
Conc: 251.58 ng/ml

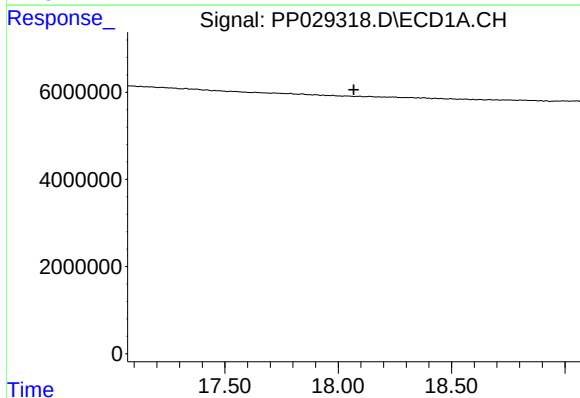

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.069 min
Response: 0
Conc: N.D.

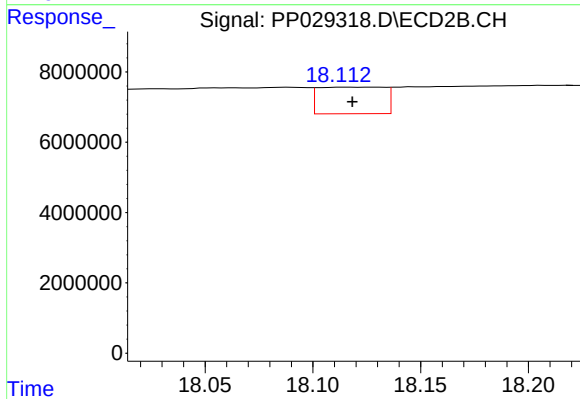

#16 DCPA

R.T.: 18.129 min
Delta R.T.: 0.010 min
Response: 16010197
Conc: 68.89 ng/ml