

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031519\
 Data File : PP029345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2019 23:24
 Operator : EI\MA
 Sample : K1087-36
 Misc : hexane
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:06:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.930	12.124	15949340	16230908	530.648	427.664
Target Compounds							
8) T	DICHLORPROP	0.000	13.554	0	523759	N.D.	15.492 #
9) T	2,4-D	0.000	14.015	0	529457	N.D.	11.677 #
10) T	Pentachlo...	0.000	14.646	0	586241	N.D.	1.139 #
11) T	2,4,5-TP ...	0.000	15.198	0	2471657	N.D.	12.151 #
12) T	2,4,5-T	0.000	15.876	0	15602276	N.D.	94.232 #
13) T	2,4-DB	16.237	0.000	20990715	0	1098.856	N.D. #
14) T	DINOSEB	17.699	16.914	5605125	26380350	38.489	201.266 #
15) T	Picloram	17.478	0.000	5039493	0	18.124	N.D. #
16) T	DCPA	0.000	18.101	0	9593541	N.D.	41.281 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031519\
Data File : PP029345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2019 23:24
Operator : EI\MA
Sample : K1087-36
Misc : hexane
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:06:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

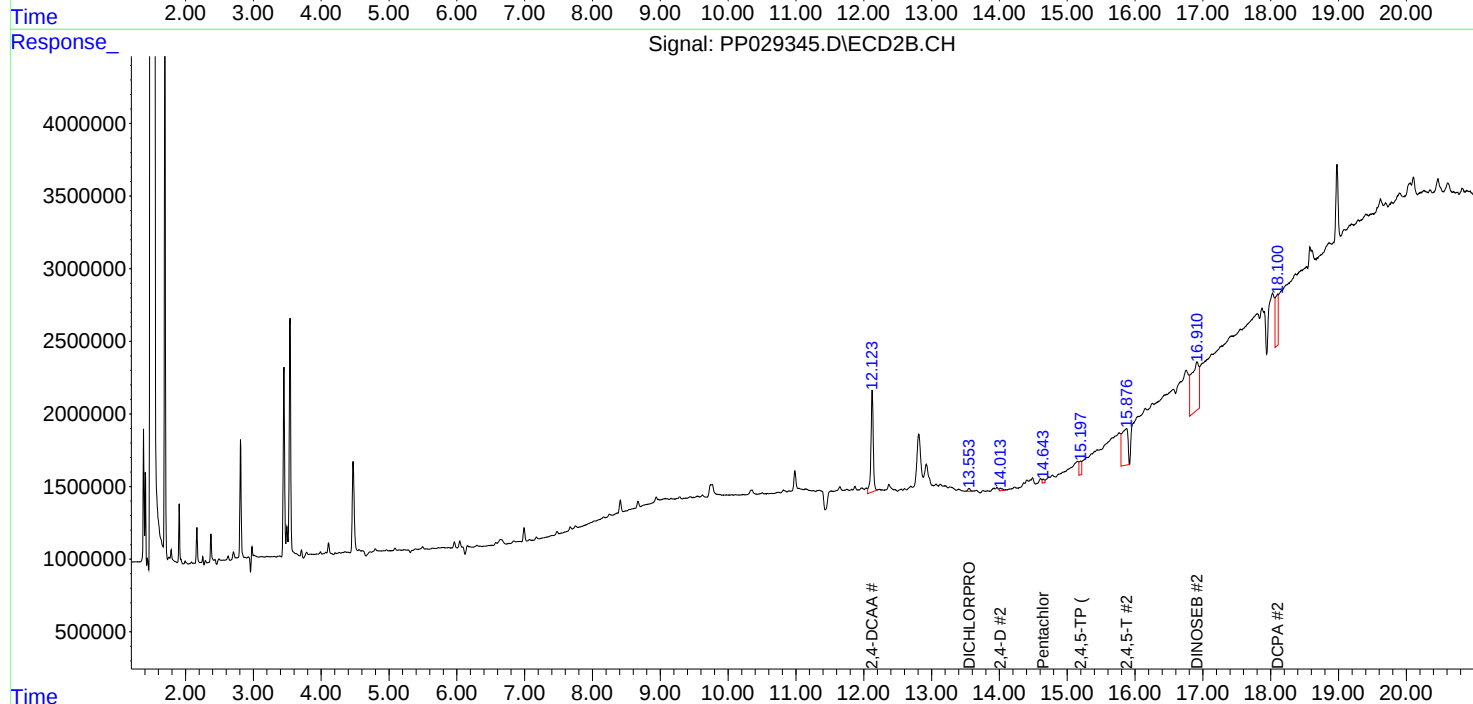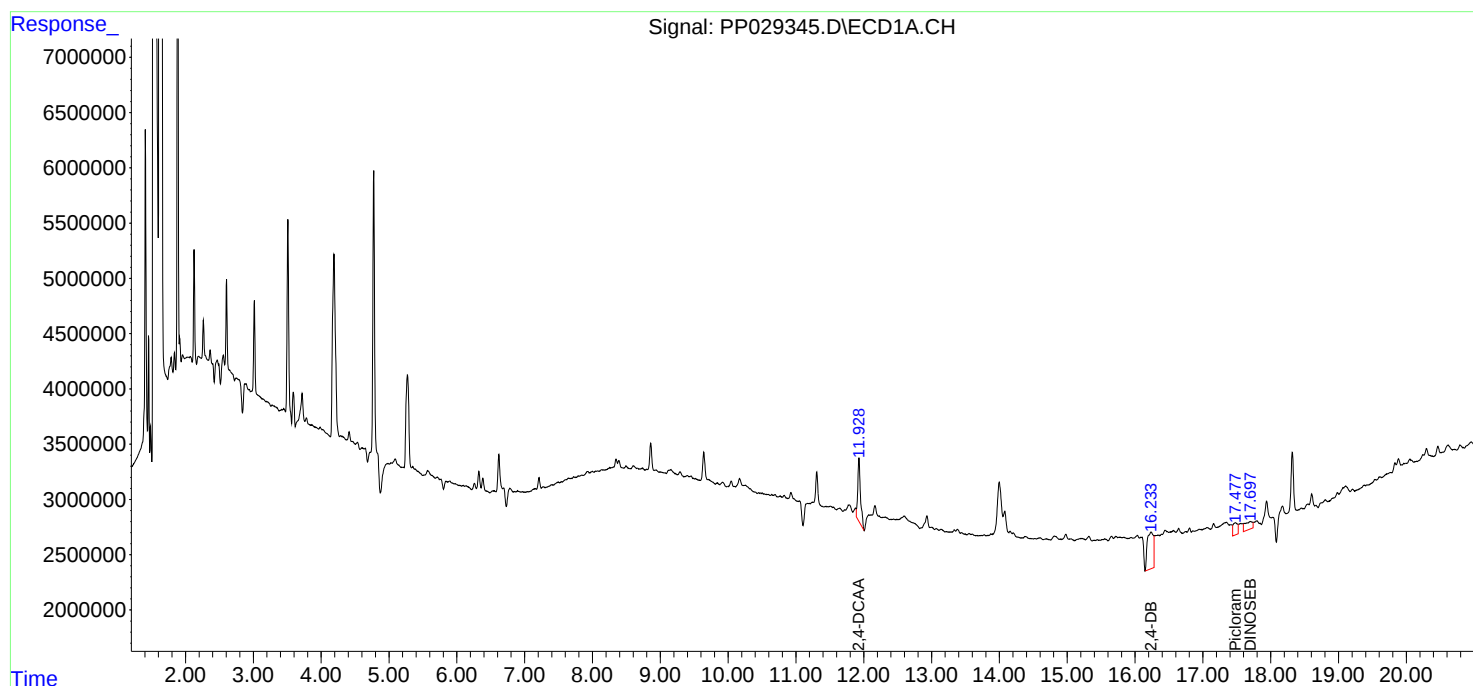


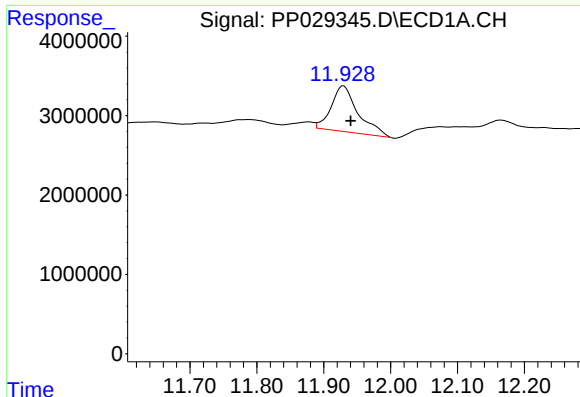

#4 2,4-DCAA


R.T.: 11.930 min
Delta R.T.: -0.011 min
Response: 15949340
Conc: 530.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11

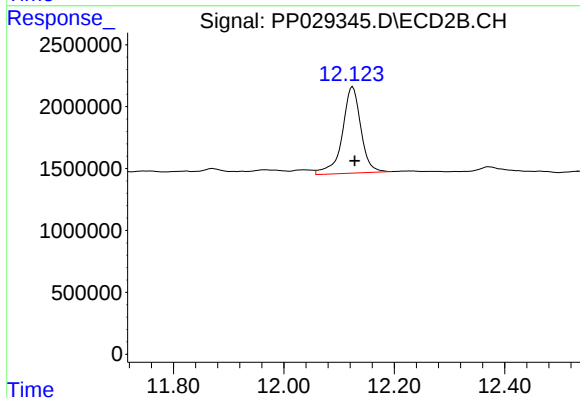


#4 2,4-DCAA

R.T.: 12.124 min
Delta R.T.: -0.004 min
Response: 16230908
Conc: 427.66 ng/ml

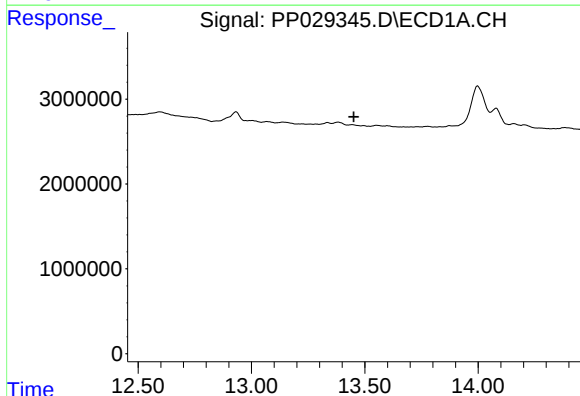


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

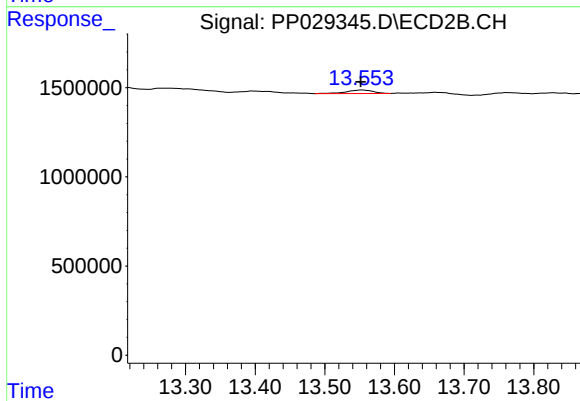

#8 DICHLORPROP


R.T.: 13.554 min
Delta R.T.: 0.003 min
Response: 523759
Conc: 15.49 ng/ml

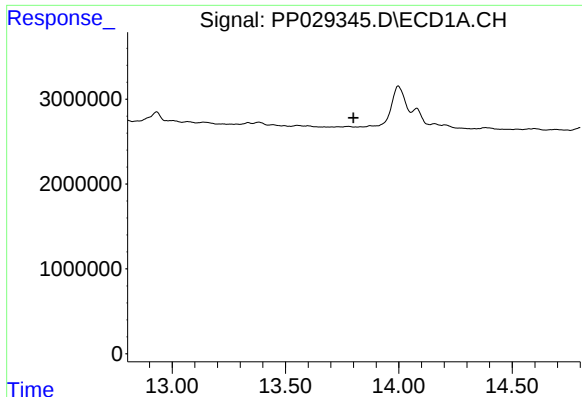

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-11

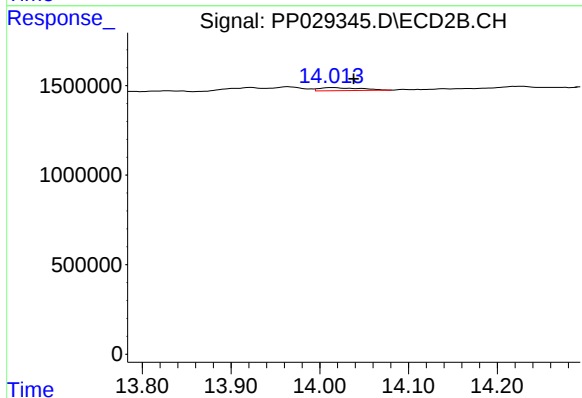


#9 2,4-D

R.T.: 14.015 min
Delta R.T.: -0.023 min
Response: 529457
Conc: 11.68 ng/ml

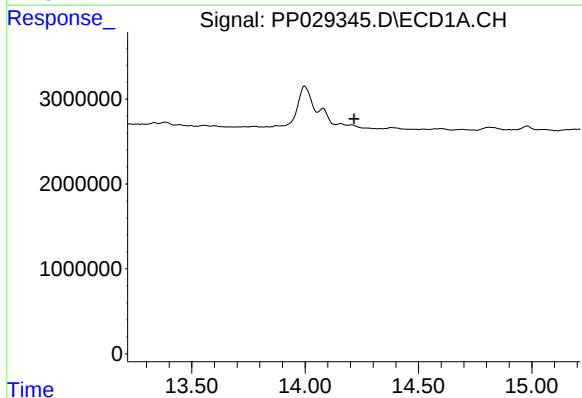


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 14.216 min
Response: 0
Conc: N.D.

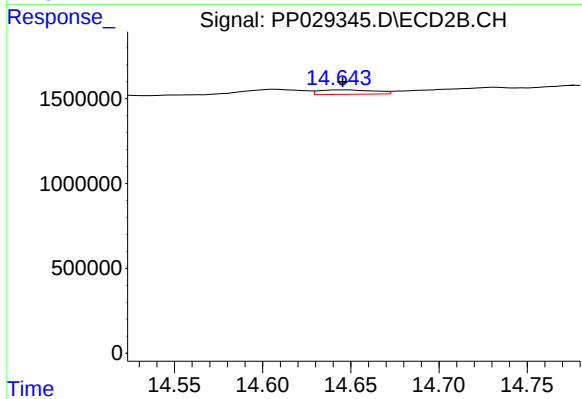

#10 Pentachlorophenol


R.T.: 14.646 min
Delta R.T.: 0.000 min
Response: 586241
Conc: 1.14 ng/ml

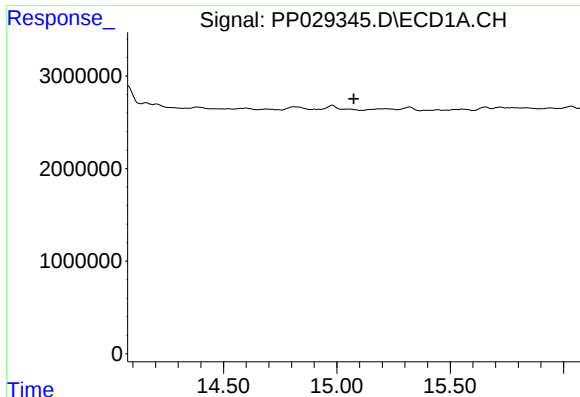

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-11

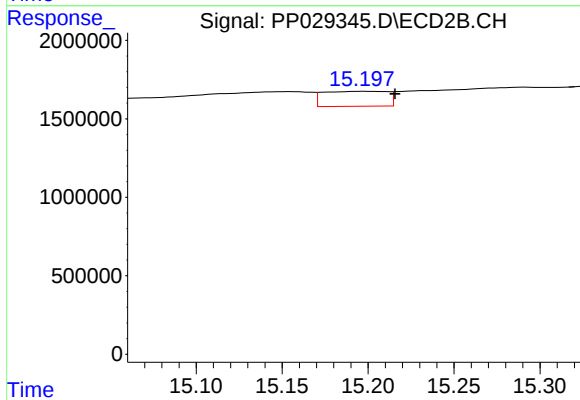


#11 2,4,5-TP (SILVEX)

R.T.: 15.198 min
Delta R.T.: -0.018 min
Response: 2471657
Conc: 12.15 ng/ml

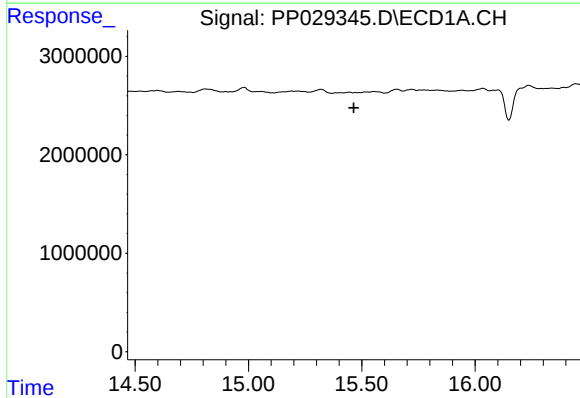


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

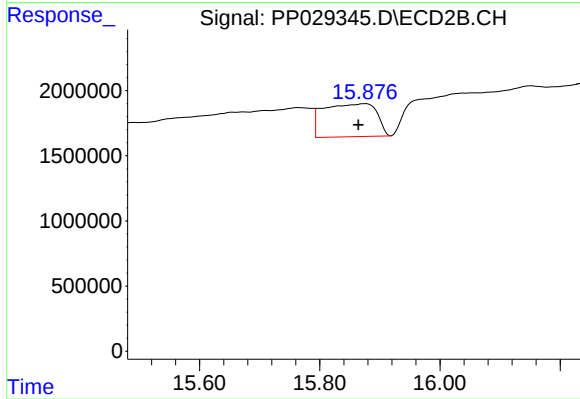

#12 2,4,5-T


R.T.: 15.876 min
Delta R.T.: 0.011 min
Response: 15602276
Conc: 94.23 ng/ml

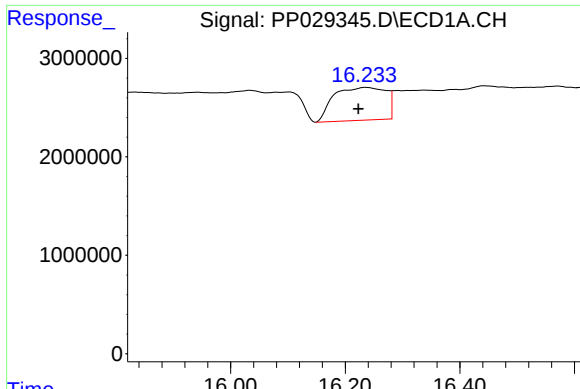

#13 2,4-DB


R.T.: 16.237 min
Delta R.T.: 0.013 min
Response: 20990715
Conc: 1098.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11

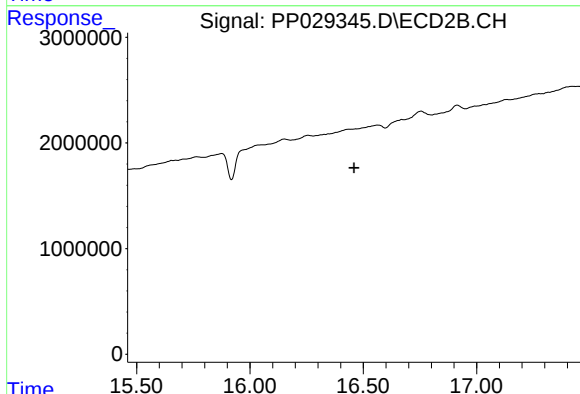


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.460 min
Response: 0
Conc: N.D.

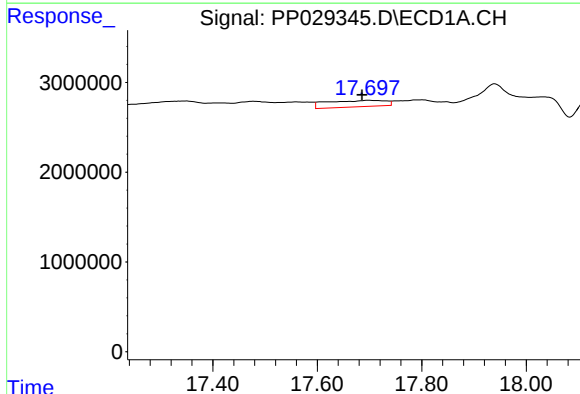


#14 DINOSEB

R.T.: 17.699 min
Delta R.T.: 0.013 min
Response: 5605125
Conc: 38.49 ng/ml

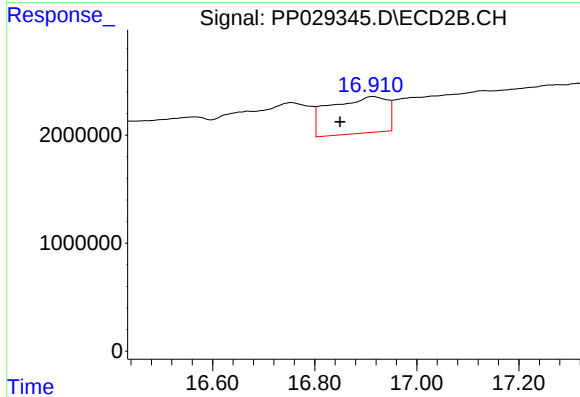

#14 DINOSEB


R.T.: 16.914 min
Delta R.T.: 0.065 min
Response: 26380350
Conc: 201.27 ng/ml

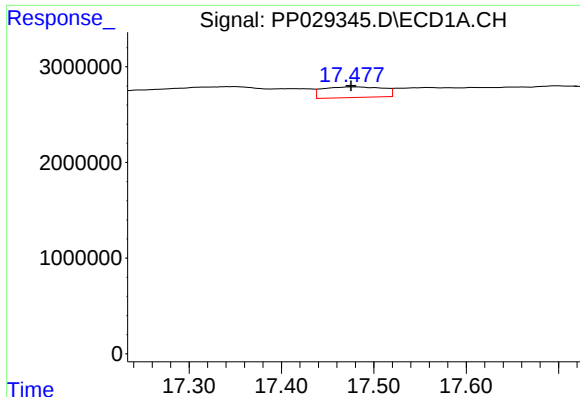

#15 Picloram


R.T.: 17.478 min
Delta R.T.: 0.003 min
Response: 5039493
Conc: 18.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11

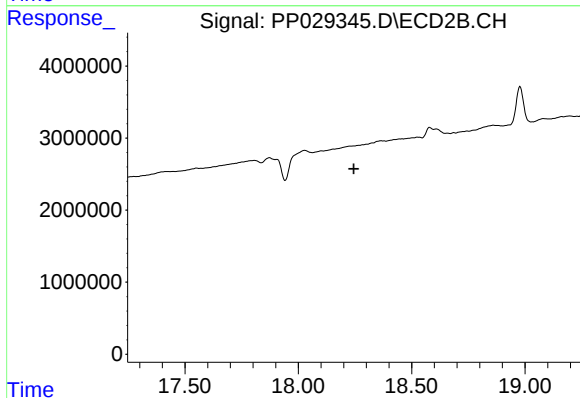


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.245 min
Response: 0
Conc: N.D.

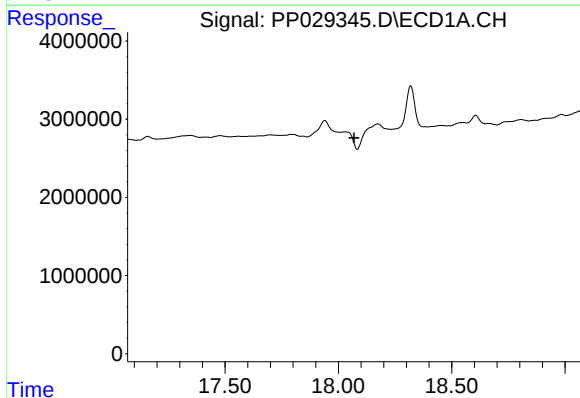

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.069 min
Response: 0
Conc: N.D.

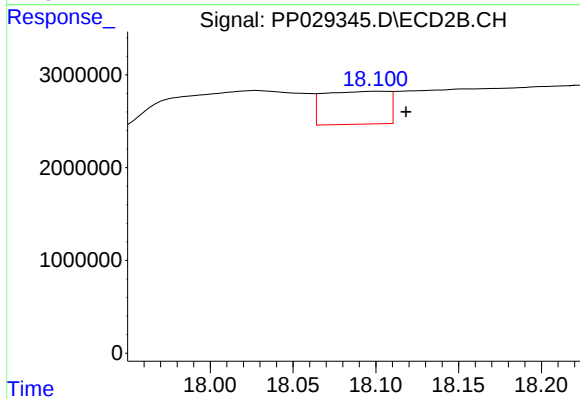

#16 DCPA

R.T.: 18.101 min
Delta R.T.: -0.017 min
Response: 9593541
Conc: 41.28 ng/ml