

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034001.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 13:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 16:09:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.265	1913581	946926	22.116	23.308
2) SA Decachlor...	10.780	9.587	2001543	633734	23.700	23.748
Target Compounds						
29) L6 AR-1254-4	7.992	0.000	1254704	0	365.799	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 13:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 16:09:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

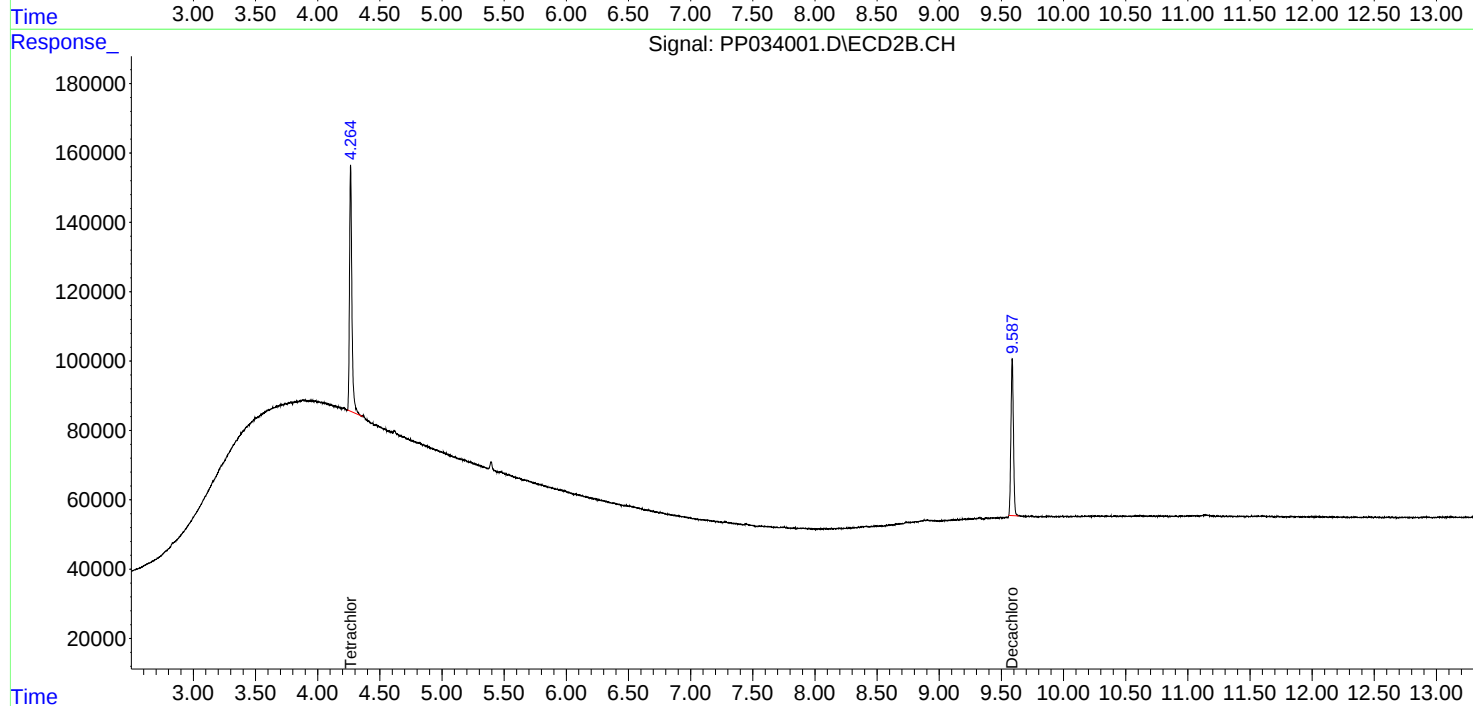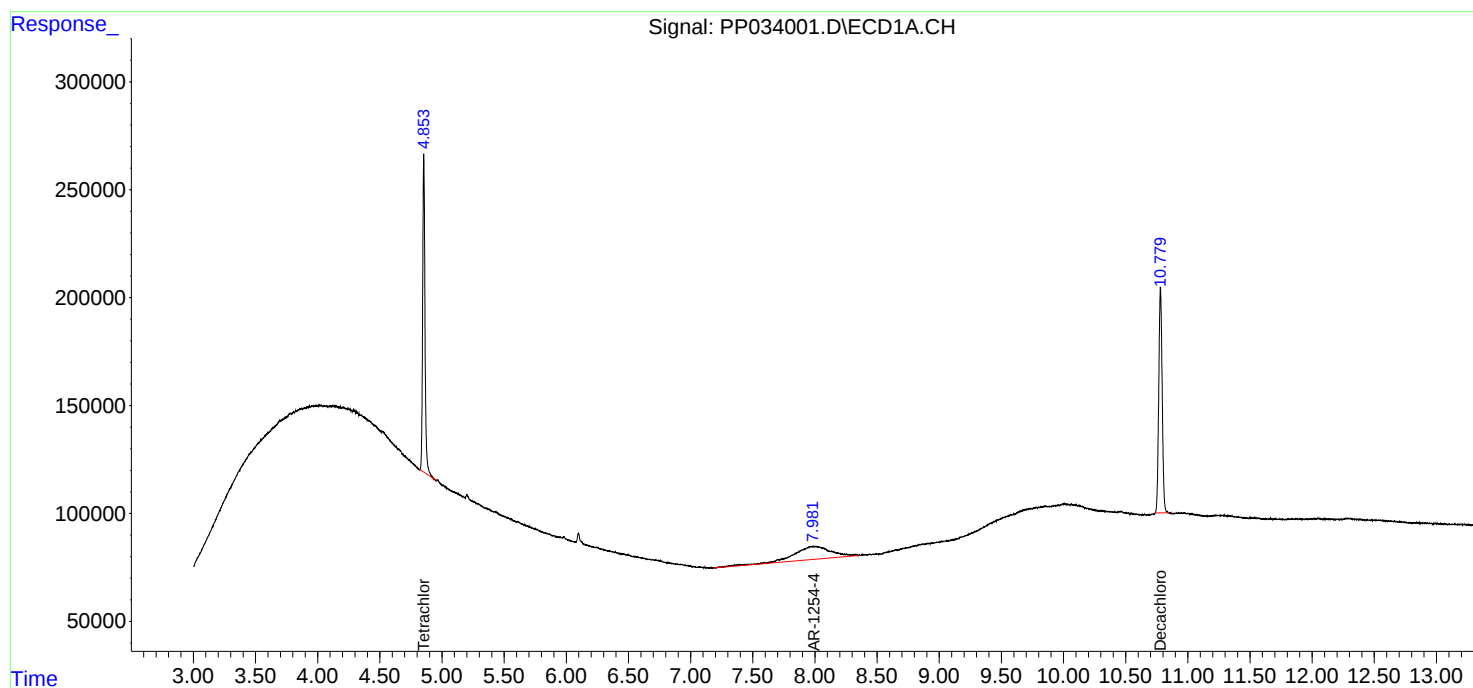


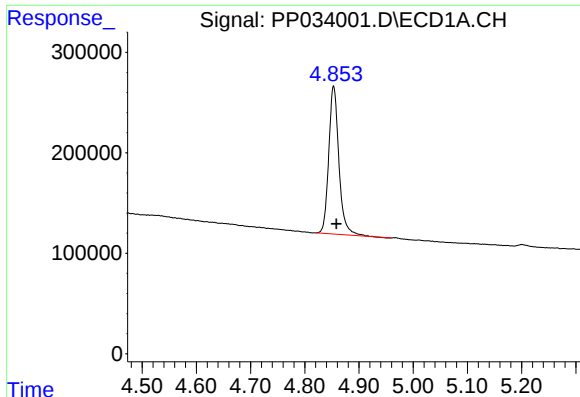

#1 Tetrachloro-m-xylene


R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 1913581
Conc: 22.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

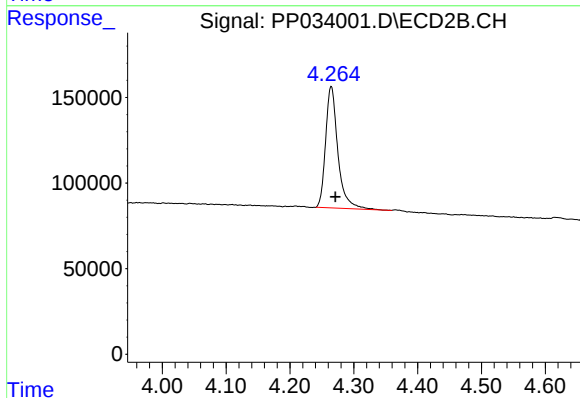


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.007 min
Response: 946926
Conc: 23.31 ng/ml

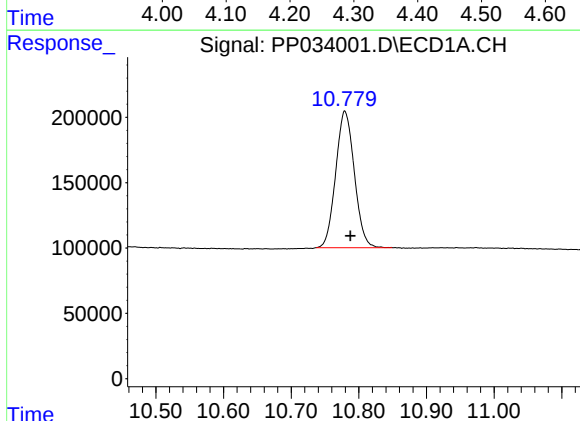


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.008 min
Response: 2001543
Conc: 23.70 ng/ml

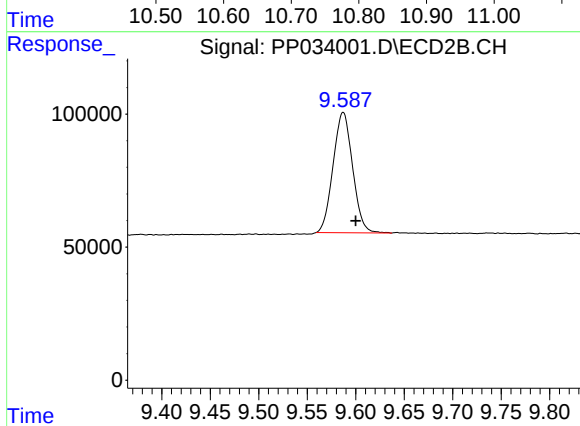

#2 Decachlorobiphenyl


R.T.: 9.587 min
Delta R.T.: -0.013 min
Response: 633734
Conc: 23.75 ng/ml

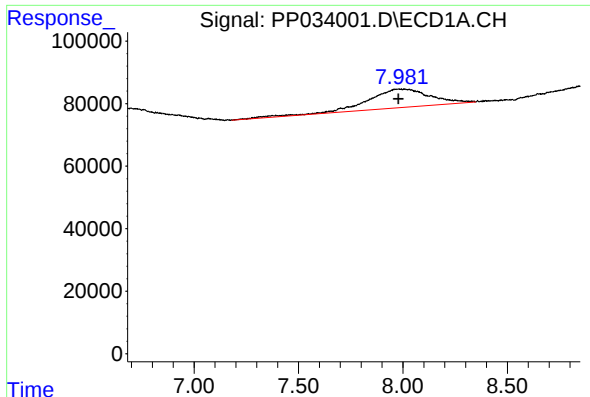

#29 AR-1254-4

R.T.: 7.992 min
Delta R.T.: 0.013 min
Response: 1254704
Conc: 365.80 ng/ml

Instrument :
ECD_P
ClientSampleId :

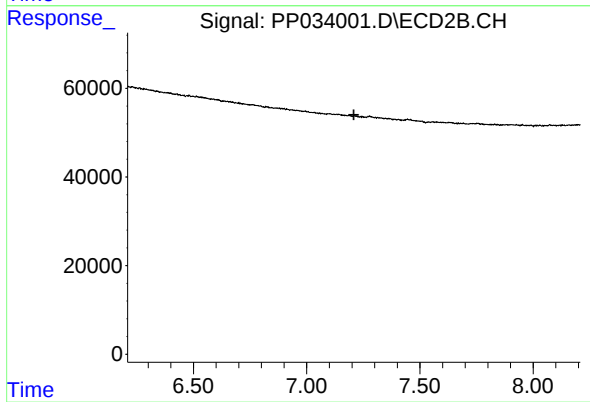

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.