

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034020.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 19:09
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:48:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.854	4.265	1867761	977378	21.586	24.058
2)	SA Decachlor...	10.783	9.587	2023220	669223	23.956	25.078
Target Compounds							
9)	L2 AR-1221-2	5.204	0.000	28580	0	40.672	N.D. #
24)	L5 AR-1248-4	7.081f	0.000	12501	0	4.519	N.D. #
26)	L6 AR-1254-1	7.081	0.000	12501	0	4.279	N.D. #
28)	L6 AR-1254-3	7.697	0.000	20771	0	4.201	N.D. #
40)	L8 AR-1262-5	0.000	9.046	0	13215	N.D.	11.593 #
43)	L9 AR-1268-3	0.000	8.739	0	21495	N.D.	6.920 #
44)	L9 AR-1268-4	0.000	9.046	0	13215	N.D.	10.888 #
45)	L9 AR-1268-5	10.462	9.327	24860	14206	0.841	1.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034020.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 19:09
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:48:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

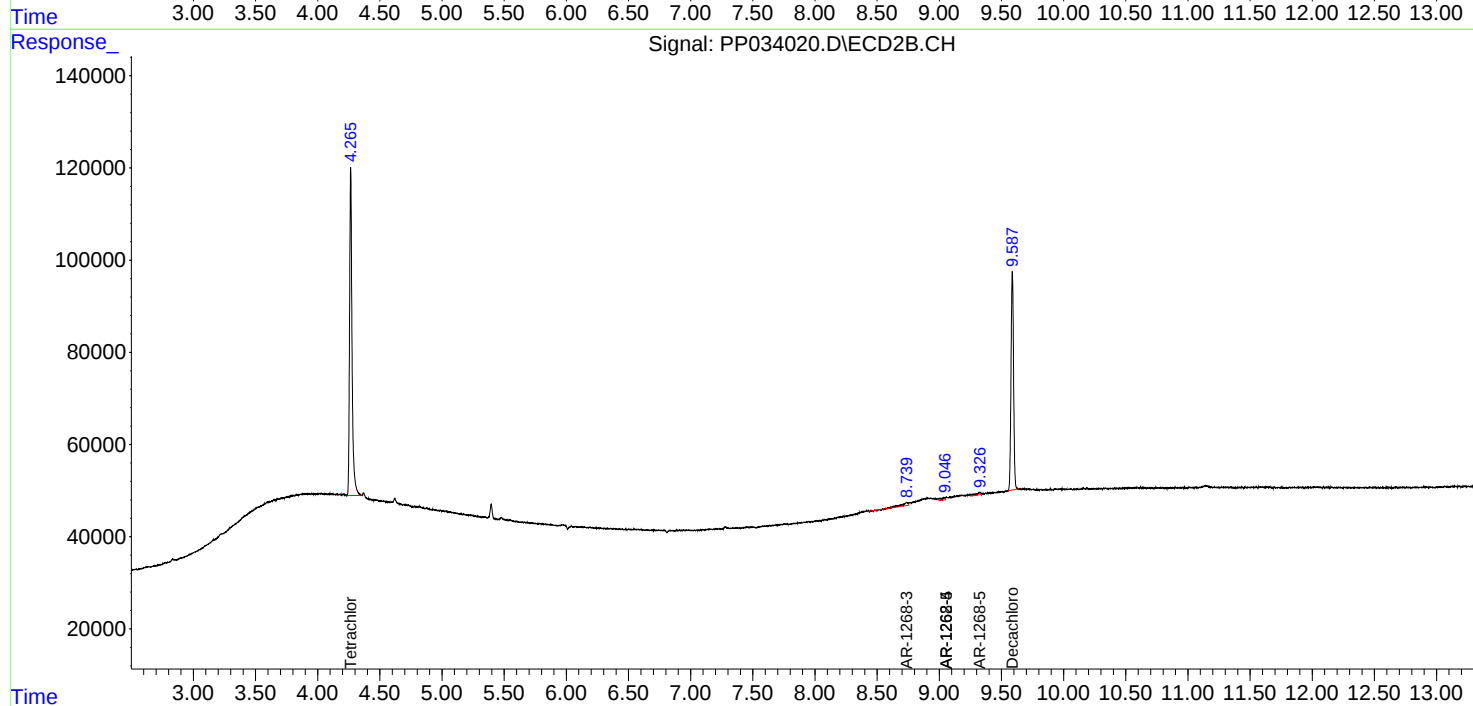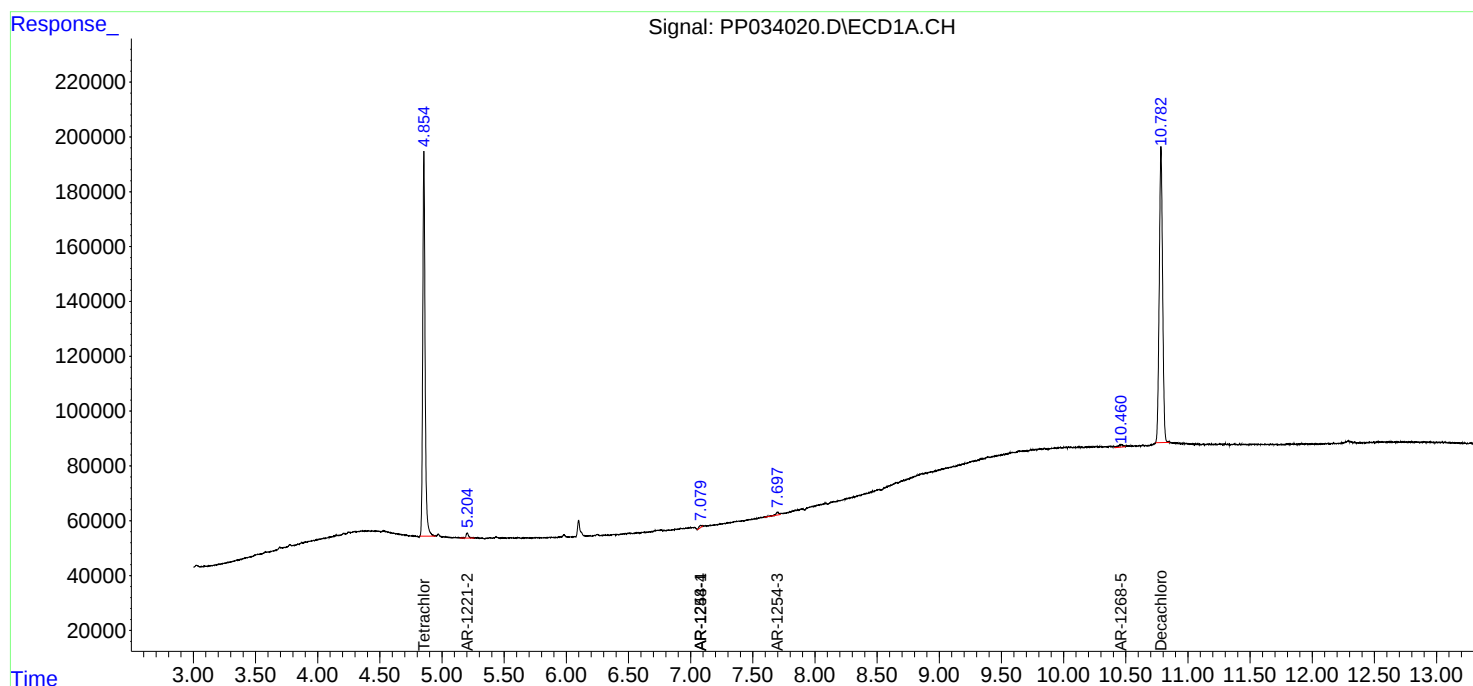


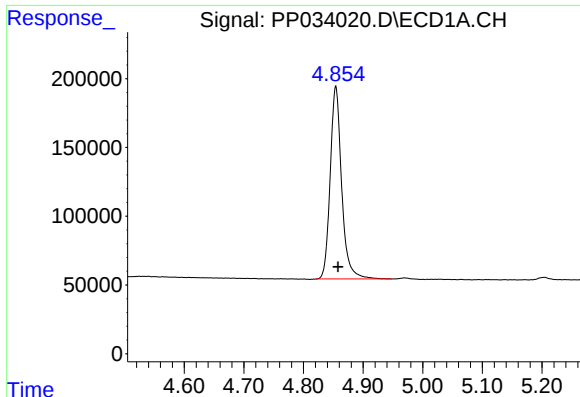

#1 Tetrachloro-m-xylene


R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 1867761
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

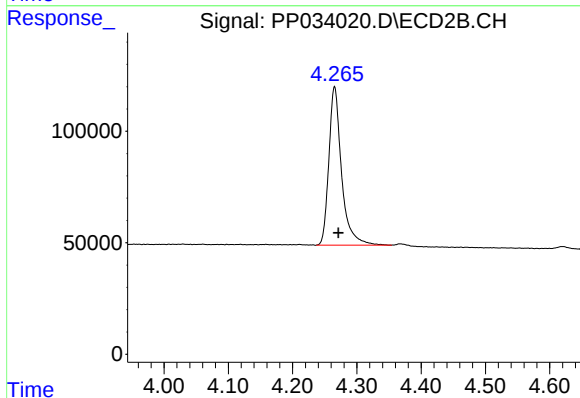


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 977378
Conc: 24.06 ng/ml

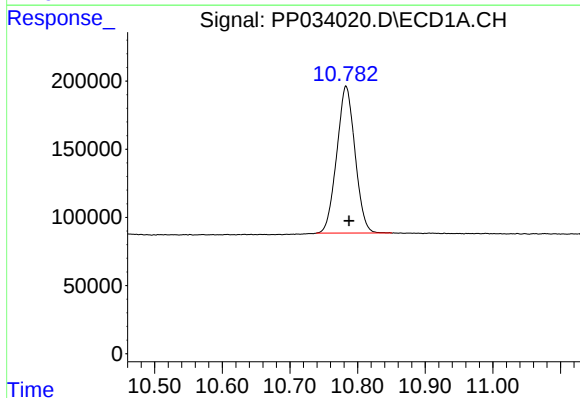


#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: -0.005 min
Response: 2023220
Conc: 23.96 ng/ml

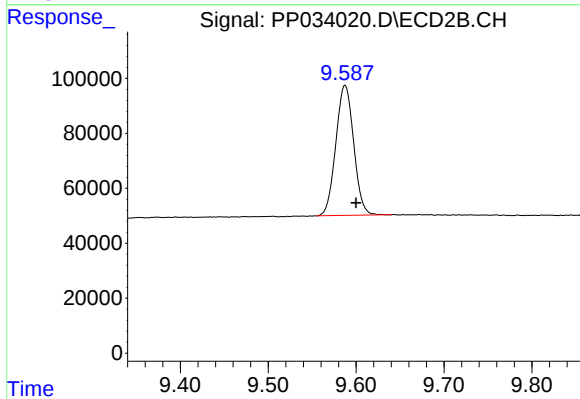

#2 Decachlorobiphenyl


R.T.: 9.587 min
Delta R.T.: -0.013 min
Response: 669223
Conc: 25.08 ng/ml

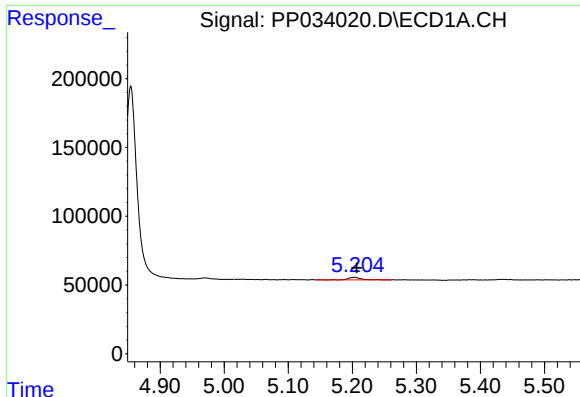

#9 AR-1221-2


R.T.: 5.204 min
Delta R.T.: -0.003 min
Response: 28580
Conc: 40.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

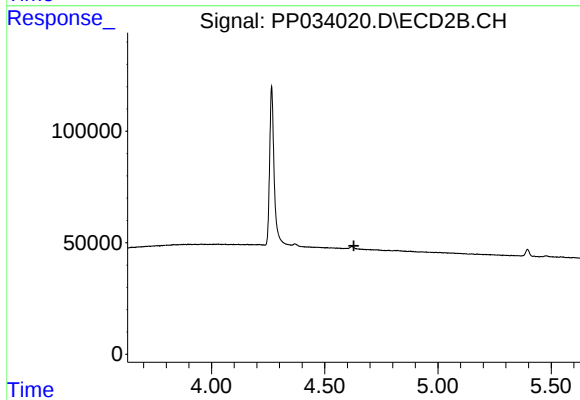


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

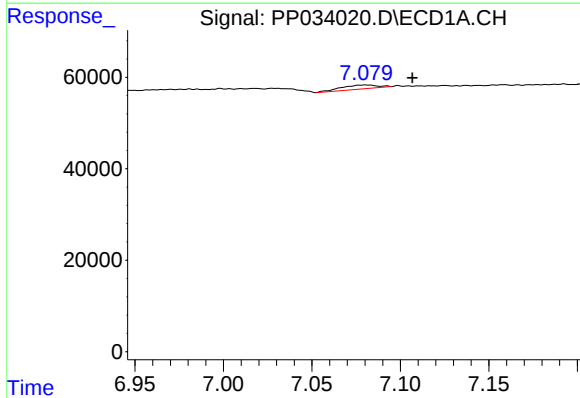


#24 AR-1248-4

R.T.: 7.081 min
Delta R.T.: -0.026 min
Response: 12501
Conc: 4.52 ng/ml

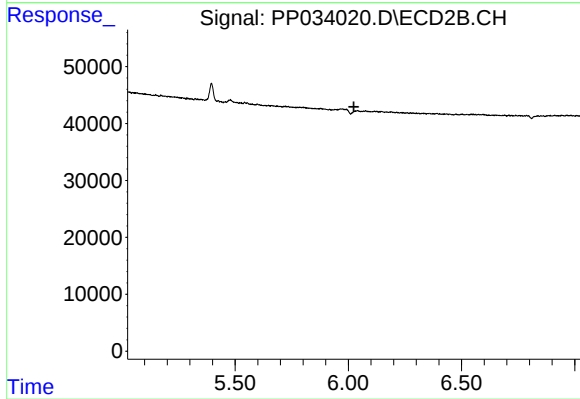

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

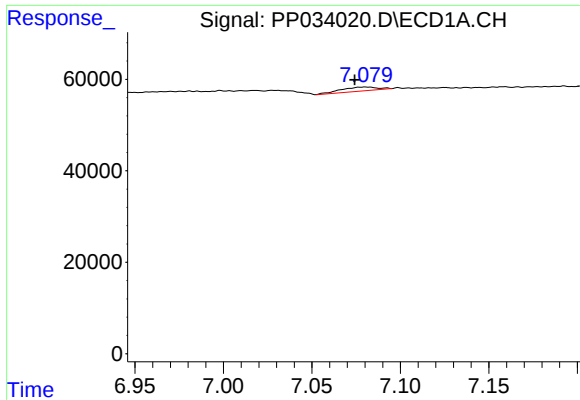

#26 AR-1254-1


R.T.: 7.081 min
Delta R.T.: 0.006 min
Response: 12501
Conc: 4.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

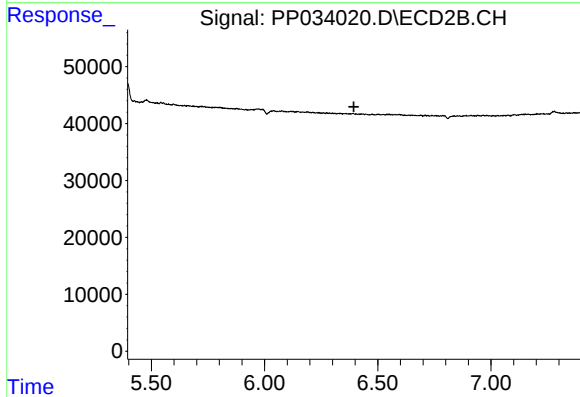


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.395 min
Response: 0
Conc: N.D.

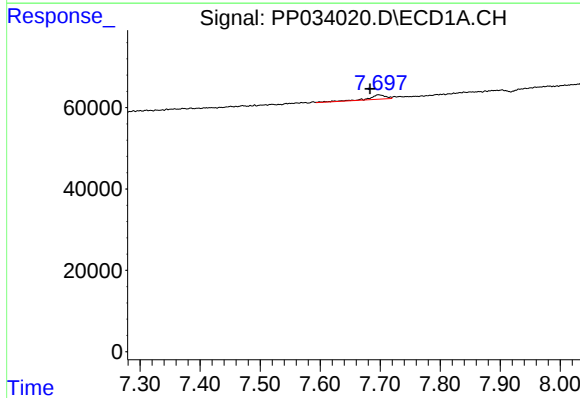


#28 AR-1254-3

R.T.: 7.697 min
Delta R.T.: 0.013 min
Response: 20771
Conc: 4.20 ng/ml

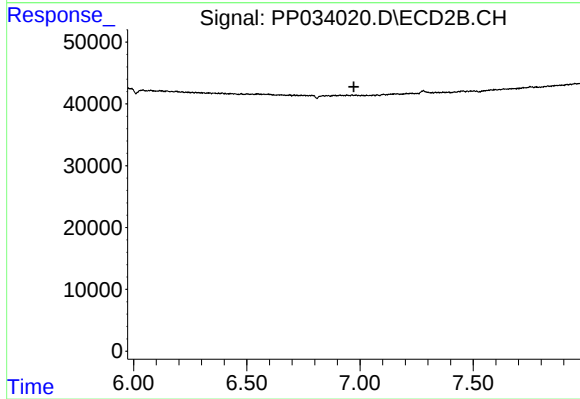

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

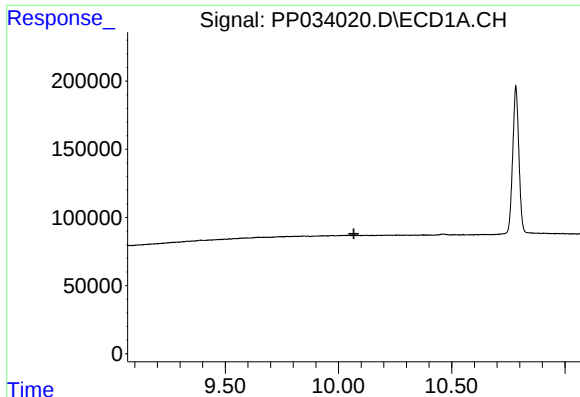

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

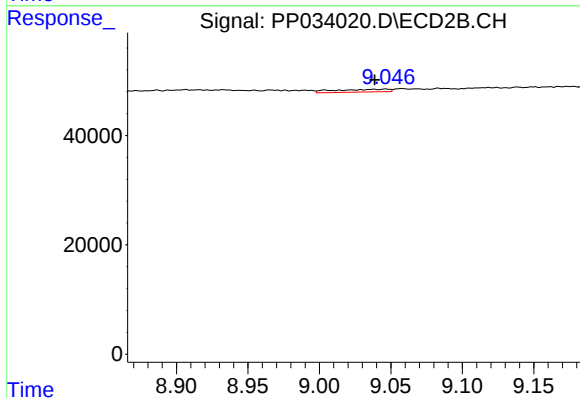


#40 AR-1262-5

R.T.: 9.046 min
Delta R.T.: 0.008 min
Response: 13215
Conc: 11.59 ng/ml

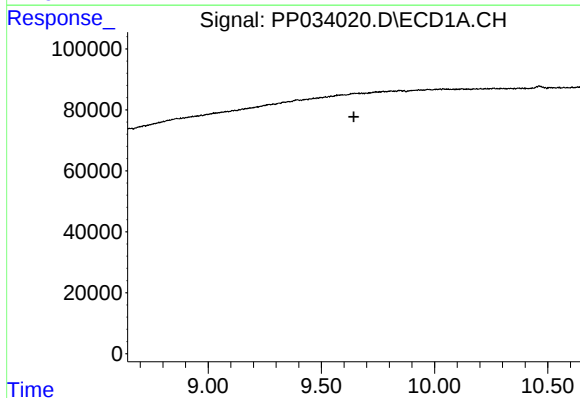


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.644 min
Response: 0
Conc: N.D.

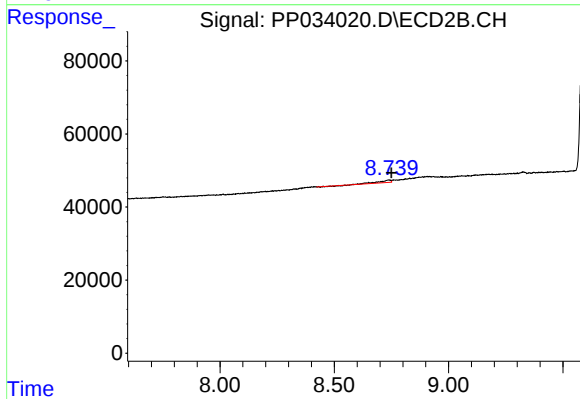

#43 AR-1268-3


R.T.: 8.739 min
Delta R.T.: -0.011 min
Response: 21495
Conc: 6.92 ng/ml

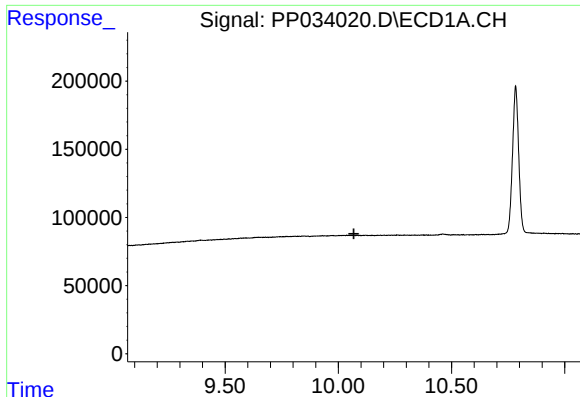

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 10.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

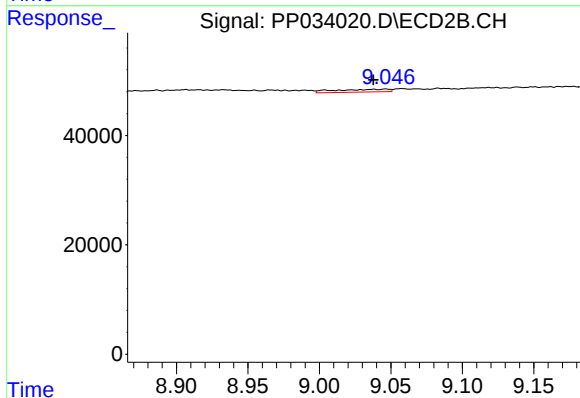


#44 AR-1268-4

R.T.: 9.046 min
Delta R.T.: 0.009 min
Response: 13215
Conc: 10.89 ng/ml

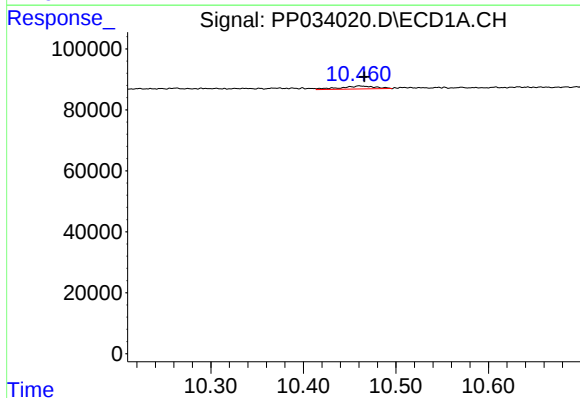

#45 AR-1268-5

R.T.: 10.462 min
Delta R.T.: -0.004 min
Response: 24860
Conc: 0.84 ng/ml

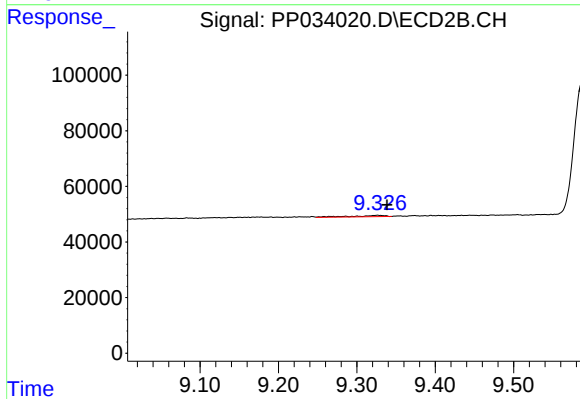

#45 AR-1268-5

R.T.: 9.327 min
Delta R.T.: -0.012 min
Response: 14206
Conc: 1.55 ng/ml