

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 22:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:53:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.852	4.264	1895291	989908	21.905	24.366
2)	SA Decachlor...	10.780	9.586	1968720	677119	23.311	25.374
Target Compounds							
9)	L2 AR-1221-2	5.202	0.000	25865	0	36.809	N.D. #
32)	L7 AR-1260-2	8.093f	0.000	129884	0	31.546	N.D. #
33)	L7 AR-1260-3	8.496	0.000	137286	0	42.414	N.D. #
35)	L7 AR-1260-5	0.000	8.189	0	2618	N.D.	0.805 #
36)	L8 AR-1262-1	8.496	0.000	137286	0	28.853	N.D. #
37)	L8 AR-1262-2	0.000	8.189	0	2618	N.D.	0.786 #
43)	L9 AR-1268-3	0.000	8.753	0	43953	N.D.	14.149 #
45)	L9 AR-1268-5	0.000	9.323f	0	179312	N.D.	19.612 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 22:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:53:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

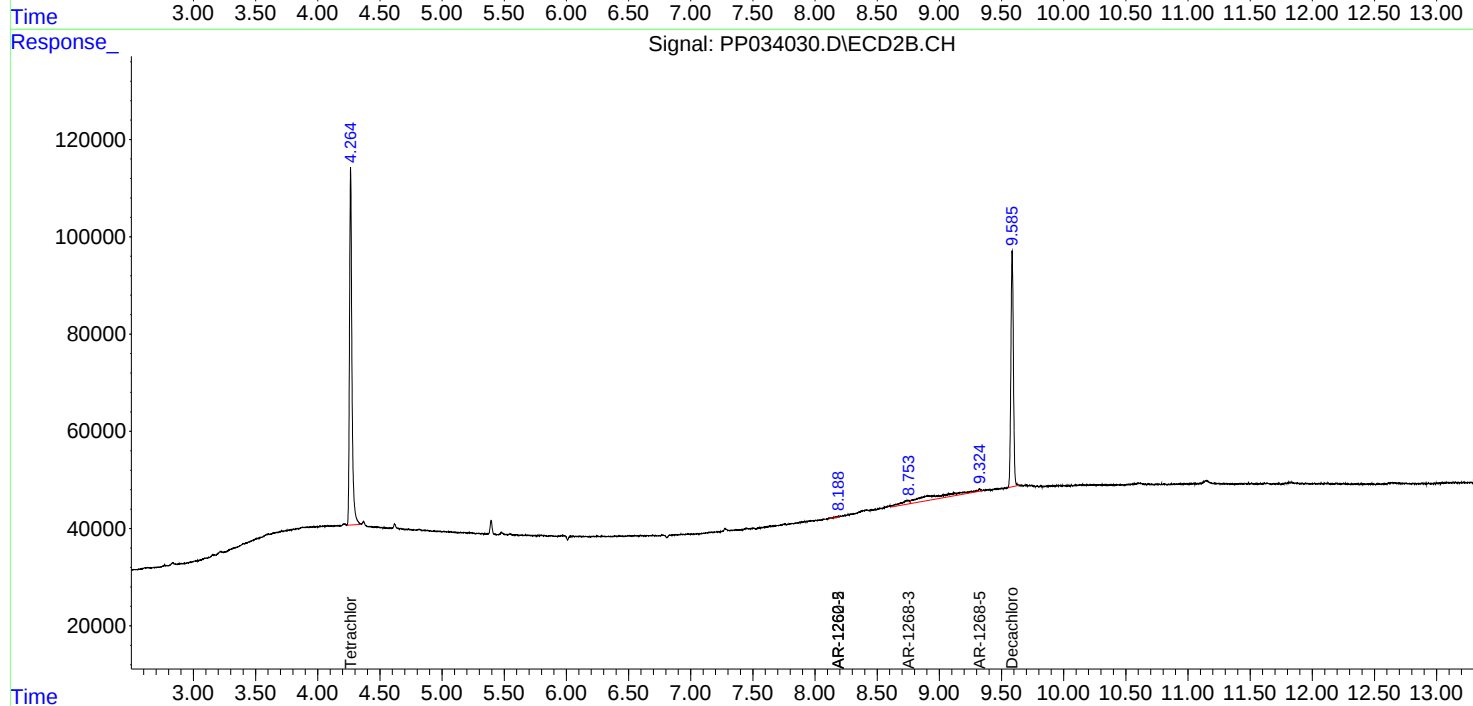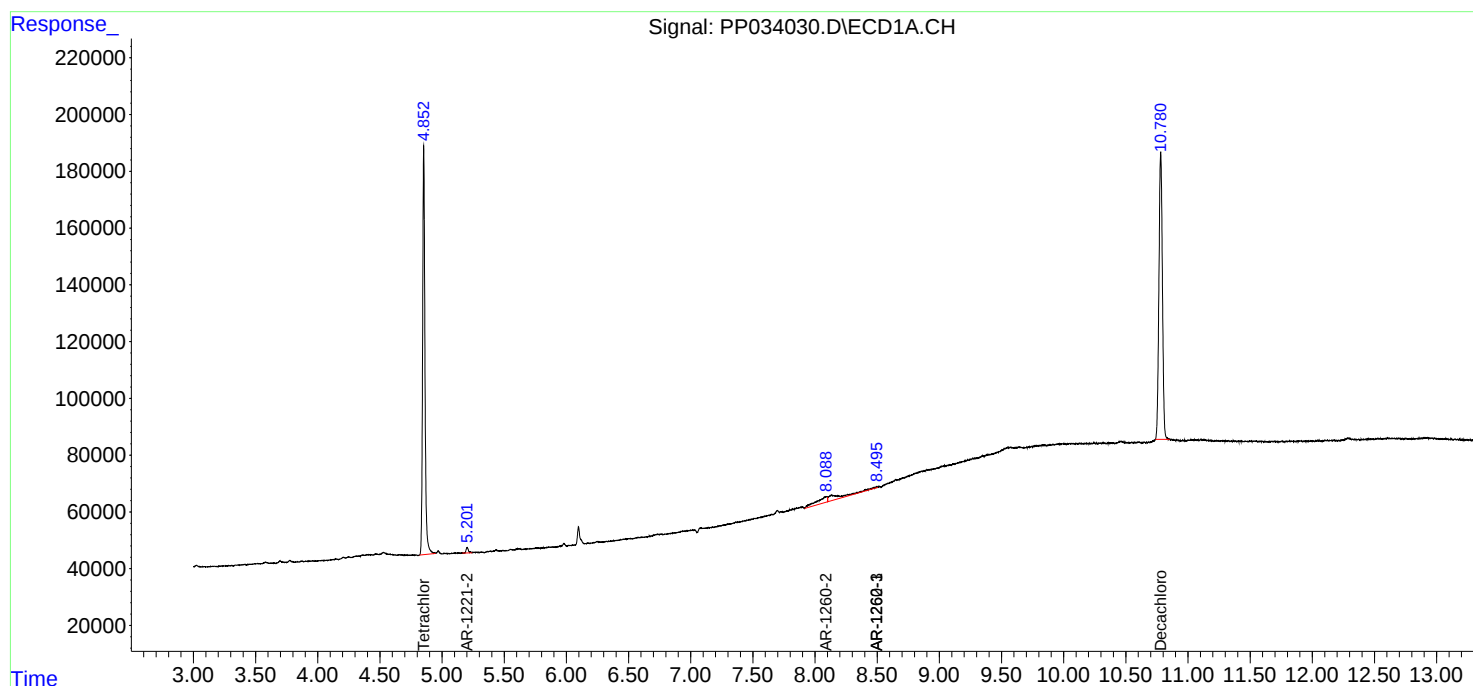


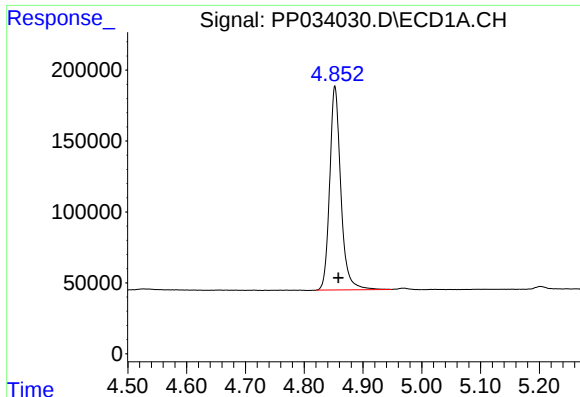

#1 Tetrachloro-m-xylene


R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 1895291
Conc: 21.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

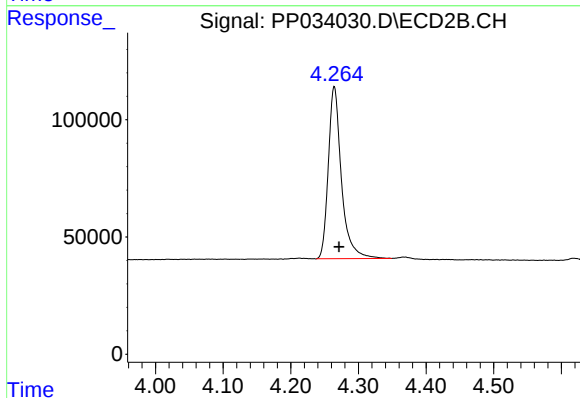


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 989908
Conc: 24.37 ng/ml

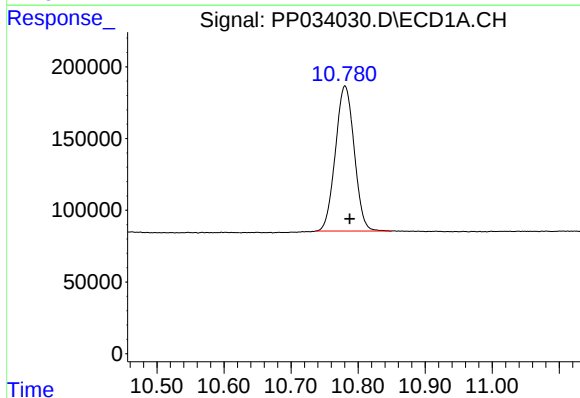


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.007 min
Response: 1968720
Conc: 23.31 ng/ml

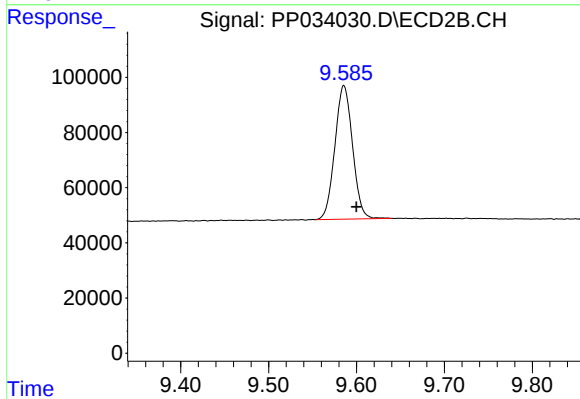

#2 Decachlorobiphenyl


R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 677119
Conc: 25.37 ng/ml

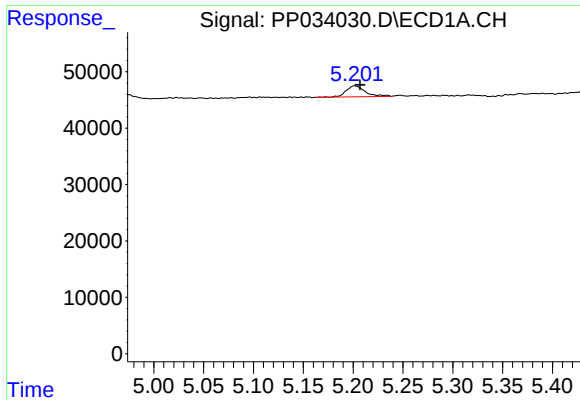

#9 AR-1221-2


R.T.: 5.202 min
Delta R.T.: -0.005 min
Response: 25865
Conc: 36.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

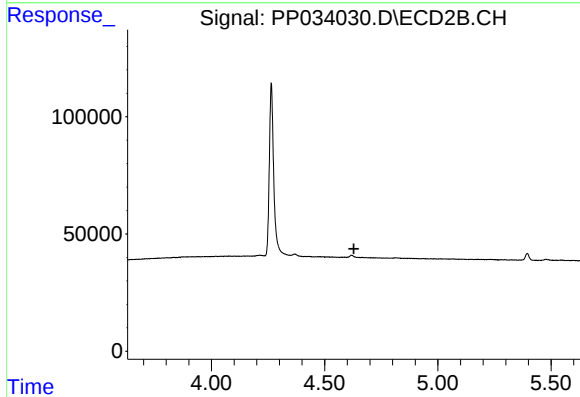


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

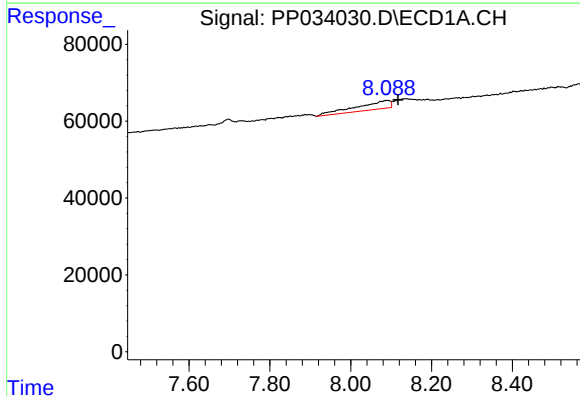


#32 AR-1260-2

R.T.: 8.093 min
Delta R.T.: -0.025 min
Response: 129884
Conc: 31.55 ng/ml

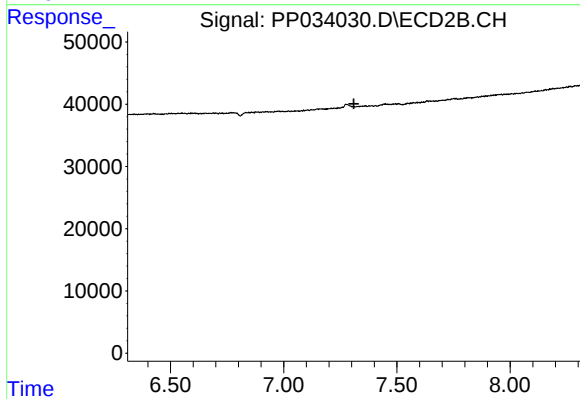

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

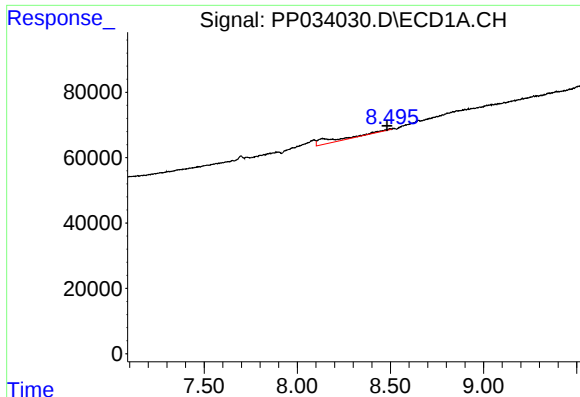

#33 AR-1260-3


R.T.: 8.496 min
Delta R.T.: 0.014 min
Response: 137286
Conc: 42.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

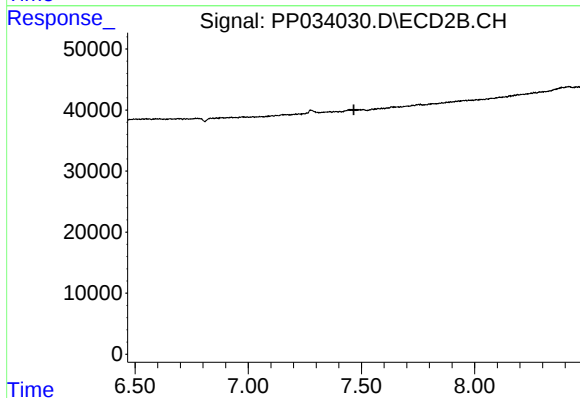


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.467 min
Response: 0
Conc: N.D.

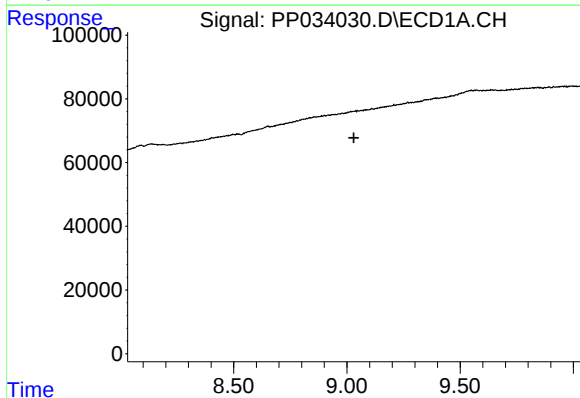


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

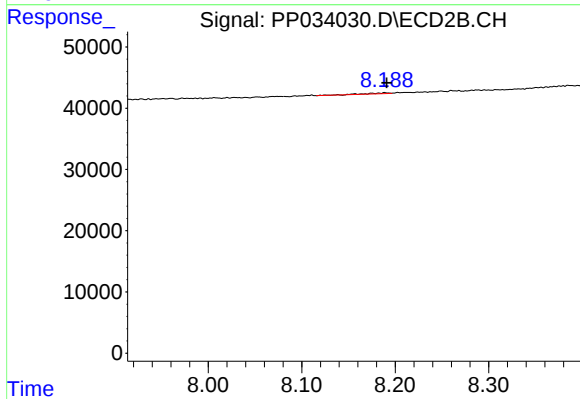

#35 AR-1260-5


R.T.: 8.189 min
Delta R.T.: -0.002 min
Response: 2618
Conc: 0.81 ng/ml

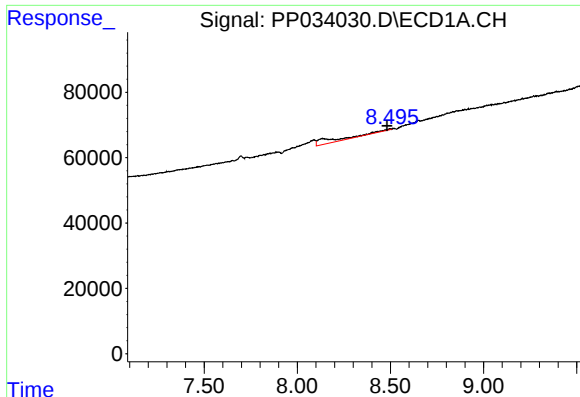

#36 AR-1262-1


R.T.: 8.496 min
Delta R.T.: 0.013 min
Response: 137286
Conc: 28.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

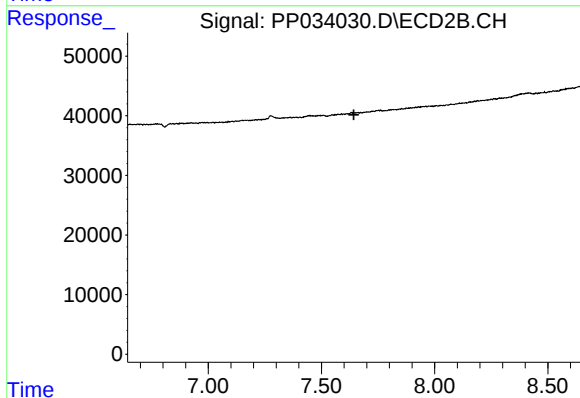


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.644 min
Response: 0
Conc: N.D.

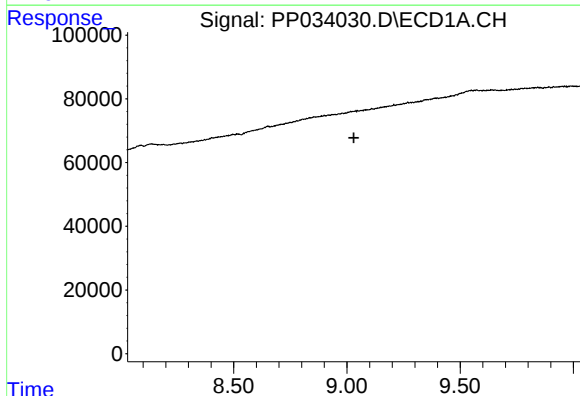


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

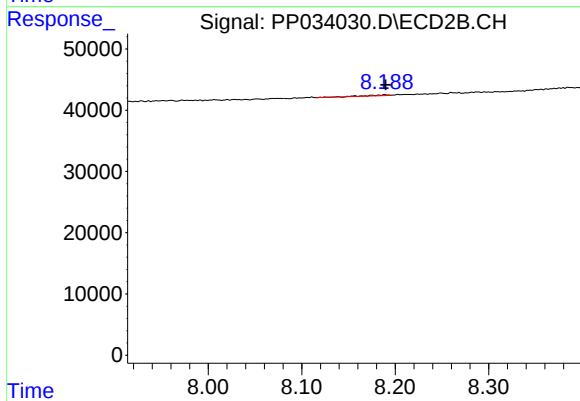

#37 AR-1262-2


R.T.: 8.189 min
Delta R.T.: 0.000 min
Response: 2618
Conc: 0.79 ng/ml

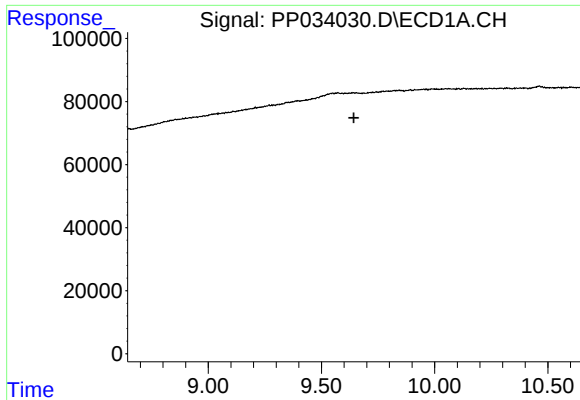

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

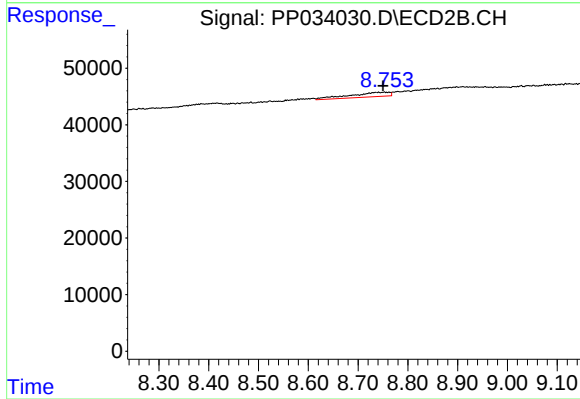


#43 AR-1268-3

R.T.: 8.753 min
Delta R.T.: 0.002 min
Response: 43953
Conc: 14.15 ng/ml

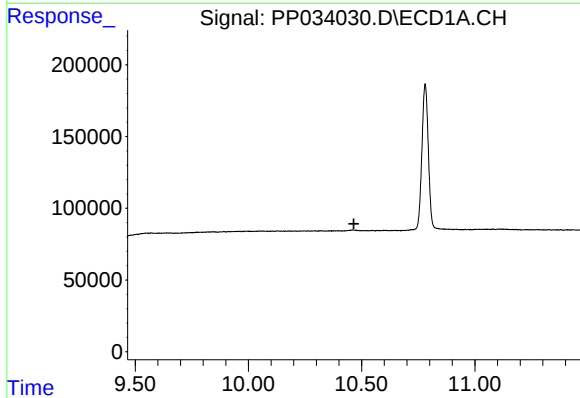

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.466 min
Response: 0
Conc: N.D.

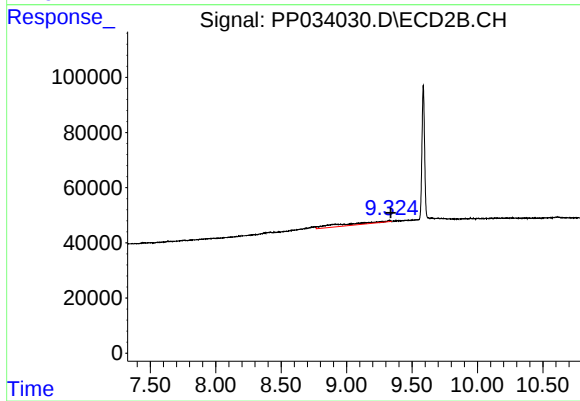

#45 AR-1268-5

R.T.: 9.323 min
Delta R.T.: -0.015 min
Response: 179312
Conc: 19.61 ng/ml