

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP033995.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 11:52
 Operator : DD\AJ
 Sample : M1660-05DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-2ADL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 16:06:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.852	4.264	380322	183230	4.396	4.510
2) SA Decachlor...	10.779	9.586	355411	111631	4.208	4.183
Target Compounds						
26) L6 AR-1254-1	7.071	6.392	623033	357808	213.273	219.471
27) L6 AR-1254-2	7.300	6.550	1789488	660835	393.545	462.701
28) L6 AR-1254-3	7.680	6.970	2813656	1337499	569.078	584.364
29) L6 AR-1254-4	7.975	7.206	2675857	987489	780.125	776.924
30) L6 AR-1254-5	8.402	7.634	4982435	2487761	1265.812	1320.804



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP033995.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 11:52
Operator : DD\AJ
Sample : M1660-05DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
X127-2ADL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 16:06:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

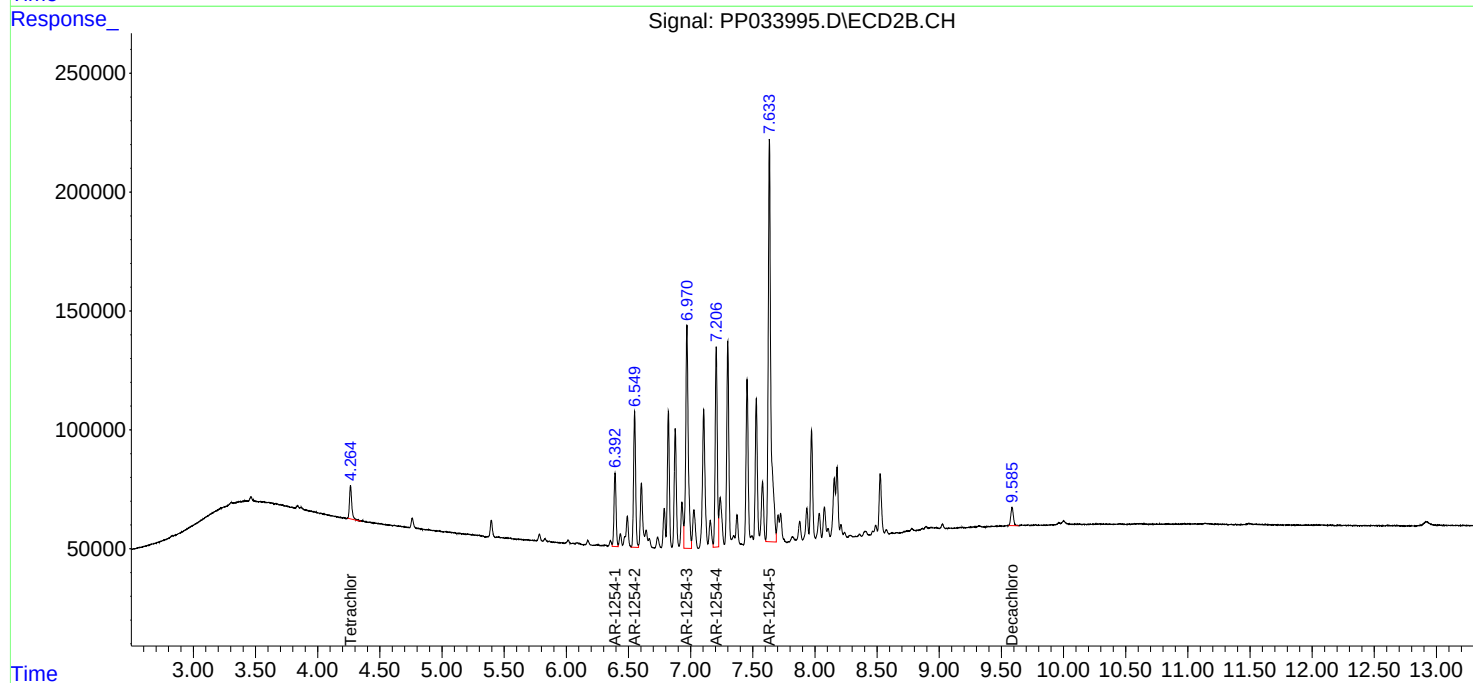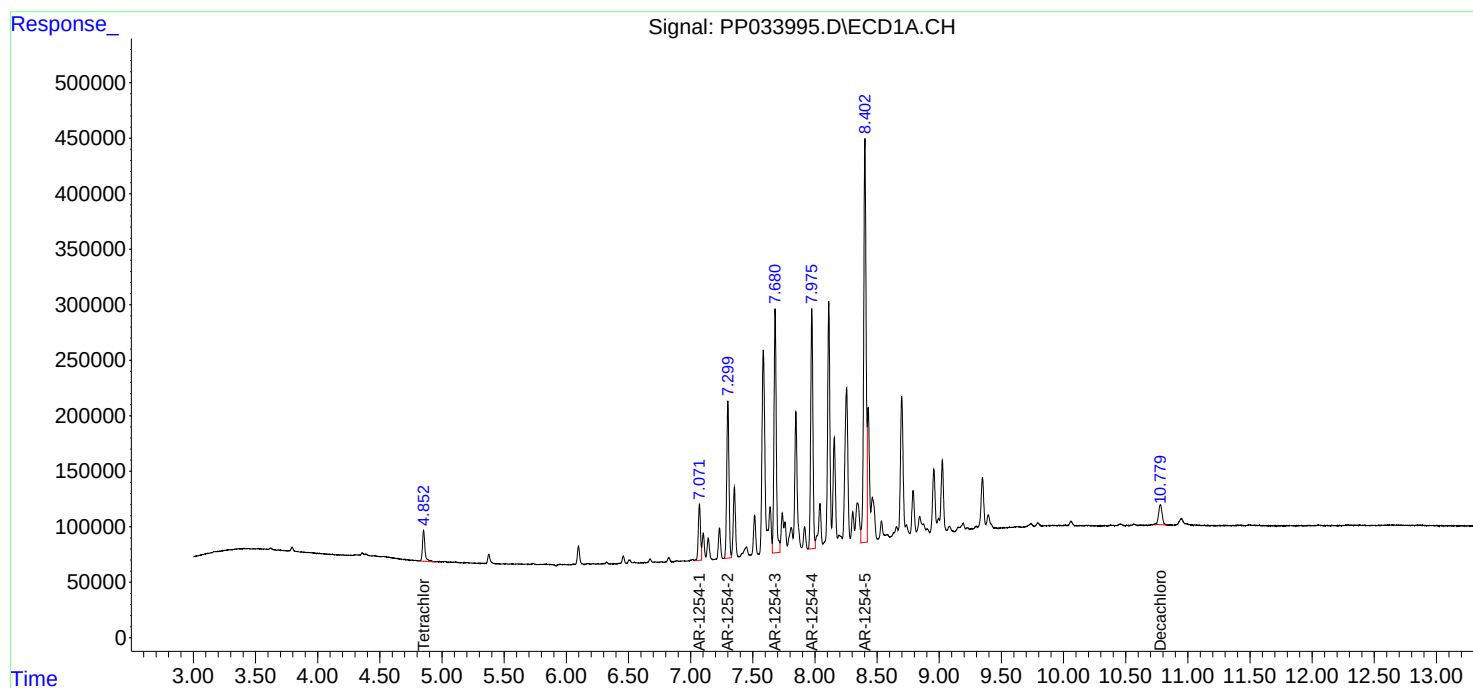


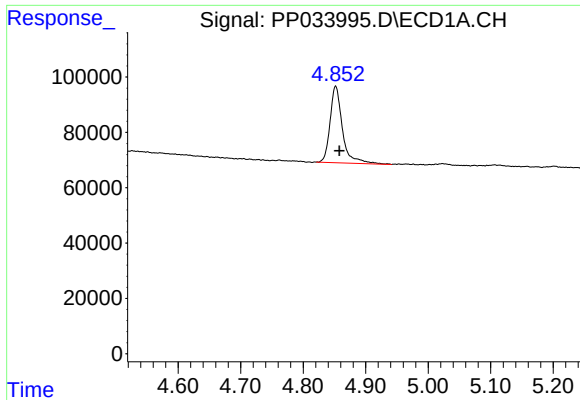

#1 Tetrachloro-m-xylene


R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 380322
Conc: 4.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2ADL

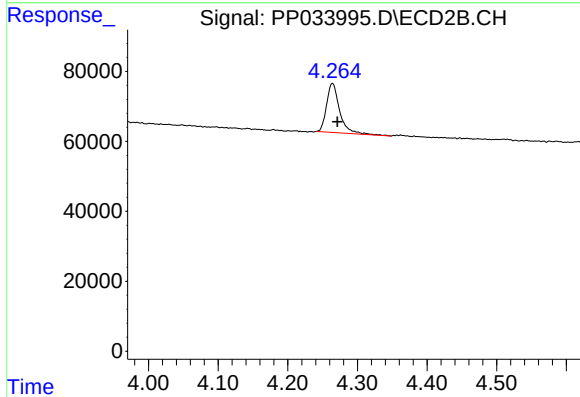


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 183230
Conc: 4.51 ng/ml

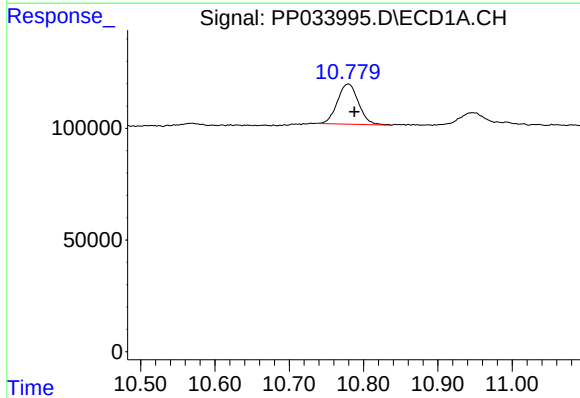


#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.008 min
Response: 355411
Conc: 4.21 ng/ml

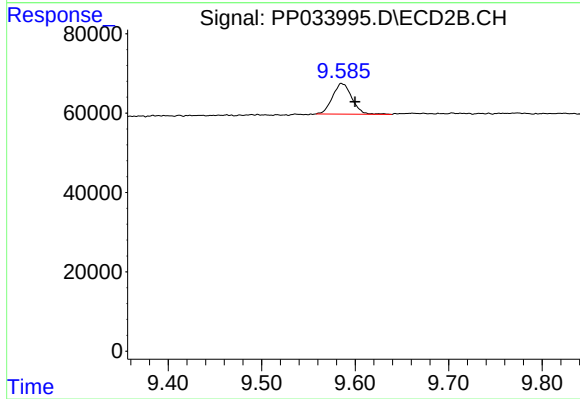

#2 Decachlorobiphenyl


R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 111631
Conc: 4.18 ng/ml

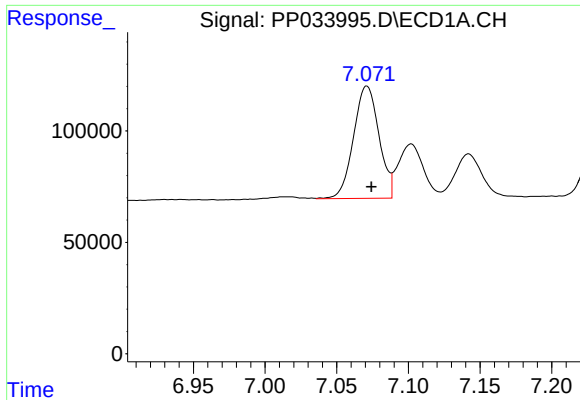

#26 AR-1254-1


R.T.: 7.071 min
Delta R.T.: -0.003 min
Response: 623033
Conc: 213.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2ADL

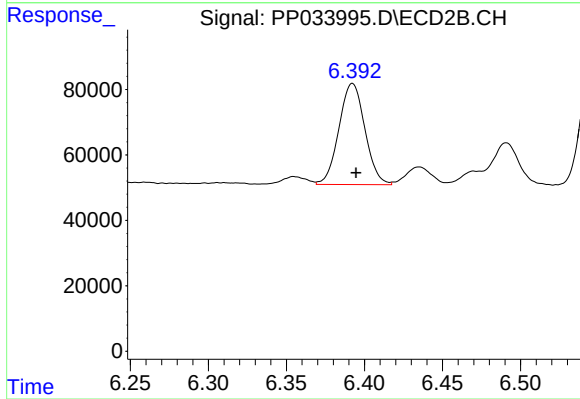


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.002 min
Response: 357808
Conc: 219.47 ng/ml

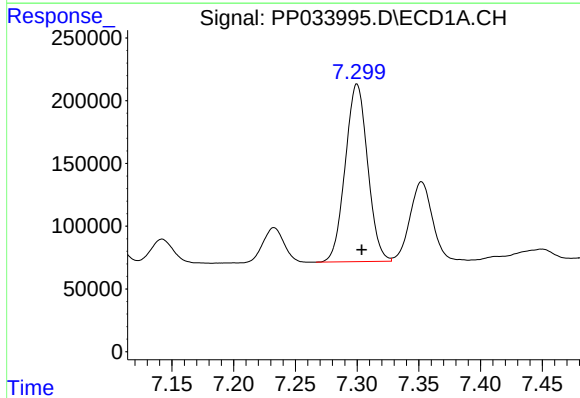


#27 AR-1254-2

R.T.: 7.300 min
Delta R.T.: -0.004 min
Response: 1789488
Conc: 393.54 ng/ml

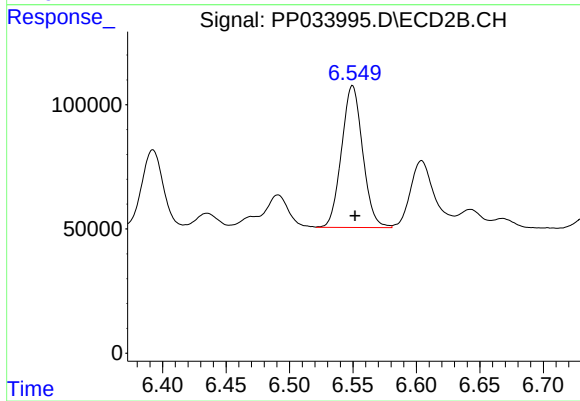

#27 AR-1254-2


R.T.: 6.550 min
Delta R.T.: -0.002 min
Response: 660835
Conc: 462.70 ng/ml

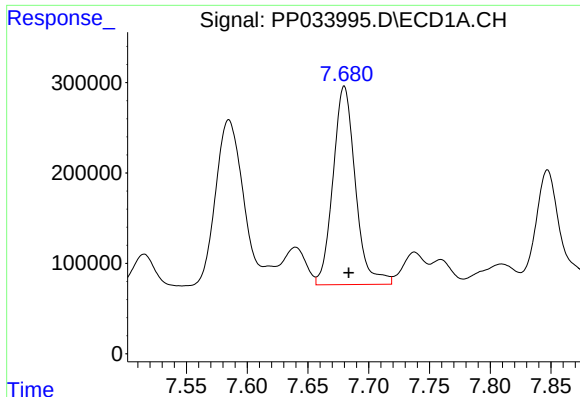

#28 AR-1254-3


R.T.: 7.680 min
Delta R.T.: -0.004 min
Response: 2813656
Conc: 569.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2ADL

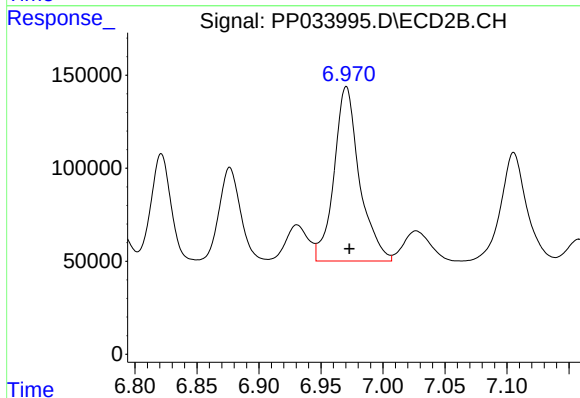


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.002 min
Response: 1337499
Conc: 584.36 ng/ml

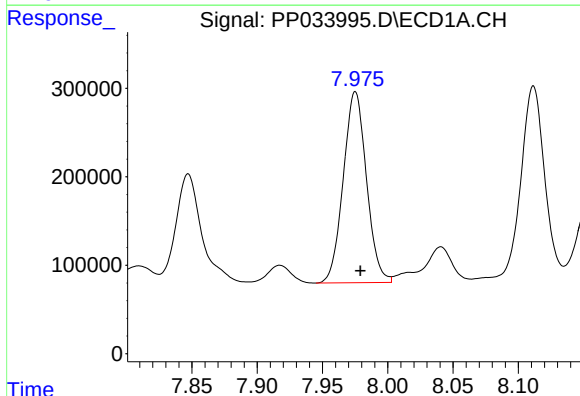


#29 AR-1254-4

R.T.: 7.975 min
Delta R.T.: -0.004 min
Response: 2675857
Conc: 780.12 ng/ml

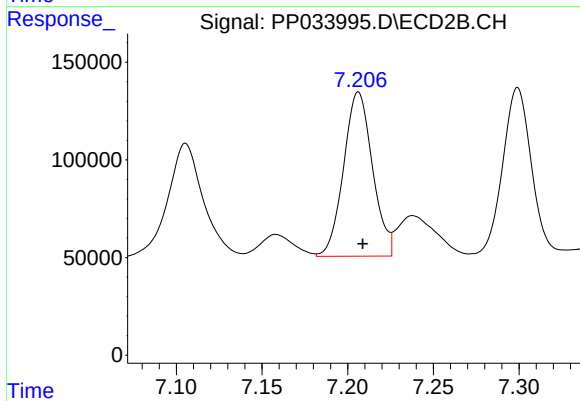

#29 AR-1254-4


R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 987489
Conc: 776.92 ng/ml

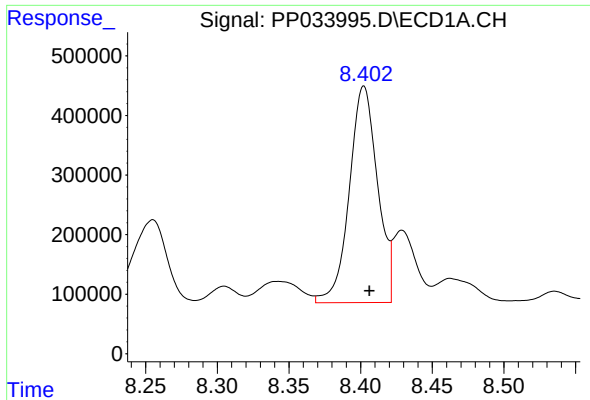

#30 AR-1254-5

R.T.: 8.402 min
Delta R.T.: -0.004 min
Response: 4982435
Conc: 1265.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2ADL

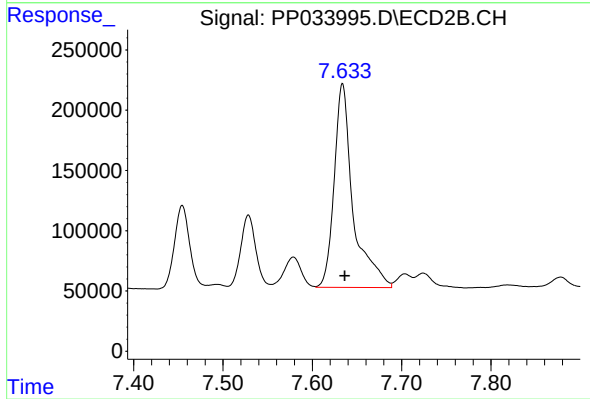

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.002 min
Response: 2487761
Conc: 1320.80 ng/ml