

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP033996.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 12:09
 Operator : DD\AJ
 Sample : M1660-08DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-3ADL

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 16:07:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.852	4.264	853588	414545	9.865	10.204
2)	SA Decachlor...	10.778	9.586	797240	249987	9.440	9.368
Target Compounds							
26)	L6 AR-1254-1	7.071	6.391	709083	390409	242.729	239.467
27)	L6 AR-1254-2	7.299	6.549	2052687	764298	451.427	535.144
28)	L6 AR-1254-3	7.679	6.970	3023856	1496302	611.592	653.747
29)	L6 AR-1254-4	7.975	7.206	3089469	1139289	900.710	896.354
30)	L6 AR-1254-5	8.402	7.633	5850867	2975193	1486.442m	1579.592

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP033996.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 12:09
Operator : DD\AJ
Sample : M1660-08DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-3ADL


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 16:07:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

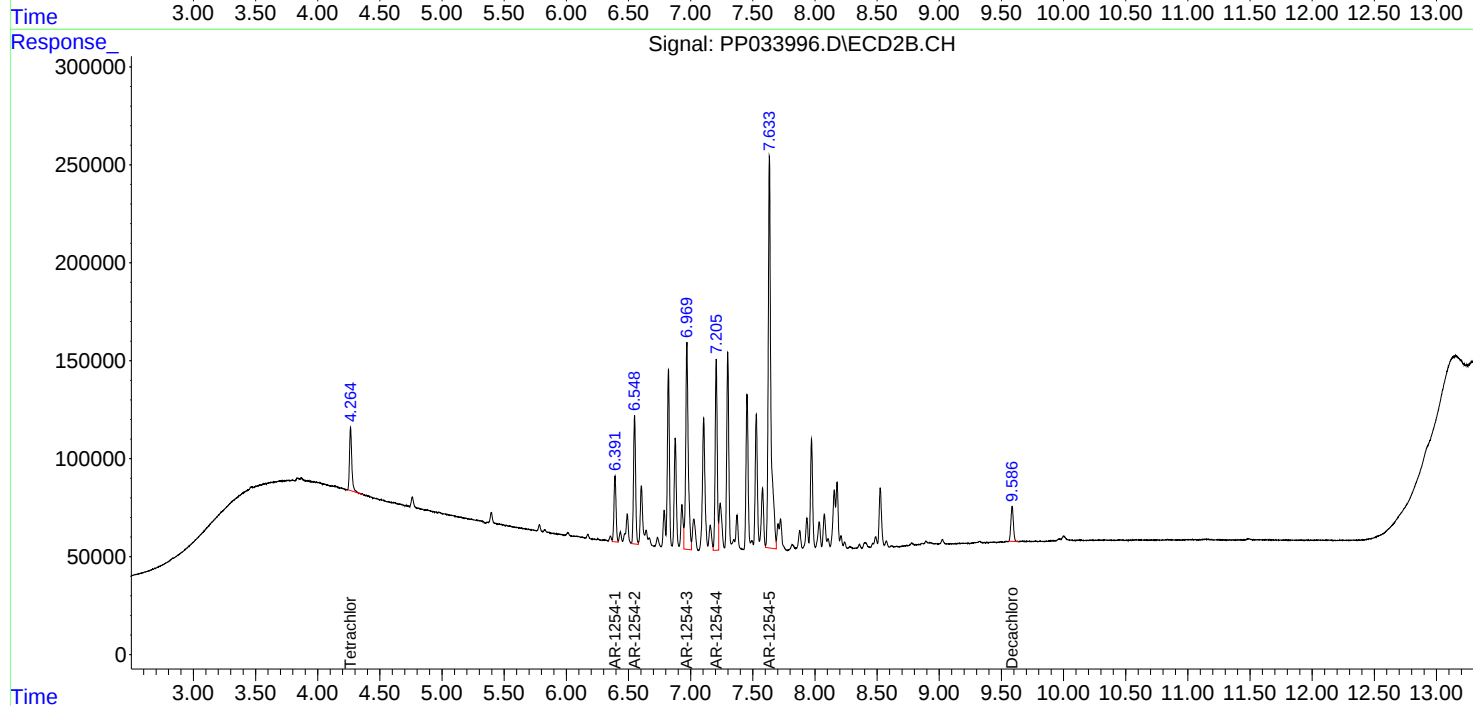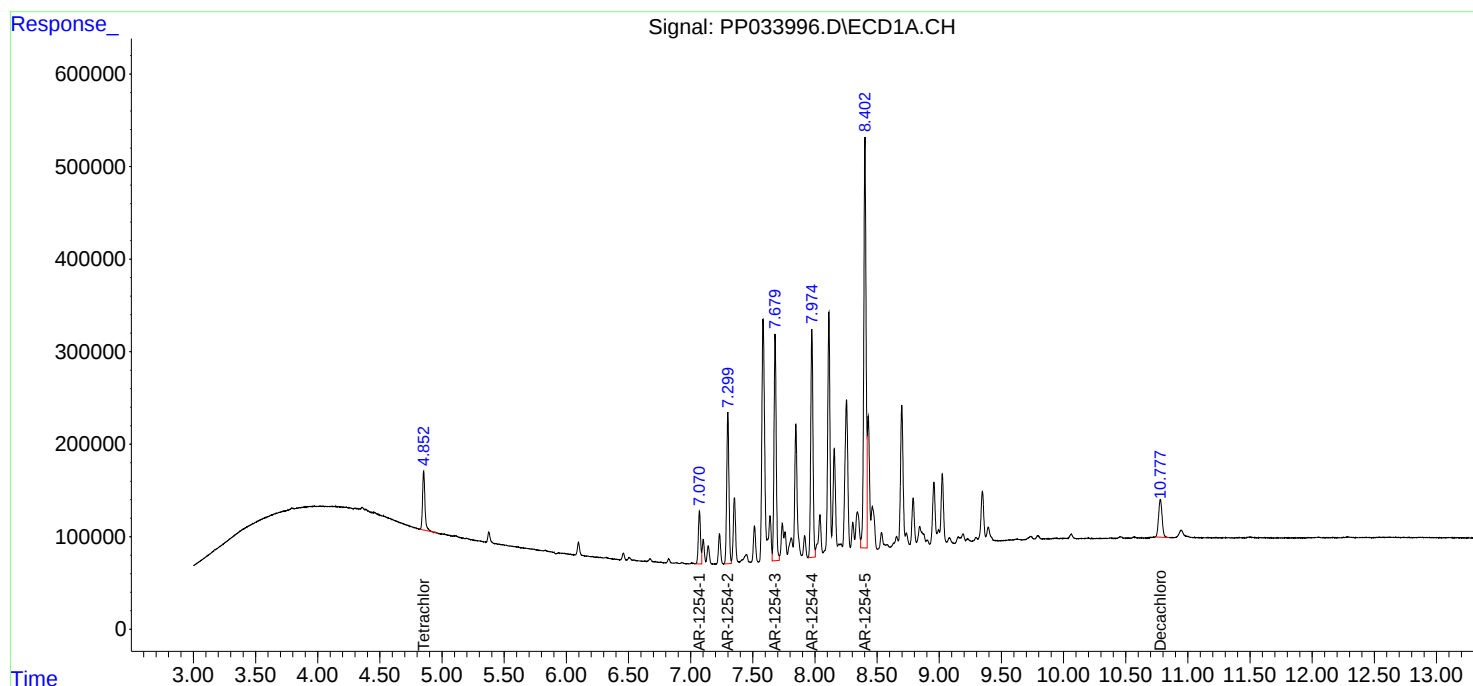

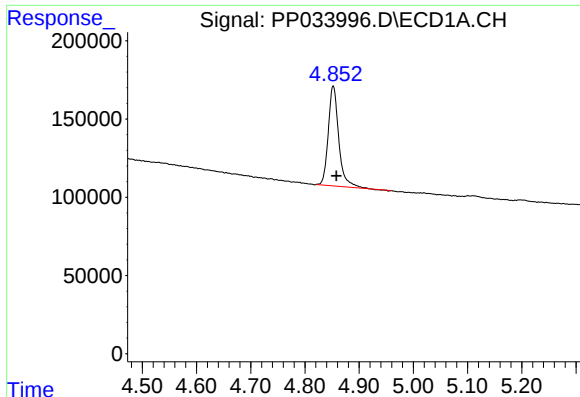


#1 Tetrachloro-m-xylene

R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 853588
Conc: 9.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3ADL


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:11 AM

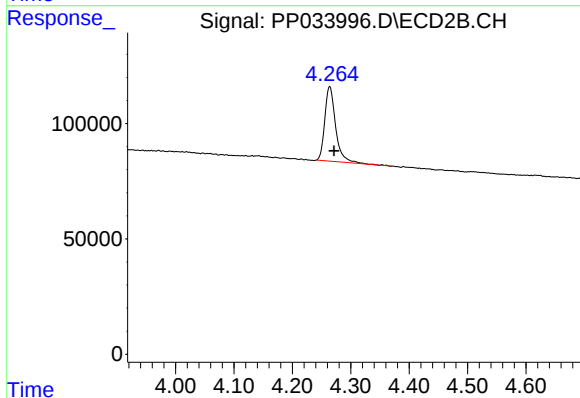


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 414545
Conc: 10.20 ng/ml

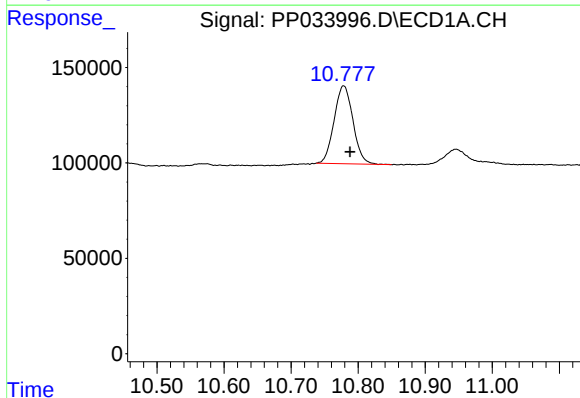


#2 Decachlorobiphenyl

R.T.: 10.778 min
Delta R.T.: -0.009 min
Response: 797240
Conc: 9.44 ng/ml

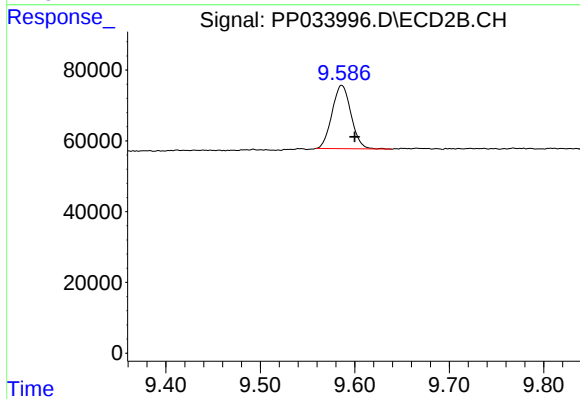

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 249987
Conc: 9.37 ng/ml

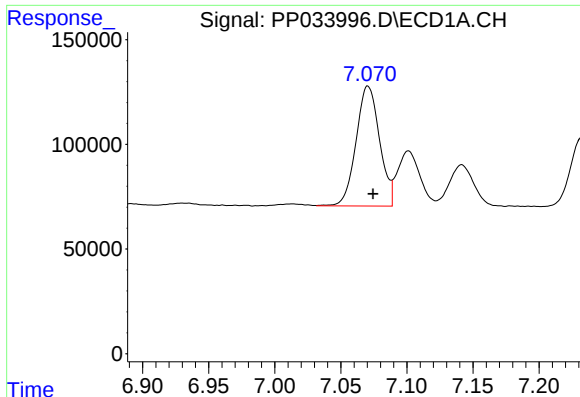


#26 AR-1254-1

R.T.: 7.071 min
Delta R.T.: -0.004 min
Response: 709083
Conc: 242.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3ADL


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:11 AM

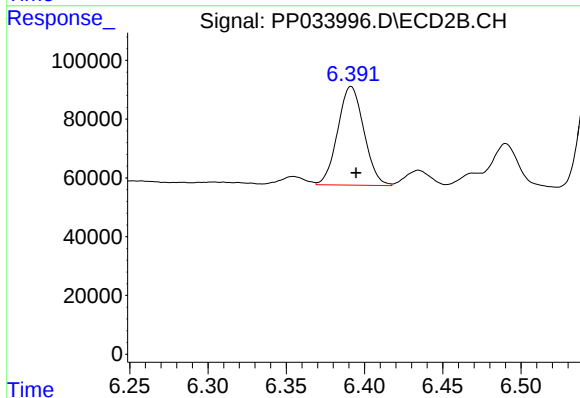


#26 AR-1254-1

R.T.: 6.391 min
Delta R.T.: -0.003 min
Response: 390409
Conc: 239.47 ng/ml

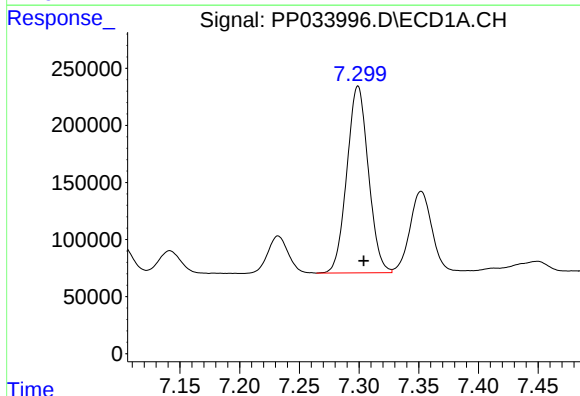


#27 AR-1254-2

R.T.: 7.299 min
Delta R.T.: -0.005 min
Response: 2052687
Conc: 451.43 ng/ml

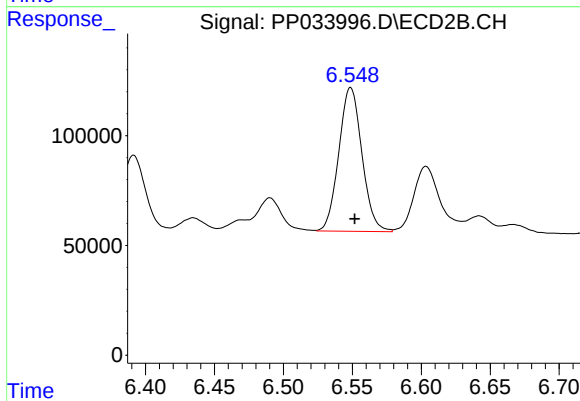

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 764298
Conc: 535.14 ng/ml

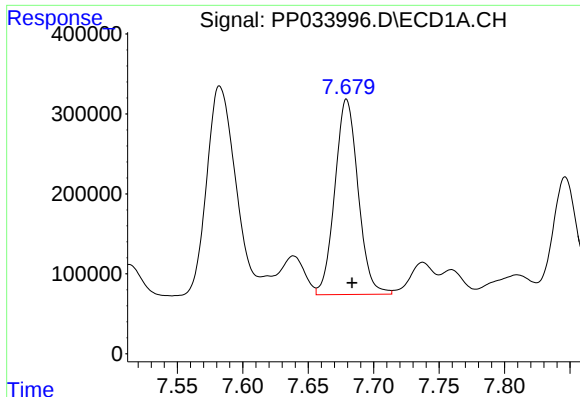


#28 AR-1254-3

R.T.: 7.679 min
Delta R.T.: -0.004 min
Response: 3023856
Conc: 611.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-3ADL


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:11 AM

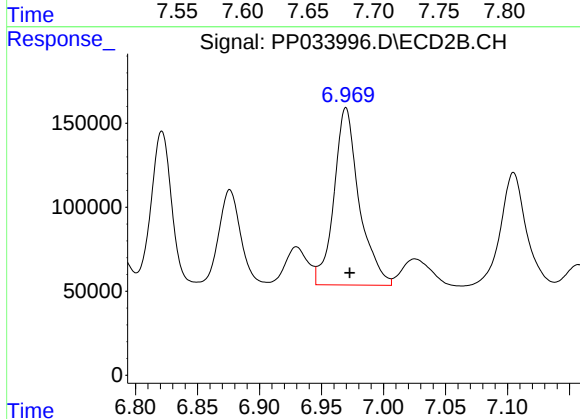


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 1496302
Conc: 653.75 ng/ml

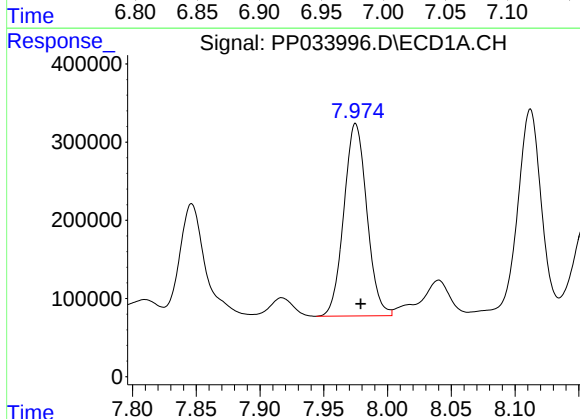


#29 AR-1254-4

R.T.: 7.975 min
Delta R.T.: -0.004 min
Response: 3089469
Conc: 900.71 ng/ml

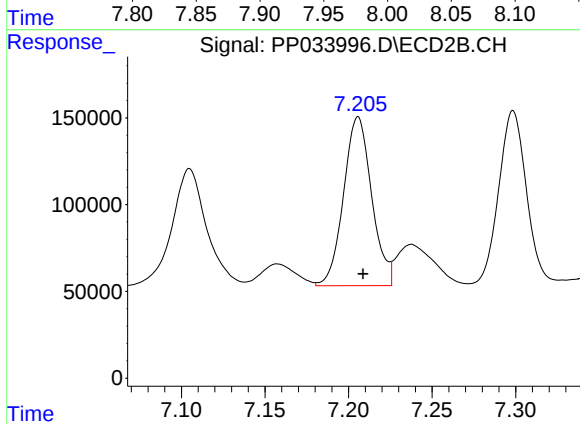

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 1139289
Conc: 896.35 ng/ml

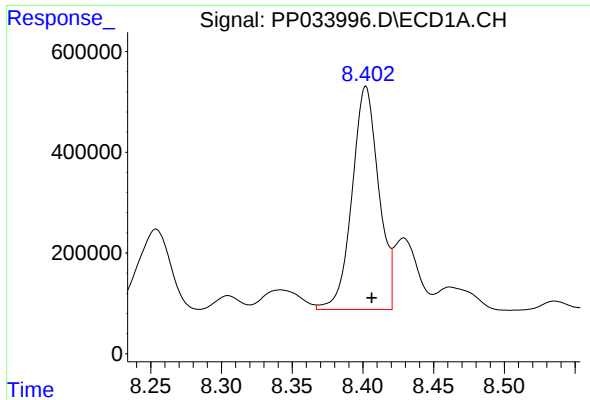


#30 AR-1254-5

R.T.: 8.402 min
Delta R.T.: -0.004 min
Response: 5850867
Conc: 1486.44 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-3ADL

Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:11 AM

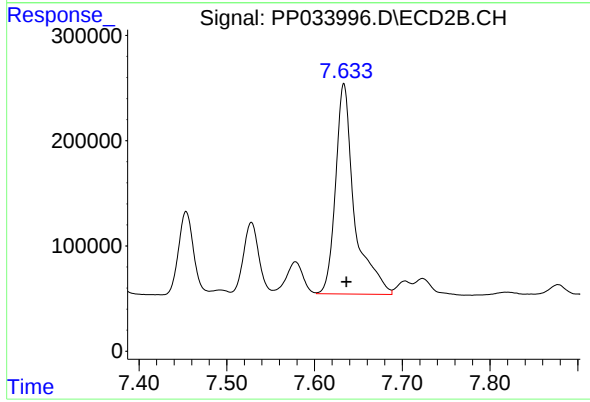

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 2975193
Conc: 1579.59 ng/ml