

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP033998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 12:42
 Operator : DD\AJ
 Sample : M1660-17DL 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-6ADL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 16:08:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.264	728531	368037	8.420	9.059
2) SA Decachlor...	10.780	9.587	651156	206744	7.710	7.748
Target Compounds						
26) L6 AR-1254-1	7.071	6.392	603285	319590	206.513	196.029
27) L6 AR-1254-2	7.300	6.549	1453885	533782	319.739	373.741
28) L6 AR-1254-3	7.681	6.970	2199857	1121341	444.933	489.923
29) L6 AR-1254-4	7.976	7.206	1784969	693723	520.394	545.798
30) L6 AR-1254-5	8.403	7.633	3865565	1967003	982.066	1044.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP033998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 12:42
Operator : DD\AJ
Sample : M1660-17DL 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
X127-6ADL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 16:08:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

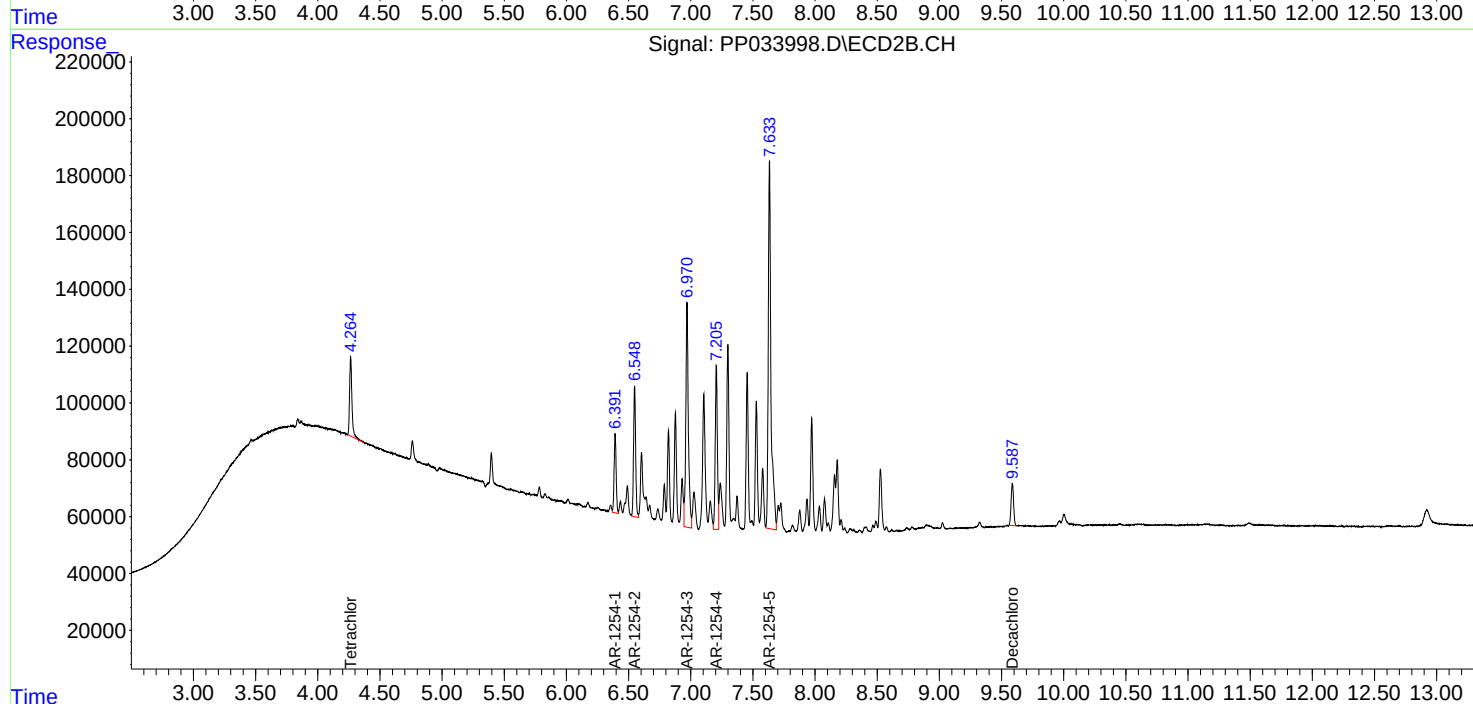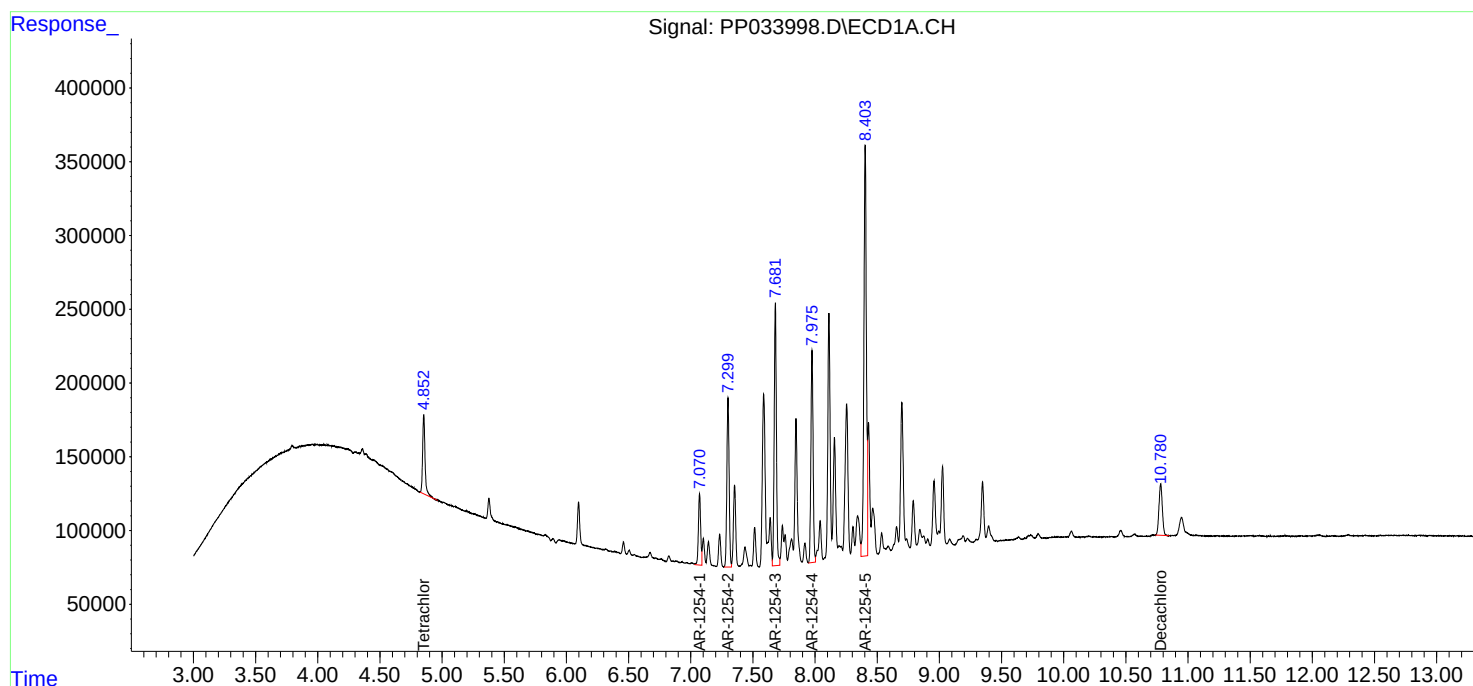


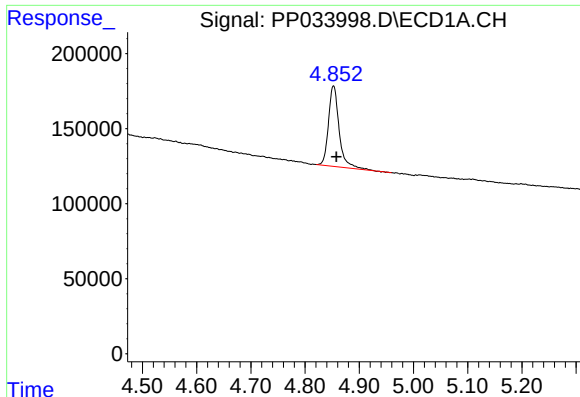

#1 Tetrachloro-m-xylene


R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 728531
Conc: 8.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6ADL

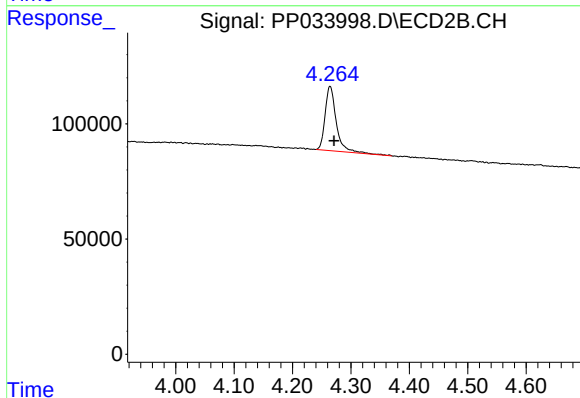


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 368037
Conc: 9.06 ng/ml

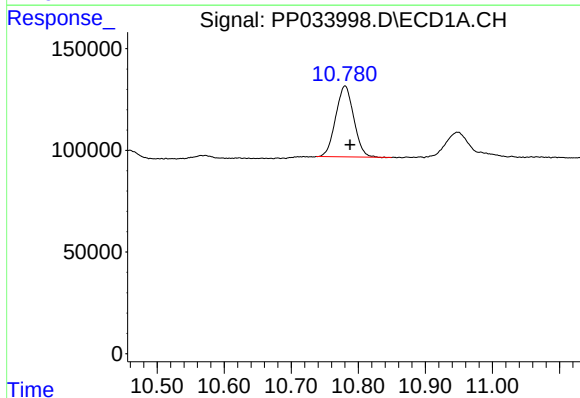


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.008 min
Response: 651156
Conc: 7.71 ng/ml

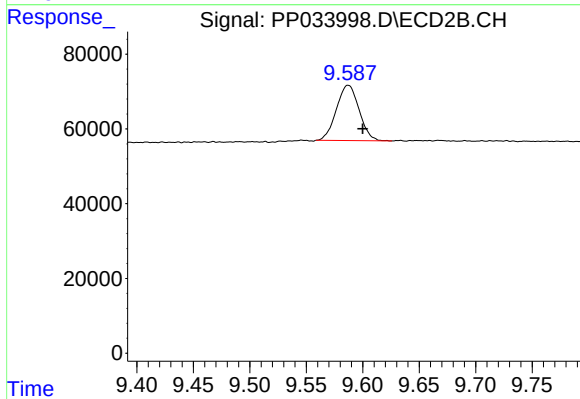

#2 Decachlorobiphenyl


R.T.: 9.587 min
Delta R.T.: -0.013 min
Response: 206744
Conc: 7.75 ng/ml

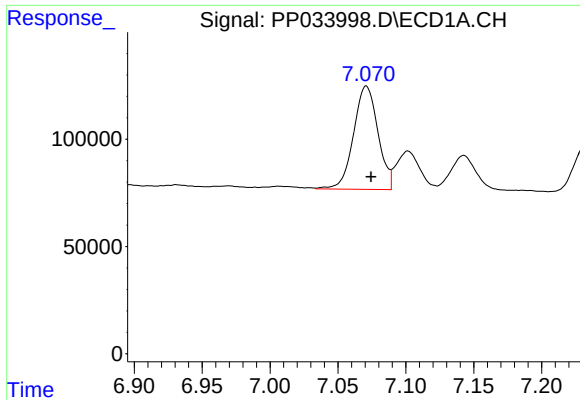

#26 AR-1254-1


R.T.: 7.071 min
Delta R.T.: -0.003 min
Response: 603285
Conc: 206.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6ADL

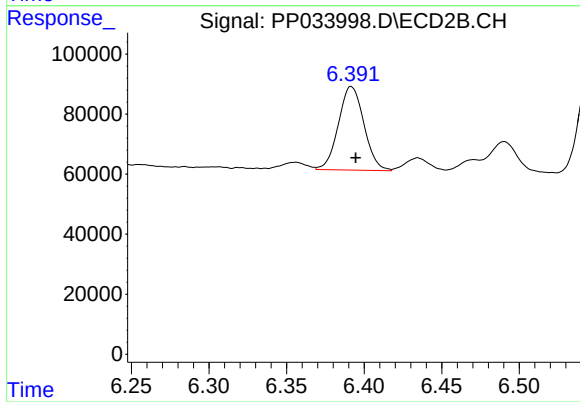


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 319590
Conc: 196.03 ng/ml

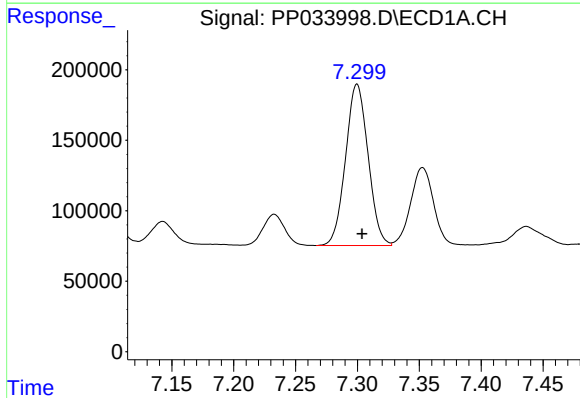


#27 AR-1254-2

R.T.: 7.300 min
Delta R.T.: -0.004 min
Response: 1453885
Conc: 319.74 ng/ml

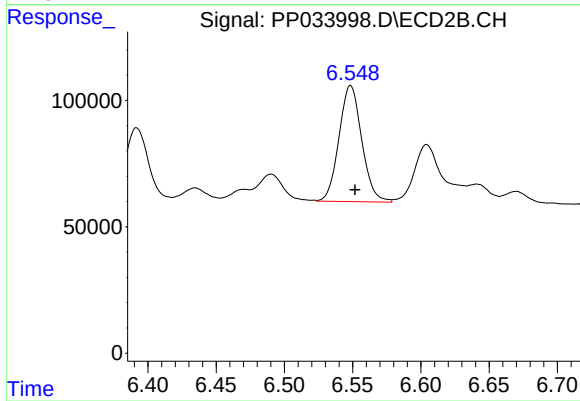

#27 AR-1254-2


R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 533782
Conc: 373.74 ng/ml

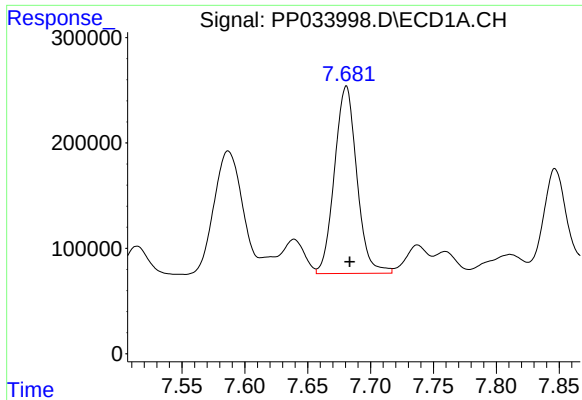

#28 AR-1254-3


R.T.: 7.681 min
Delta R.T.: -0.003 min
Response: 2199857
Conc: 444.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6ADL

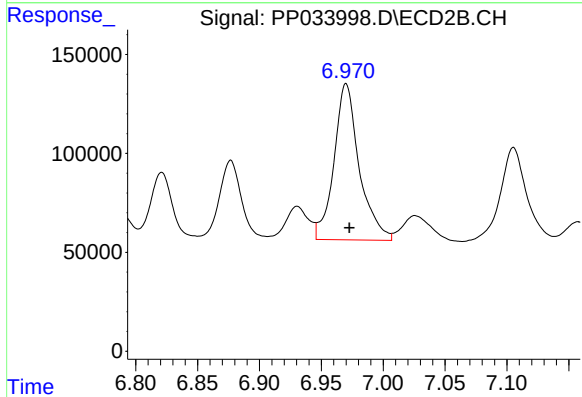


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 1121341
Conc: 489.92 ng/ml

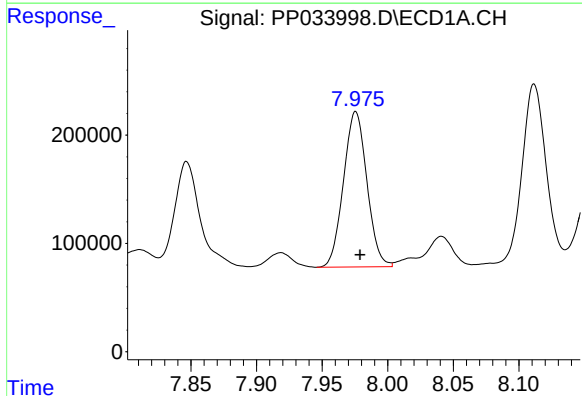


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 1784969
Conc: 520.39 ng/ml

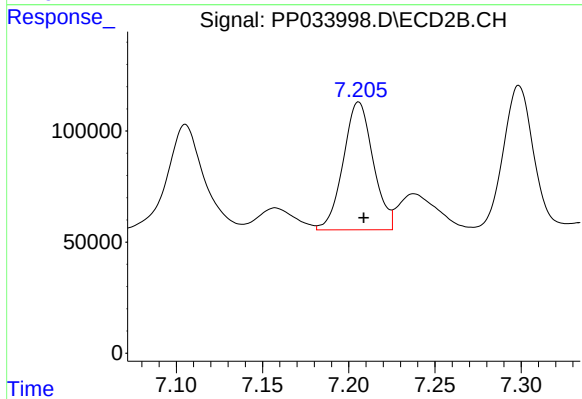

#29 AR-1254-4


R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 693723
Conc: 545.80 ng/ml

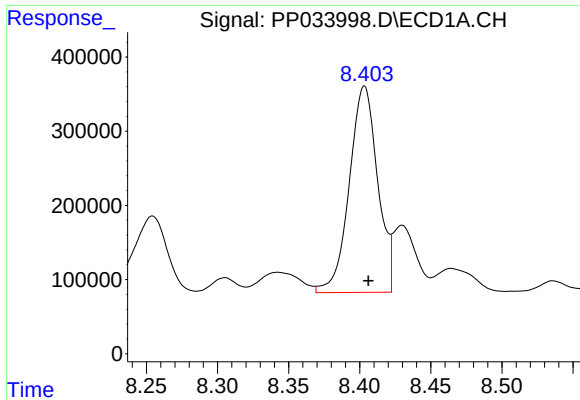

#30 AR-1254-5

R.T.: 8.403 min
Delta R.T.: -0.003 min
Response: 3865565
Conc: 982.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6ADL

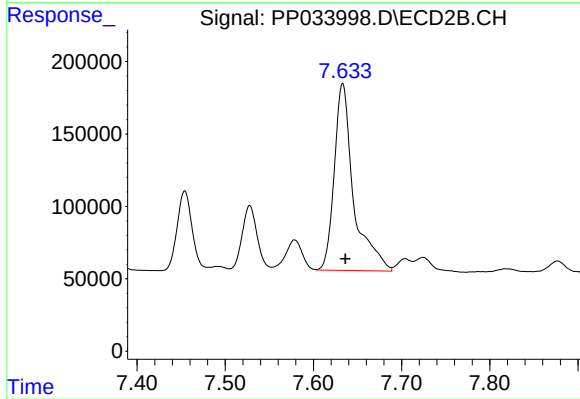

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 1967003
Conc: 1044.32 ng/ml