

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034004.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 14:23
 Operator : DD\AJ
 Sample : M1661-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-7A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 16:10:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.852	4.264	405914	200551	4.691	4.937
2)	SA Decachlor...	10.781	9.586	574663	188764	6.804	7.074
Target Compounds							
26)	L6 AR-1254-1	7.071	6.393	249981	131935	85.572	80.926
27)	L6 AR-1254-2	7.299	6.549	632622	251205	139.126	175.888 #
28)	L6 AR-1254-3	7.681	6.970	1012741	545276	204.833	238.236
29)	L6 AR-1254-4	7.976	7.206	763805	302087	222.681	237.672
30)	L6 AR-1254-5	8.404	7.634	2027372	1262067	515.064	670.058 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034004.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 14:23
Operator : DD\AJ
Sample : M1661-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
X127-7A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 16:10:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

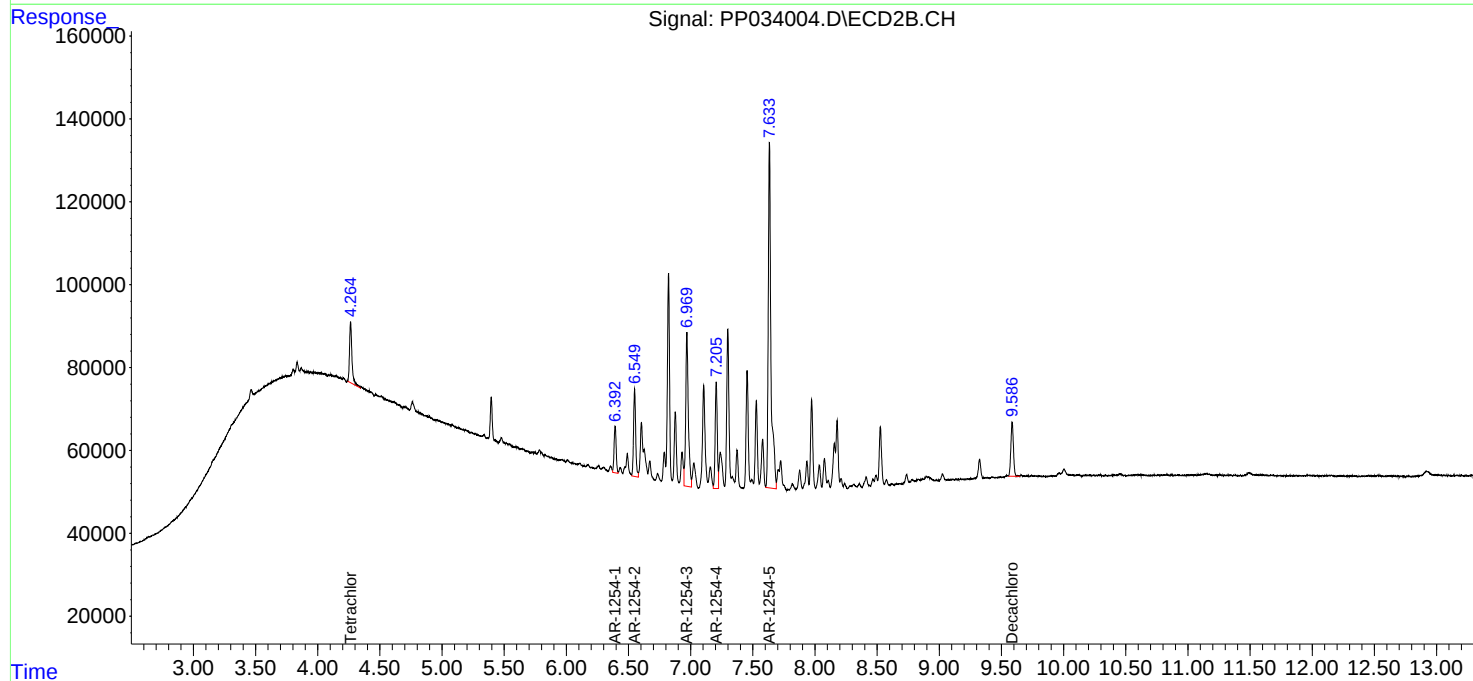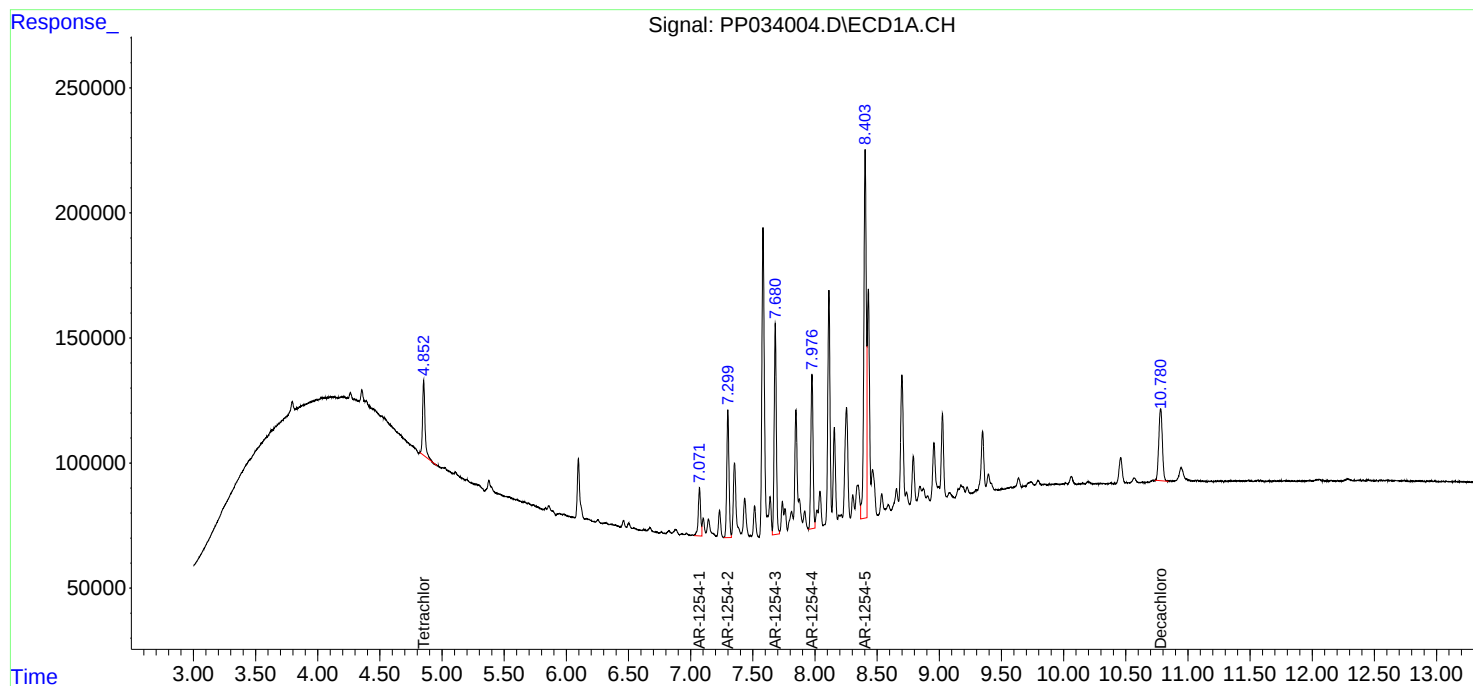


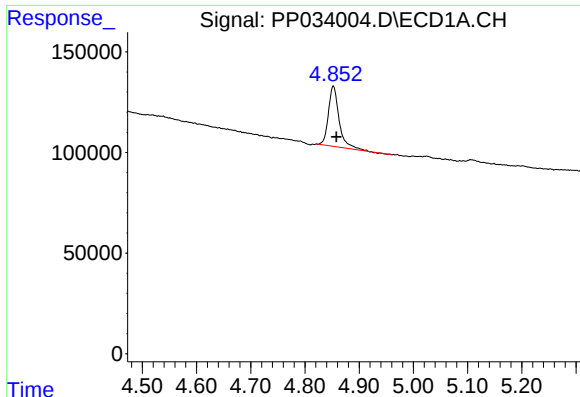

#1 Tetrachloro-m-xylene


R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 405914
Conc: 4.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-7A

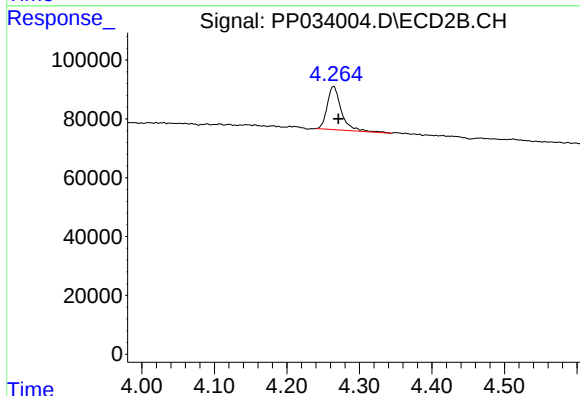


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 200551
Conc: 4.94 ng/ml

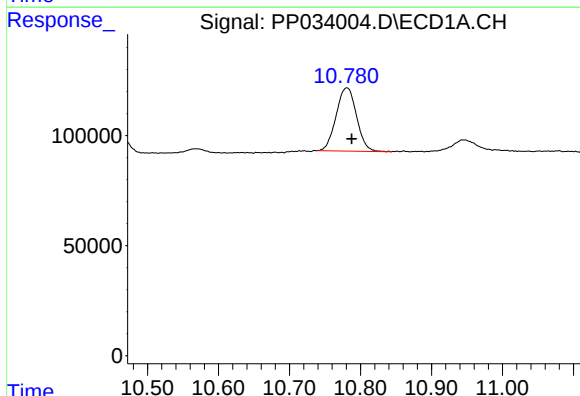


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 574663
Conc: 6.80 ng/ml

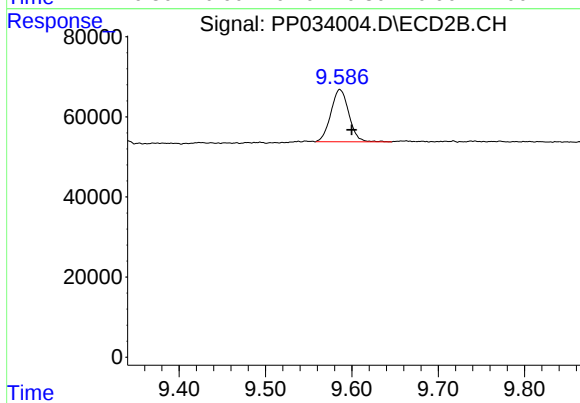

#2 Decachlorobiphenyl


R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 188764
Conc: 7.07 ng/ml

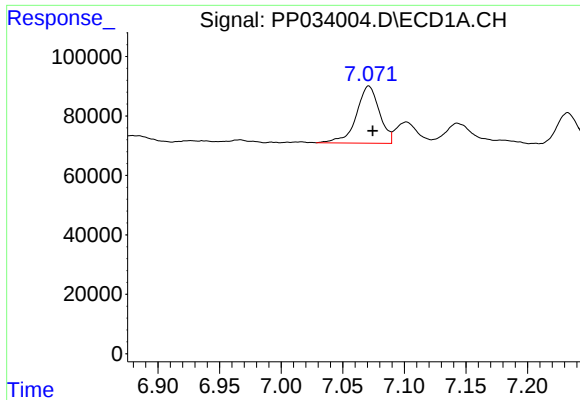

#26 AR-1254-1


R.T.: 7.071 min
Delta R.T.: -0.003 min
Response: 249981
Conc: 85.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-7A

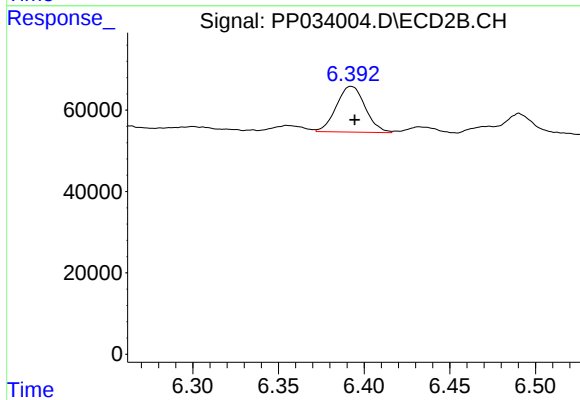


#26 AR-1254-1

R.T.: 6.393 min
Delta R.T.: -0.002 min
Response: 131935
Conc: 80.93 ng/ml

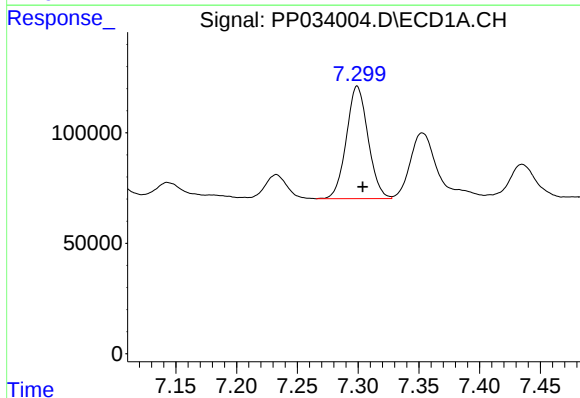


#27 AR-1254-2

R.T.: 7.299 min
Delta R.T.: -0.005 min
Response: 632622
Conc: 139.13 ng/ml

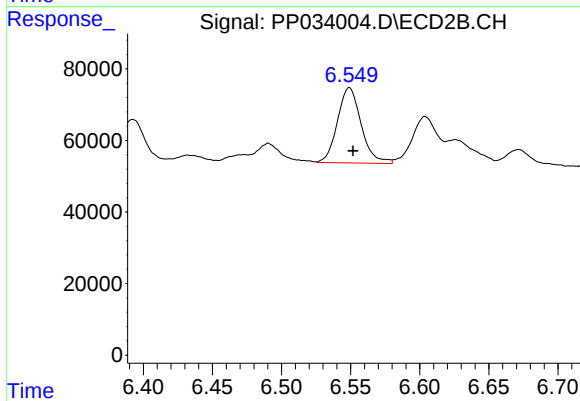

#27 AR-1254-2


R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 251205
Conc: 175.89 ng/ml

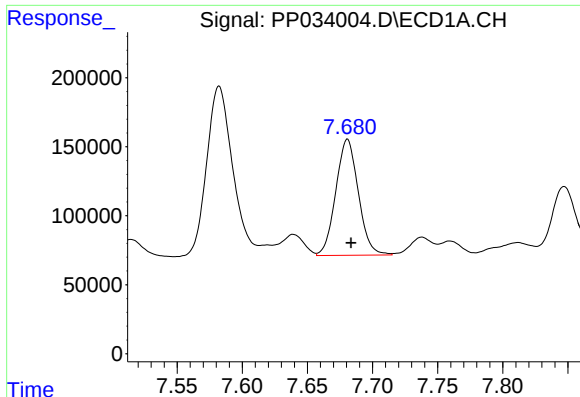

#28 AR-1254-3


R.T.: 7.681 min
Delta R.T.: -0.003 min
Response: 1012741
Conc: 204.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-7A

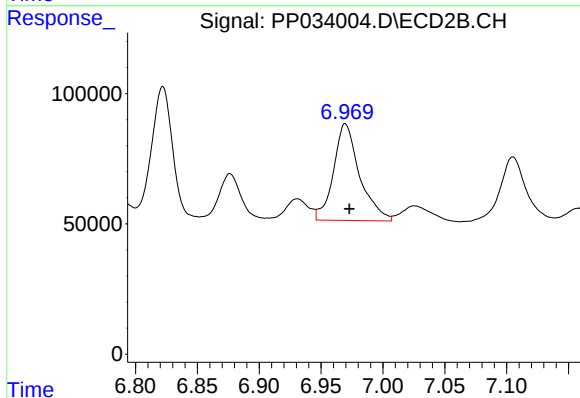


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 545276
Conc: 238.24 ng/ml

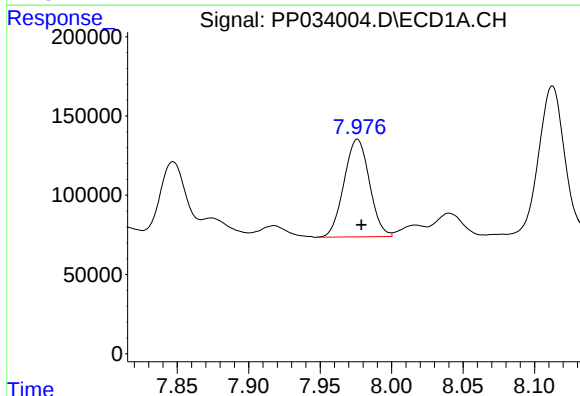


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 763805
Conc: 222.68 ng/ml

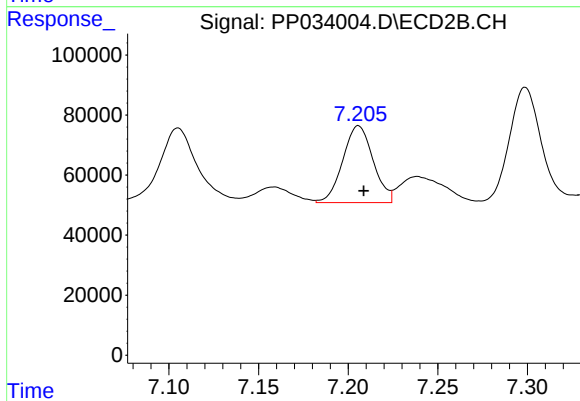

#29 AR-1254-4


R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 302087
Conc: 237.67 ng/ml

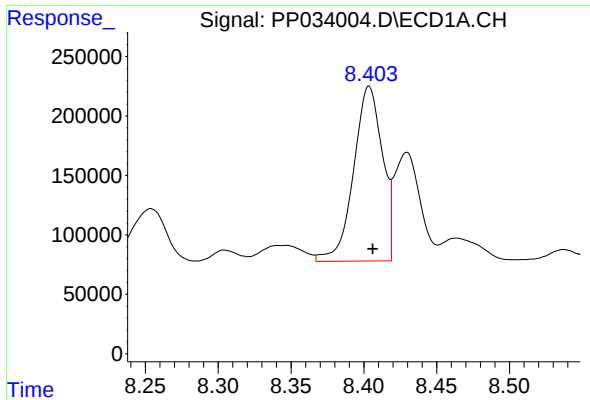

#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.003 min
Response: 2027372
Conc: 515.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-7A

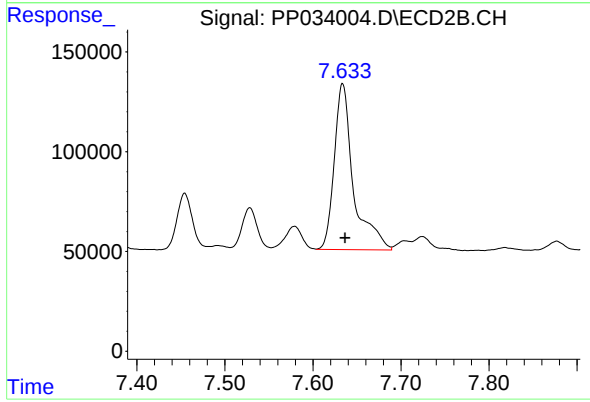

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.003 min
Response: 1262067
Conc: 670.06 ng/ml