

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034009.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 15:47
 Operator : DD\AJ
 Sample : M1661-18 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-12A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:44:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.265	397401	205820	4.593	5.066
2) SA Decachlor...	10.781	9.586	379787	127405	4.497	4.774
Target Compounds						
26) L6 AR-1254-1	7.072	6.392	123251	66215	42.191m	40.614
27) L6 AR-1254-2	7.301	6.549	395123	163987	86.895	114.820 #
28) L6 AR-1254-3	7.681	6.970	689158	398344	139.386	174.040
29) L6 AR-1254-4	7.976	7.206	632553	257064	184.416	202.250
30) L6 AR-1254-5	8.405	7.633	2016882	1208954	512.399	641.859 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034009.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 15:47
Operator : DD\AJ
Sample : M1661-18 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-12A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:44:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

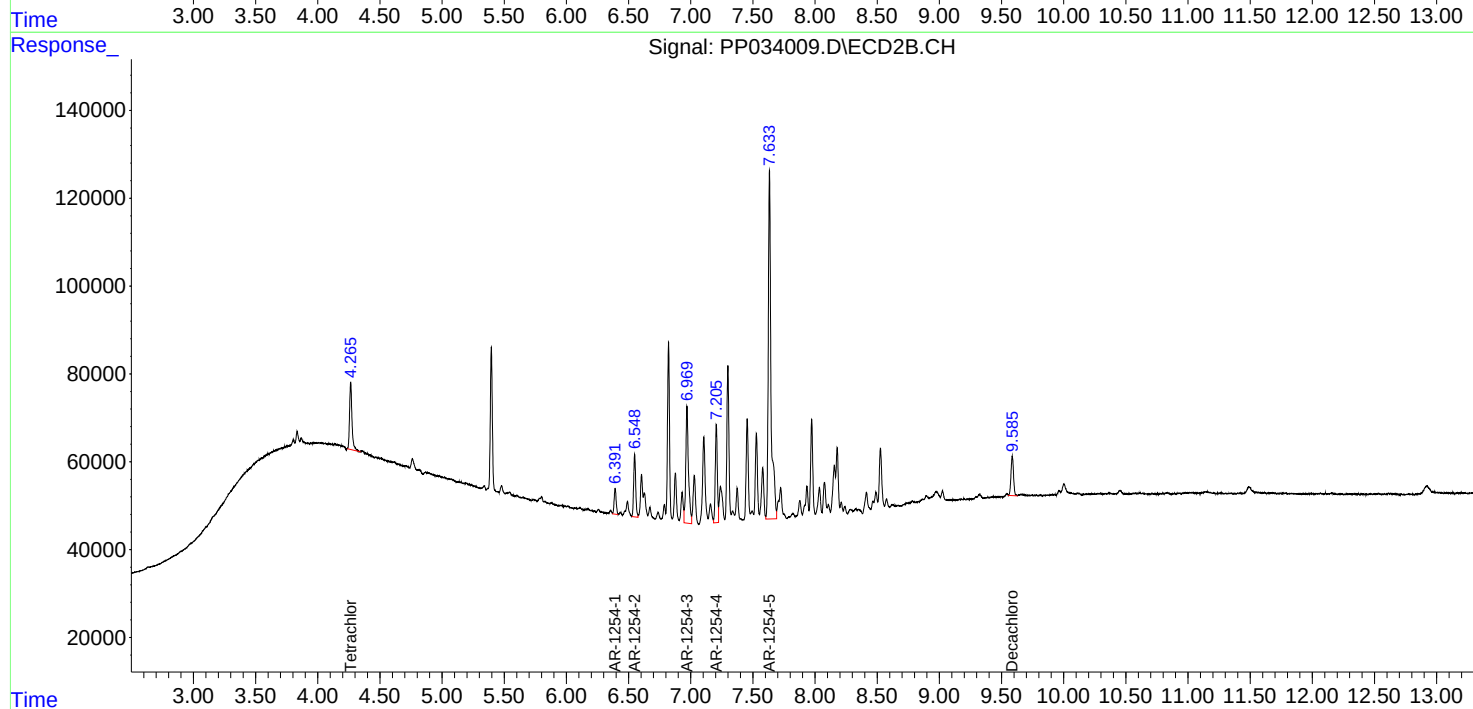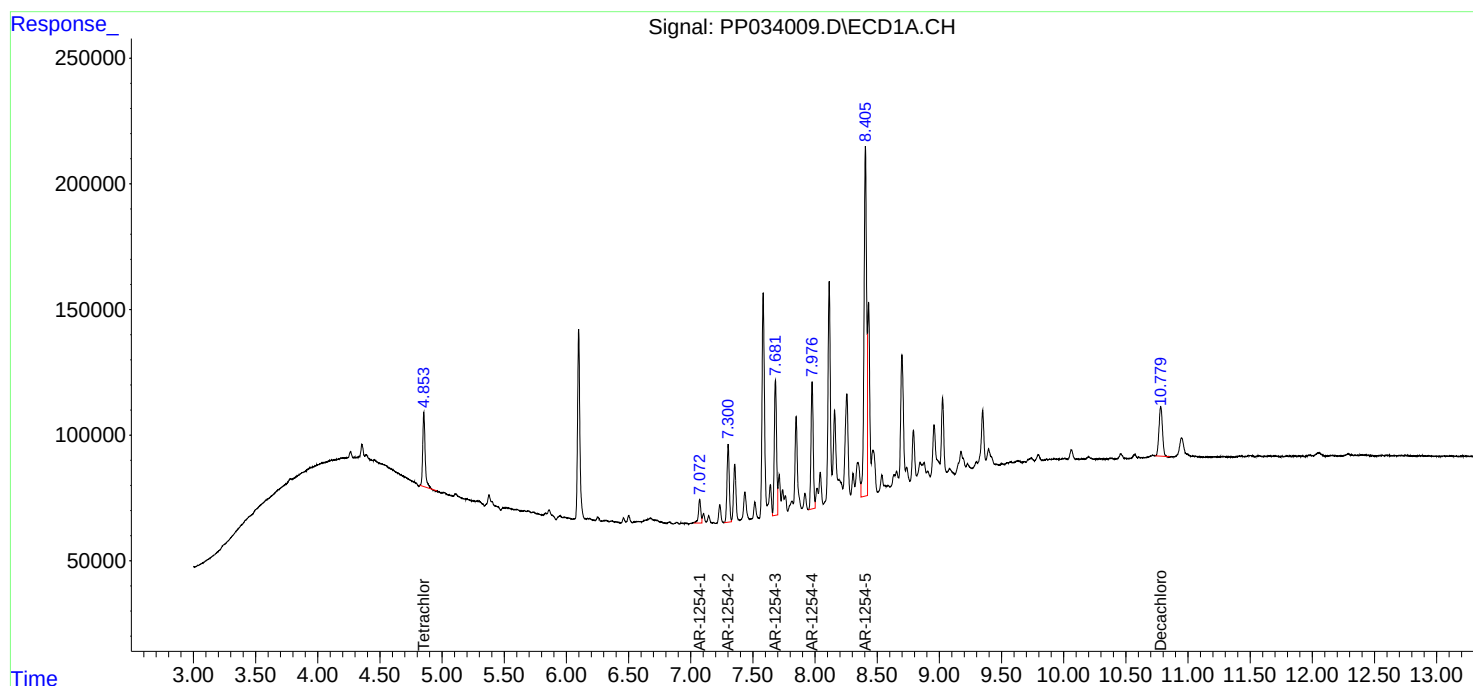

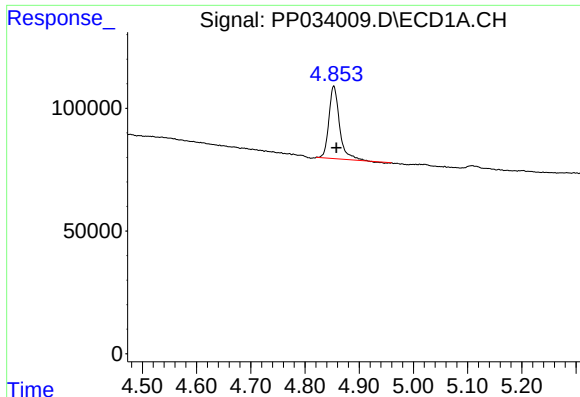


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 397401
Conc: 4.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-12A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:17 AM

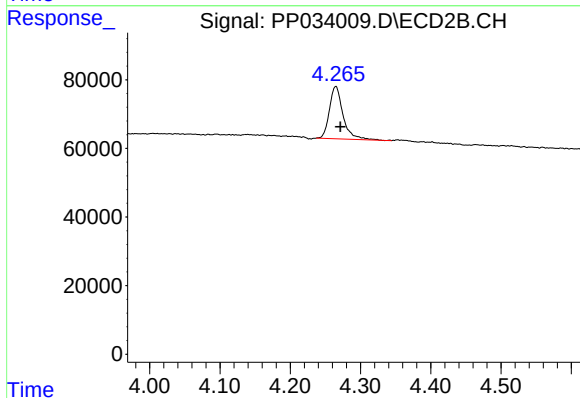


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 205820
Conc: 5.07 ng/ml

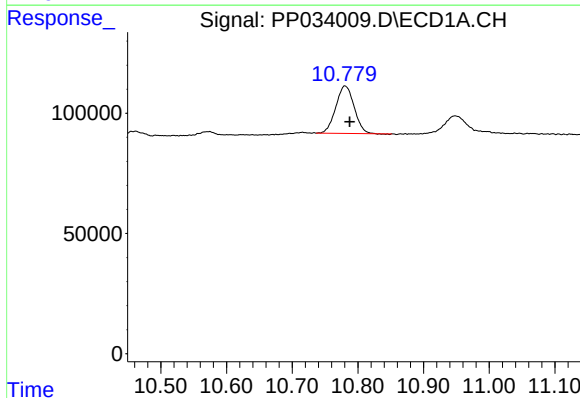


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 379787
Conc: 4.50 ng/ml

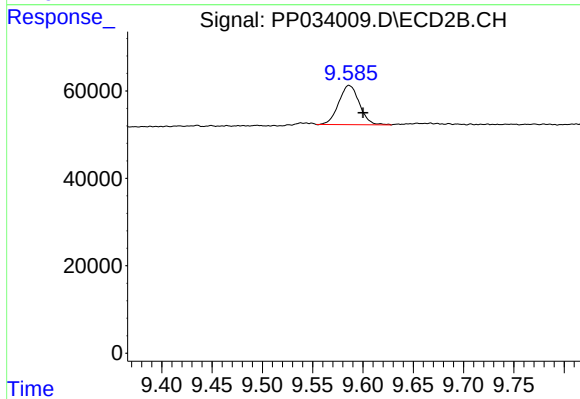

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 127405
Conc: 4.77 ng/ml

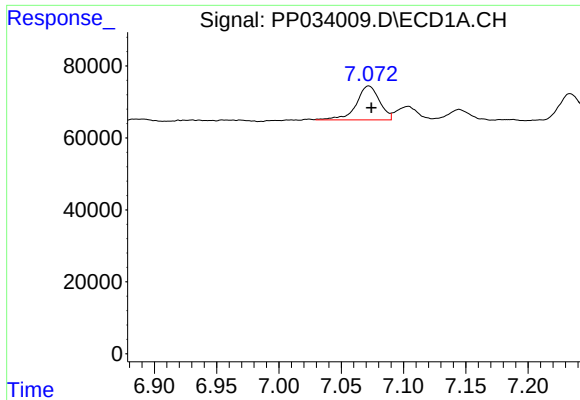


#26 AR-1254-1

R.T.: 7.072 min
Delta R.T.: -0.003 min
Response: 123251
Conc: 42.19 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-12A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:17 AM

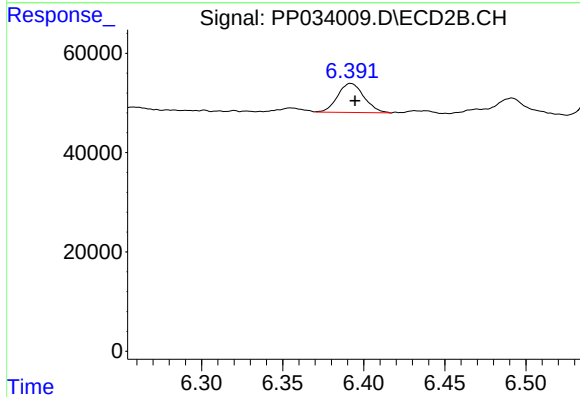


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 66215
Conc: 40.61 ng/ml

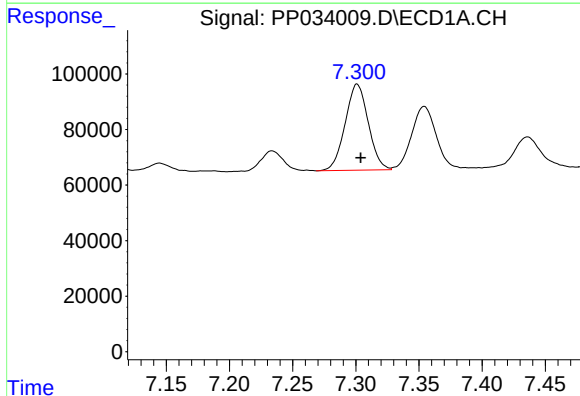


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.003 min
Response: 395123
Conc: 86.90 ng/ml

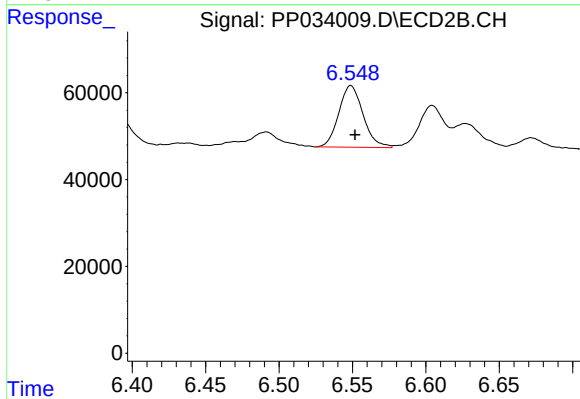

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 163987
Conc: 114.82 ng/ml

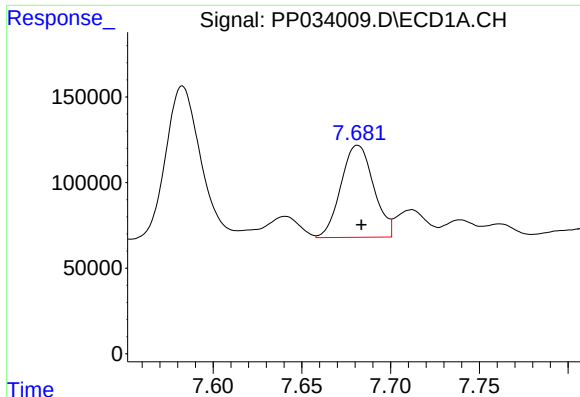


#28 AR-1254-3

R.T.: 7.681 min
Delta R.T.: -0.002 min
Response: 689158
Conc: 139.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-12A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:17 AM

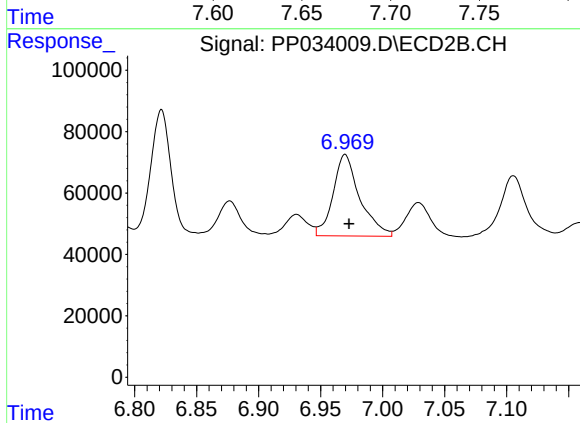


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 398344
Conc: 174.04 ng/ml

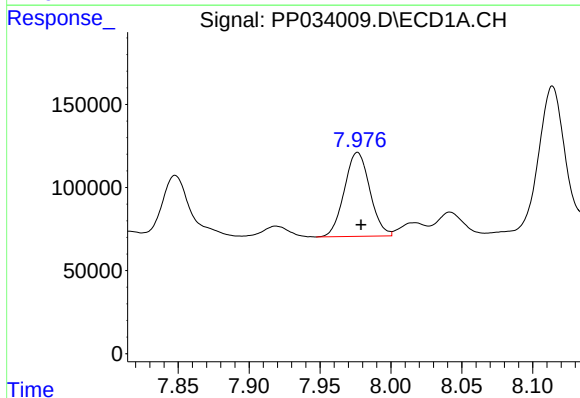


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 632553
Conc: 184.42 ng/ml

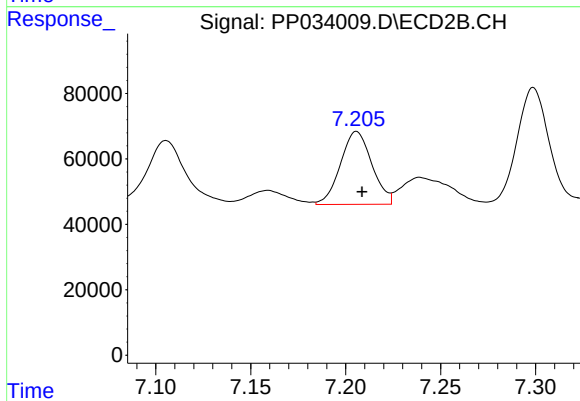

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 257064
Conc: 202.25 ng/ml

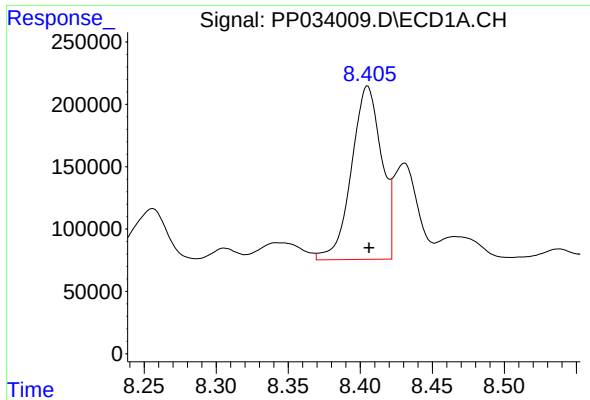


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.001 min
Response: 2016882
Conc: 512.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-12A

Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:17 AM

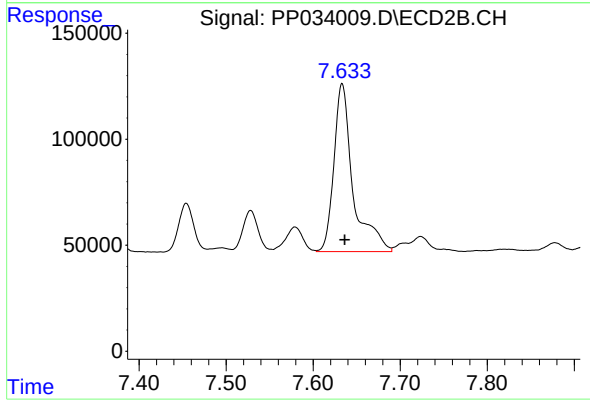

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 1208954
Conc: 641.86 ng/ml