

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034010.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 16:04
 Operator : DD\AJ
 Sample : M1662-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-13A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:45:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.264	444455	213357	5.137	5.252
2) SA Decachlor...	10.782	9.587	412435	134372	4.884	5.035
Target Compounds						
26) L6 AR-1254-1	7.071	6.392	124118	73682	42.487m	45.195
27) L6 AR-1254-2	7.301	6.549	210835	69441	46.367	48.621
28) L6 AR-1254-3	7.681	6.970	621855	343729	125.774	150.178
29) L6 AR-1254-4	7.975	7.206	289904	112979	84.519	88.888
30) L6 AR-1254-5	8.404	7.633	1263957	1121262	321.115	595.301 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 16:04
Operator : DD\AJ
Sample : M1662-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
Client Sampled :
X127-13A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:45:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

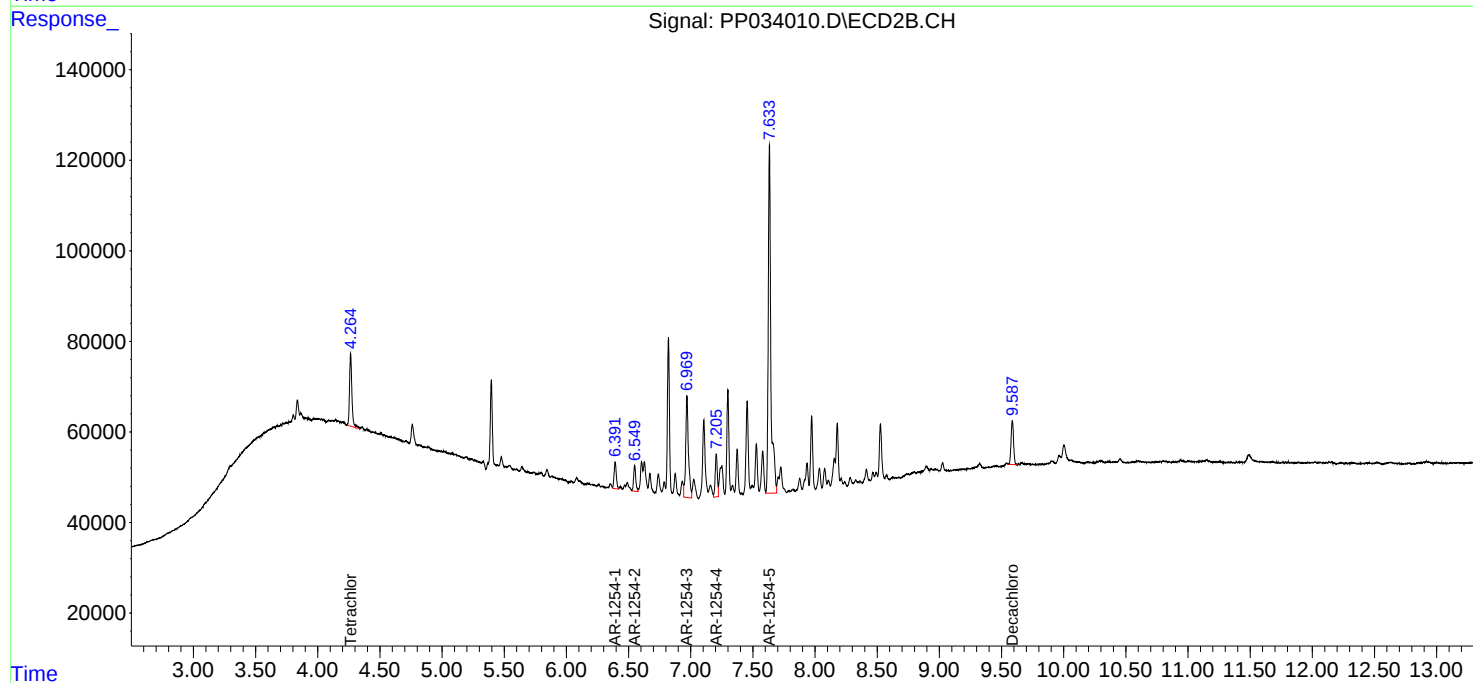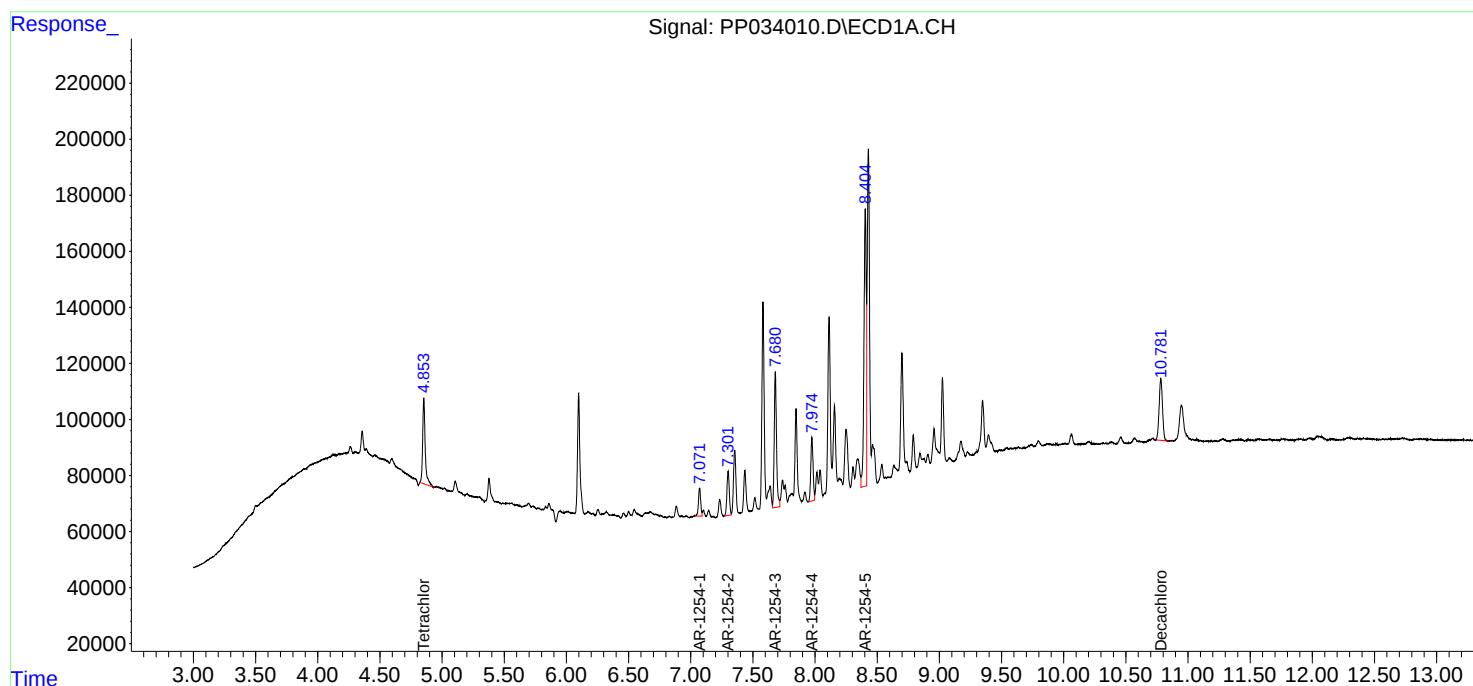

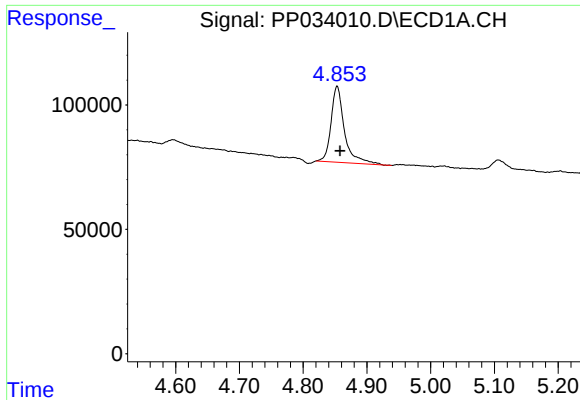


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 444455
Conc: 5.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-13A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:19 AM

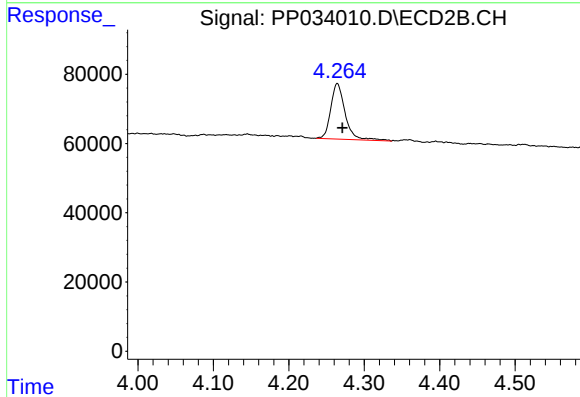


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 213357
Conc: 5.25 ng/ml

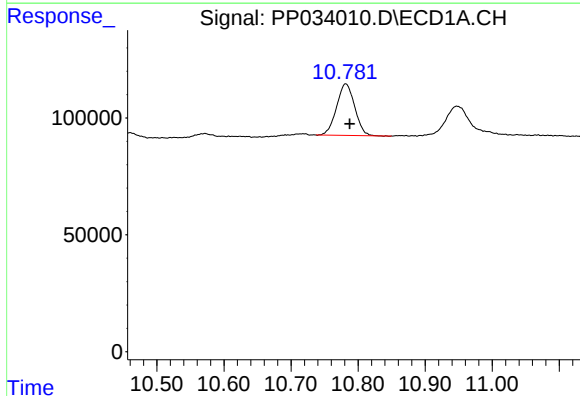


#2 Decachlorobiphenyl

R.T.: 10.782 min
Delta R.T.: -0.006 min
Response: 412435
Conc: 4.88 ng/ml

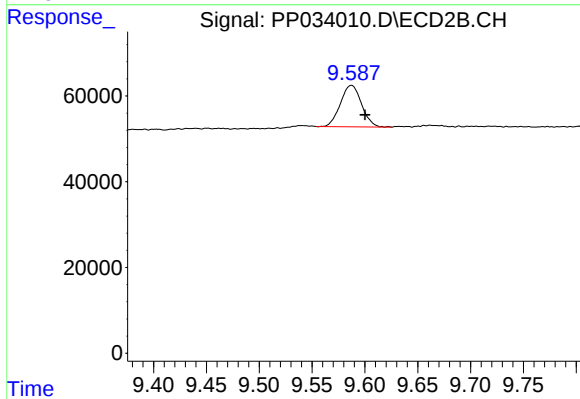

#2 Decachlorobiphenyl

R.T.: 9.587 min
Delta R.T.: -0.013 min
Response: 134372
Conc: 5.04 ng/ml

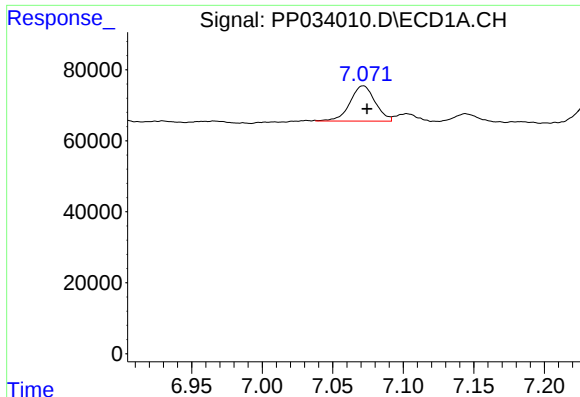


#26 AR-1254-1

R.T.: 7.071 min
Delta R.T.: -0.003 min
Response: 124118
Conc: 42.49 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-13A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:19 AM

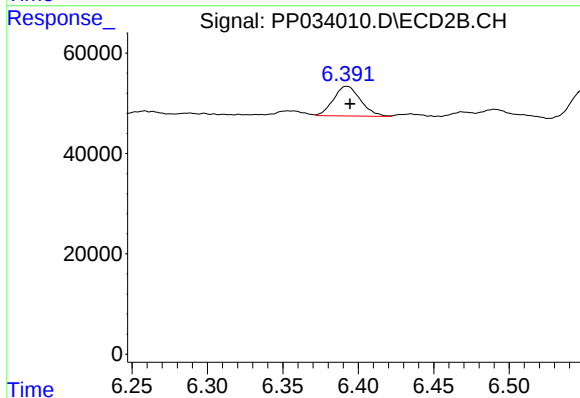


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.002 min
Response: 73682
Conc: 45.20 ng/ml

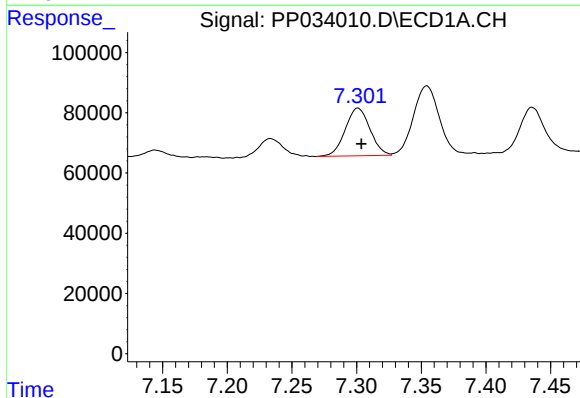


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.003 min
Response: 210835
Conc: 46.37 ng/ml

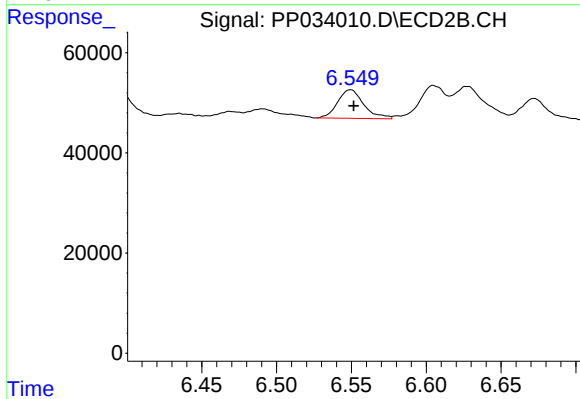

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.002 min
Response: 69441
Conc: 48.62 ng/ml

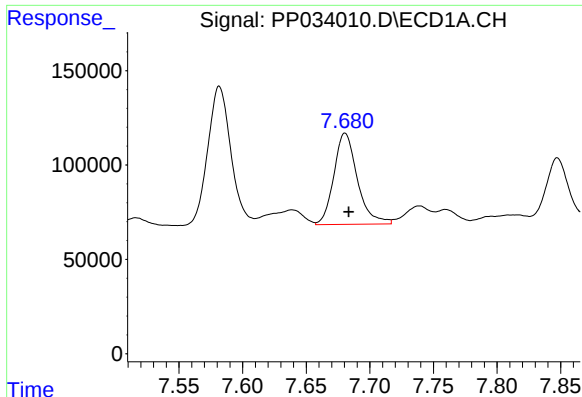


#28 AR-1254-3

R.T.: 7.681 min
Delta R.T.: -0.003 min
Response: 621855
Conc: 125.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-13A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:19 AM

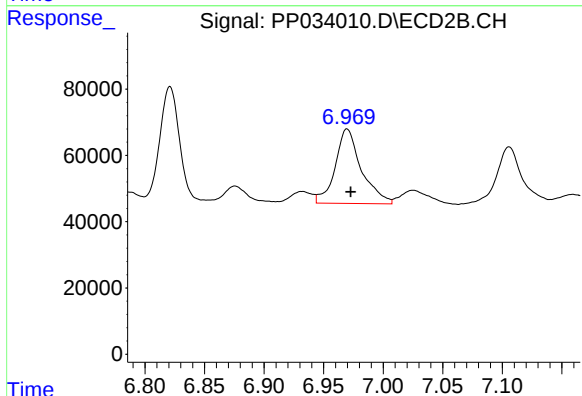


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 343729
Conc: 150.18 ng/ml

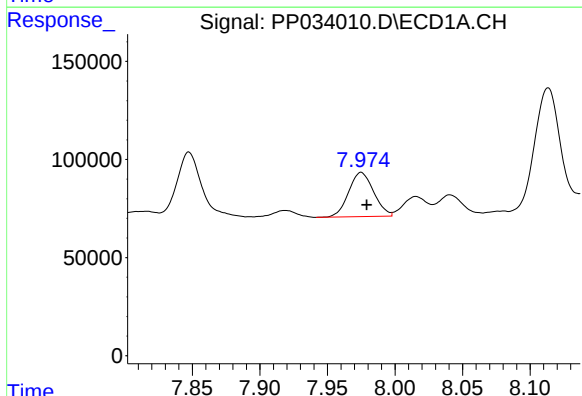


#29 AR-1254-4

R.T.: 7.975 min
Delta R.T.: -0.004 min
Response: 289904
Conc: 84.52 ng/ml

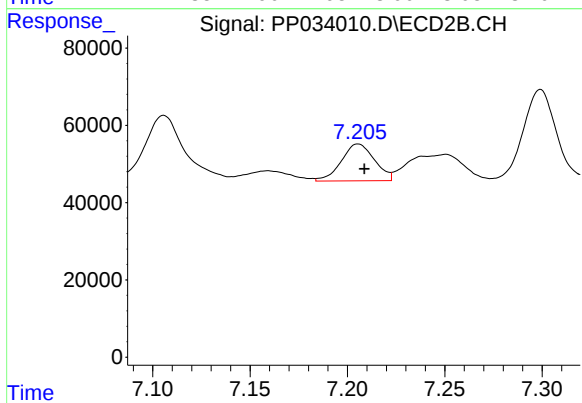

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 112979
Conc: 88.89 ng/ml

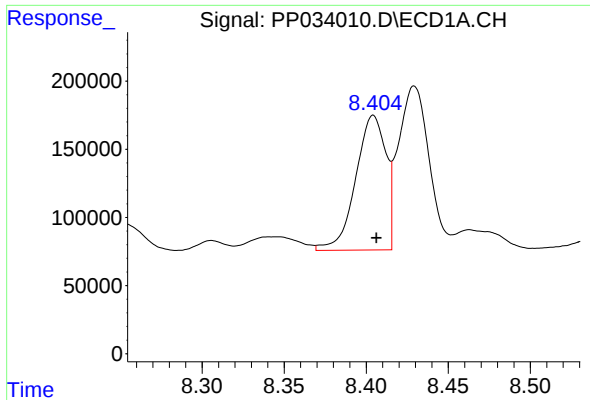


#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 1263957
Conc: 321.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-13A

Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:19 AM

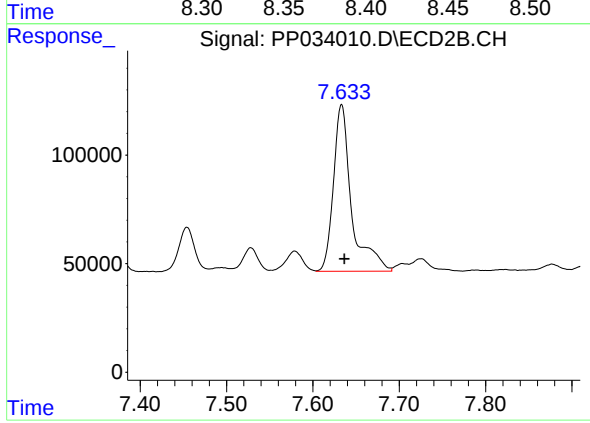

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 1121262
Conc: 595.30 ng/ml