

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 19:26
 Operator : DD\AJ
 Sample : M1663-01 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-19A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:49:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.265	411298	212703	4.754	5.236
2) SA Decachlor...	10.781	9.586	340804	118363	4.035	4.436

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 19:26
Operator : DD\AJ
Sample : M1663-01 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-19A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:49:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

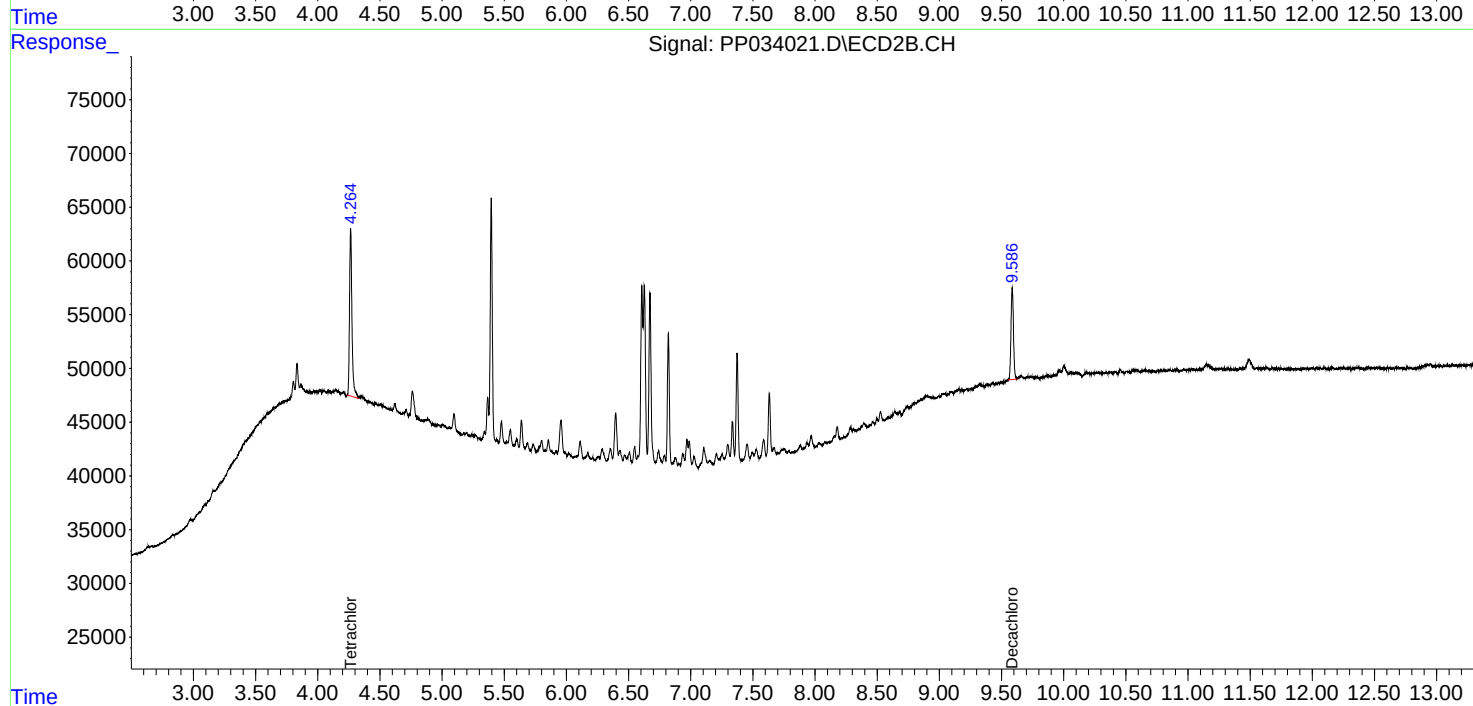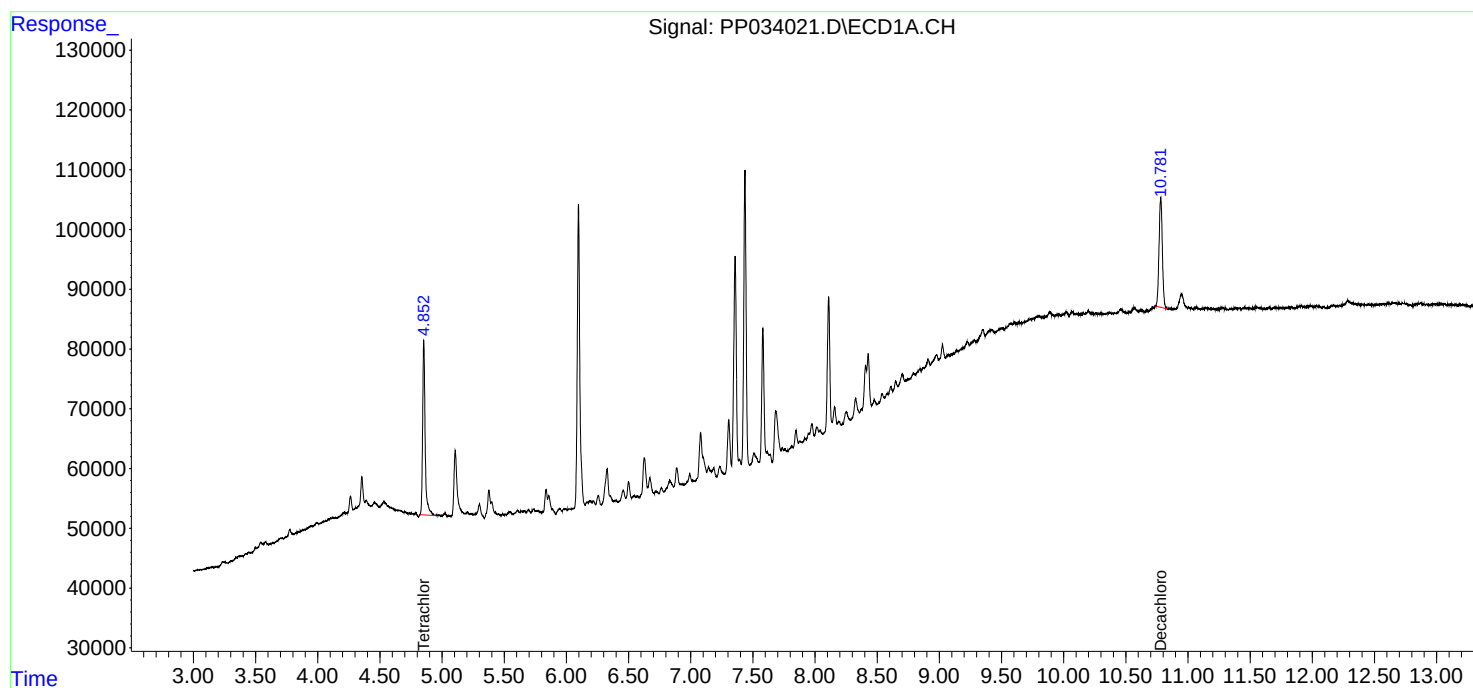

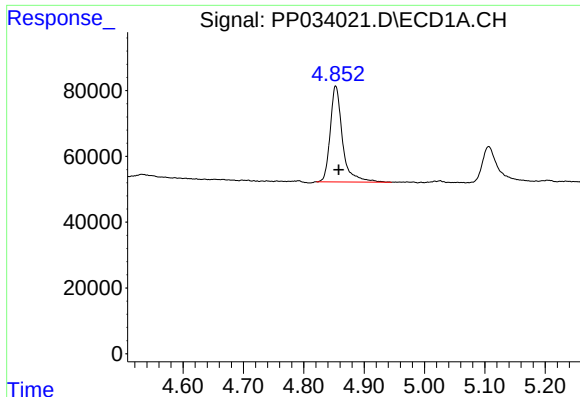


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 411298
Conc: 4.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-19A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:29 AM

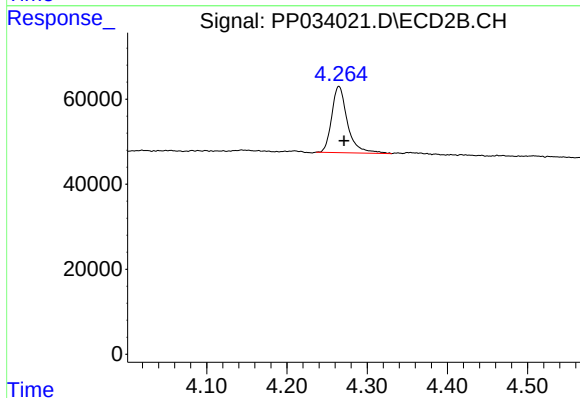


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 212703
Conc: 5.24 ng/ml

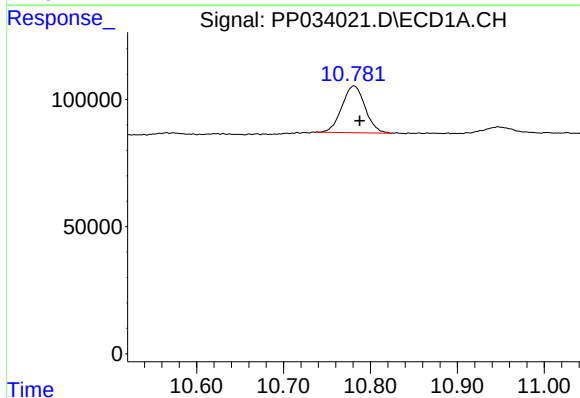

#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 340804
Conc: 4.04 ng/ml

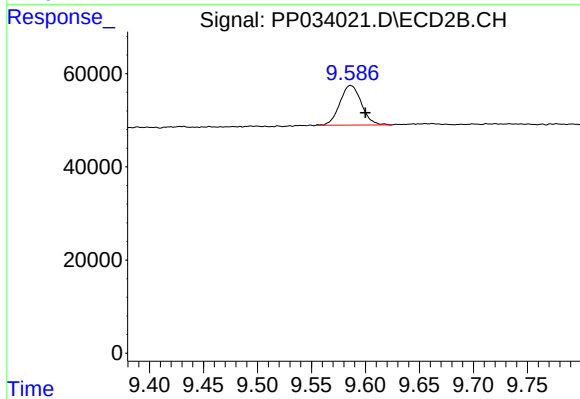

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 118363
Conc: 4.44 ng/ml