

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 20:17
 Operator : DD\AJ
 Sample : M1663-12 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-22A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:50:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.854	4.264	427346	226627	4.939	5.578
2)	SA Decachlor...	10.781	9.586	361443	128678	4.280	4.822
Target Compounds							
26)	L6 AR-1254-1	7.077	6.395	160175	78057	54.830m	47.879
27)	L6 AR-1254-2	7.303	6.548	218218	59729	47.990	41.821m
28)	L6 AR-1254-3	7.682	6.969	353318	159134	71.461	69.527
29)	L6 AR-1254-4	7.976	7.206	183176	75280	53.403	59.227
30)	L6 AR-1254-5	8.404	7.633	516438	422312	131.204	224.214 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 20:17
Operator : DD\AJ
Sample : M1663-12 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:50:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

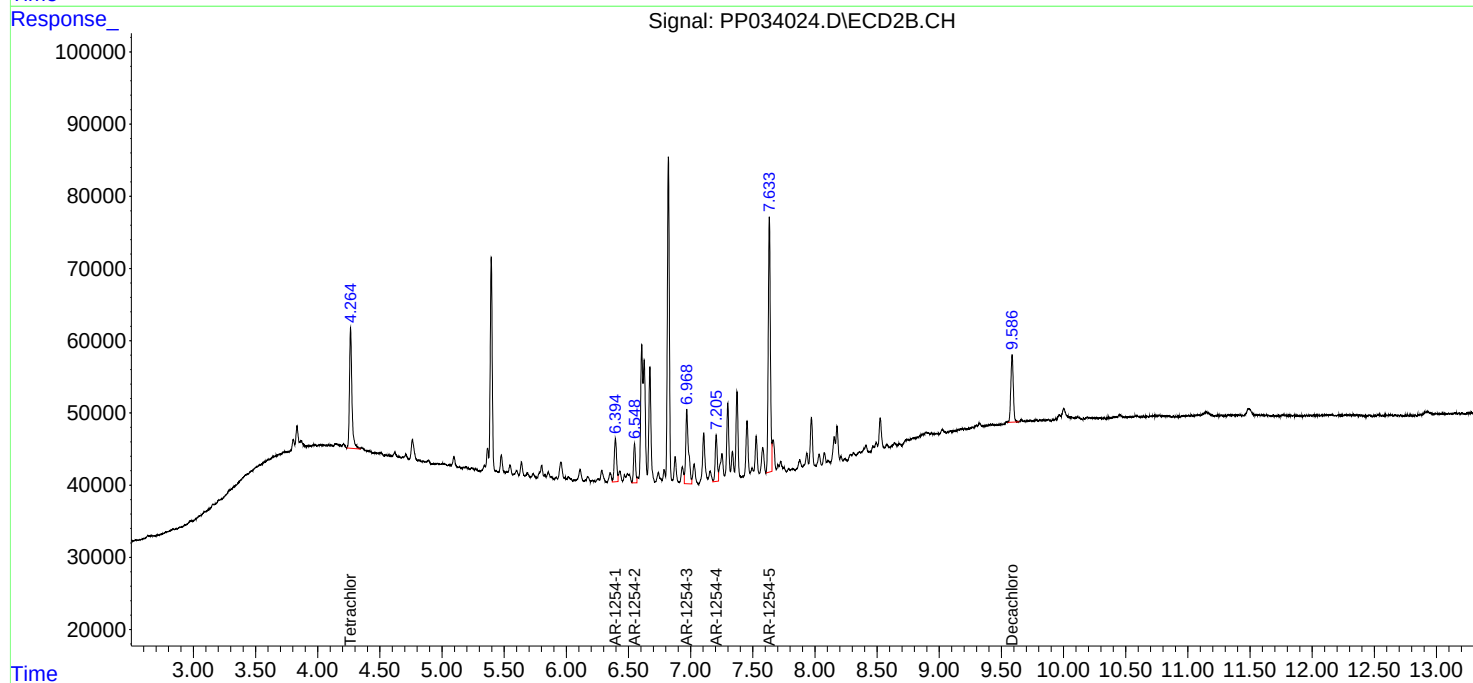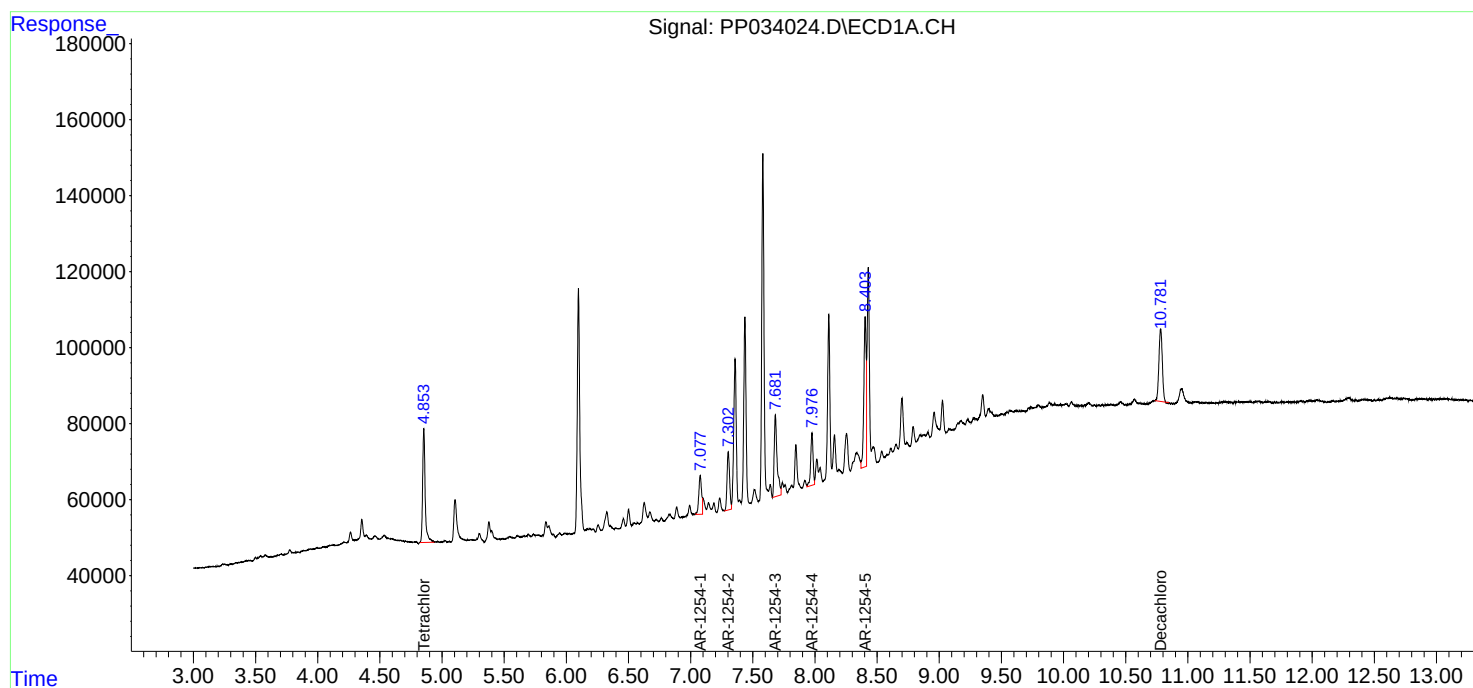

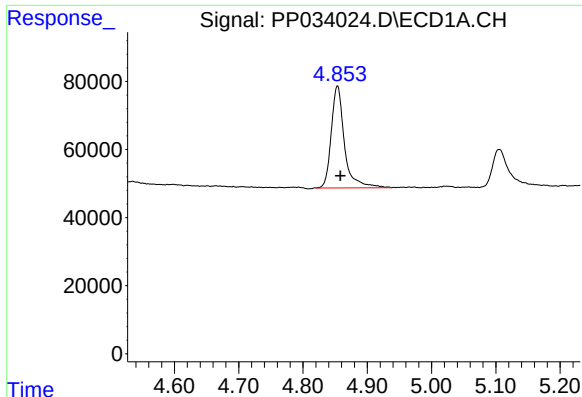


#1 Tetrachloro-m-xylene

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 427346
Conc: 4.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:33 AM

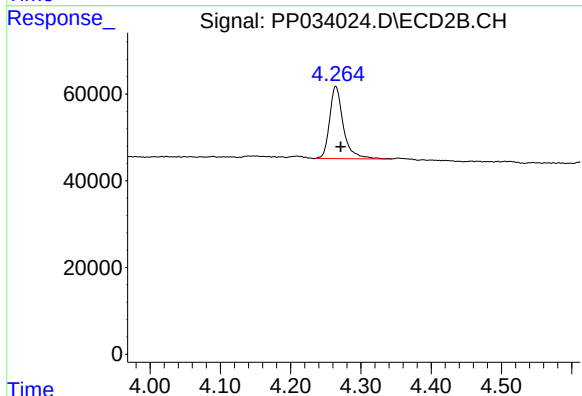


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 226627
Conc: 5.58 ng/ml

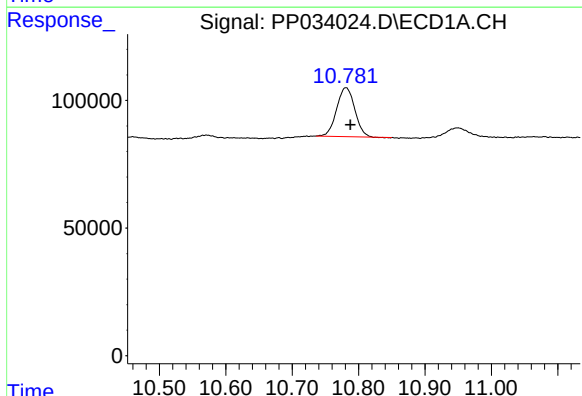


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 361443
Conc: 4.28 ng/ml

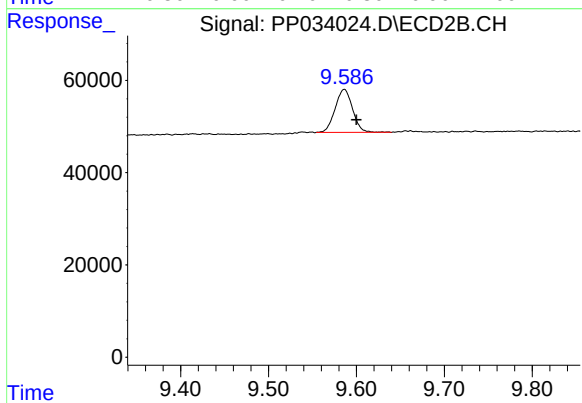

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 128678
Conc: 4.82 ng/ml

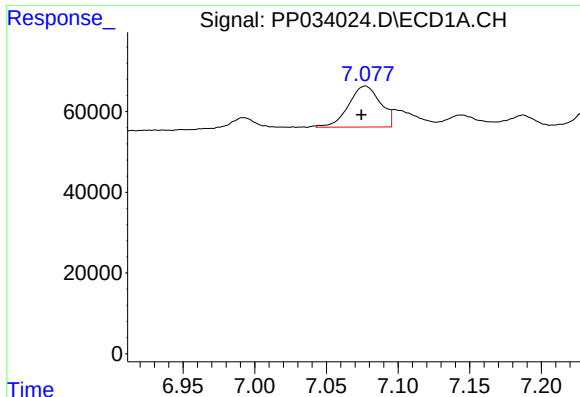


#26 AR-1254-1

R.T.: 7.077 min
Delta R.T.: 0.003 min
Response: 160175
Conc: 54.83 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:33 AM

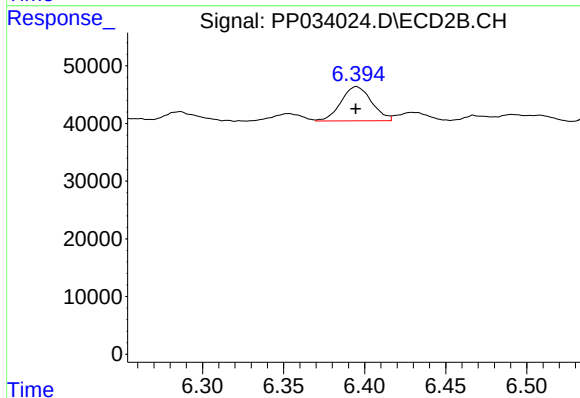


#26 AR-1254-1

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 78057
Conc: 47.88 ng/ml

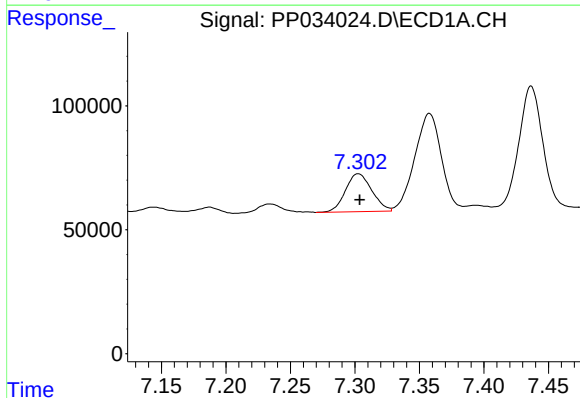


#27 AR-1254-2

R.T.: 7.303 min
Delta R.T.: -0.001 min
Response: 218218
Conc: 47.99 ng/ml

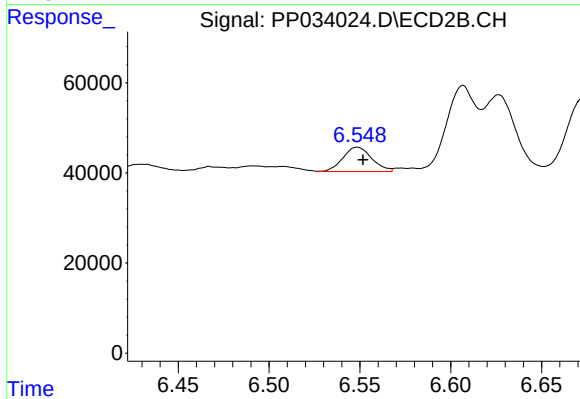

#27 AR-1254-2

R.T.: 6.548 min
Delta R.T.: -0.003 min
Response: 59729
Conc: 41.82 ng/ml m

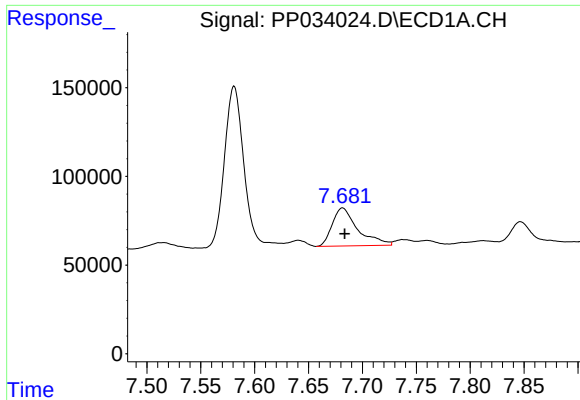


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.002 min
Response: 353318
Conc: 71.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:33 AM

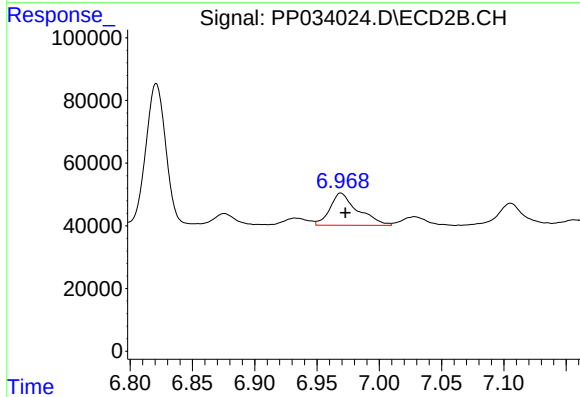


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: -0.004 min
Response: 159134
Conc: 69.53 ng/ml

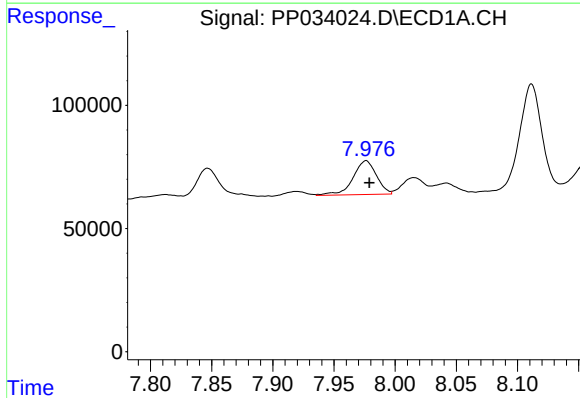


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 183176
Conc: 53.40 ng/ml

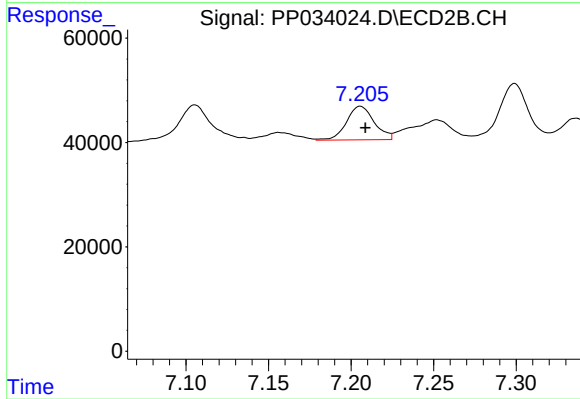

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 75280
Conc: 59.23 ng/ml

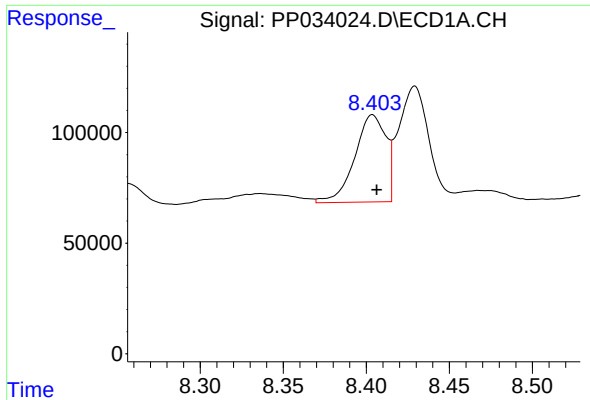


#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 516438
Conc: 131.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A

Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:33 AM

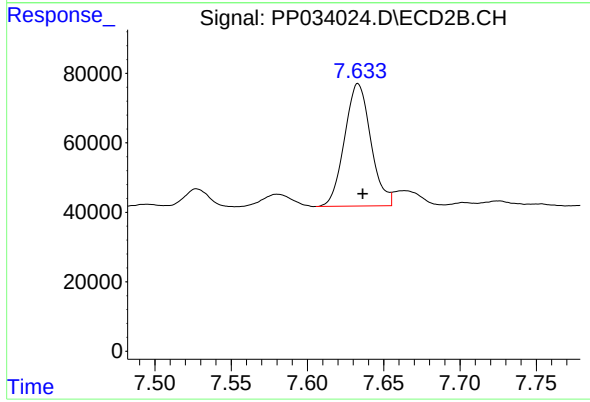

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 422312
Conc: 224.21 ng/ml