

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
 Data File : PP034025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 20:33
 Operator : DD\AJ
 Sample : M1663-15 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-23A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:17:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:50:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.852	4.264	436223	222043	5.042	5.466
2) SA Decachlor...	10.779	9.586	333480	117399	3.949	4.399
Target Compounds						
26) L6 AR-1254-1	7.076	6.394	140566	78376	48.118m	48.074
27) L6 AR-1254-2	7.303	6.549	209444	56571	46.061	39.610
28) L6 AR-1254-3	7.681	6.969	343918	167360	69.559	73.121
29) L6 AR-1254-4	7.975	7.205	186845	74299	54.473	58.456
30) L6 AR-1254-5	8.403	7.632	510382	446565	129.665	237.091 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031521\
Data File : PP034025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 20:33
Operator : DD\AJ
Sample : M1663-15 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:50:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

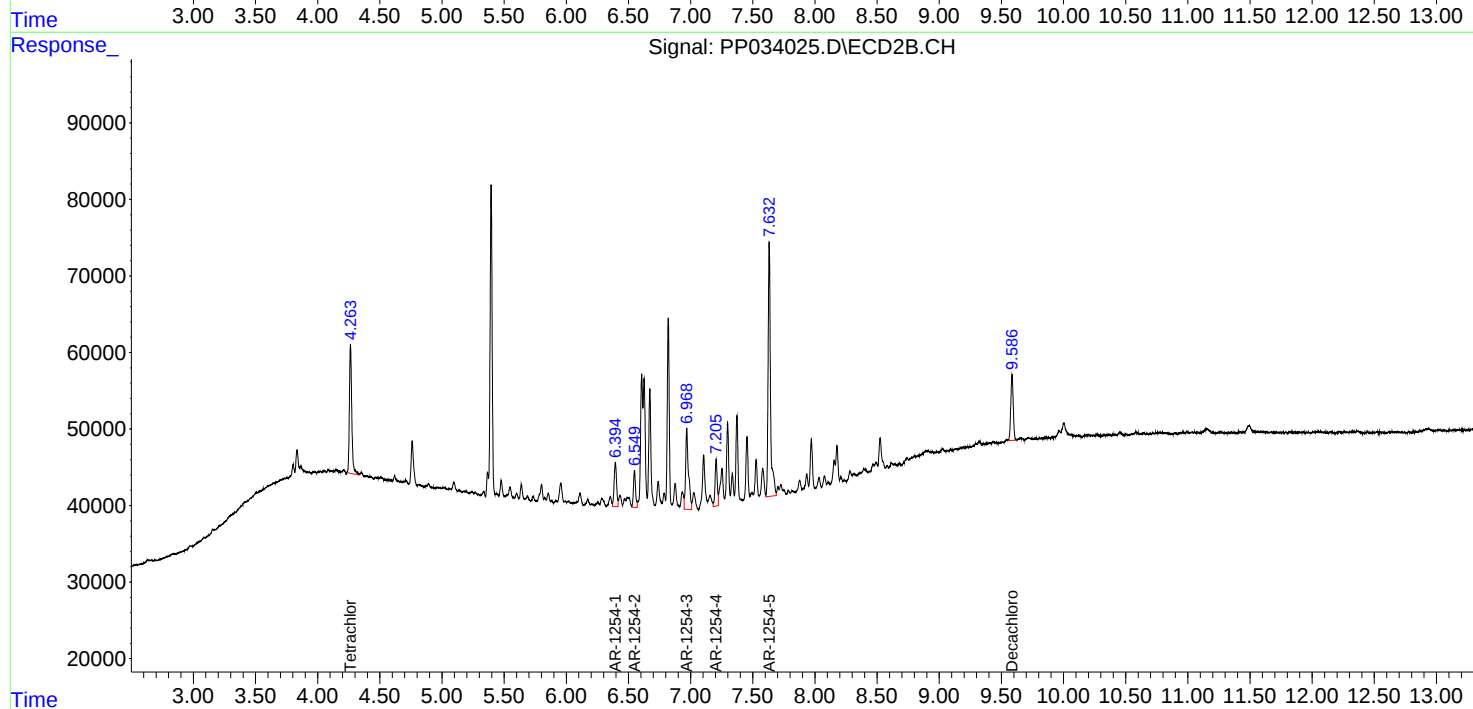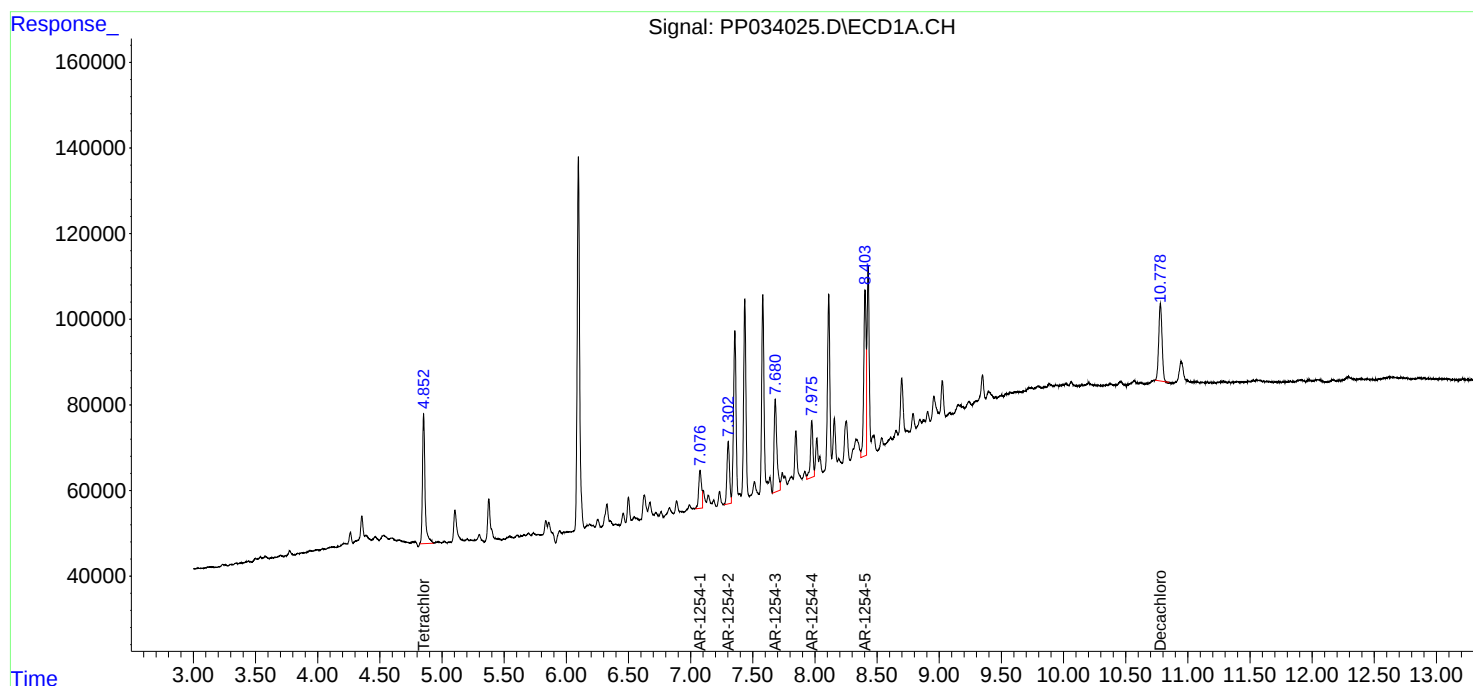

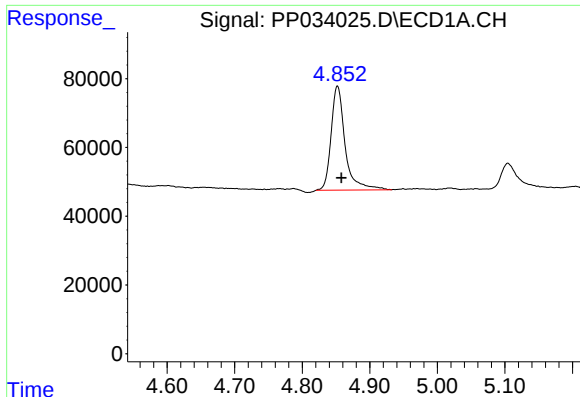


#1 Tetrachloro-m-xylene

R.T.: 4.852 min
Delta R.T.: -0.006 min
Response: 436223
Conc: 5.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:35 AM

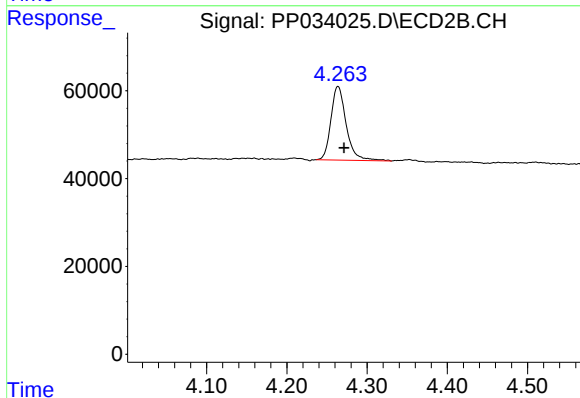


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.007 min
Response: 222043
Conc: 5.47 ng/ml

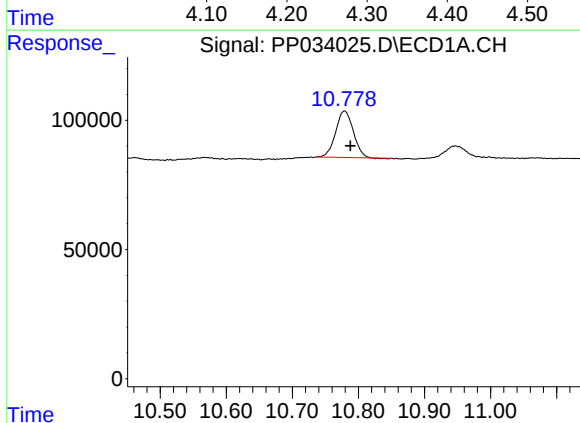


#2 Decachlorobiphenyl

R.T.: 10.779 min
Delta R.T.: -0.009 min
Response: 333480
Conc: 3.95 ng/ml

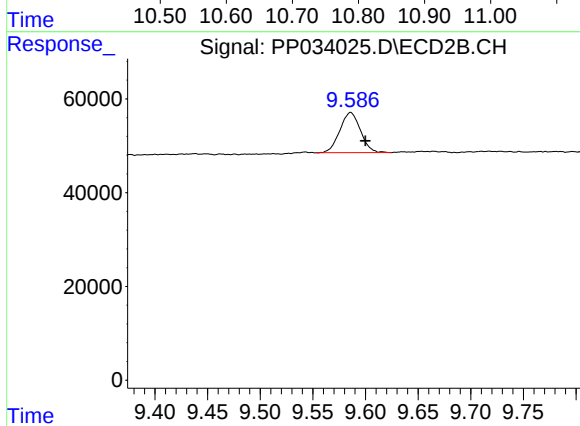

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.014 min
Response: 117399
Conc: 4.40 ng/ml

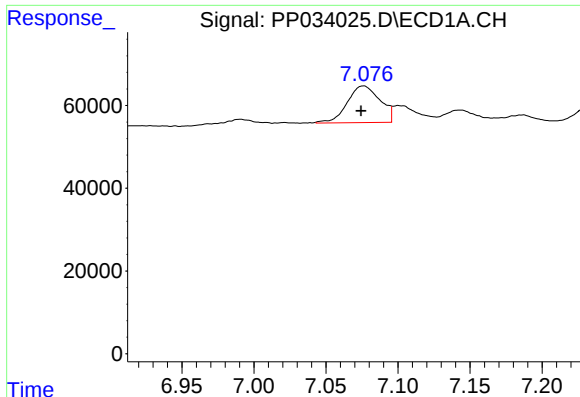


#26 AR-1254-1

R.T.: 7.076 min
Delta R.T.: 0.002 min
Response: 140566
Conc: 48.12 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:35 AM

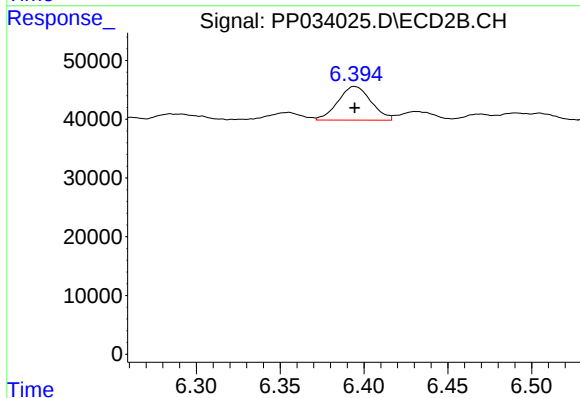


#26 AR-1254-1

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 78376
Conc: 48.07 ng/ml

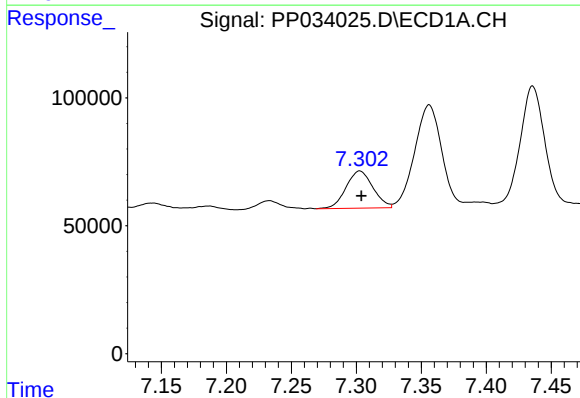


#27 AR-1254-2

R.T.: 7.303 min
Delta R.T.: -0.001 min
Response: 209444
Conc: 46.06 ng/ml

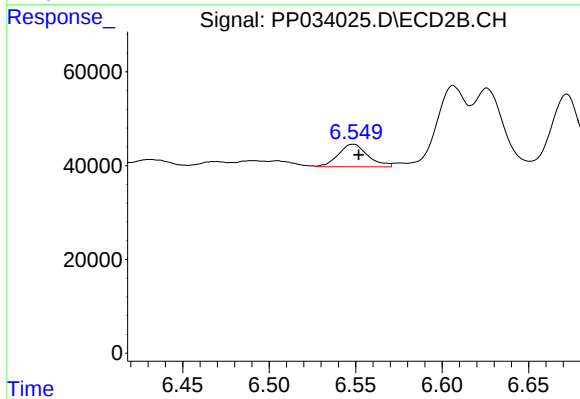

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 56571
Conc: 39.61 ng/ml

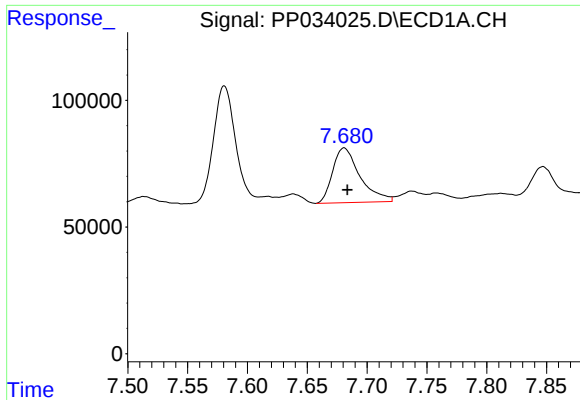


#28 AR-1254-3

R.T.: 7.681 min
Delta R.T.: -0.003 min
Response: 343918
Conc: 69.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:35 AM

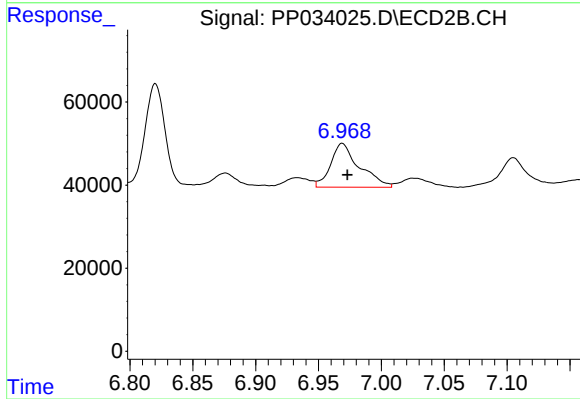


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: -0.004 min
Response: 167360
Conc: 73.12 ng/ml

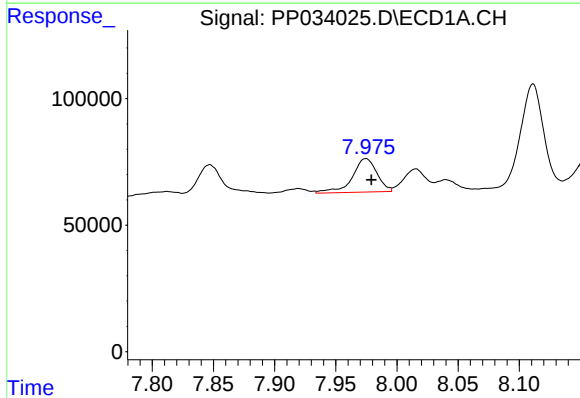


#29 AR-1254-4

R.T.: 7.975 min
Delta R.T.: -0.004 min
Response: 186845
Conc: 54.47 ng/ml

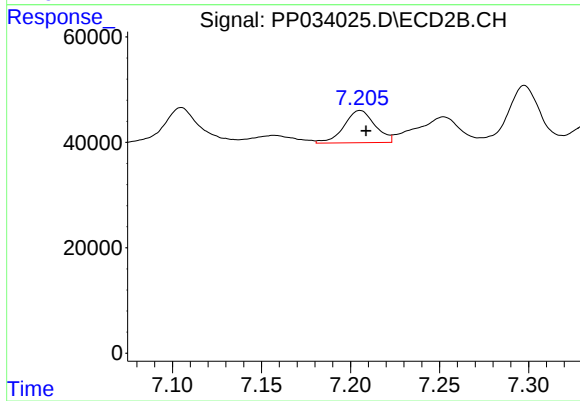

#29 AR-1254-4

R.T.: 7.205 min
Delta R.T.: -0.003 min
Response: 74299
Conc: 58.46 ng/ml

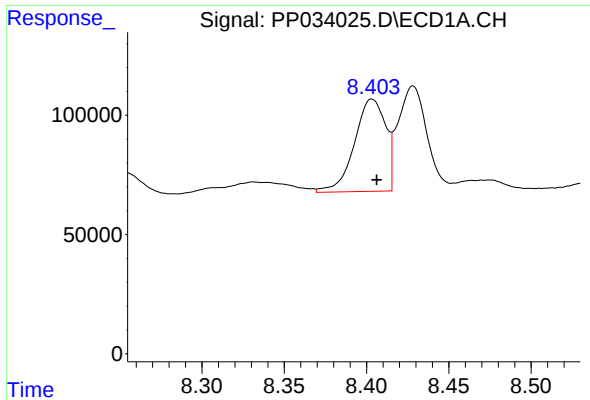


#30 AR-1254-5

R.T.: 8.403 min
Delta R.T.: -0.003 min
Response: 510382
Conc: 129.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A

Manual Integrations
APPROVED

Ankita
3/16/2021 11:17:35 AM

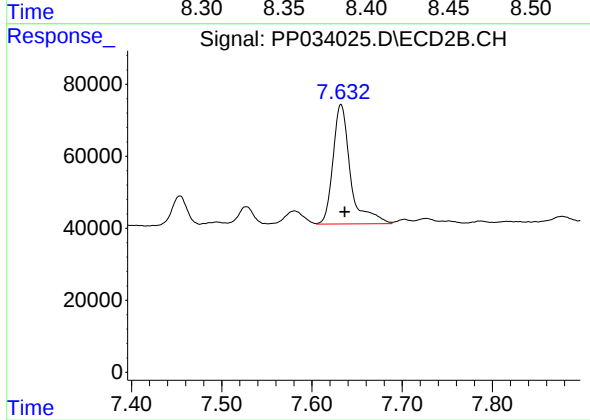

#30 AR-1254-5

R.T.: 7.632 min
Delta R.T.: -0.004 min
Response: 446565
Conc: 237.09 ng/ml