

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
 Data File : PP063473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2024 11:47
 Operator : YP\AJ
 Sample : P1746-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-01-4.0-6.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:31:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.641	47641340	48757776	21.200	21.194
2) SA Decachlor...	10.367	8.686	39155960	45902290	20.207	22.500
Target Compounds						
9) L2 AR-1221-2	0.000	3.944	0	909513	N.D.	47.084 #
20) L4 AR-1242-5	6.597	0.000	3437027	0	90.567	N.D. #
25) L5 AR-1248-5	6.597	0.000	3437027	0	50.594	N.D. #
32) L7 AR-1260-2	0.000	6.399	0	509292	N.D.	3.634 #
34) L7 AR-1260-4	8.122f	0.000	1119138	0	12.261	N.D. #
35) L7 AR-1260-5	0.000	7.274	0	442512	N.D.	2.412 #
39) L8 AR-1262-4	0.000	7.638	0	437144	N.D.	2.495 #
42) L9 AR-1268-2	0.000	7.638	0	437144	N.D.	1.559 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
Data File : PP063473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2024 11:47
Operator : YP\AJ
Sample : P1746-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:31:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

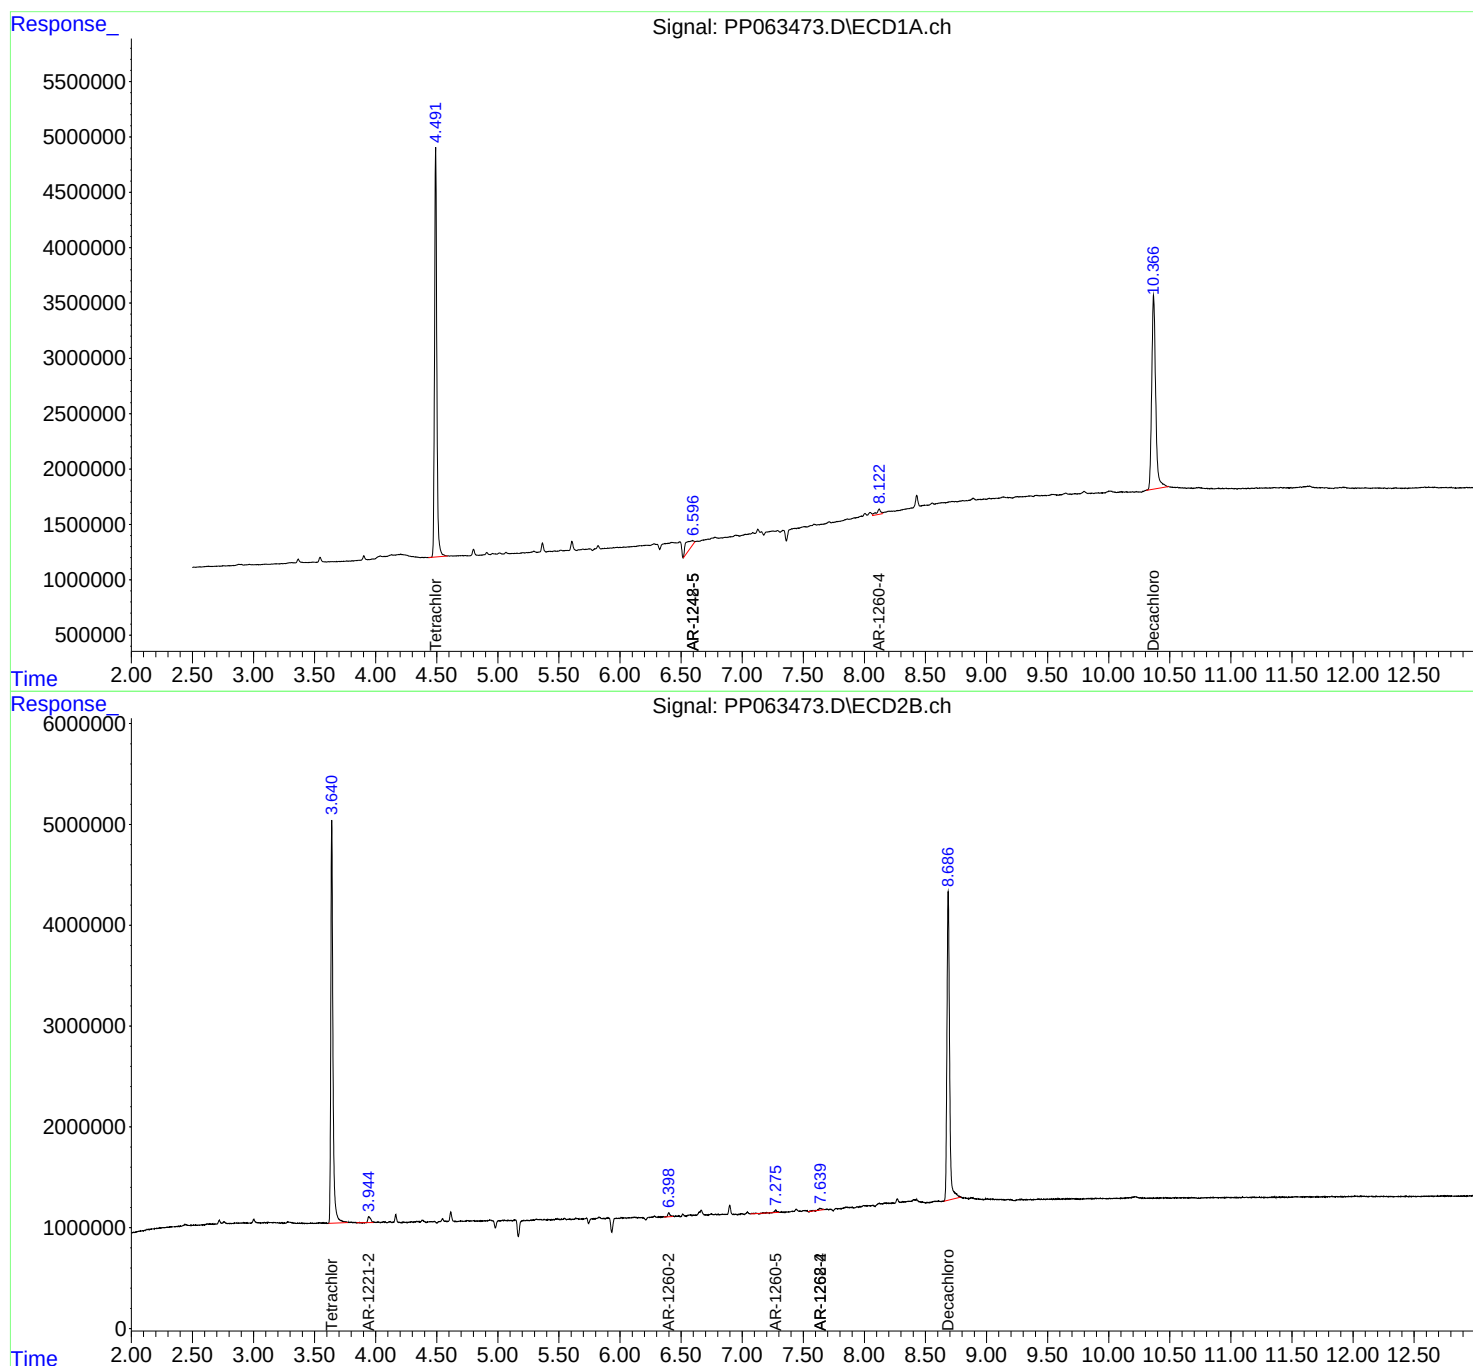


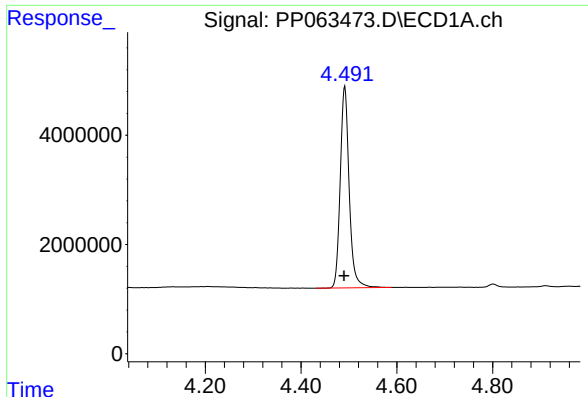

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.001 min
Response: 47641340
Conc: 21.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

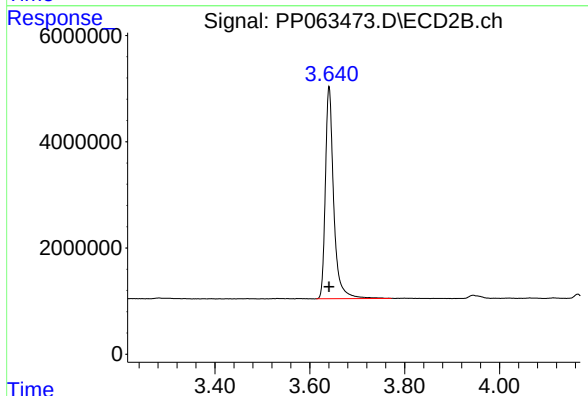


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 48757776
Conc: 21.19 ng/ml

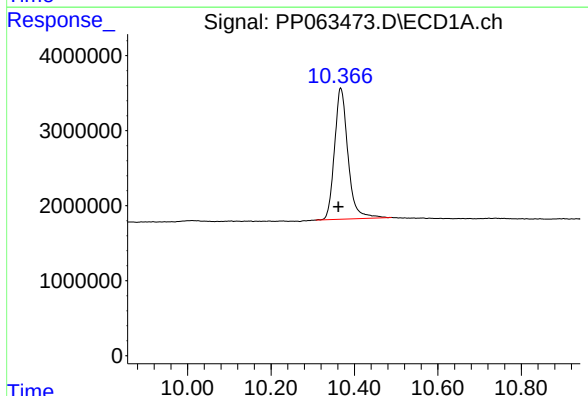


#2 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: 0.005 min
Response: 39155960
Conc: 20.21 ng/ml

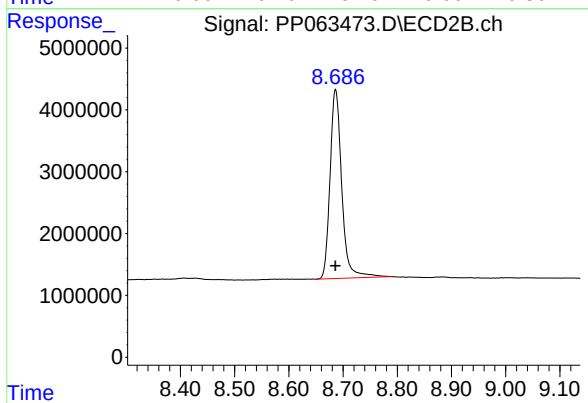

#2 Decachlorobiphenyl


R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 45902290
Conc: 22.50 ng/ml

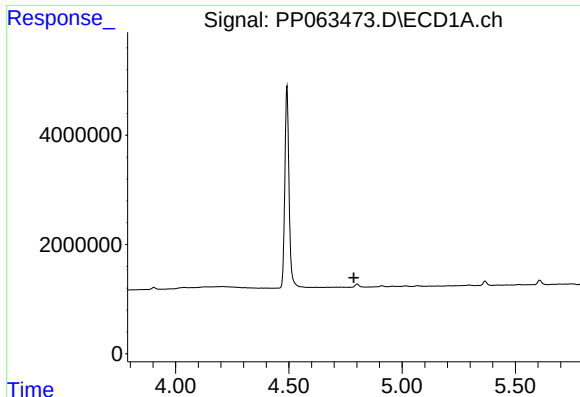

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

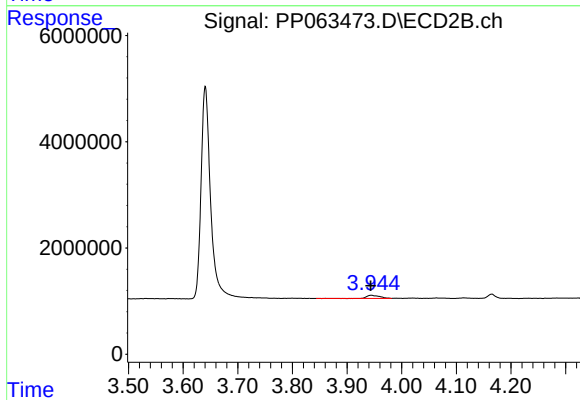


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 909513
Conc: 47.08 ng/ml

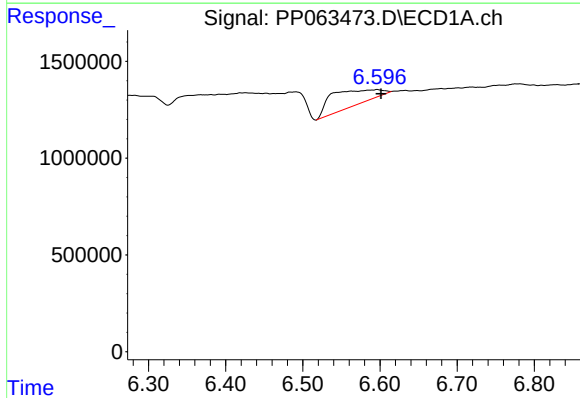


#20 AR-1242-5

R.T.: 6.597 min
Delta R.T.: -0.004 min
Response: 3437027
Conc: 90.57 ng/ml

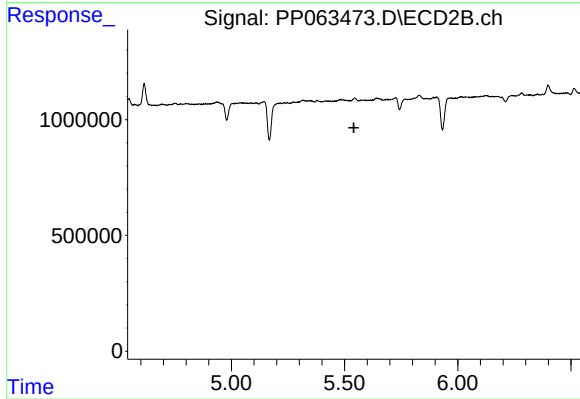

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 5.541 min
Response: 0
Conc: N.D.

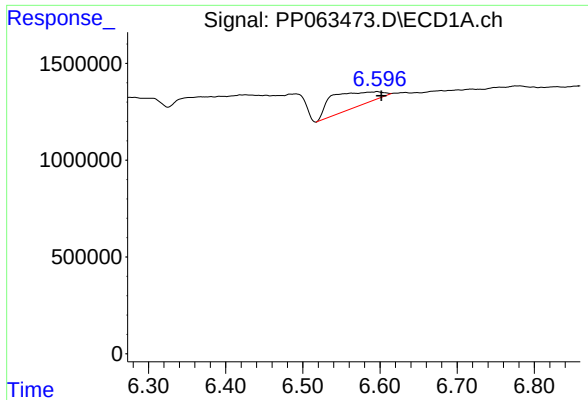

#25 AR-1248-5


R.T.: 6.597 min
Delta R.T.: -0.005 min
Response: 3437027
Conc: 50.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

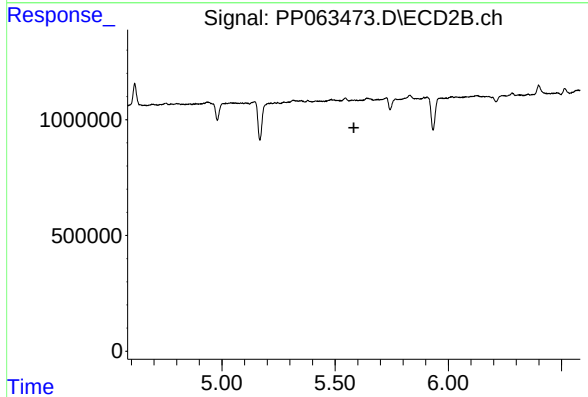


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.583 min
Response: 0
Conc: N.D.

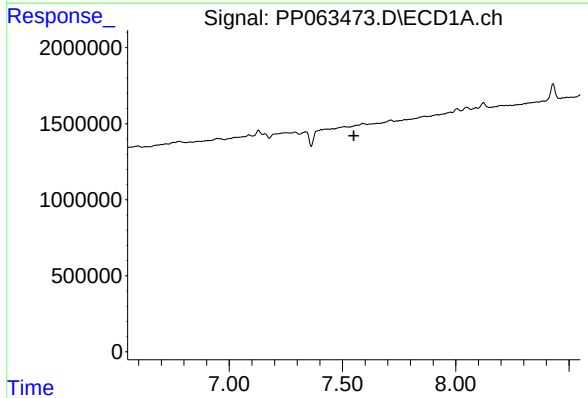


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.550 min
Response: 0
Conc: N.D.

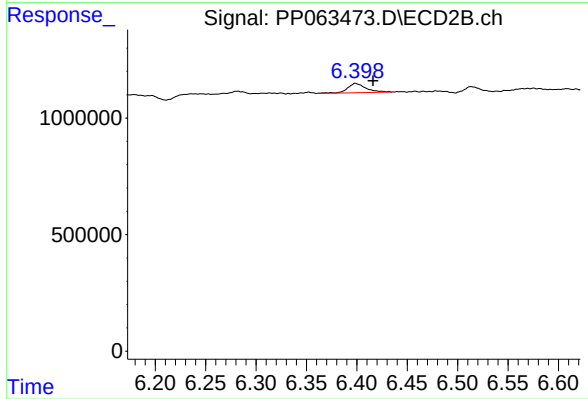

#32 AR-1260-2


R.T.: 6.399 min
Delta R.T.: -0.017 min
Response: 509292
Conc: 3.63 ng/ml

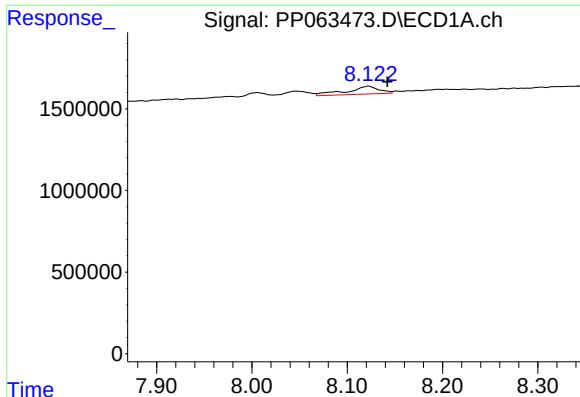

#34 AR-1260-4


R.T.: 8.122 min
Delta R.T.: -0.020 min
Response: 1119138
Conc: 12.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

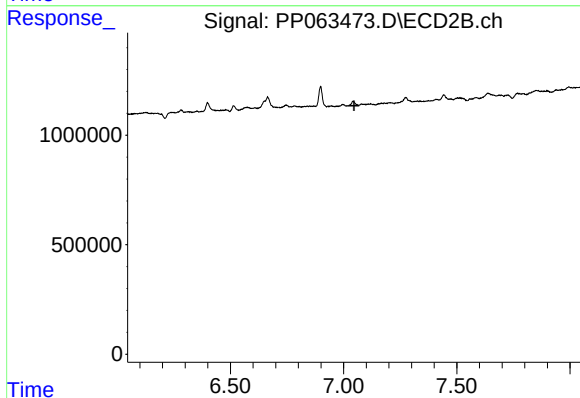


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

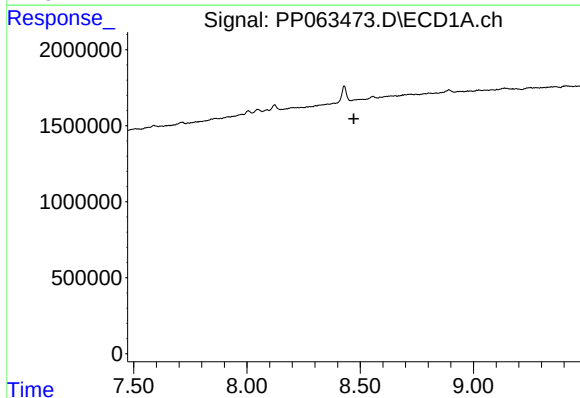


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

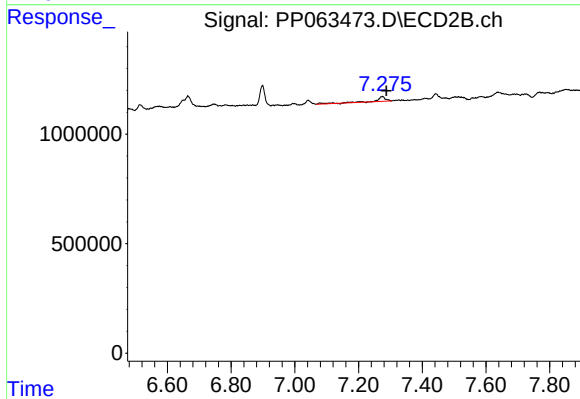

#35 AR-1260-5


R.T.: 7.274 min
Delta R.T.: -0.013 min
Response: 442512
Conc: 2.41 ng/ml

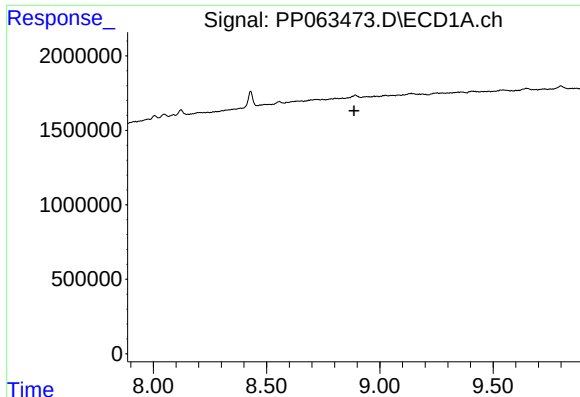

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SB-01-4.0-6.0

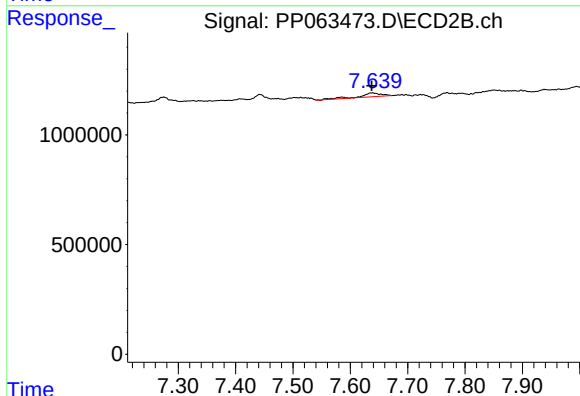


#39 AR-1262-4

R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 437144
Conc: 2.49 ng/ml

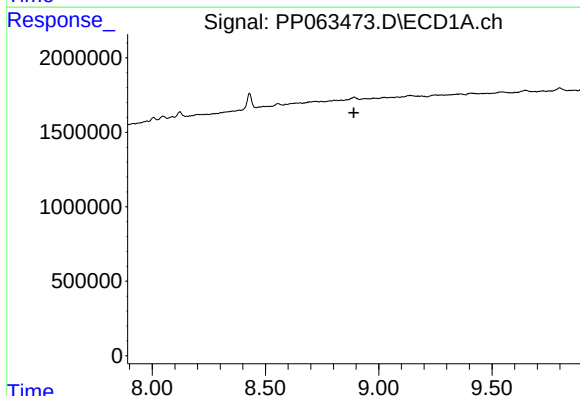

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.890 min
Response: 0
Conc: N.D.

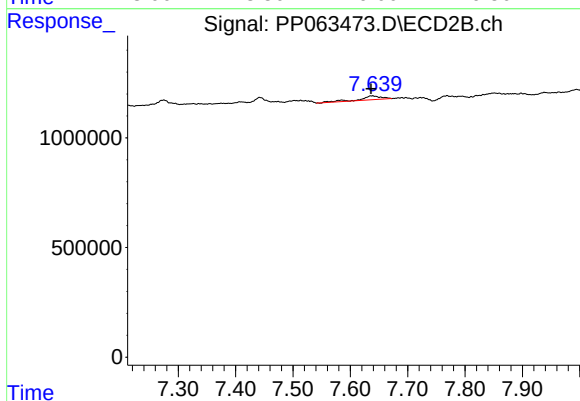

#42 AR-1268-2

R.T.: 7.638 min
Delta R.T.: 0.002 min
Response: 437144
Conc: 1.56 ng/ml