

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
 Data File : PP063479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2024 14:35
 Operator : YP\AJ
 Sample : P1764-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:33:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.490	3.640	46339033	46833016	20.621	20.358
2)	SA Decachlor...	10.365	8.685	36193597	42097862	18.678	20.635
Target Compounds							
9)	L2 AR-1221-2	0.000	3.941	0	892968	N.D.	46.227 #
20)	L4 AR-1242-5	0.000	5.542	0	405960	N.D.	8.005 #
26)	L6 AR-1254-1	0.000	5.542	0	405960	N.D.	3.546 #
30)	L6 AR-1254-5	0.000	6.746	0	352196	N.D.	2.575 #
34)	L7 AR-1260-4	0.000	7.041	0	338897	N.D.	3.344 #
35)	L7 AR-1260-5	0.000	7.271	0	698960	N.D.	3.809 #
37)	L8 AR-1262-2	0.000	7.041	0	338897	N.D.	2.343 #
39)	L8 AR-1262-4	0.000	7.637	0	611664	N.D.	3.491 #
42)	L9 AR-1268-2	0.000	7.637	0	611664	N.D.	2.182 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
Data File : PP063479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2024 14:35
Operator : YP\AJ
Sample : P1764-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:33:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

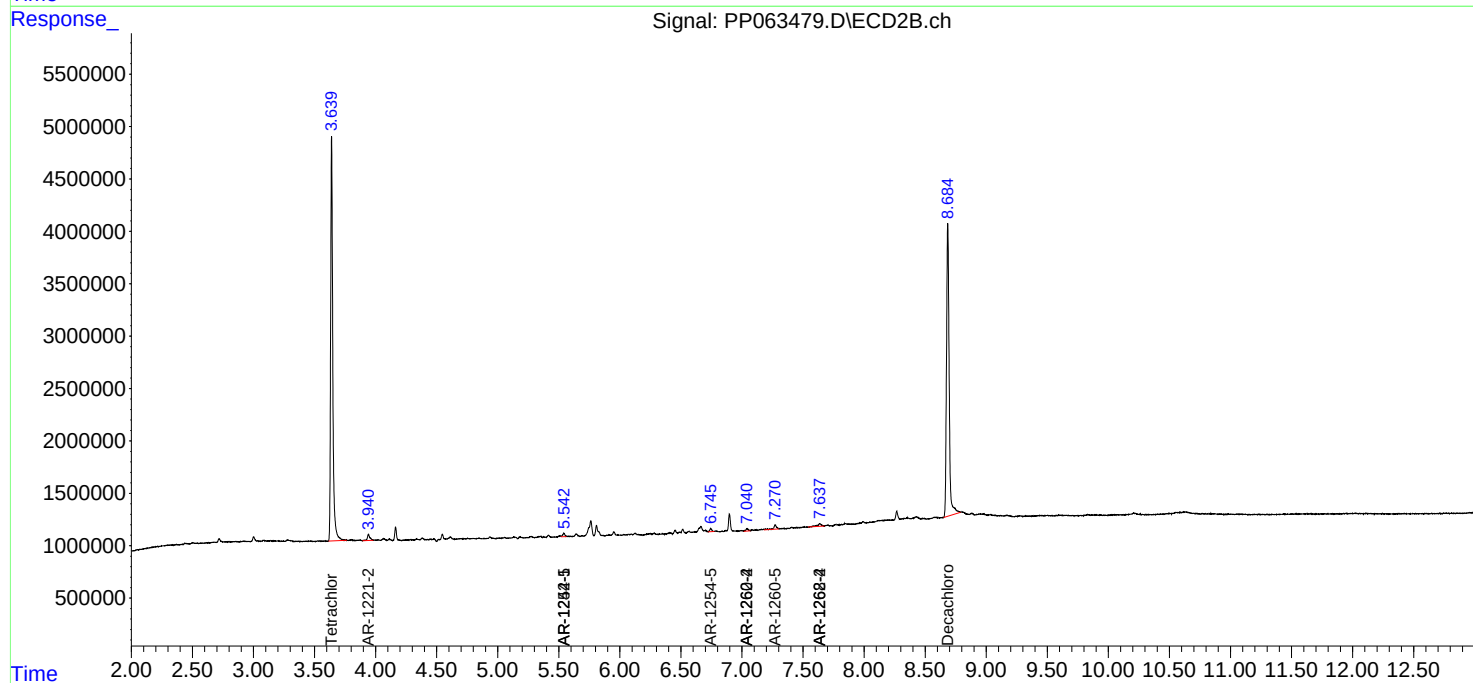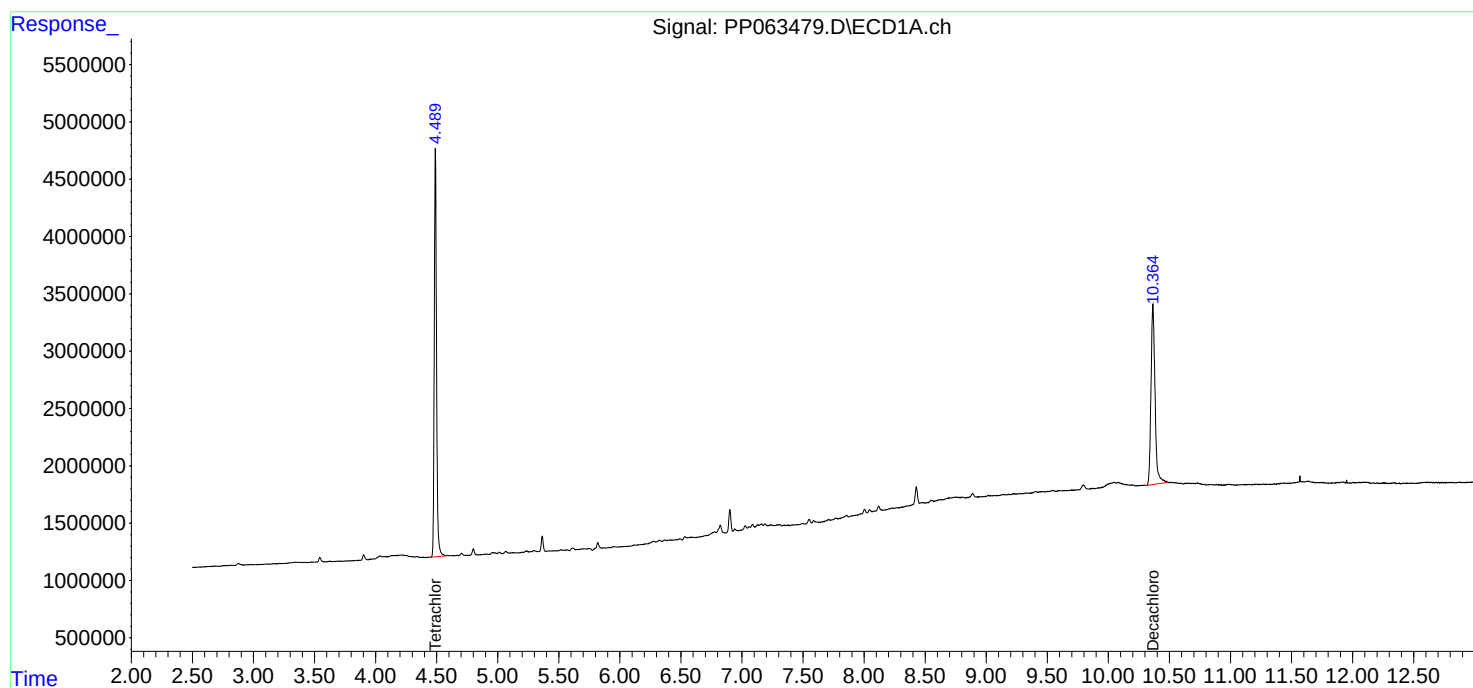


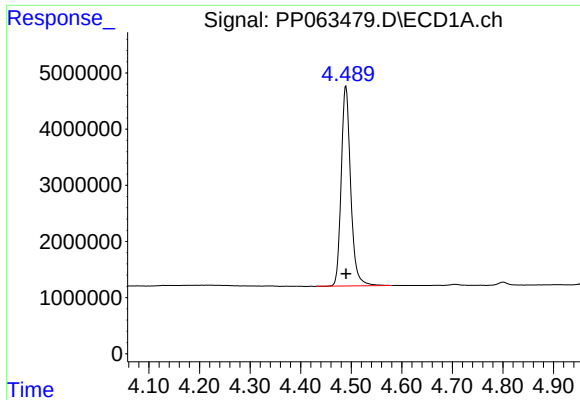

#1 Tetrachloro-m-xylene


R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 46339033
Conc: 20.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-2

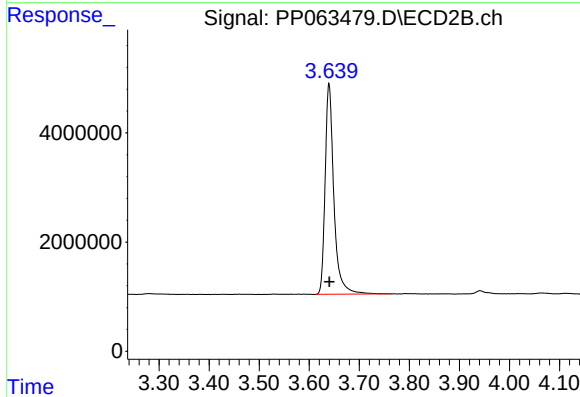


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 46833016
Conc: 20.36 ng/ml

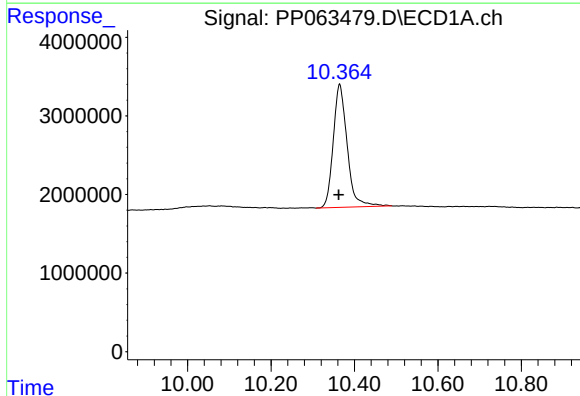


#2 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.003 min
Response: 36193597
Conc: 18.68 ng/ml

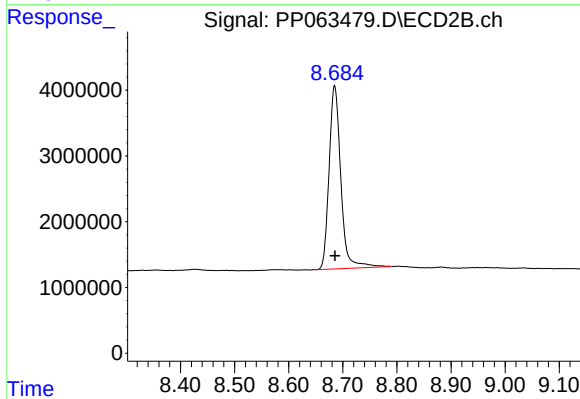

#2 Decachlorobiphenyl


R.T.: 8.685 min
Delta R.T.: 0.000 min
Response: 42097862
Conc: 20.63 ng/ml

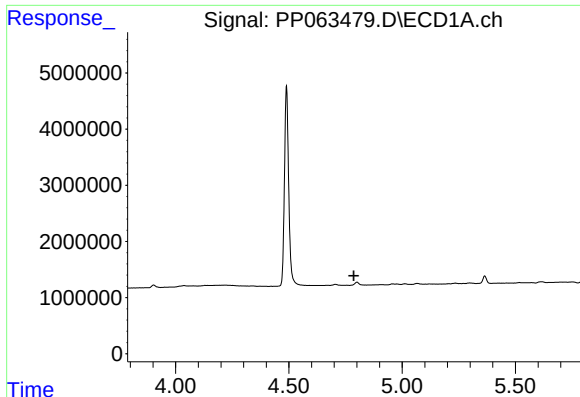

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
COMP-2

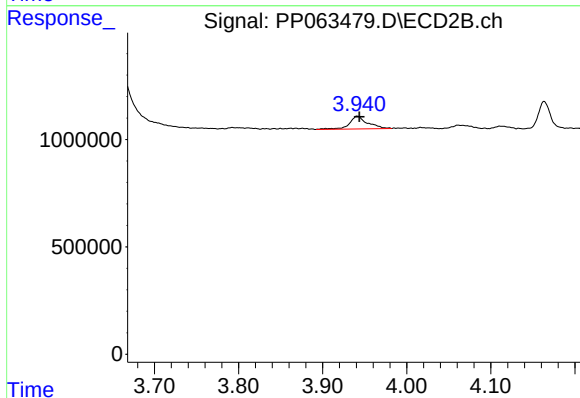


#9 AR-1221-2

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 892968
Conc: 46.23 ng/ml

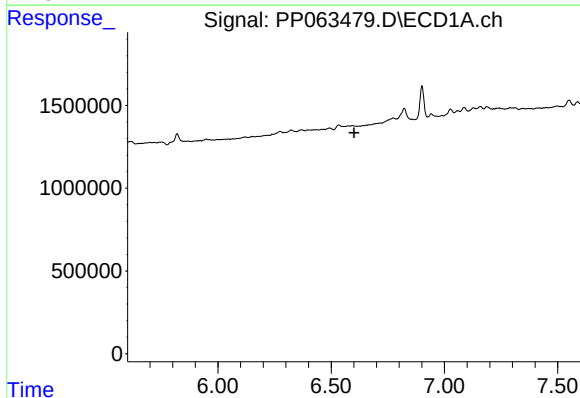


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.601 min
Response: 0
Conc: N.D.

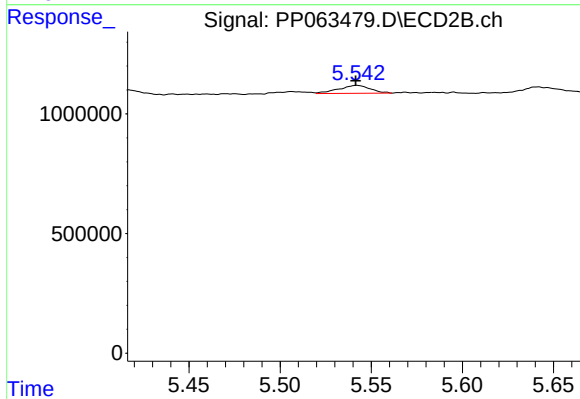

#20 AR-1242-5


R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 405960
Conc: 8.01 ng/ml

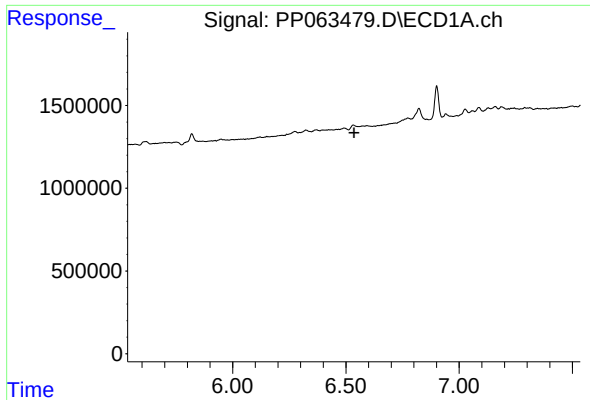

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.536 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
COMP-2

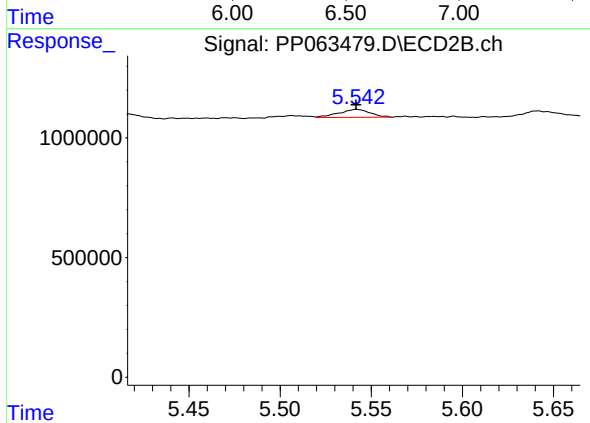


#26 AR-1254-1

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 405960
Conc: 3.55 ng/ml

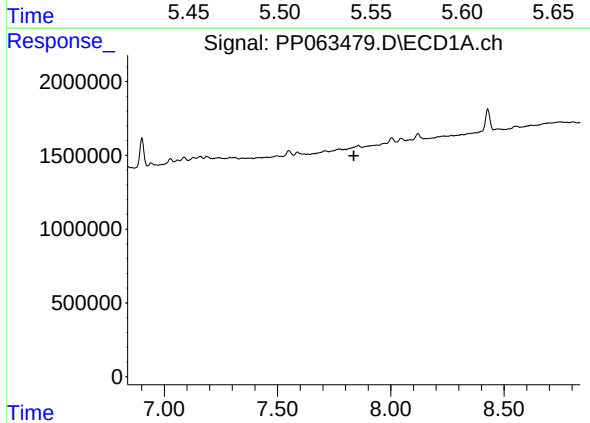


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.836 min
Response: 0
Conc: N.D.

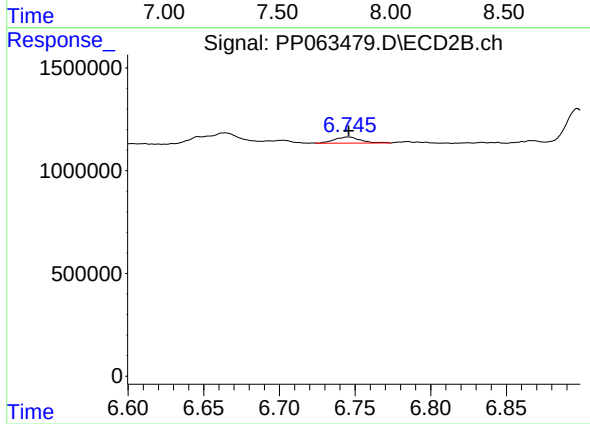

#30 AR-1254-5


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 352196
Conc: 2.58 ng/ml

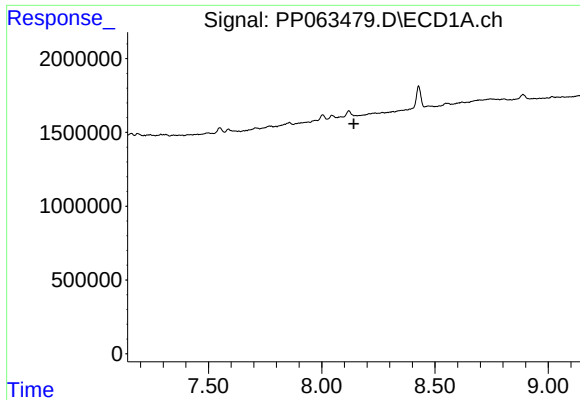

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
COMP-2

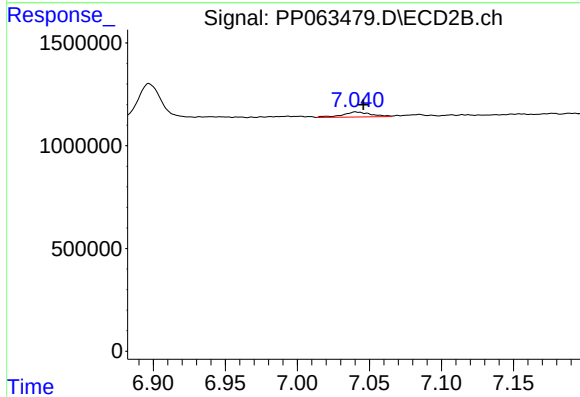


#34 AR-1260-4

R.T.: 7.041 min
Delta R.T.: -0.005 min
Response: 338897
Conc: 3.34 ng/ml

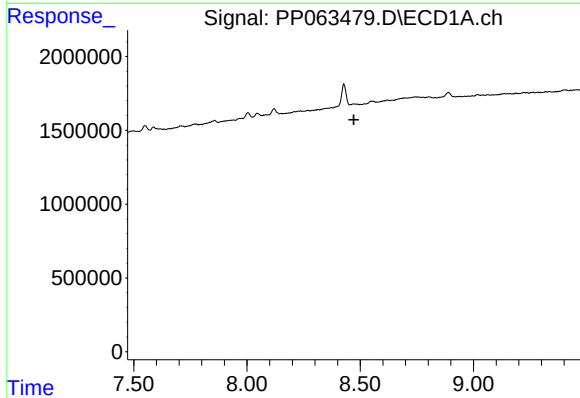


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

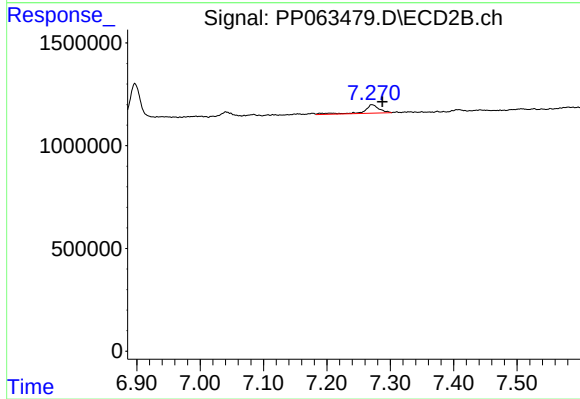

#35 AR-1260-5


R.T.: 7.271 min
Delta R.T.: -0.017 min
Response: 698960
Conc: 3.81 ng/ml

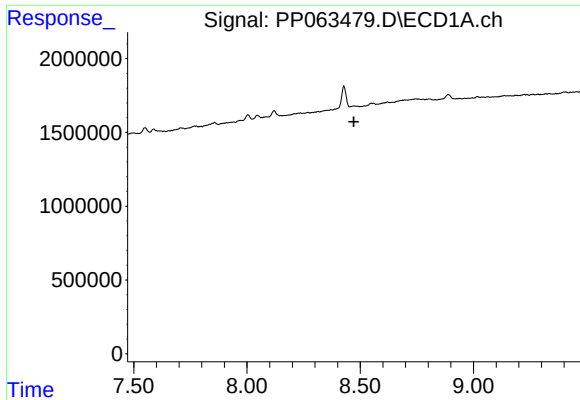

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
COMP-2

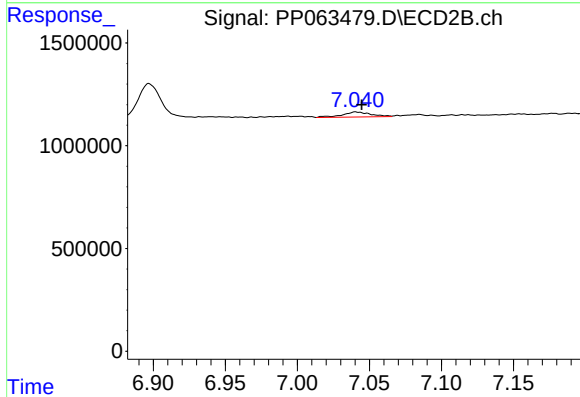


#37 AR-1262-2

R.T.: 7.041 min
Delta R.T.: -0.004 min
Response: 338897
Conc: 2.34 ng/ml

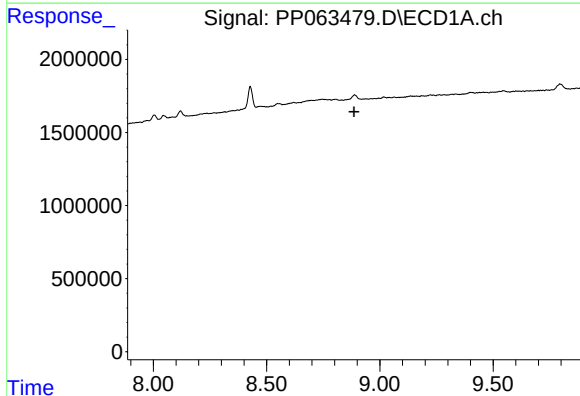


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.886 min
Response: 0
Conc: N.D.

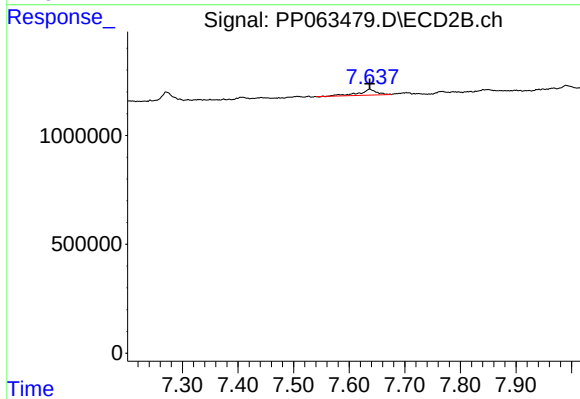

#39 AR-1262-4


R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 611664
Conc: 3.49 ng/ml

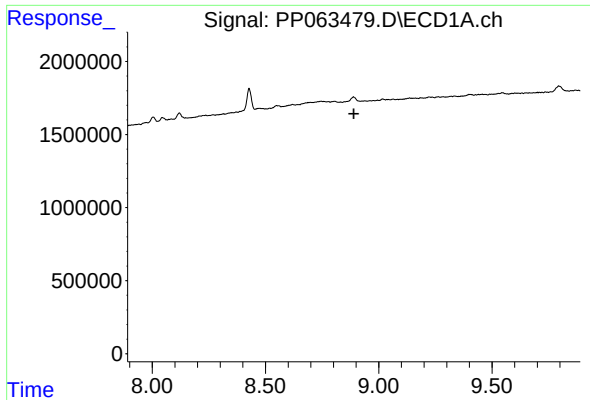

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
COMP-2

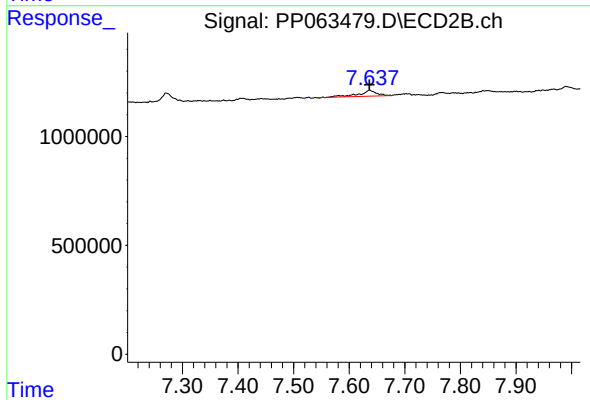

#42 AR-1268-2

R.T.: 7.637 min
Delta R.T.: 0.000 min
Response: 611664
Conc: 2.18 ng/ml