

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
 Data File : PP063537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2024 09:55
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:25:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.489	3.639	40681689	41073816	18.103	17.854
2)	SA Decachlor...	10.361	8.680	42004682	42353916	21.677	20.760
Target Compounds							
6)	L1 AR-1016-4	0.000	4.996f	0	225316	N.D.	4.464 #
9)	L2 AR-1221-2	0.000	3.941	0	619344	N.D.	32.062 #
14)	L3 AR-1232-4	0.000	4.996f	0	225316	N.D.	8.944 #
19)	L4 AR-1242-4	0.000	4.996f	0	225316	N.D.	4.799 #
22)	L5 AR-1248-2	0.000	4.996f	0	225316	N.D.	3.372 #
23)	L5 AR-1248-3	0.000	4.996f	0	225316	N.D.	3.231 #
32)	L7 AR-1260-2	0.000	6.395f	0	897968	N.D.	6.407 #
36)	L8 AR-1262-1	7.981	0.000	4095186	0	79.151	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
Data File : PP063537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2024 09:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:25:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

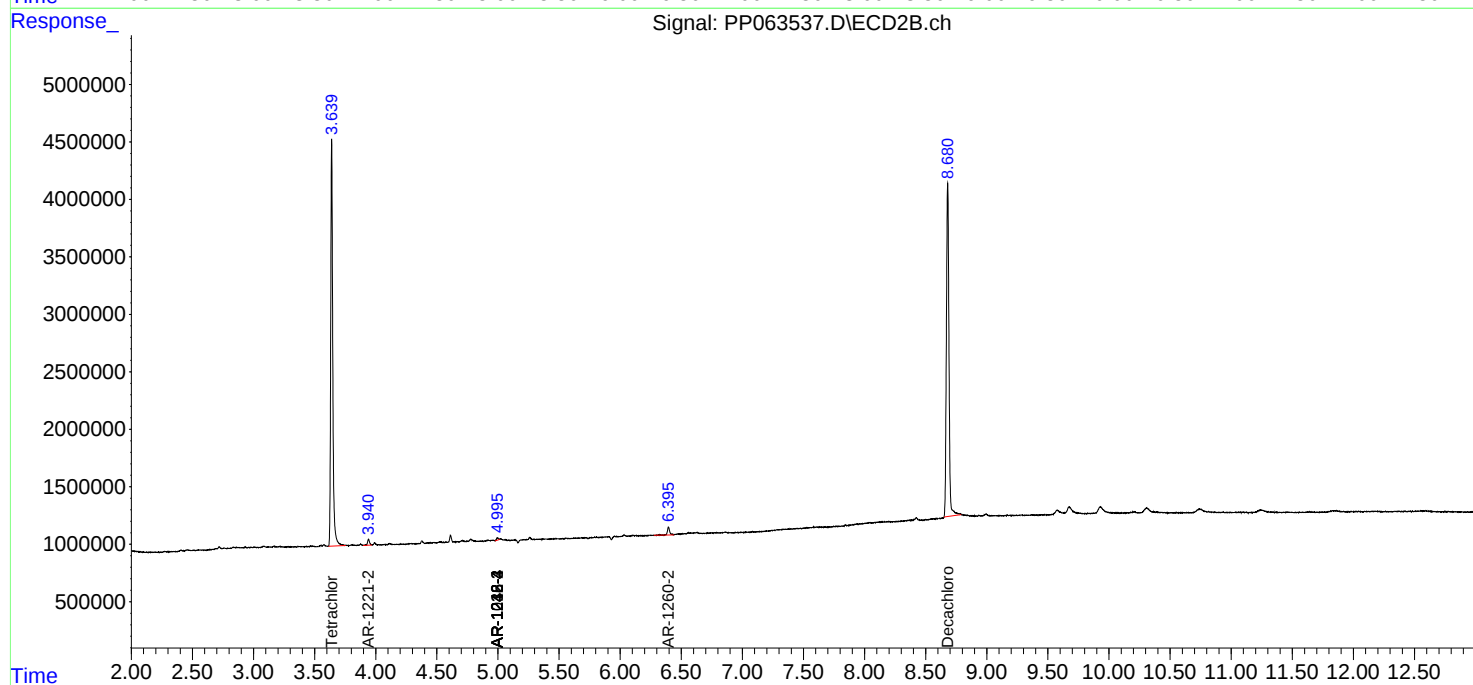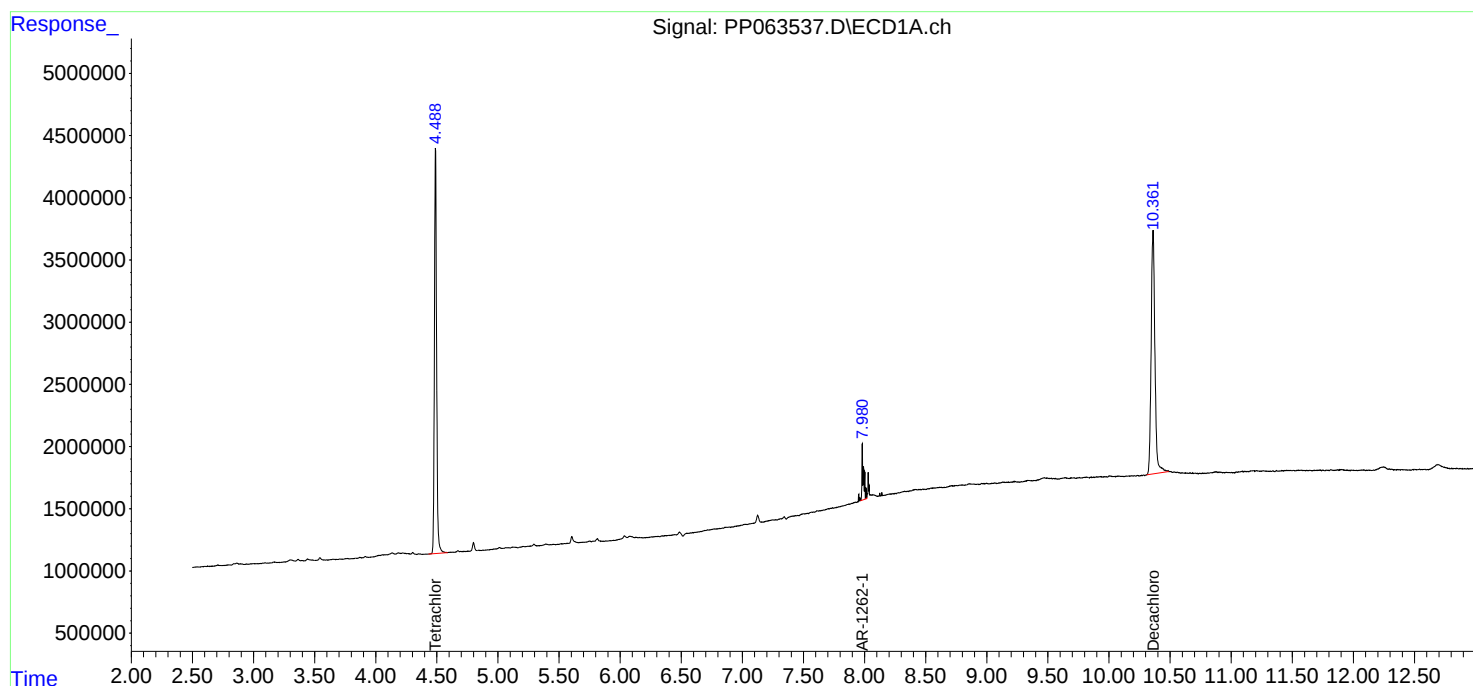


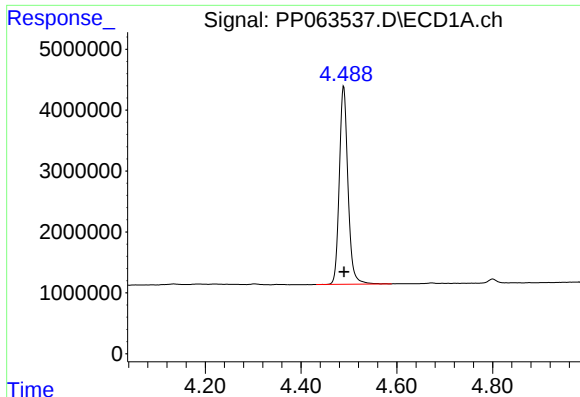

#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 40681689
Conc: 18.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

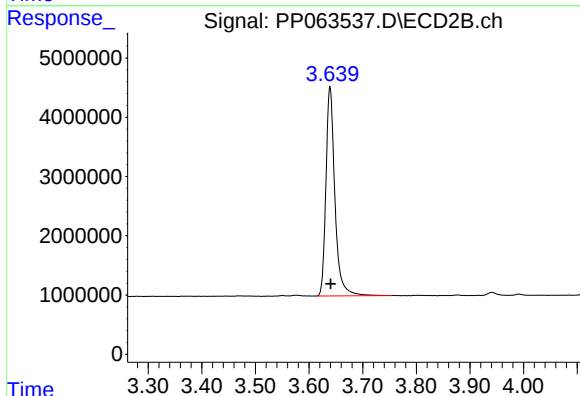


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 41073816
Conc: 17.85 ng/ml

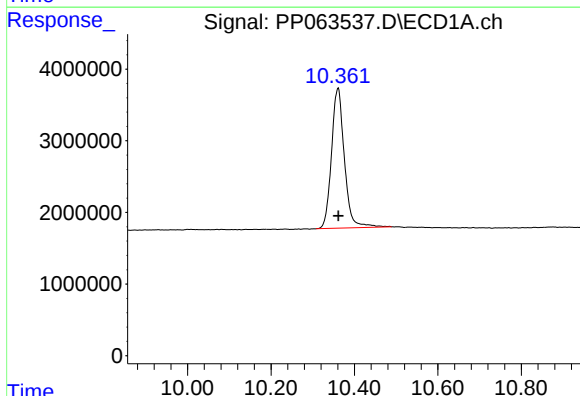


#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.001 min
Response: 42004682
Conc: 21.68 ng/ml

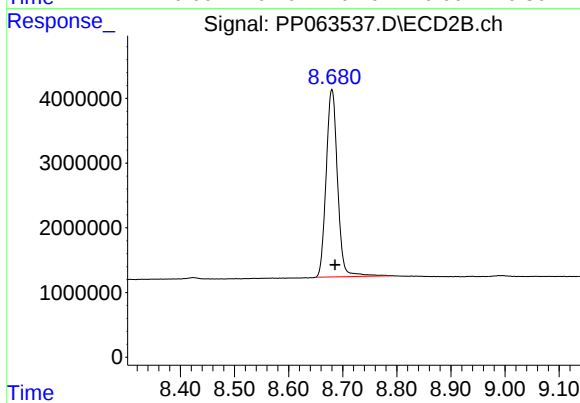

#2 Decachlorobiphenyl


R.T.: 8.680 min
Delta R.T.: -0.006 min
Response: 42353916
Conc: 20.76 ng/ml

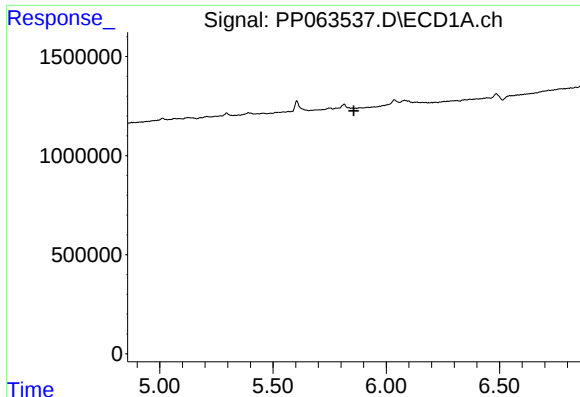

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

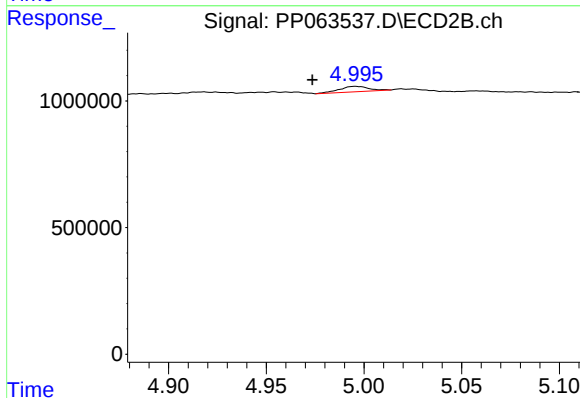


#6 AR-1016-4

R.T.: 4.996 min
Delta R.T.: 0.022 min
Response: 225316
Conc: 4.46 ng/ml

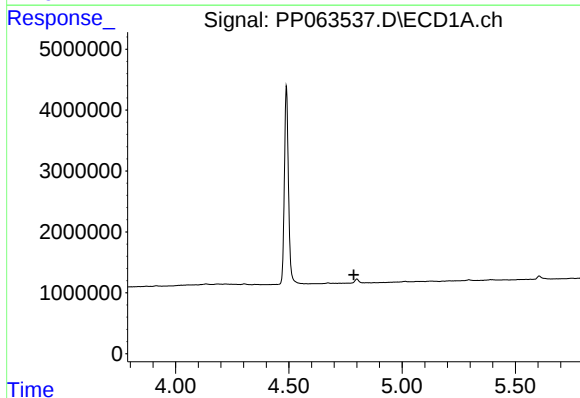


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.787 min
Response: 0
Conc: N.D.

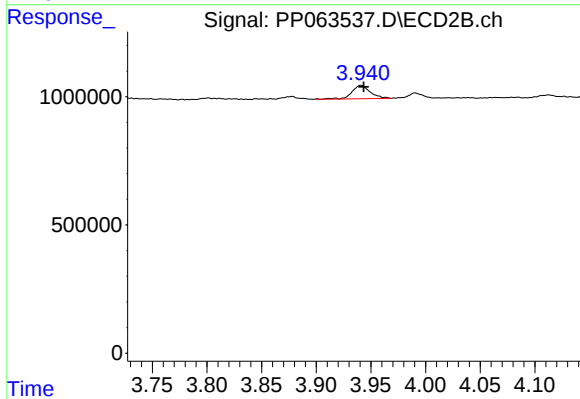

#9 AR-1221-2


R.T.: 3.941 min
Delta R.T.: -0.003 min
Response: 619344
Conc: 32.06 ng/ml

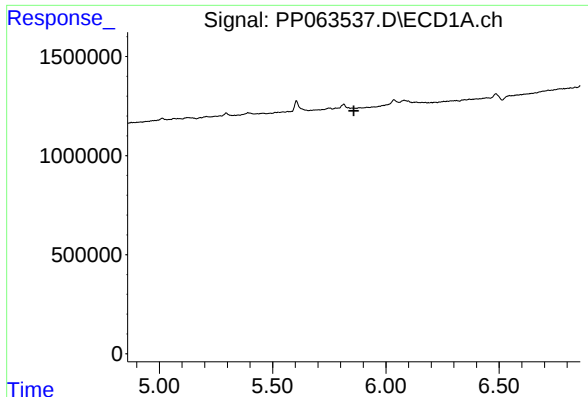

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.858 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

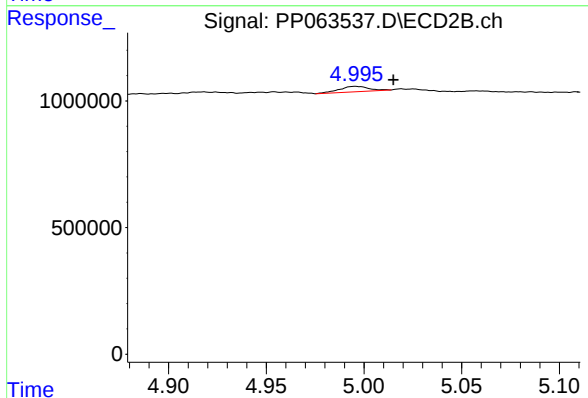


#14 AR-1232-4

R.T.: 4.996 min
Delta R.T.: -0.020 min
Response: 225316
Conc: 8.94 ng/ml

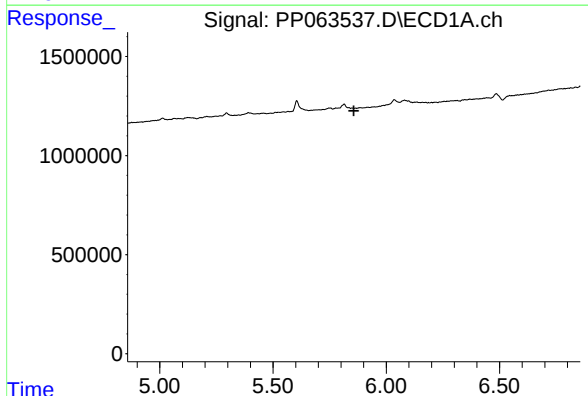


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.857 min
Response: 0
Conc: N.D.

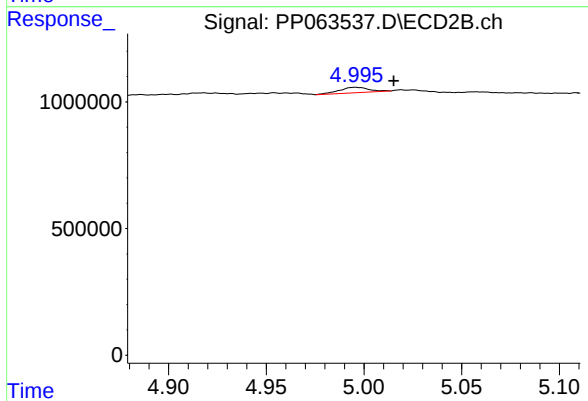

#19 AR-1242-4


R.T.: 4.996 min
Delta R.T.: -0.020 min
Response: 225316
Conc: 4.80 ng/ml

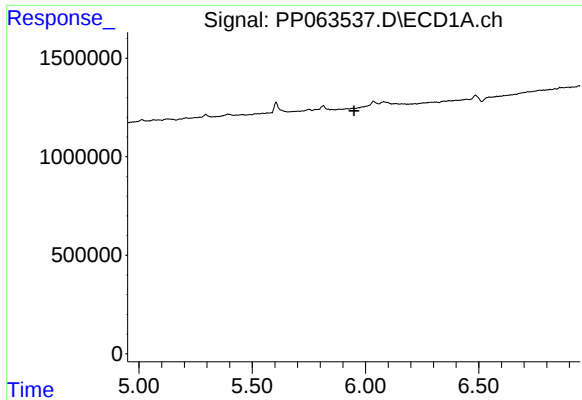

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

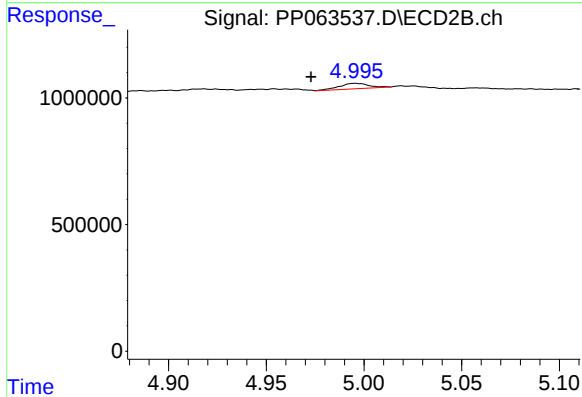


#22 AR-1248-2

R.T.: 4.996 min
Delta R.T.: 0.023 min
Response: 225316
Conc: 3.37 ng/ml

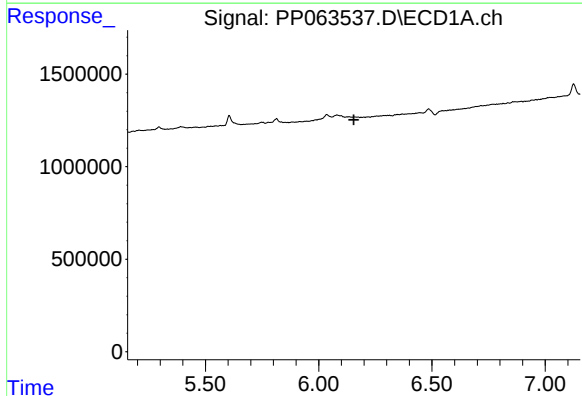


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.156 min
Response: 0
Conc: N.D.

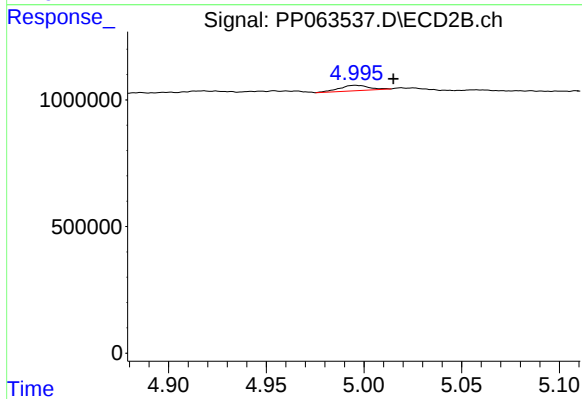

#23 AR-1248-3


R.T.: 4.996 min
Delta R.T.: -0.020 min
Response: 225316
Conc: 3.23 ng/ml

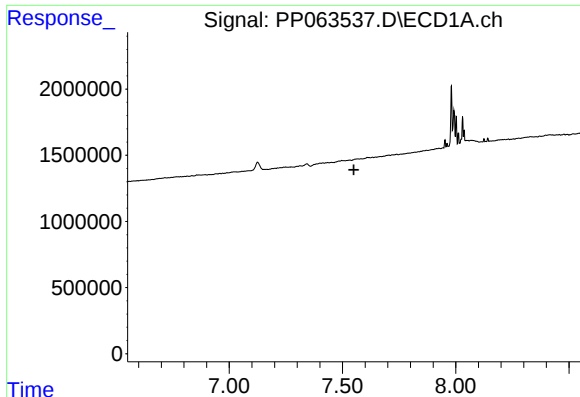

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

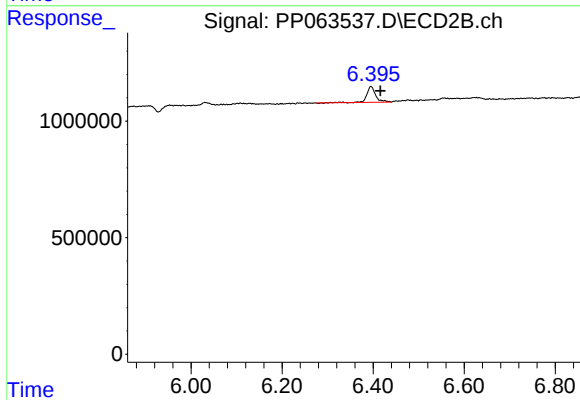


#32 AR-1260-2

R.T.: 6.395 min
Delta R.T.: -0.021 min
Response: 897968
Conc: 6.41 ng/ml

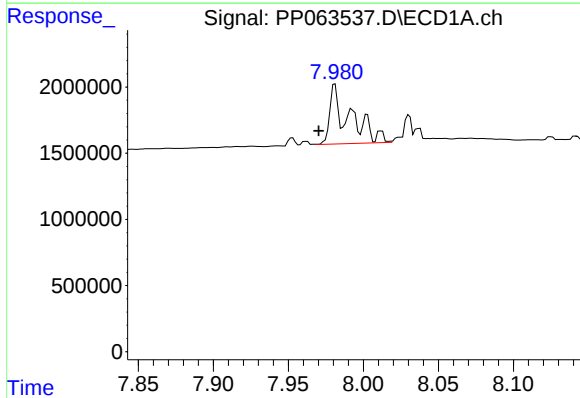

#36 AR-1262-1

R.T.: 7.981 min
Delta R.T.: 0.011 min
Response: 4095186
Conc: 79.15 ng/ml

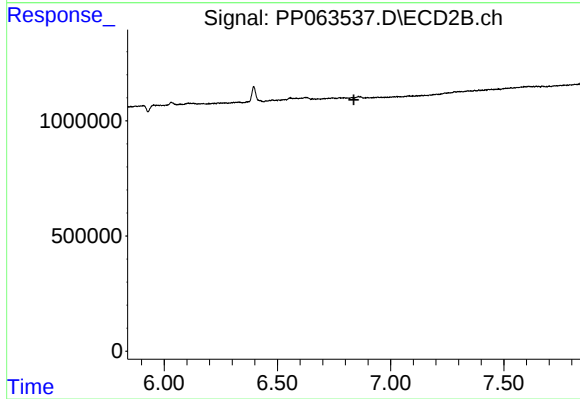

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.