

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
 Data File : PP063503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2024 22:06
 Operator : YP\AJ
 Sample : P1769-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FB-3-14-24

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2024
 Supervised By :Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:42:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.641	49779827	50766496	22.152m	22.068
2) SA Decachlor...	10.363	8.683	31546026	35854620	16.279	17.575

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
Data File : PP063503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2024 22:06
Operator : YP\AJ
Sample : P1769-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FB-3-14-24


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2024
Supervised By :Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:42:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

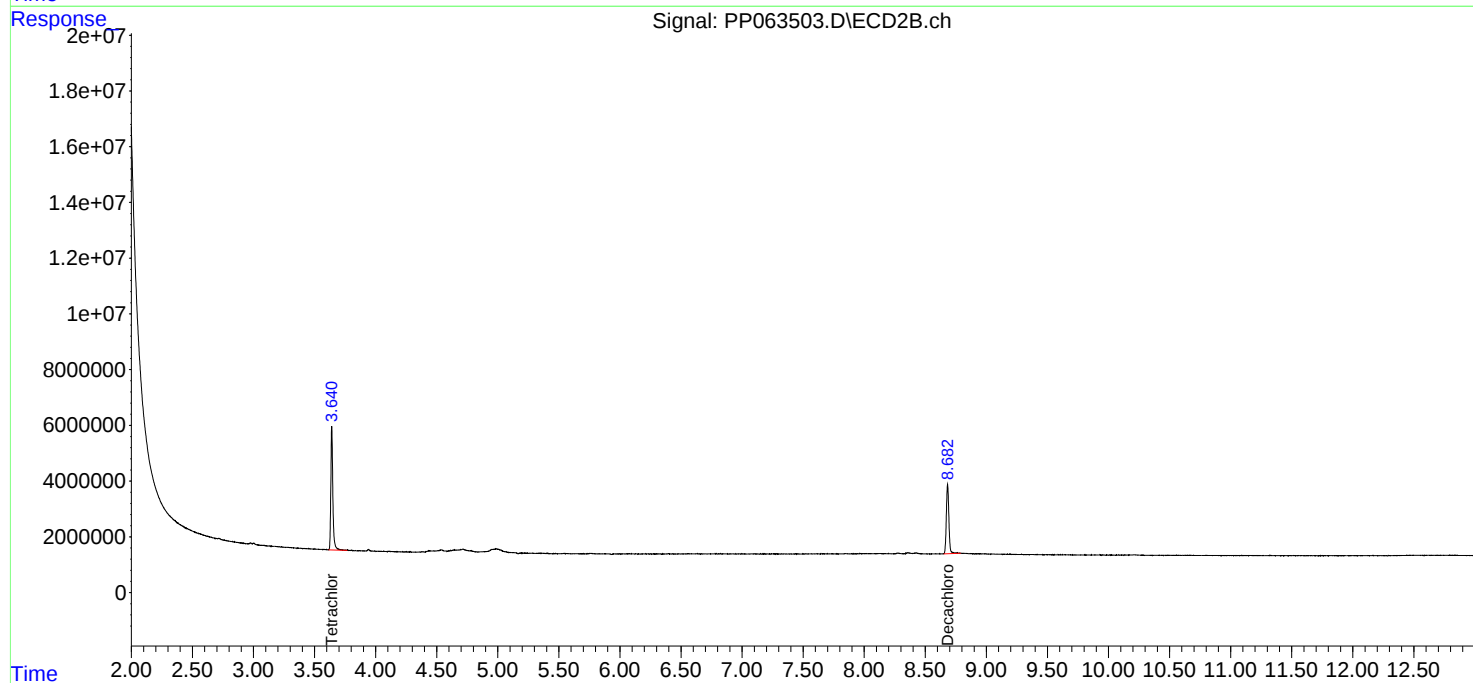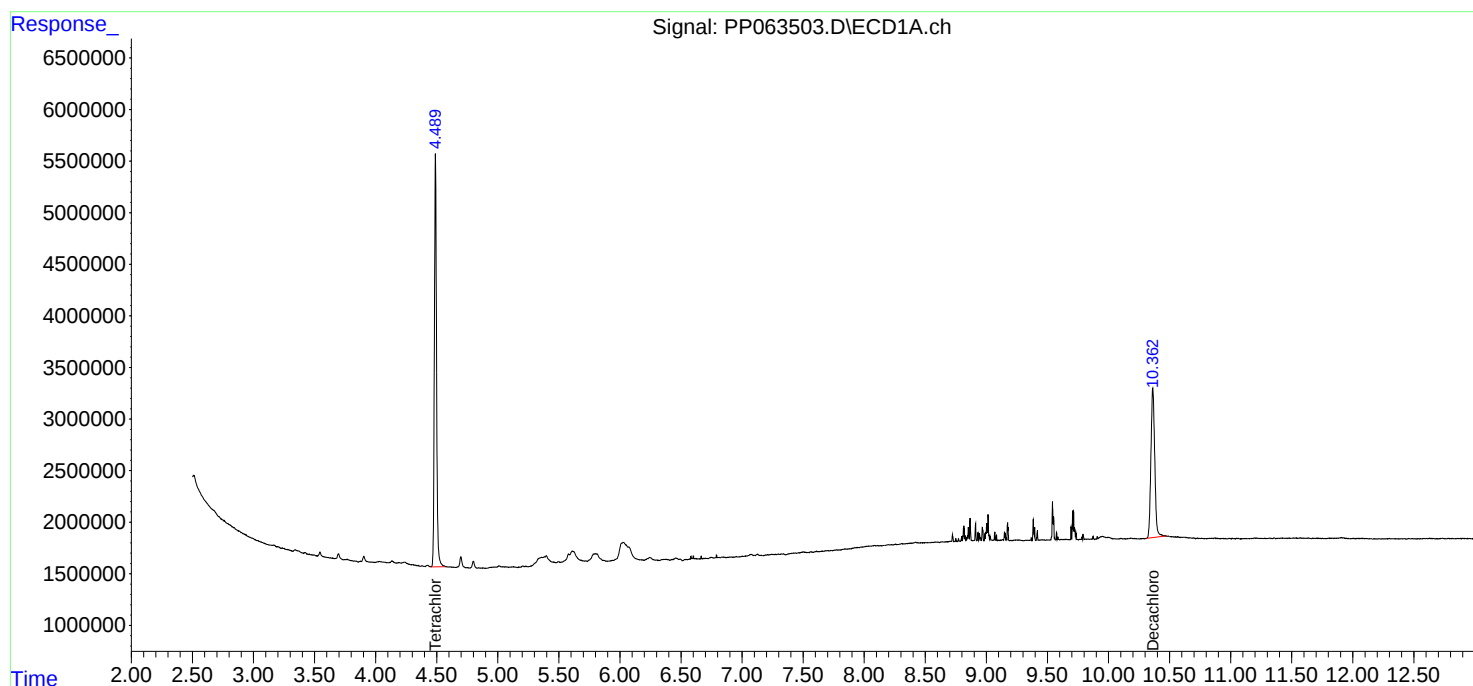

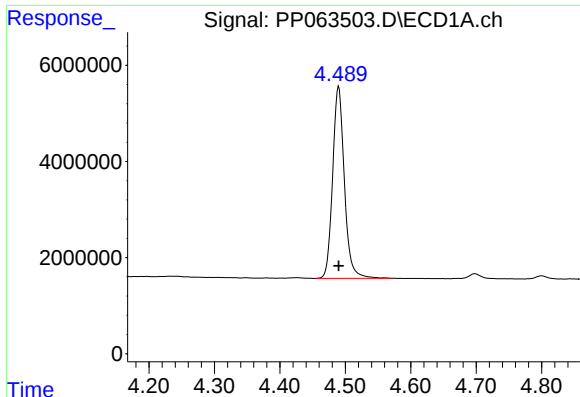


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 49779827
Conc: 22.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
FB-3-14-24


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2024
Supervised By :Ankita Jodhani 03/18/2024

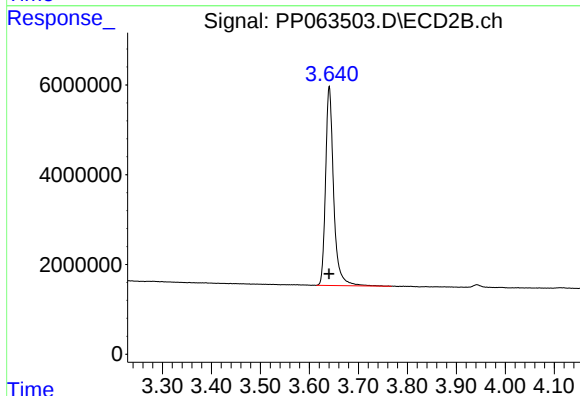


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 50766496
Conc: 22.07 ng/ml

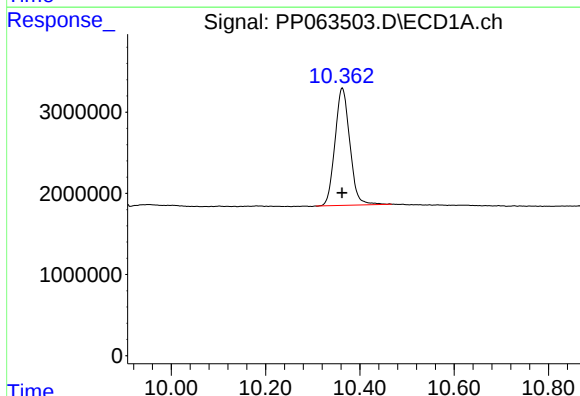

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.000 min
Response: 31546026
Conc: 16.28 ng/ml

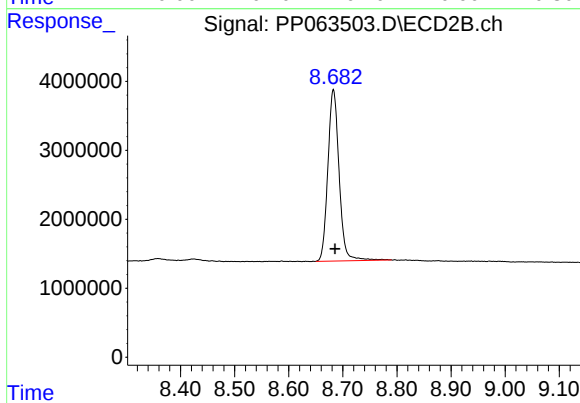

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.003 min
Response: 35854620
Conc: 17.57 ng/ml