

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
 Data File : PP063531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2024 06:54
 Operator : YP\AJ
 Sample : P1768-05 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226477L02-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2024
 Supervised By :Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 07:20:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.639	2477592	2113102	1.103m	0.919m
2) SA Decachlor...	10.359	8.682	4938650	2666047	2.549	1.307m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031524\
Data File : PP063531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2024 06:54
Operator : YP\AJ
Sample : P1768-05 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC226477L02-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2024
Supervised By :Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 07:20:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

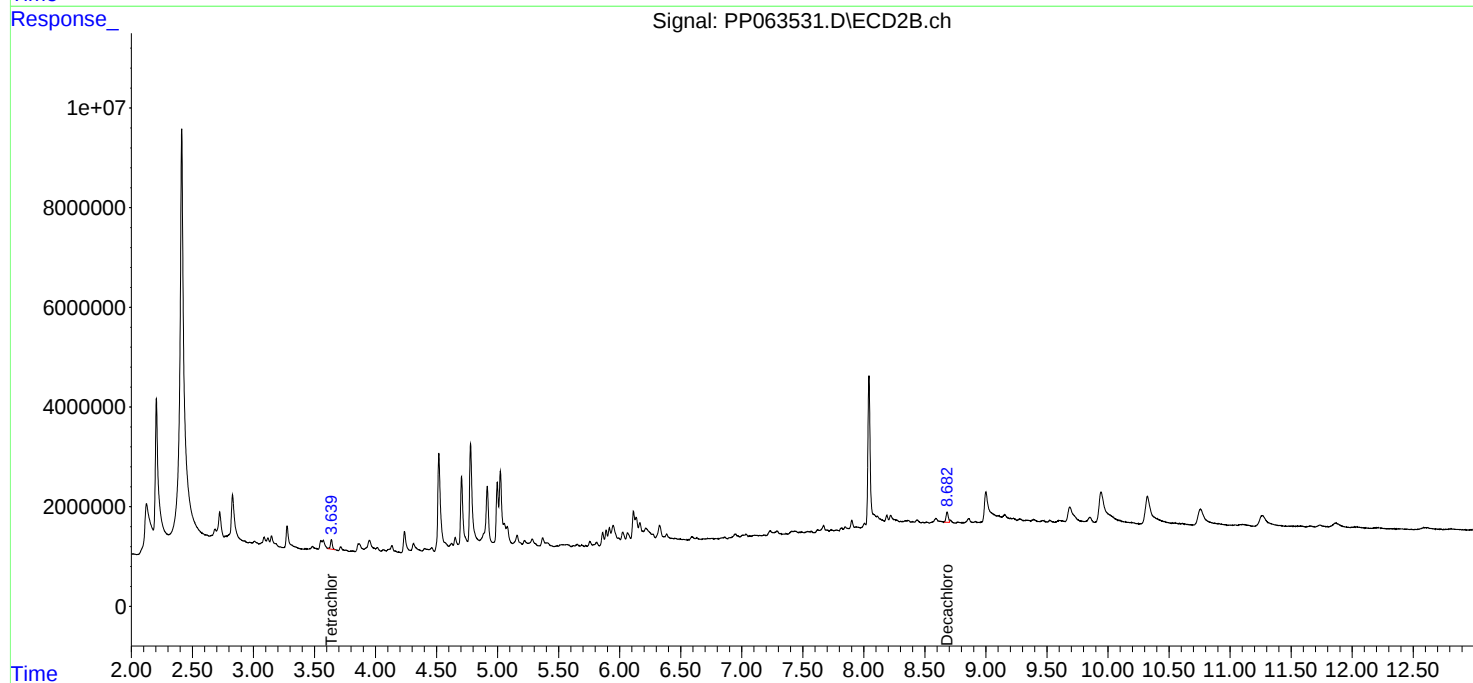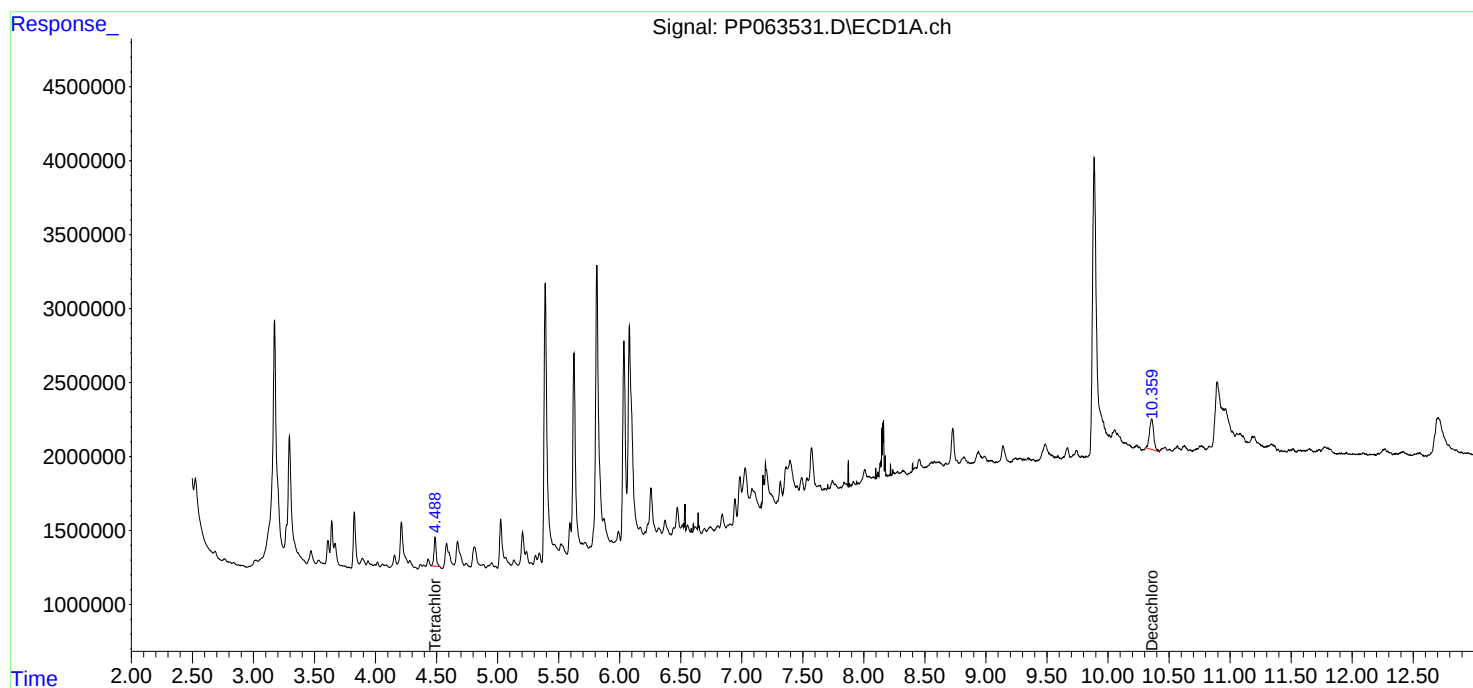

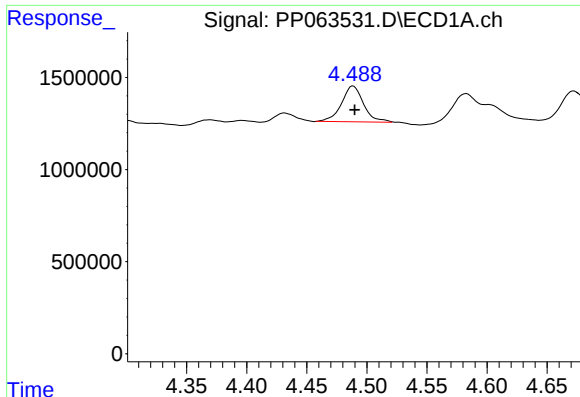


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.002 min
Response: 2477592
Conc: 1.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226477L02-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2024
Supervised By :Ankita Jodhani 03/18/2024

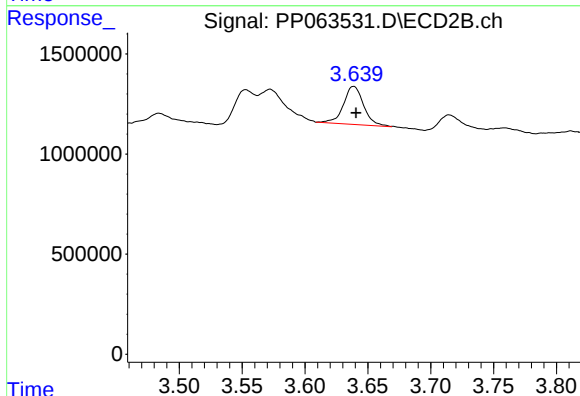


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 2113102
Conc: 0.92 ng/ml m

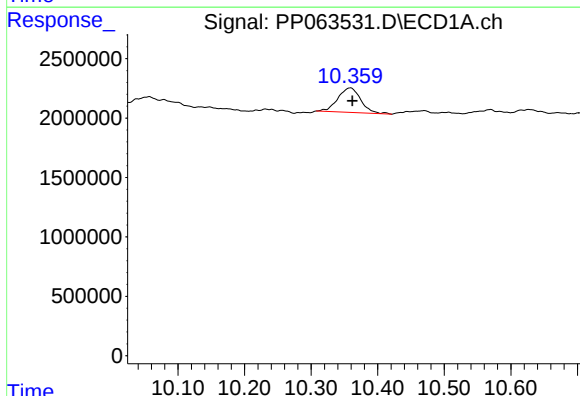

#2 Decachlorobiphenyl

R.T.: 10.359 min
Delta R.T.: -0.003 min
Response: 4938650
Conc: 2.55 ng/ml

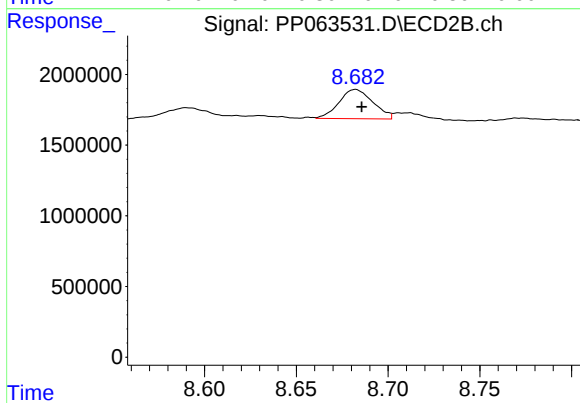

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.004 min
Response: 2666047
Conc: 1.31 ng/ml m