

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP031621\  
 Data File : PP034052.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 16 Mar 2021 11:14  
 Operator : DD\AJ  
 Sample : M1662-07  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 X127-15A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 17 06:04:31 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP030921.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 12 12:21:17 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|--------|--------|--------|
| -----                       |        |       |         |        |        |        |
| System Monitoring Compounds |        |       |         |        |        |        |
| 1) SA Tetrachlo...          | 4.853  | 4.264 | 1821758 | 961313 | 21.055 | 23.663 |
| 2) SA Decachlor...          | 10.781 | 9.585 | 1636478 | 563211 | 19.377 | 21.106 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP031621\  
Data File : PP034052.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 16 Mar 2021 11:14  
Operator : DD\AJ  
Sample : M1662-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
X127-15A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 17 06:04:31 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP030921.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Mar 12 12:21:17 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

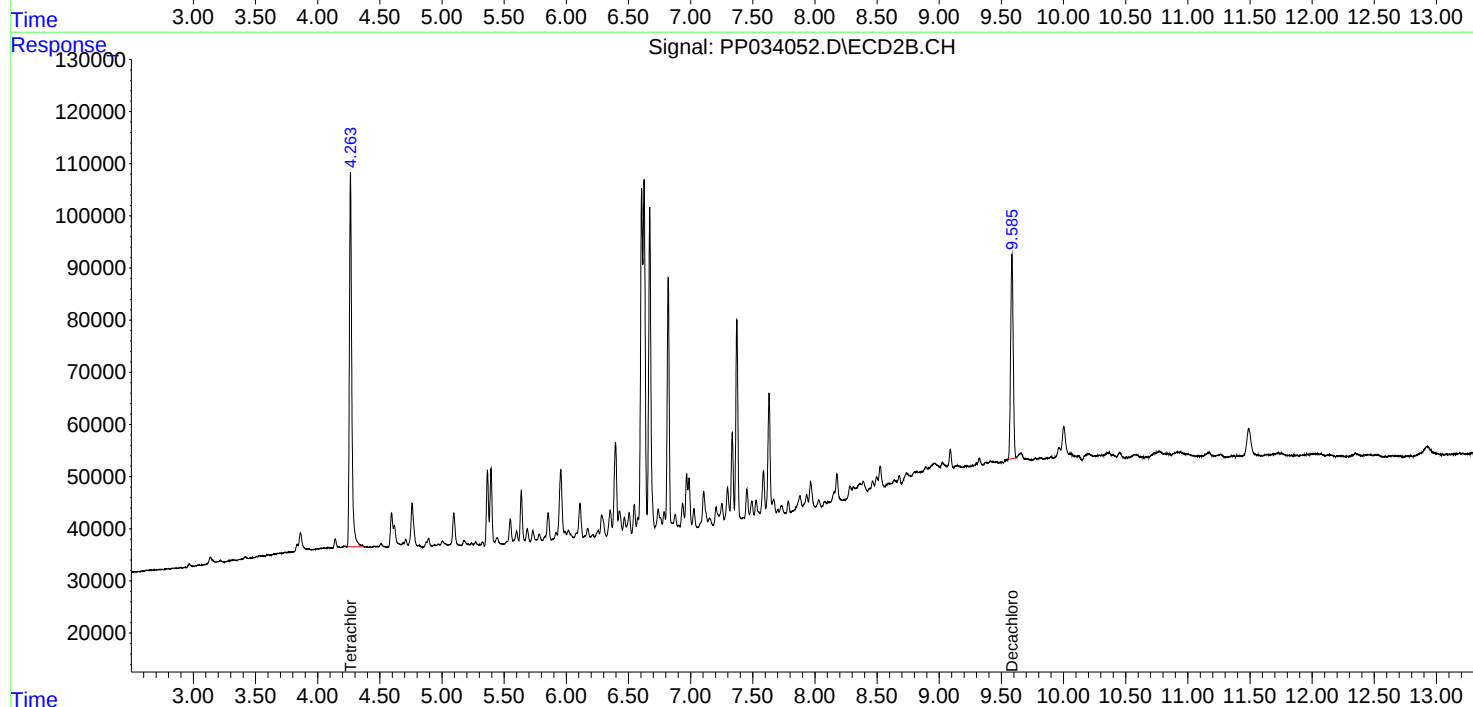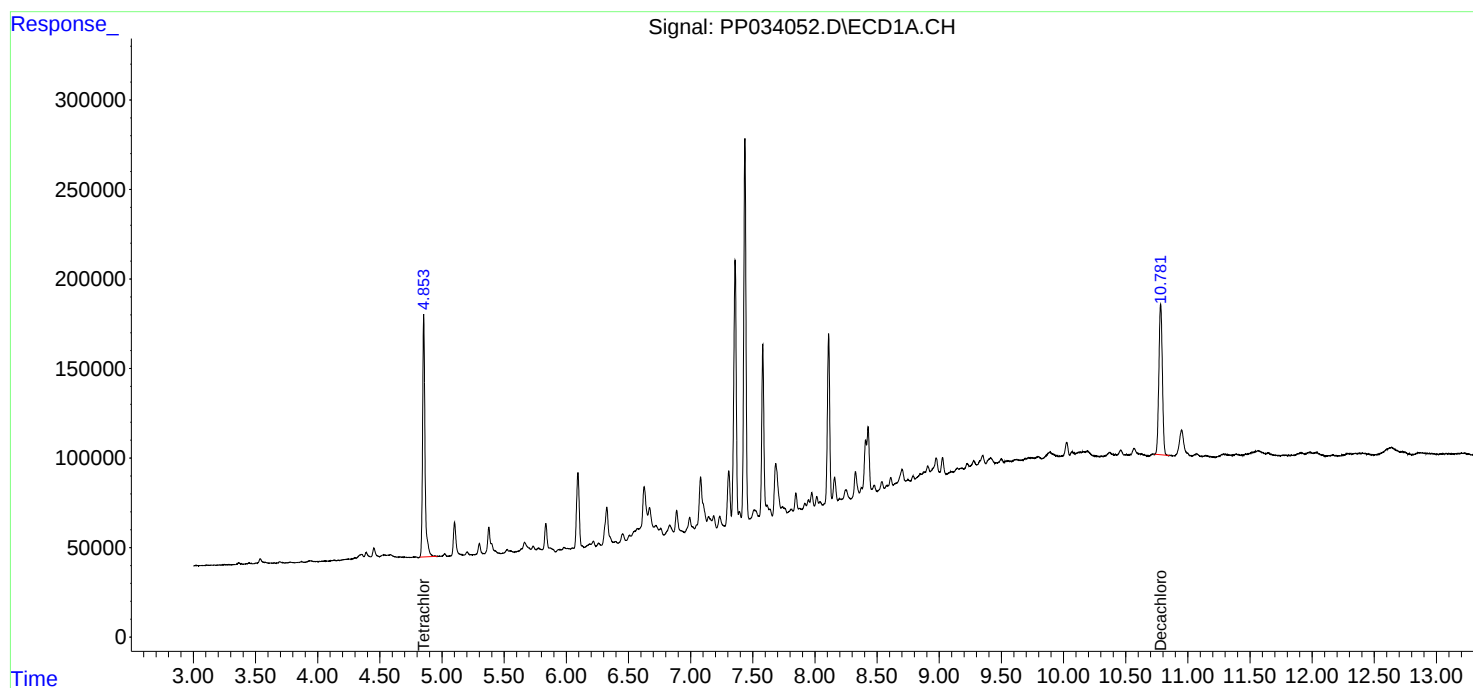


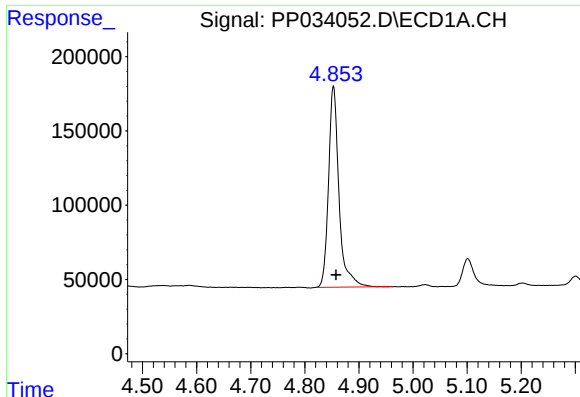

#1 Tetrachloro-m-xylene


R.T.: 4.853 min  
Delta R.T.: -0.005 min  
Response: 1821758  
Conc: 21.05 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
X127-15A

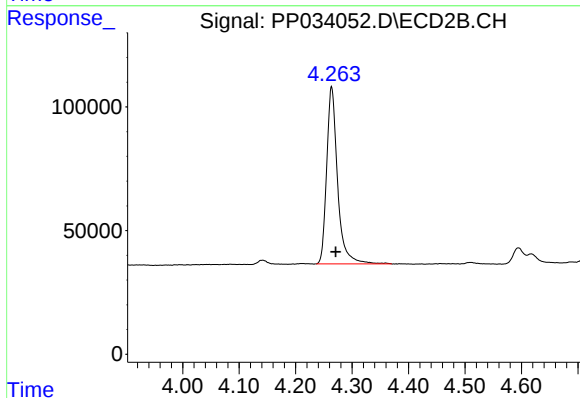


#1 Tetrachloro-m-xylene

R.T.: 4.264 min  
Delta R.T.: -0.007 min  
Response: 961313  
Conc: 23.66 ng/ml

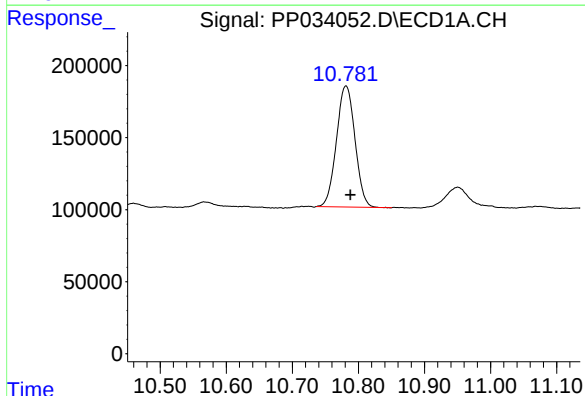

#2 Decachlorobiphenyl

R.T.: 10.781 min  
Delta R.T.: -0.007 min  
Response: 1636478  
Conc: 19.38 ng/ml

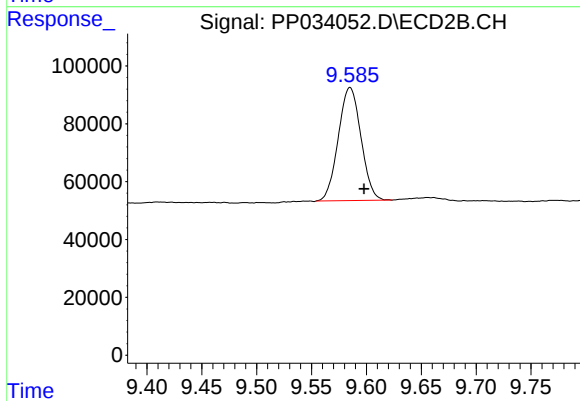

#2 Decachlorobiphenyl

R.T.: 9.585 min  
Delta R.T.: -0.013 min  
Response: 563211  
Conc: 21.11 ng/ml