

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
 Data File : PP034060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 13:28
 Operator : DD\AJ
 Sample : M1663-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-22A

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:36:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 06:07:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.854	4.265	1484289	854297	17.154	21.028
2) SA Decachlor...	10.781	9.586	1284048	479941	15.204	17.985
Target Compounds						
26) L6 AR-1254-1	7.077	6.395	756966	304329	259.120	186.668 #
27) L6 AR-1254-2	7.304	6.549	727221	225219	159.930	157.693
28) L6 AR-1254-3	7.683	6.970	1186659	572696	240.009	250.215
29) L6 AR-1254-4	7.977	7.205	637469	276168	185.849	217.279
30) L6 AR-1254-5	8.405	7.633	1859047	1867245	472.300	991.359m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
Data File : PP034060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 13:28
Operator : DD\AJ
Sample : M1663-12
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-22A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 06:07:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

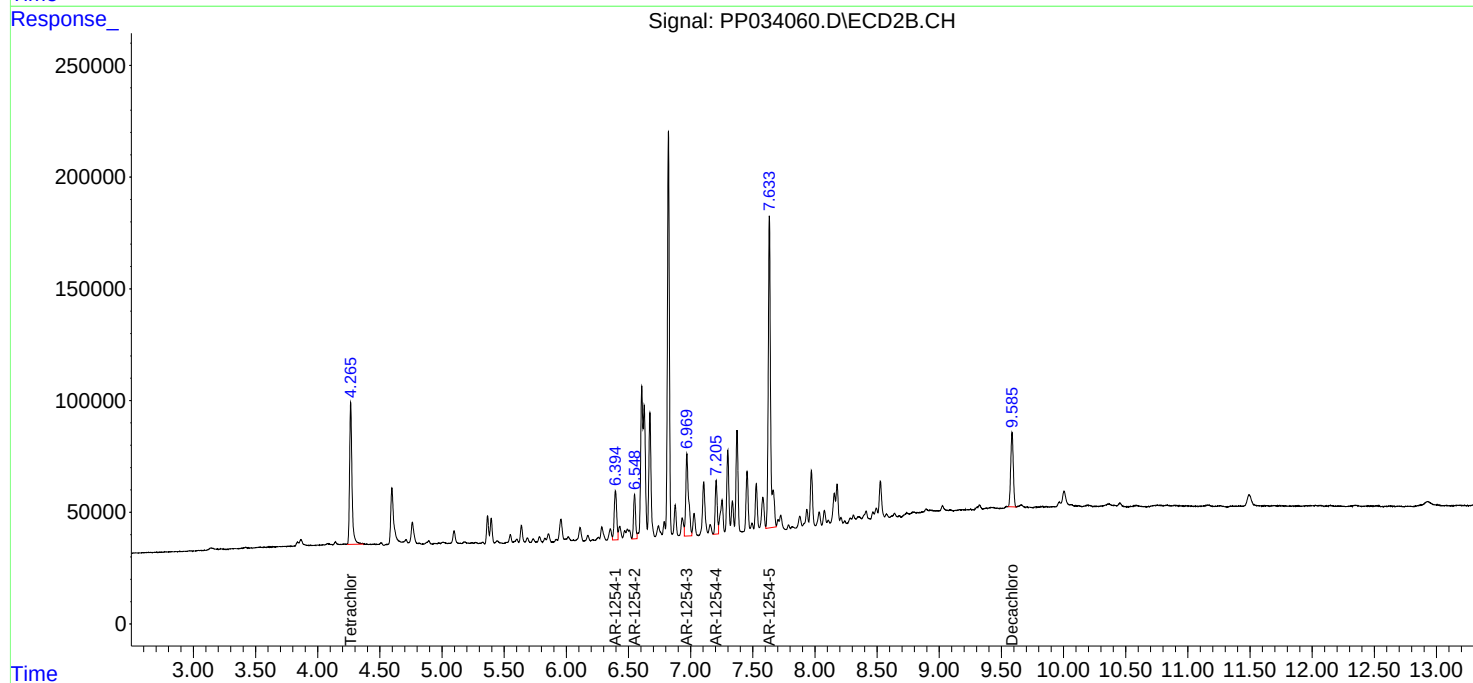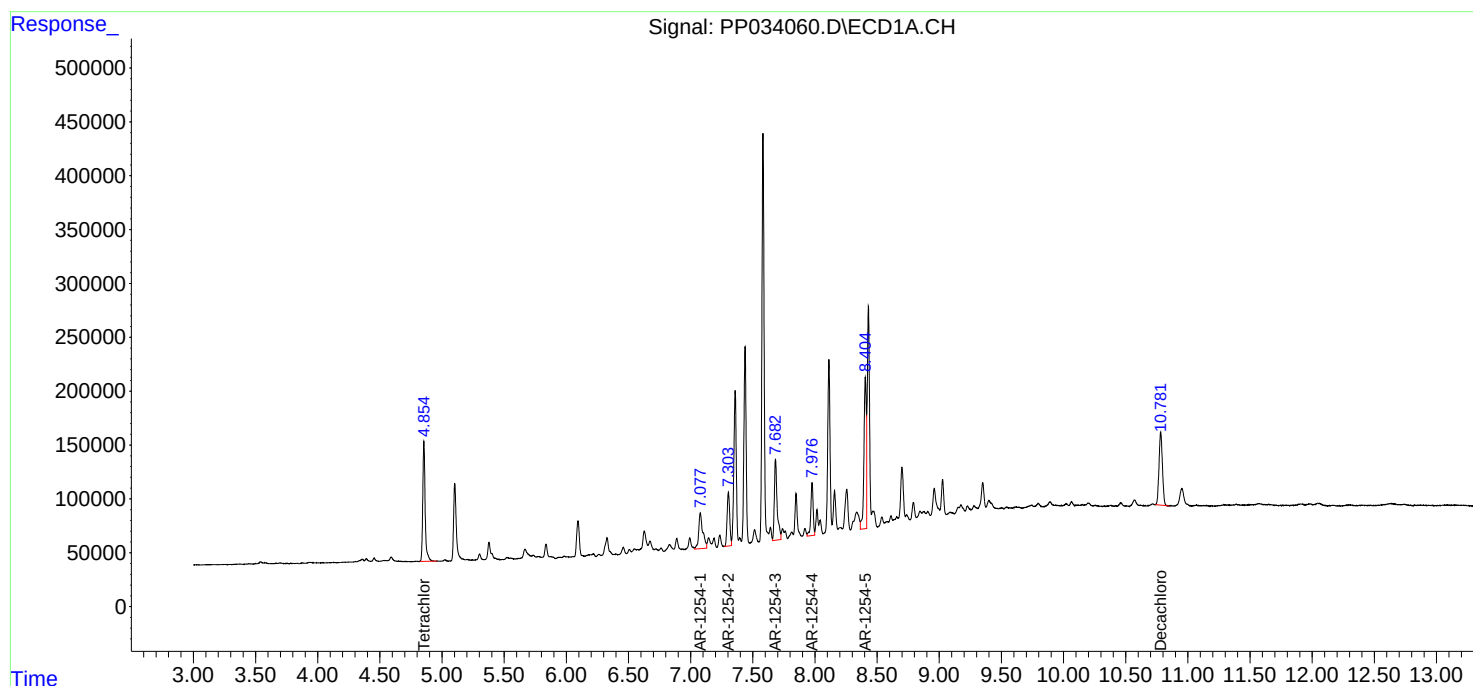

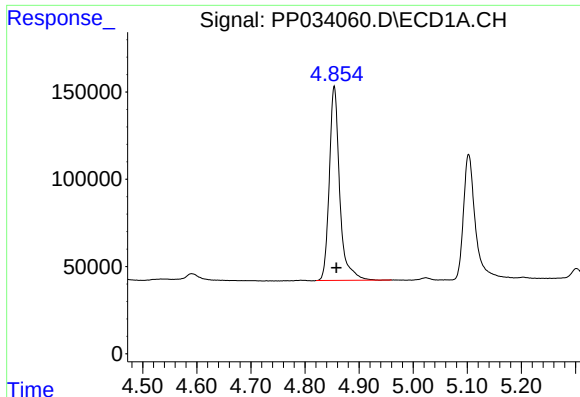


#1 Tetrachloro-m-xylene

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 1484289
Conc: 17.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:35 PM

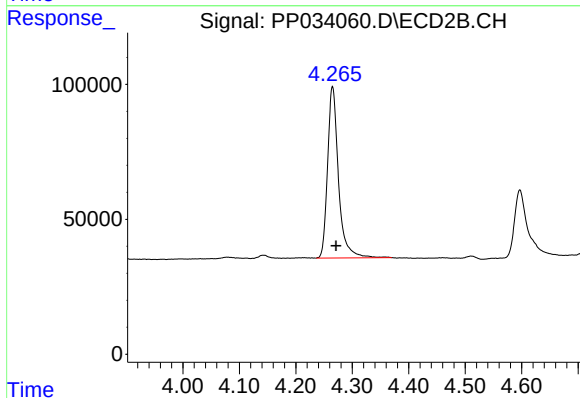


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 854297
Conc: 21.03 ng/ml

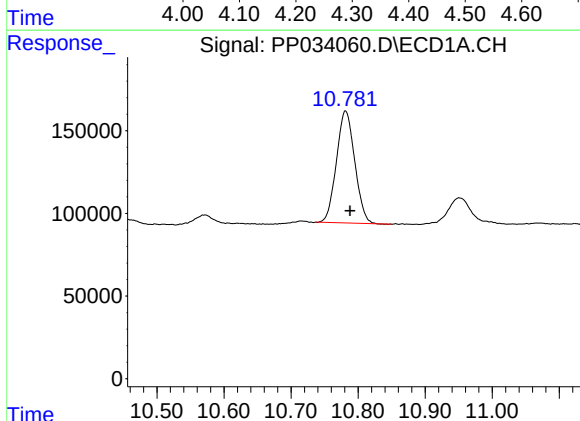


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 1284048
Conc: 15.20 ng/ml

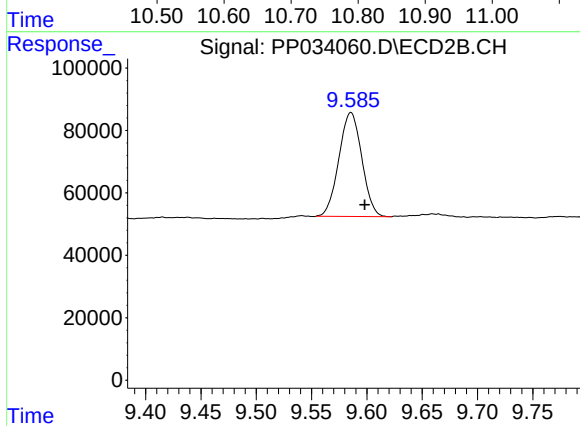

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.012 min
Response: 479941
Conc: 17.99 ng/ml

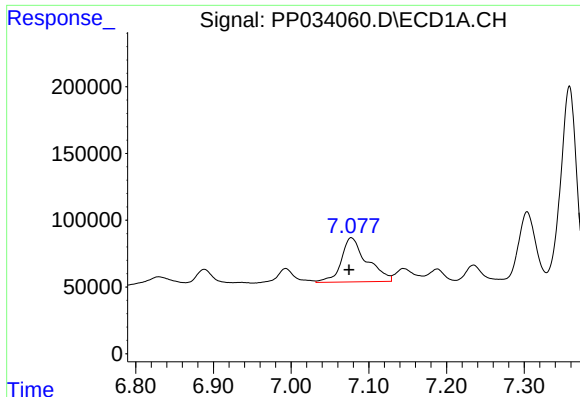


#26 AR-1254-1

R.T.: 7.077 min
Delta R.T.: 0.003 min
Response: 756966
Conc: 259.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:35 PM

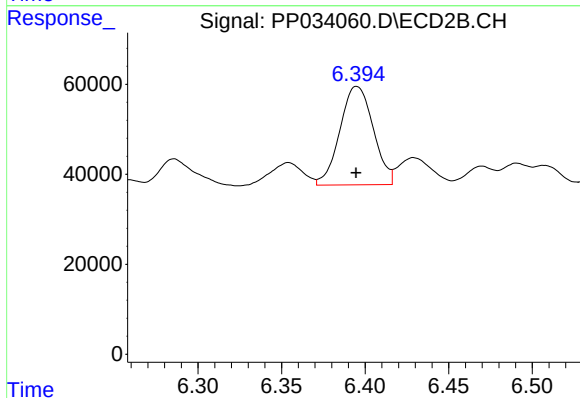


#26 AR-1254-1

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 304329
Conc: 186.67 ng/ml

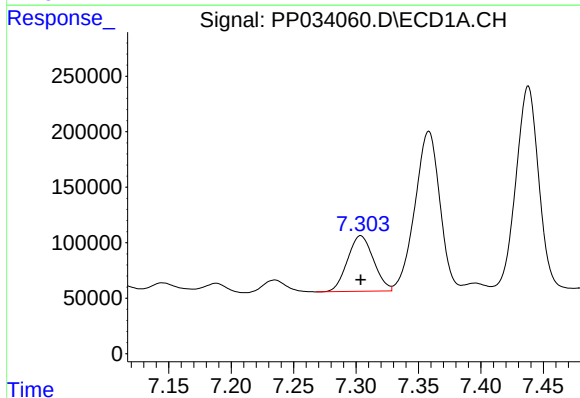


#27 AR-1254-2

R.T.: 7.304 min
Delta R.T.: 0.000 min
Response: 727221
Conc: 159.93 ng/ml

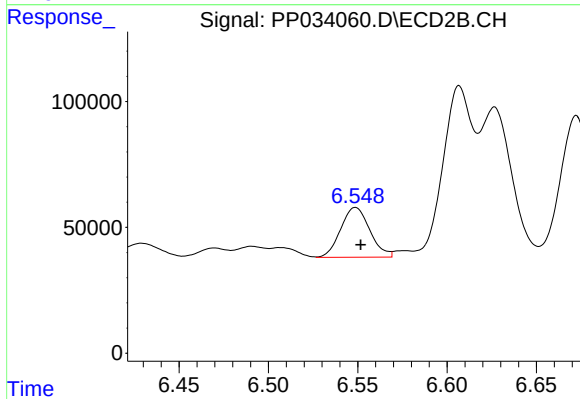

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 225219
Conc: 157.69 ng/ml

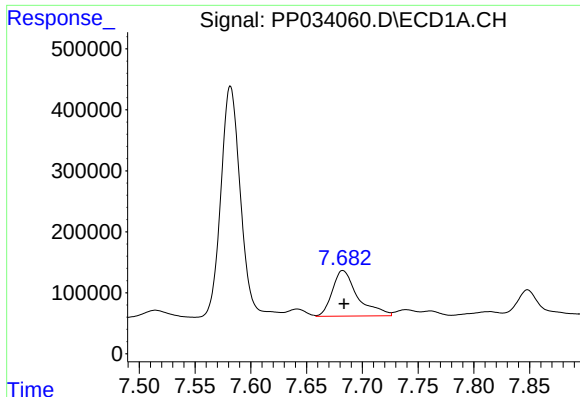


#28 AR-1254-3

R.T.: 7.683 min
Delta R.T.: 0.000 min
Response: 1186659
Conc: 240.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:35 PM

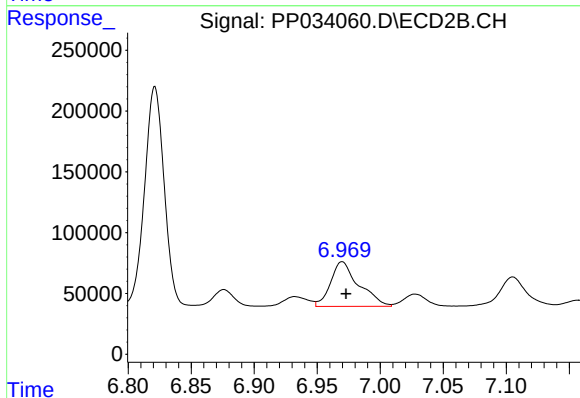


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 572696
Conc: 250.22 ng/ml

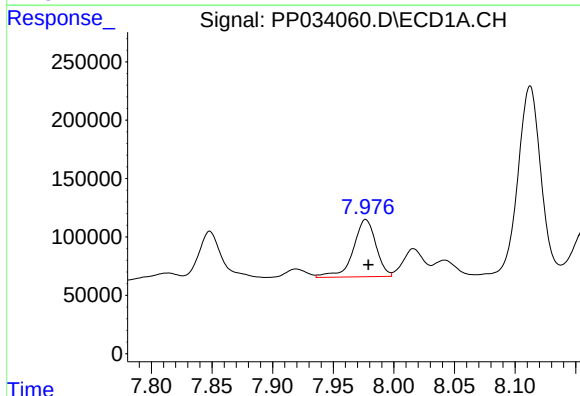


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.002 min
Response: 637469
Conc: 185.85 ng/ml

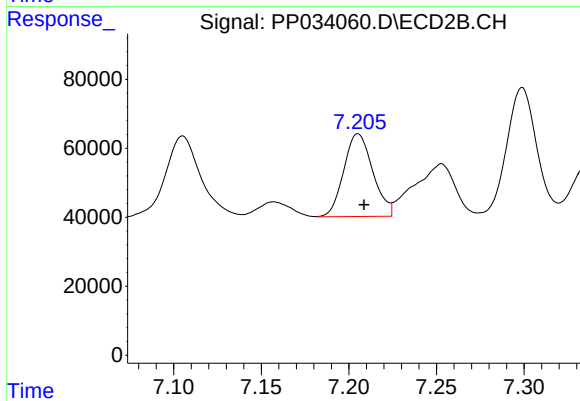

#29 AR-1254-4

R.T.: 7.205 min
Delta R.T.: -0.003 min
Response: 276168
Conc: 217.28 ng/ml

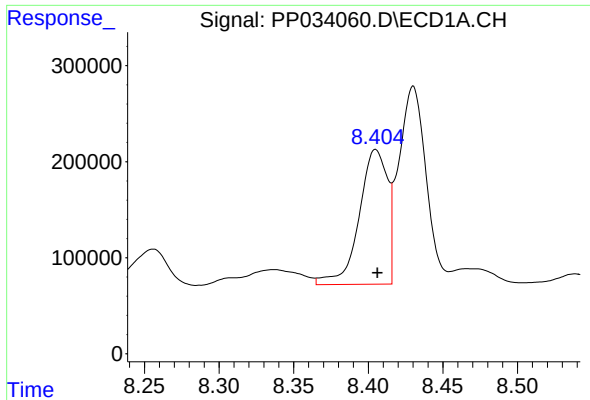


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.001 min
Response: 1859047
Conc: 472.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-22A

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:35 PM

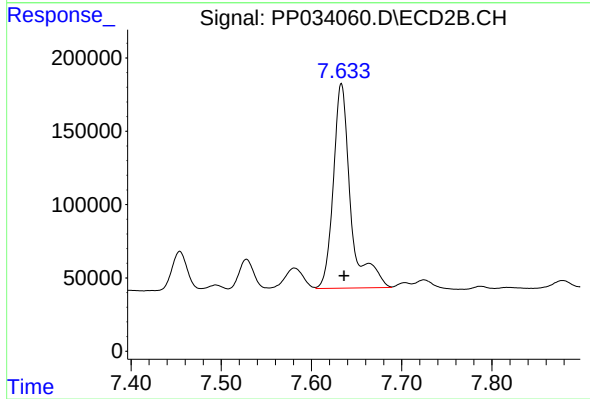

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.004 min
Response: 1867245
Conc: 991.36 ng/ml m