

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
 Data File : PP034061.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 13:45
 Operator : DD\AJ
 Sample : M1663-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-23A

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:36:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 06:08:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.853	4.265	1504914	855853	17.393	21.067
2) SA Decachlor...	10.781	9.586	1214903	437467	14.385	16.394
Target Compounds						
26) L6 AR-1254-1	7.076	6.395	435449	293621	149.060m	180.100
27) L6 AR-1254-2	7.303	6.549	692534	200963	152.302	140.710
28) L6 AR-1254-3	7.682	6.970	1127473	582317	228.038	254.419
29) L6 AR-1254-4	7.976	7.206	600055	258298	174.941	203.220
30) L6 AR-1254-5	8.404	7.633	1798842	1781983	457.005	946.092 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
Data File : PP034061.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 13:45
Operator : DD\AJ
Sample : M1663-15
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-23A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 06:08:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

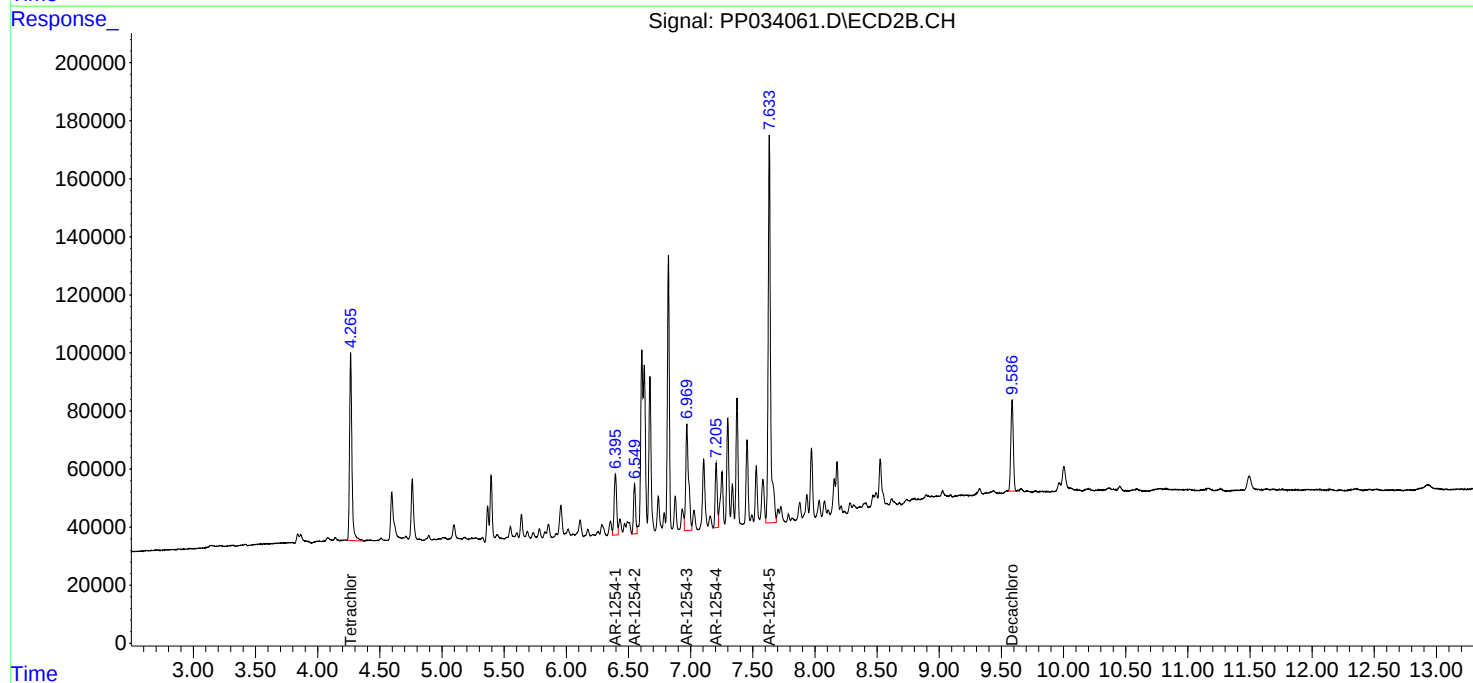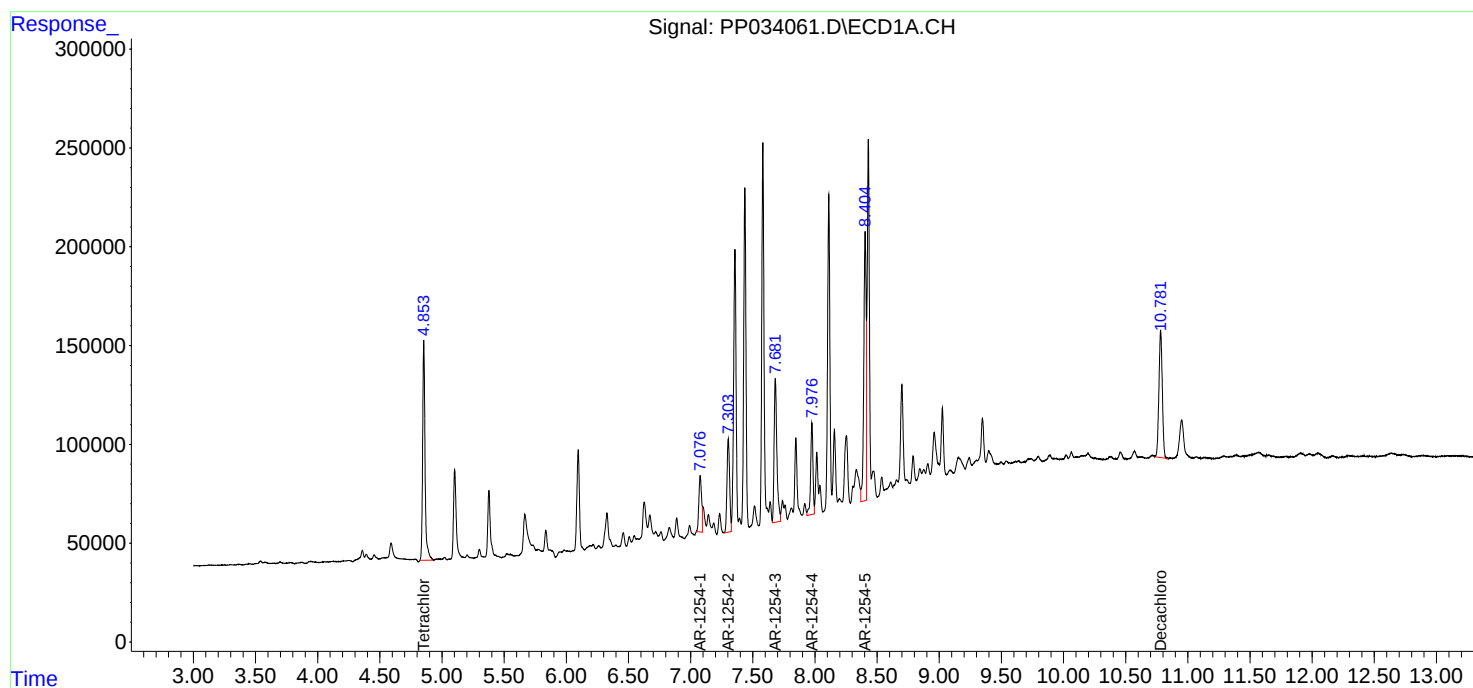

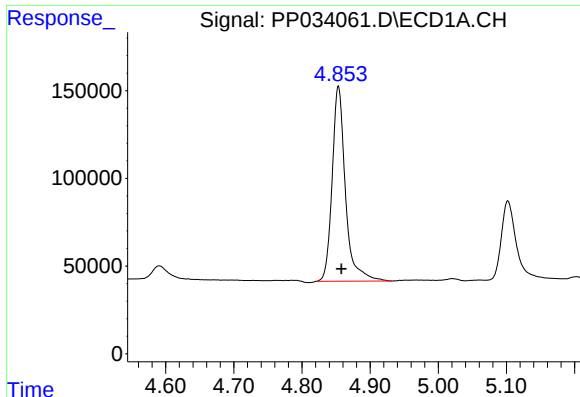


#1 Tetrachloro-m-xylene

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 1504914
Conc: 17.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:37 PM

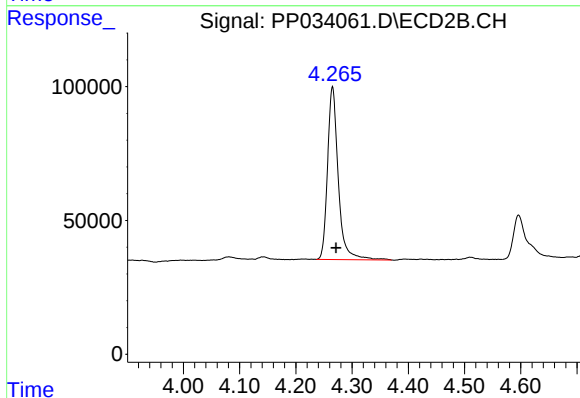

#1 Tetrachloro-m-xylene


R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 855853
Conc: 21.07 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 1214903
Conc: 14.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.012 min
Response: 437467
Conc: 16.39 ng/ml

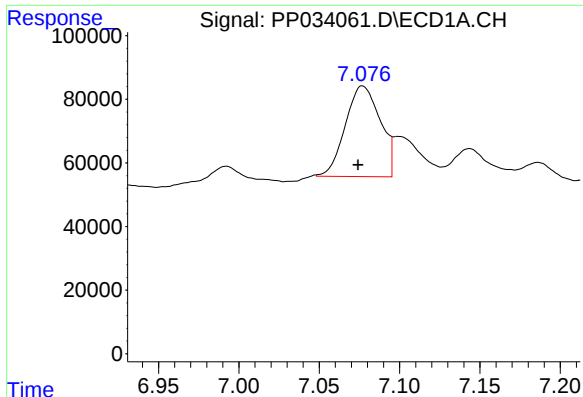


#26 AR-1254-1

R.T.: 7.076 min
Delta R.T.: 0.002 min
Response: 435449
Conc: 149.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:37 PM

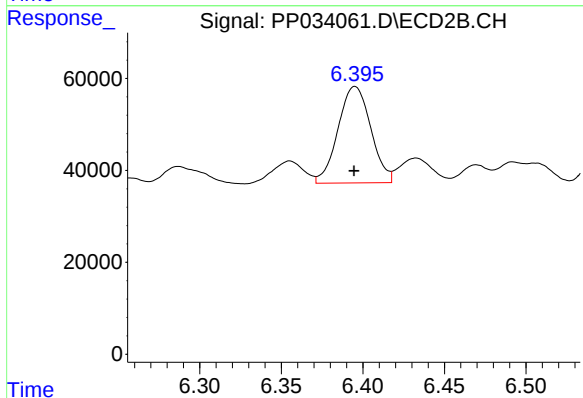


#26 AR-1254-1

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 293621
Conc: 180.10 ng/ml

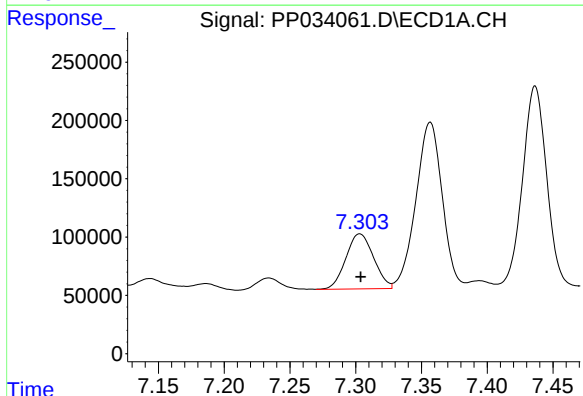


#27 AR-1254-2

R.T.: 7.303 min
Delta R.T.: 0.000 min
Response: 692534
Conc: 152.30 ng/ml

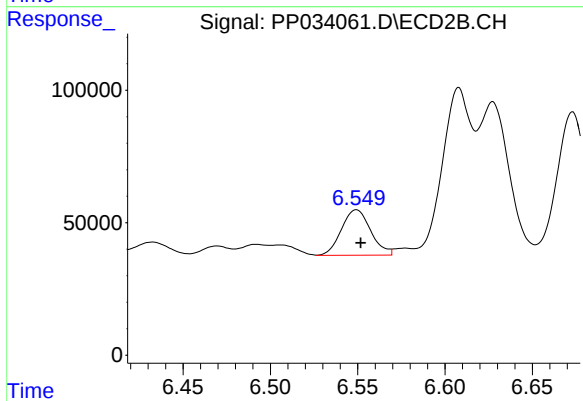

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.002 min
Response: 200963
Conc: 140.71 ng/ml

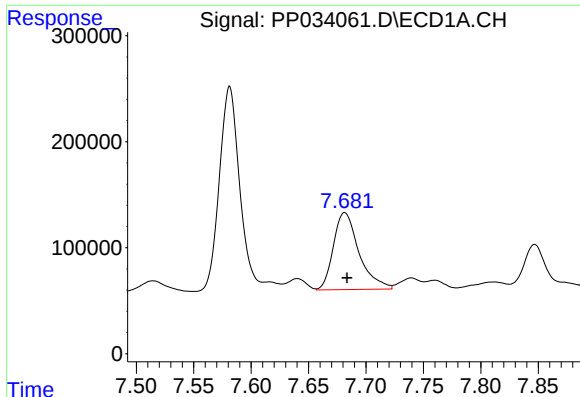


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.002 min
Response: 1127473
Conc: 228.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:37 PM

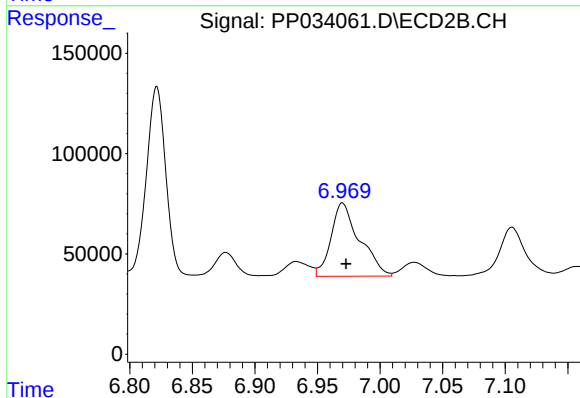


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 582317
Conc: 254.42 ng/ml

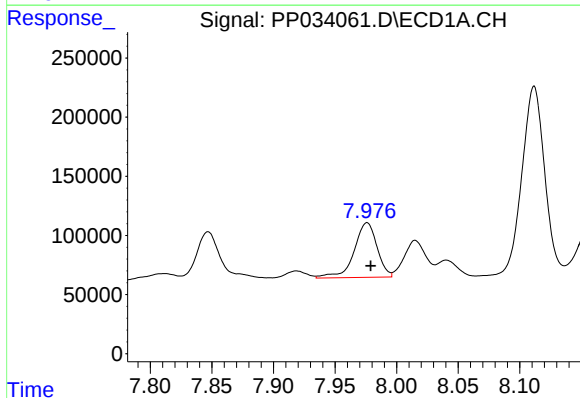


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 600055
Conc: 174.94 ng/ml

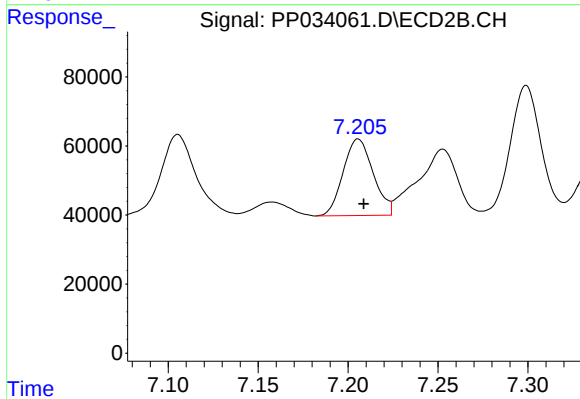

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 258298
Conc: 203.22 ng/ml

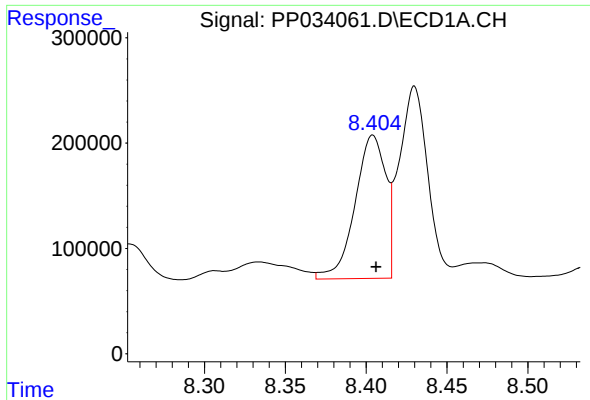


#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 1798842
Conc: 457.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-23A

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:37 PM

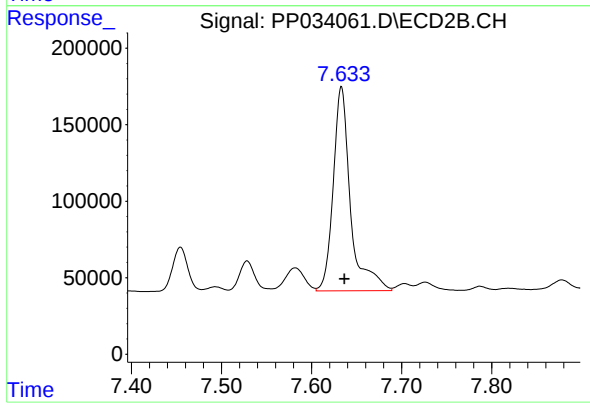

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 1781983
Conc: 946.09 ng/ml