

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
 Data File : PP034064.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 14:36
 Operator : DD\AJ
 Sample : M1661-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-7A

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:36:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 06:09:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.854	4.265	373295	205399	4.314	5.056
2)	SA Decachlor...	10.781	9.586	488675	177197	5.786	6.640
Target Compounds							
26)	L6 AR-1254-1	7.078	6.392	1328814	123083	454.872m	75.496m#
27)	L6 AR-1254-2	7.301	6.549	522616	258656	114.934m	181.105m#
28)	L6 AR-1254-3	7.685	6.970	1445875	559668	292.436m	244.524
29)	L6 AR-1254-4	7.976	7.206	684764	323802	199.638m	254.757 #
30)	L6 AR-1254-5	8.404	7.634	1570079	1282873	398.886m	681.104 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
Data File : PP034064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 14:36
Operator : DD\AJ
Sample : M1661-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-7A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 06:09:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

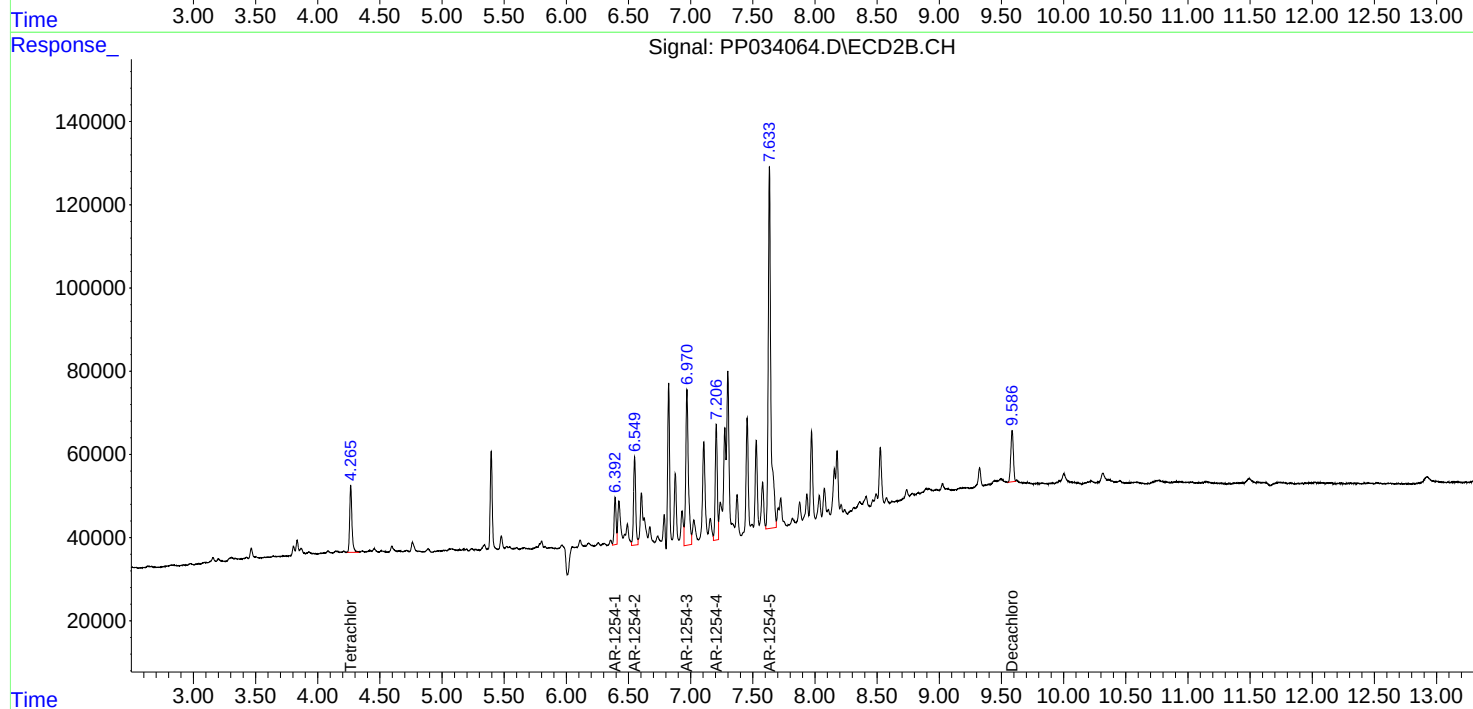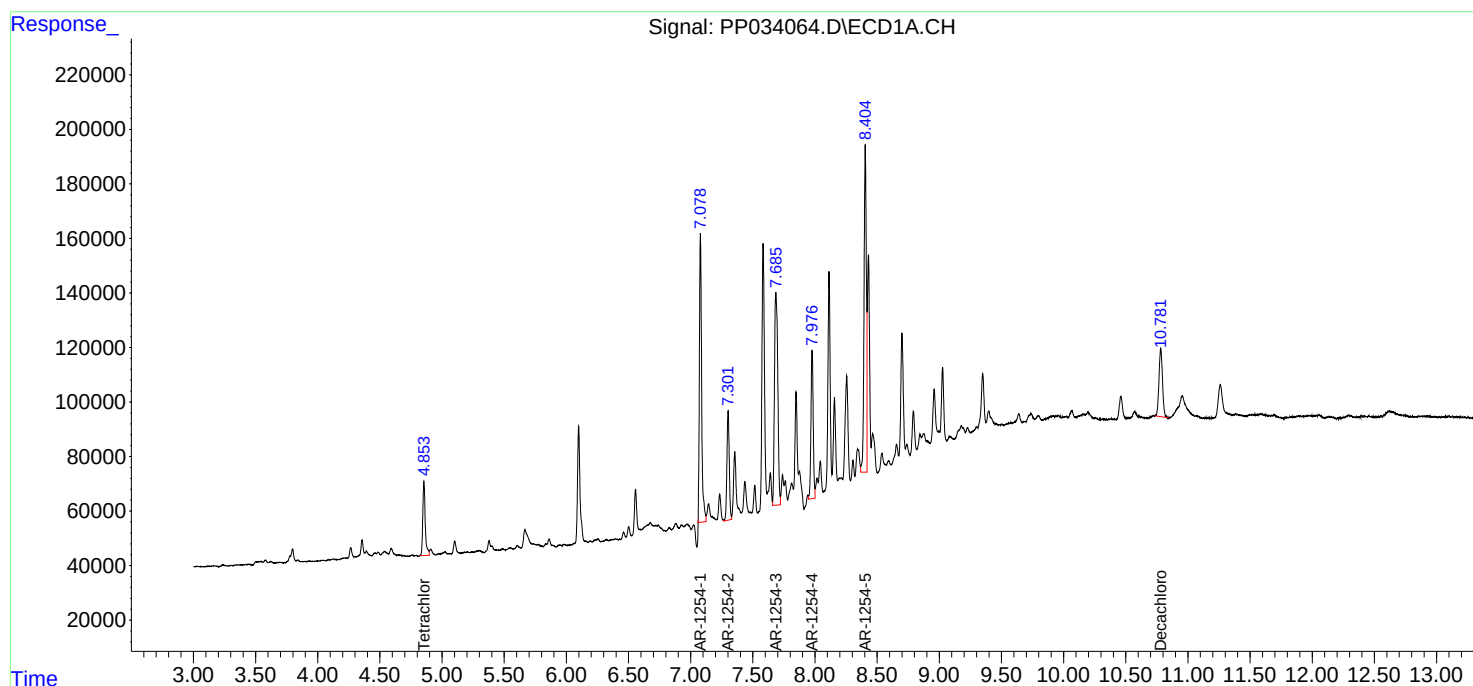

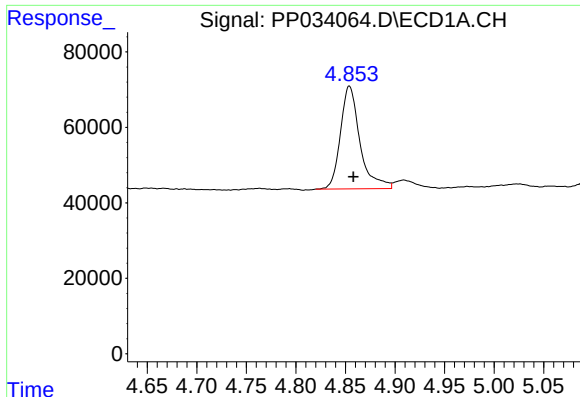


#1 Tetrachloro-m-xylene

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 373295
Conc: 4.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-7A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:39 PM

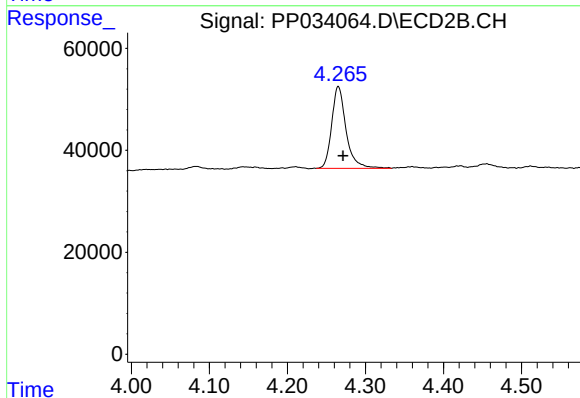


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 205399
Conc: 5.06 ng/ml

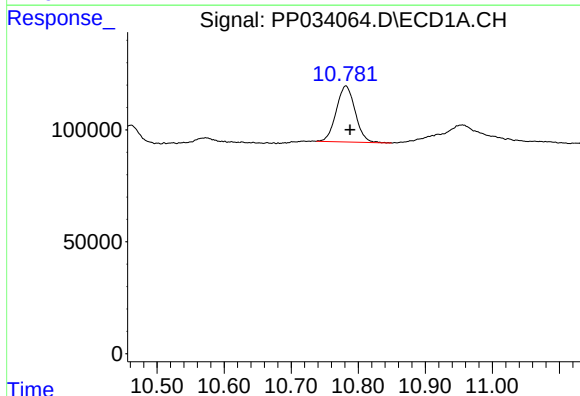


#2 Decachlorobiphenyl

R.T.: 10.781 min
Delta R.T.: -0.007 min
Response: 488675
Conc: 5.79 ng/ml

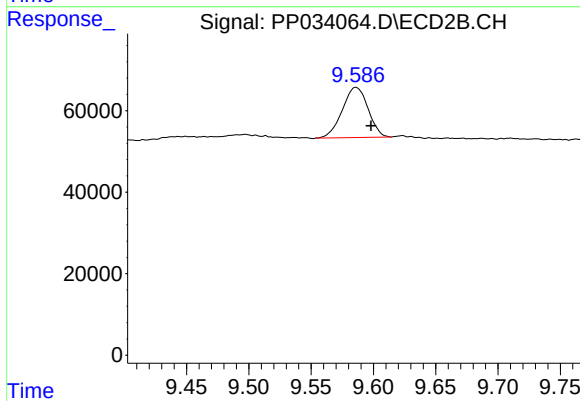

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.012 min
Response: 177197
Conc: 6.64 ng/ml

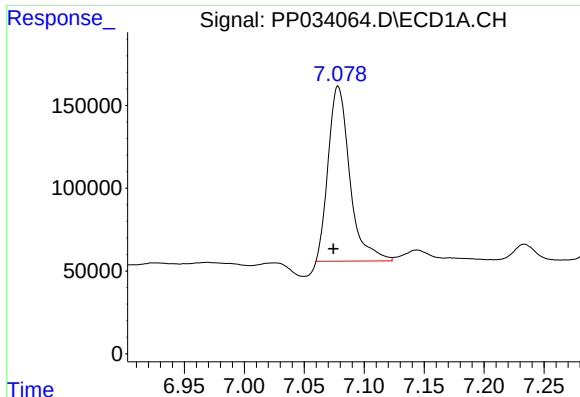


#26 AR-1254-1

R.T.: 7.078 min
Delta R.T.: 0.003 min
Response: 1328814
Conc: 454.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-7A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:39 PM

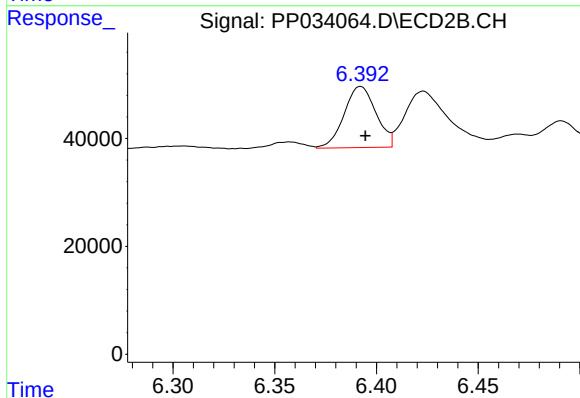


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 123083
Conc: 75.50 ng/ml m

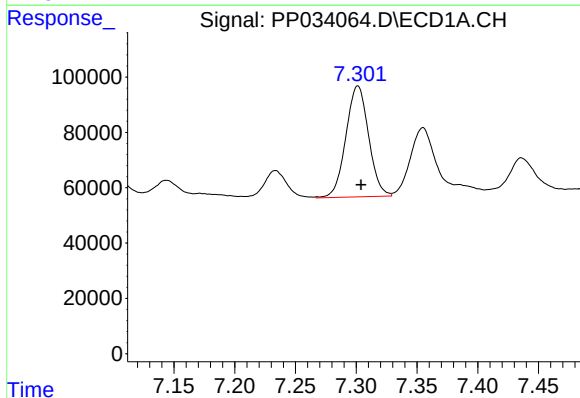


#27 AR-1254-2

R.T.: 7.301 min
Delta R.T.: -0.003 min
Response: 522616
Conc: 114.93 ng/ml m

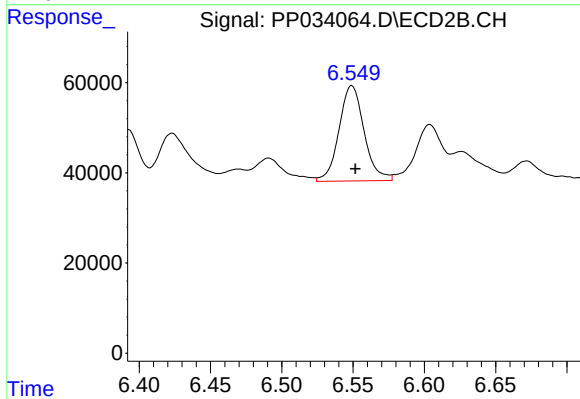

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 258656
Conc: 181.11 ng/ml m

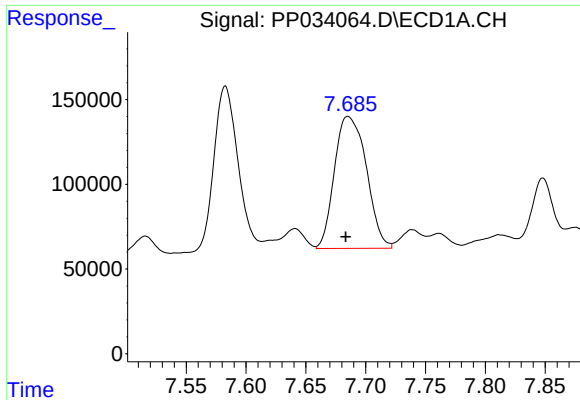


#28 AR-1254-3

R.T.: 7.685 min
Delta R.T.: 0.001 min
Response: 1445875
Conc: 292.44 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-7A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:39 PM

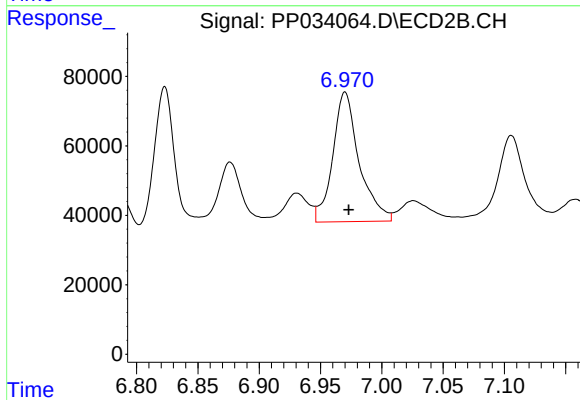


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 559668
Conc: 244.52 ng/ml

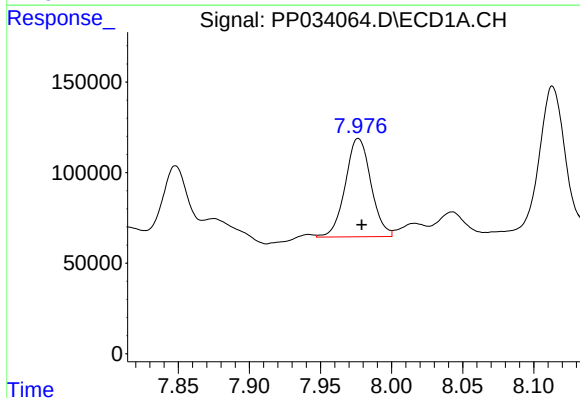


#29 AR-1254-4

R.T.: 7.976 min
Delta R.T.: -0.003 min
Response: 684764
Conc: 199.64 ng/ml m

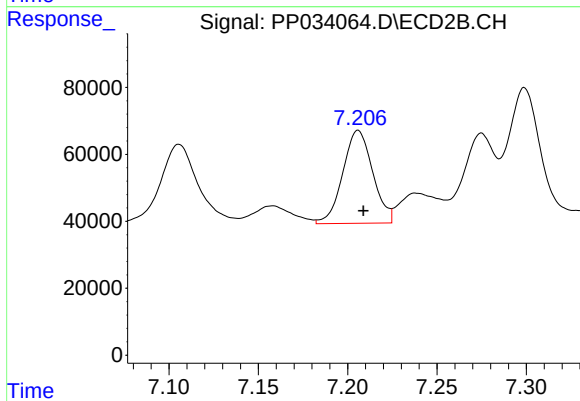

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 323802
Conc: 254.76 ng/ml

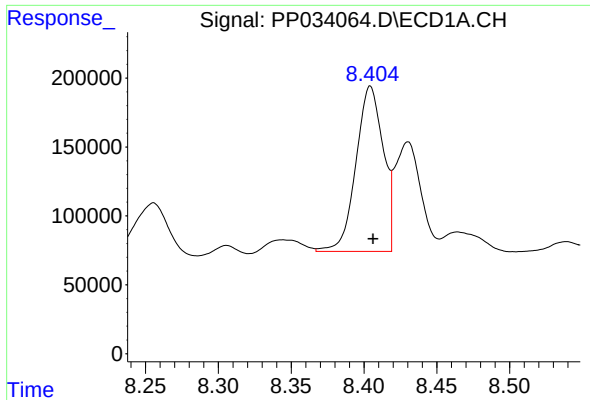


#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 1570079
Conc: 398.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-7A

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:39 PM

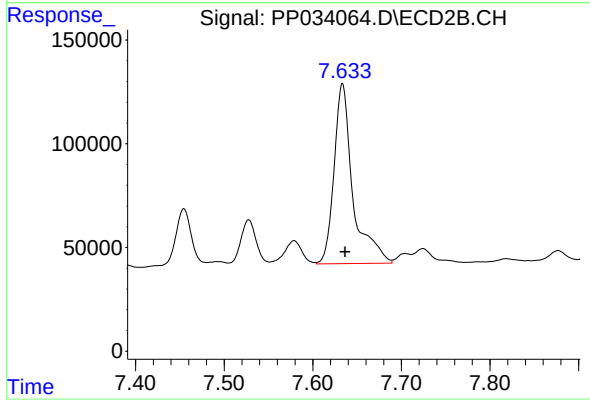

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.003 min
Response: 1282873
Conc: 681.10 ng/ml