

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
 Data File : PP034065.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 14:53
 Operator : DD\AJ
 Sample : M1661-04DL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-8ADL

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:36:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 06:09:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.854	4.265	190152	102322	2.198m	2.519
2) SA Decachlor...	10.783	9.586	153755	58469	1.821	2.191
Target Compounds						
26) L6 AR-1254-1	7.073	6.392	462647	317742	158.371	194.895
27) L6 AR-1254-2	7.302	6.549	1303501	582643	286.666	407.953 #
28) L6 AR-1254-3	7.682	6.970	2063059	1185858	417.265	518.111
29) L6 AR-1254-4	7.978	7.206	2009013	891045	585.712	701.044
30) L6 AR-1254-5	8.406	7.634	4502981	2779649	1144.004	1475.773 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
Data File : PP034065.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 14:53
Operator : DD\AJ
Sample : M1661-04DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-8ADL


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 06:09:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

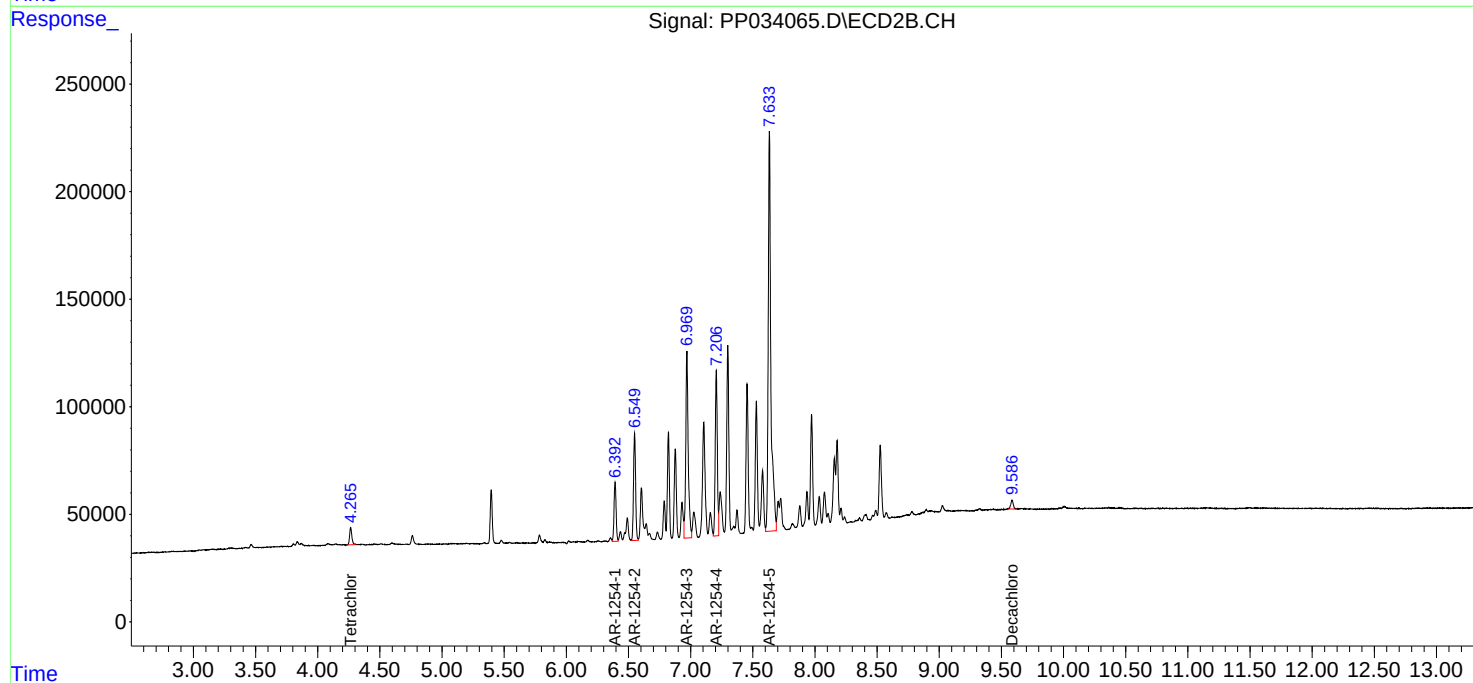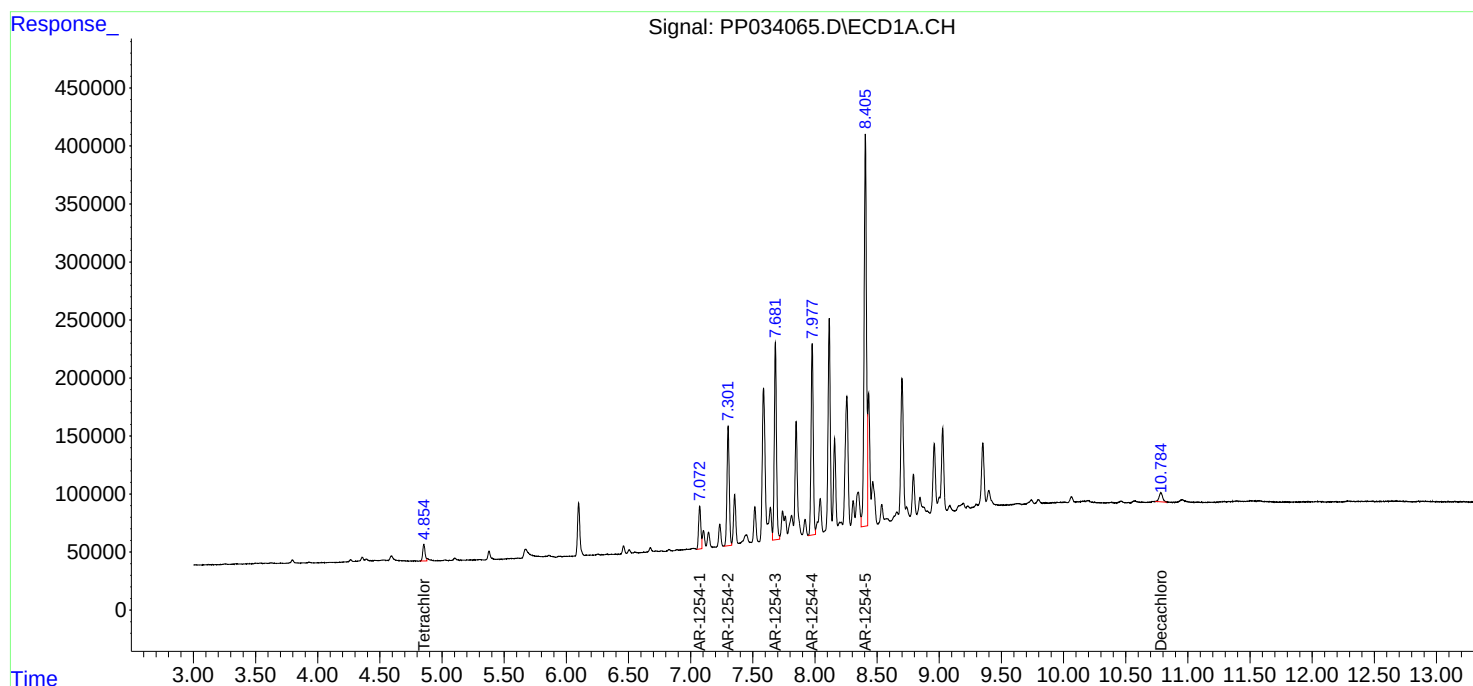

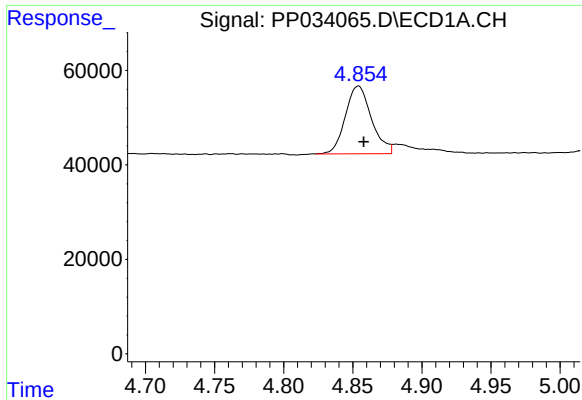


#1 Tetrachloro-m-xylene

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 190152
Conc: 2.20 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-8ADL


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:41 PM

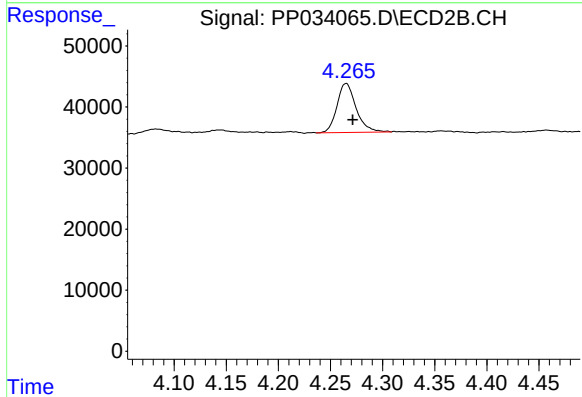


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.006 min
Response: 102322
Conc: 2.52 ng/ml

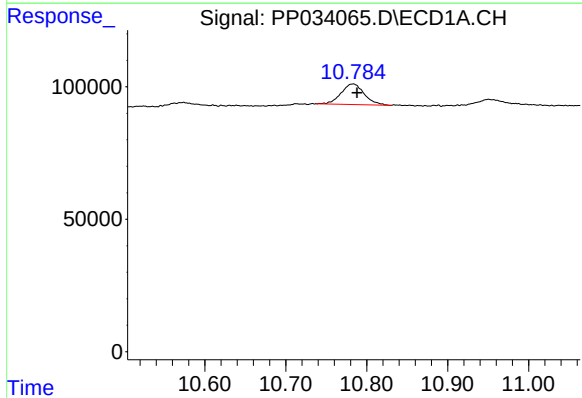


#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: -0.005 min
Response: 153755
Conc: 1.82 ng/ml

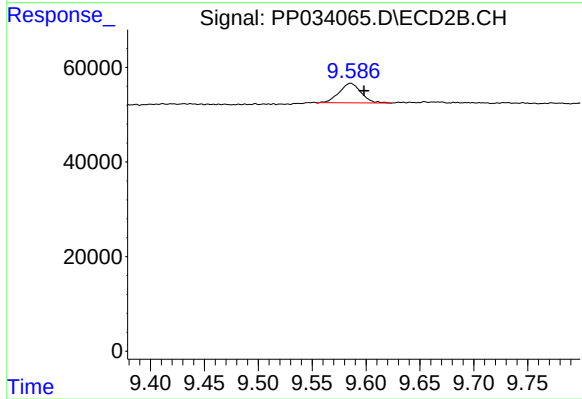

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.012 min
Response: 58469
Conc: 2.19 ng/ml

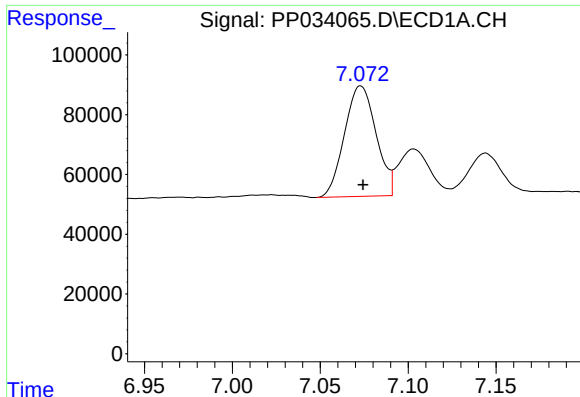


#26 AR-1254-1

R.T.: 7.073 min
Delta R.T.: -0.001 min
Response: 462647
Conc: 158.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-8ADL


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:41 PM

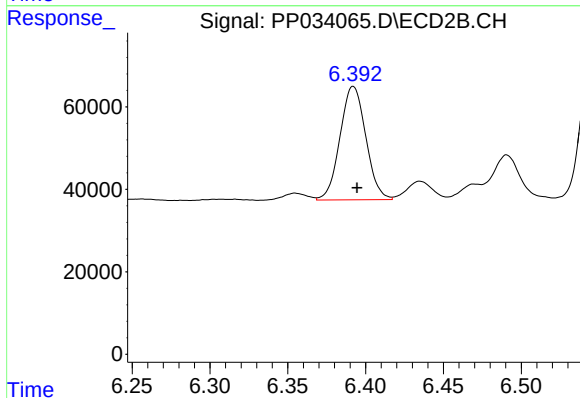


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: -0.002 min
Response: 317742
Conc: 194.90 ng/ml

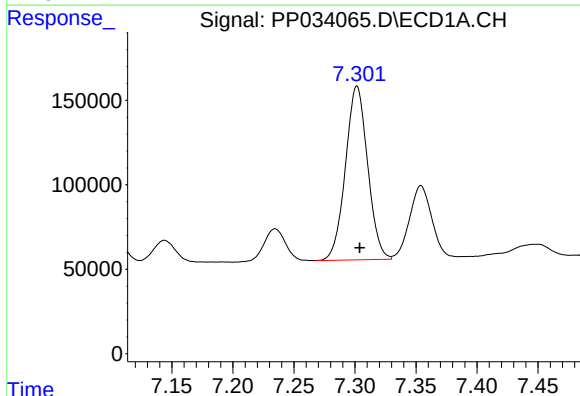


#27 AR-1254-2

R.T.: 7.302 min
Delta R.T.: -0.002 min
Response: 1303501
Conc: 286.67 ng/ml

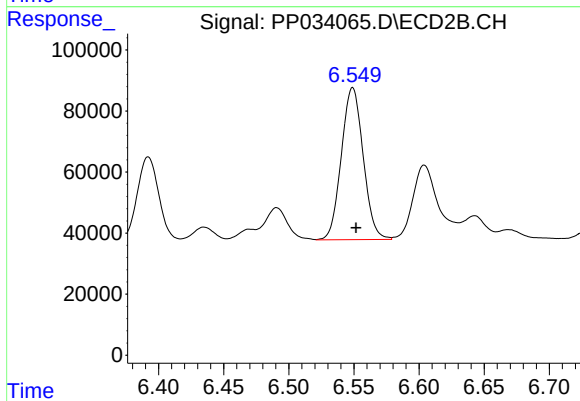

#27 AR-1254-2

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 582643
Conc: 407.95 ng/ml

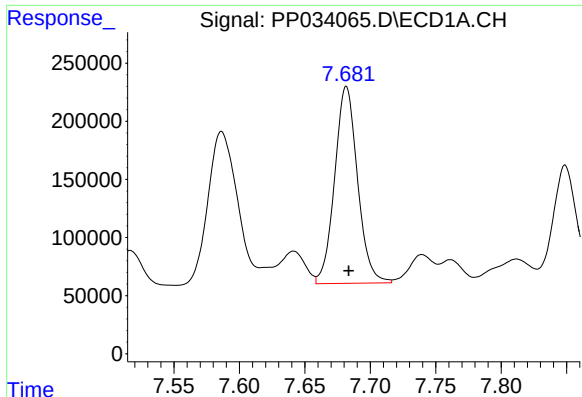


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.002 min
Response: 2063059
Conc: 417.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-8ADL


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:41 PM

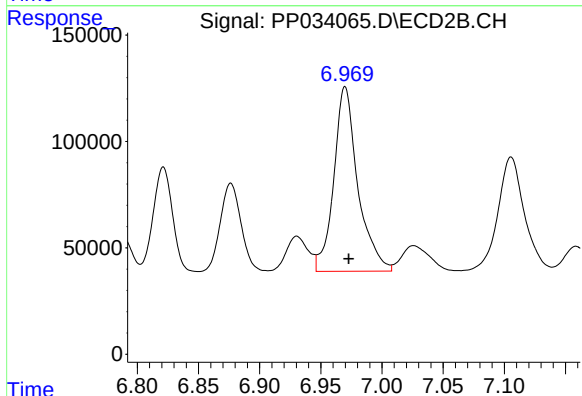


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 1185858
Conc: 518.11 ng/ml

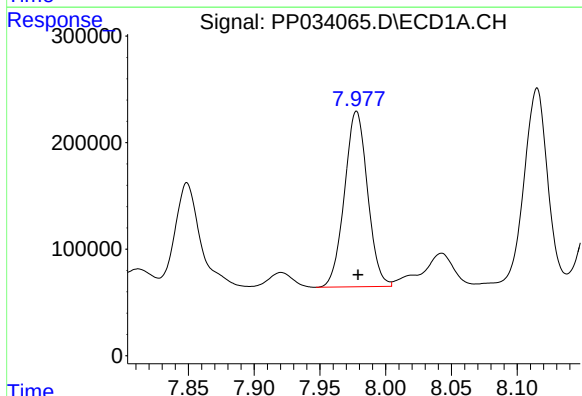


#29 AR-1254-4

R.T.: 7.978 min
Delta R.T.: -0.001 min
Response: 2009013
Conc: 585.71 ng/ml

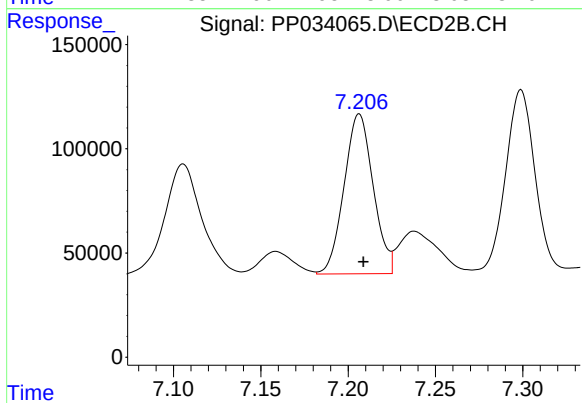

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 891045
Conc: 701.04 ng/ml

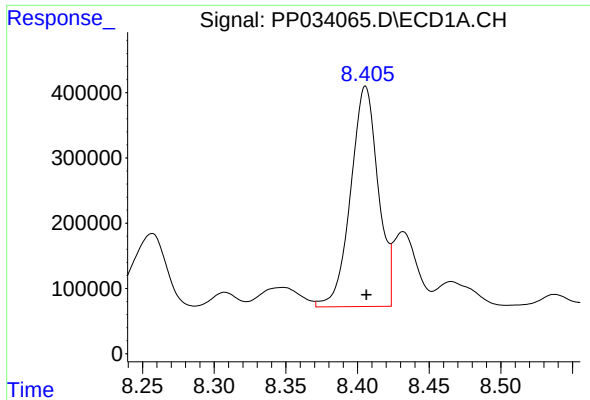


#30 AR-1254-5

R.T.: 8.406 min
Delta R.T.: 0.000 min
Response: 4502981
Conc: 1144.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-8ADL

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:41 PM

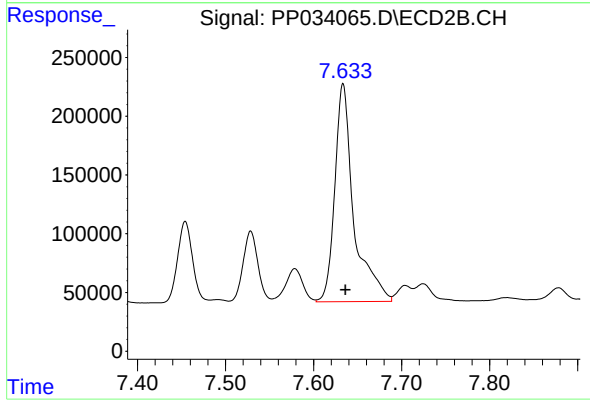

#30 AR-1254-5

R.T.: 7.634 min
Delta R.T.: -0.003 min
Response: 2779649
Conc: 1475.77 ng/ml