

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
 Data File : PP034066.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 15:10
 Operator : DD\AJ
 Sample : M1661-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-10A

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:36:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 06:10:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 12 12:21:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.855	4.266	1634794	897958	18.894	22.103
2)	SA Decachlor...	10.784	9.581f	1575155	996032	18.651	37.325m#
Target Compounds							
26)	L6 AR-1254-1	7.072	6.393	250973	183768	85.912	112.719 #
27)	L6 AR-1254-2	7.302	6.550	787208	365418	173.123	255.857 #
28)	L6 AR-1254-3	7.682	6.970	1671474	963433	338.065	420.932
29)	L6 AR-1254-4	7.977	7.206	1121469	485609	326.955	382.061
30)	L6 AR-1254-5	8.405	7.633	3942234	4097609	1001.544	2175.506 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031621\
Data File : PP034066.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 15:10
Operator : DD\AJ
Sample : M1661-10
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-10A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 06:10:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 12 12:21:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

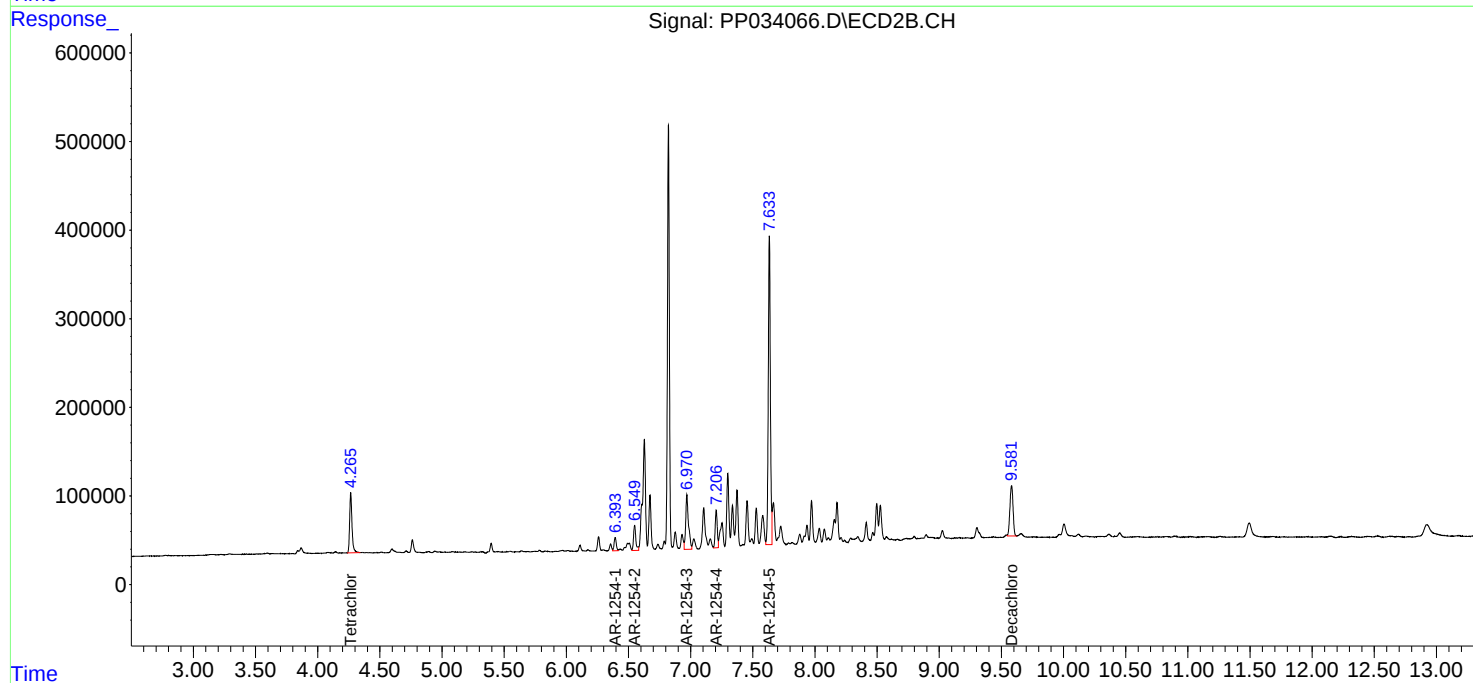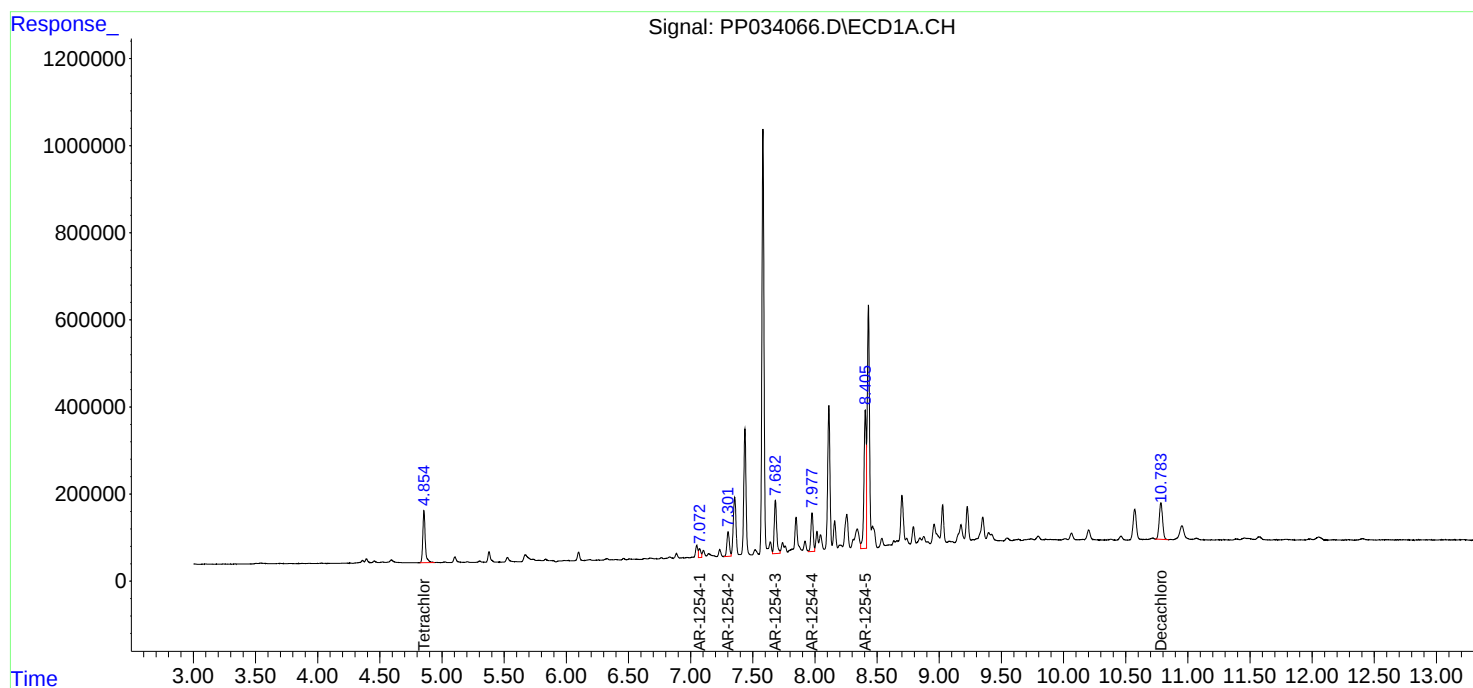

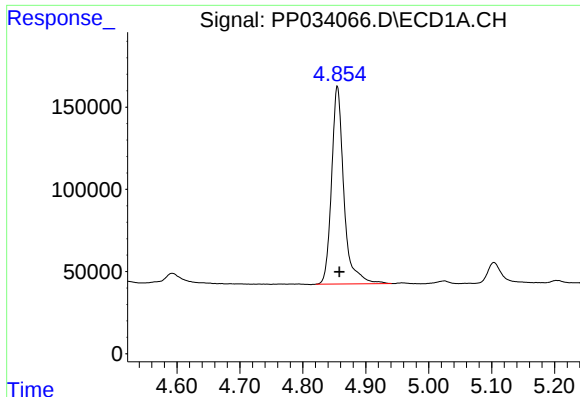


#1 Tetrachloro-m-xylene

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 1634794
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-10A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:43 PM

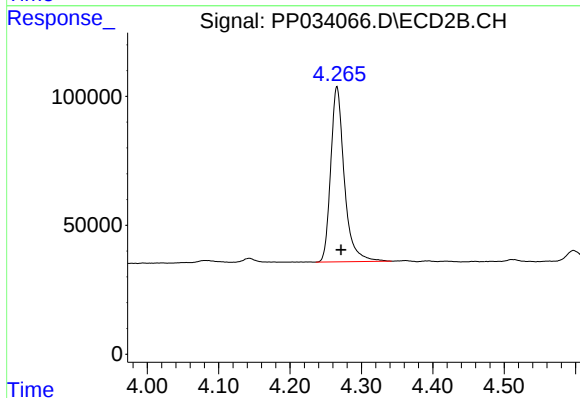


#1 Tetrachloro-m-xylene

R.T.: 4.266 min
Delta R.T.: -0.005 min
Response: 897958
Conc: 22.10 ng/ml

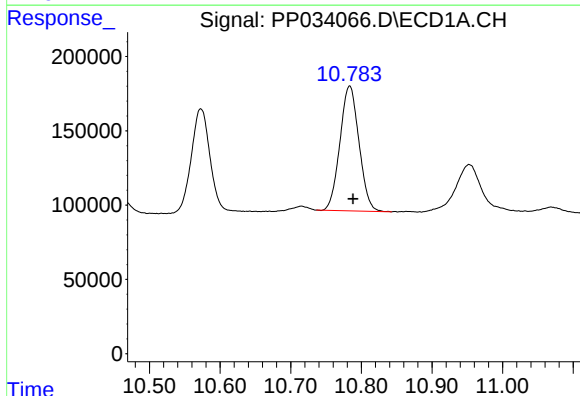


#2 Decachlorobiphenyl

R.T.: 10.784 min
Delta R.T.: -0.004 min
Response: 1575155
Conc: 18.65 ng/ml

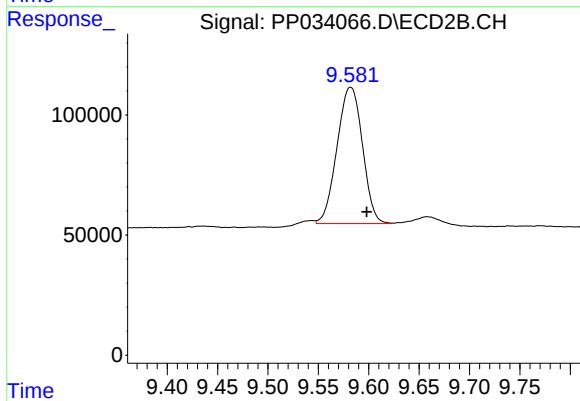

#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: -0.017 min
Response: 996032
Conc: 37.33 ng/ml m

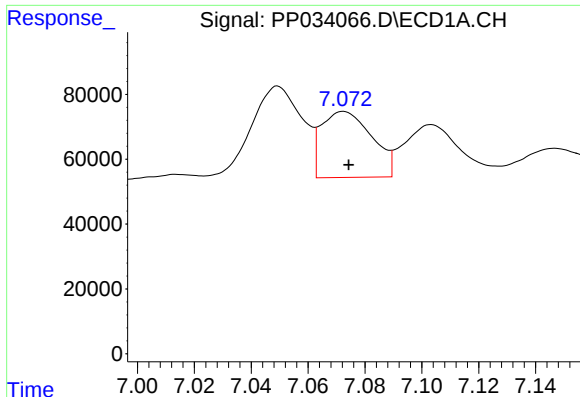


#26 AR-1254-1

R.T.: 7.072 min
Delta R.T.: -0.002 min
Response: 250973
Conc: 85.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-10A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:43 PM

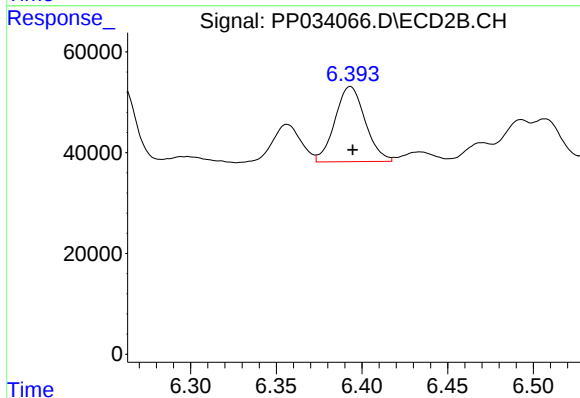


#26 AR-1254-1

R.T.: 6.393 min
Delta R.T.: -0.001 min
Response: 183768
Conc: 112.72 ng/ml

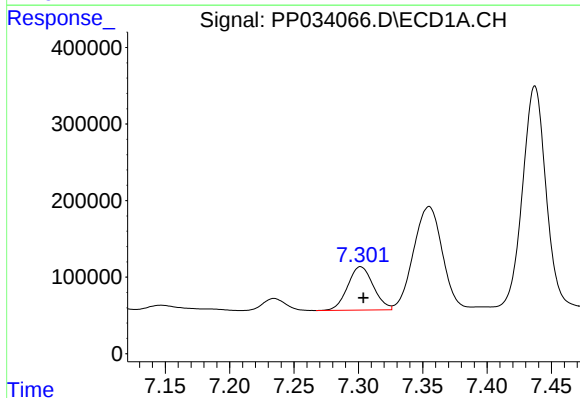


#27 AR-1254-2

R.T.: 7.302 min
Delta R.T.: -0.002 min
Response: 787208
Conc: 173.12 ng/ml

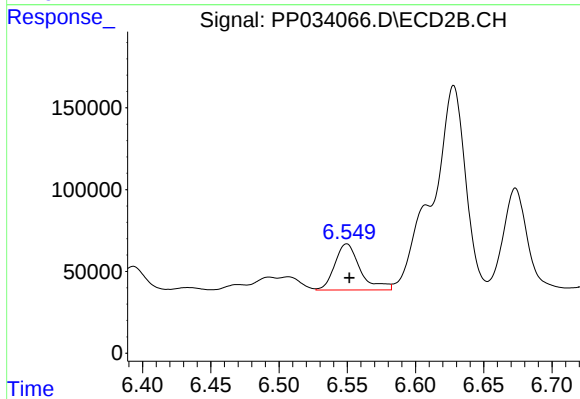

#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.002 min
Response: 365418
Conc: 255.86 ng/ml

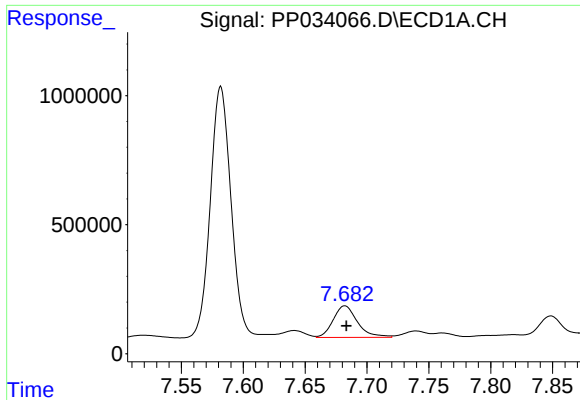


#28 AR-1254-3

R.T.: 7.682 min
Delta R.T.: -0.001 min
Response: 1671474
Conc: 338.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-10A


Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:43 PM

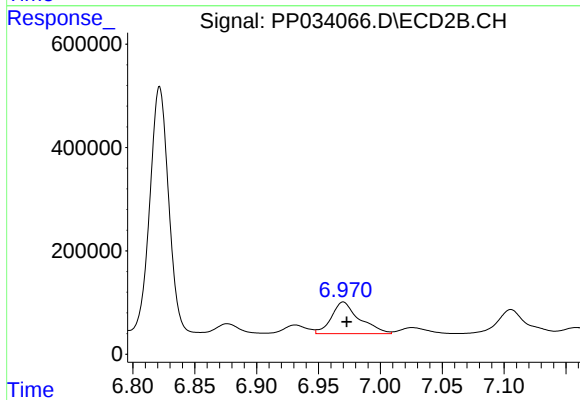


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: -0.003 min
Response: 963433
Conc: 420.93 ng/ml

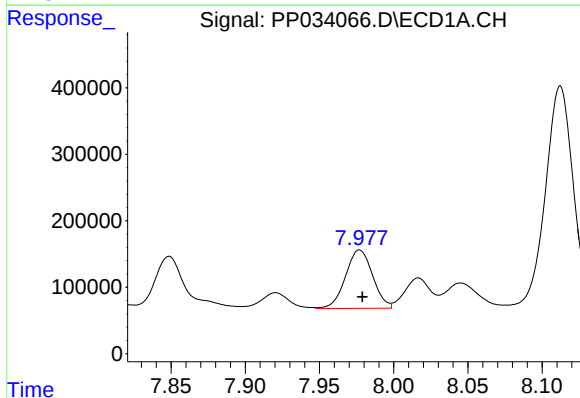


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.002 min
Response: 1121469
Conc: 326.96 ng/ml

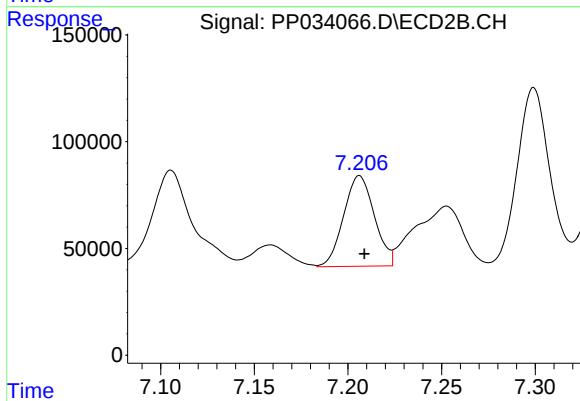

#29 AR-1254-4

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 485609
Conc: 382.06 ng/ml

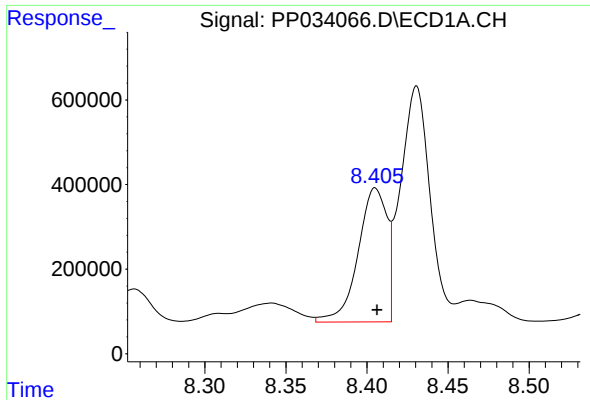


#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.001 min
Response: 3942234
Conc: 1001.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-10A

Manual Integrations
APPROVED

Ankita
3/17/2021 4:36:43 PM

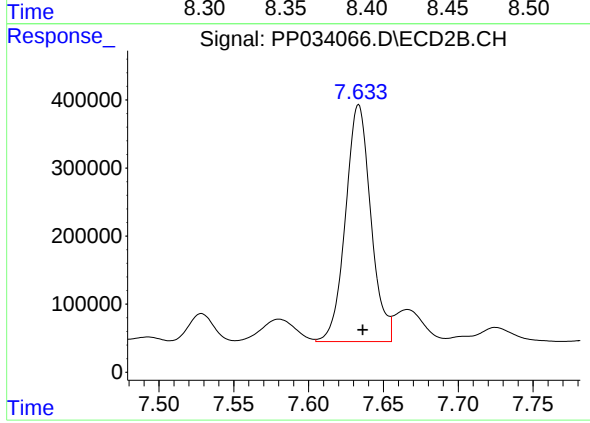

#30 AR-1254-5

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 4097609
Conc: 2175.51 ng/ml