

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031622\
 Data File : PP044799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 11:37
 Operator : YP\AJ
 Sample : N1946-01 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WIPE-NWB-1755A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:56:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.902	3.166	4510544	10182025	2.177m	5.820m#
2) SA Decachlor...	10.032	8.520	2844247	2247088	2.066	1.465 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031622\
Data File : PP044799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 11:37
Operator : YP\AJ
Sample : N1946-01 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WIPE-NWB-1755A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:56:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

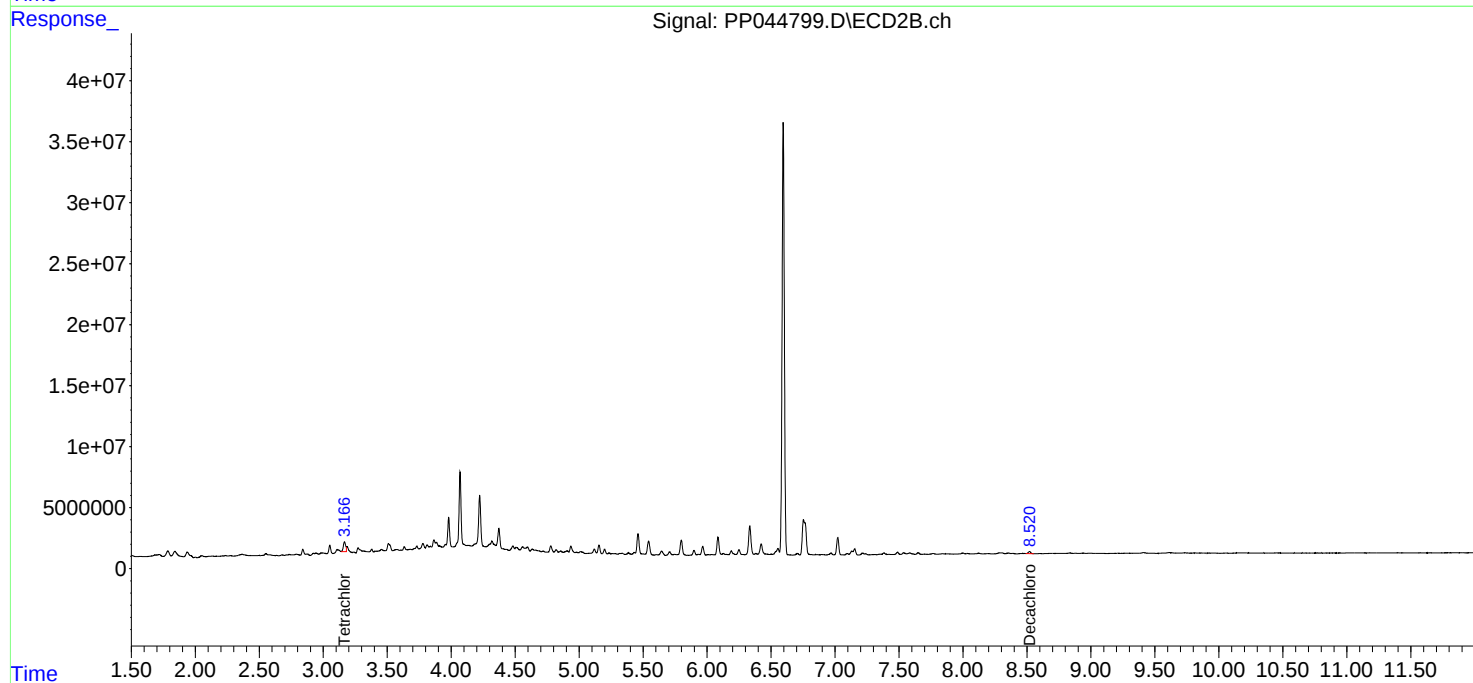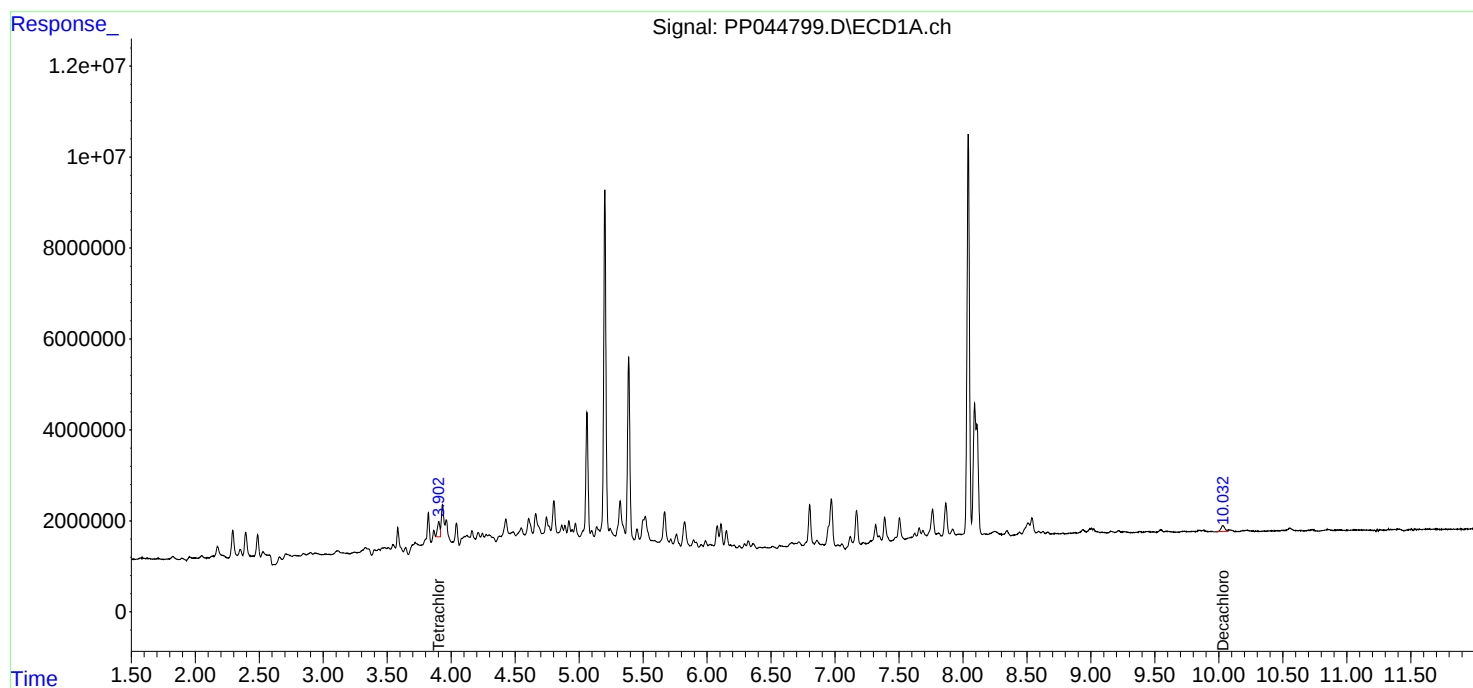


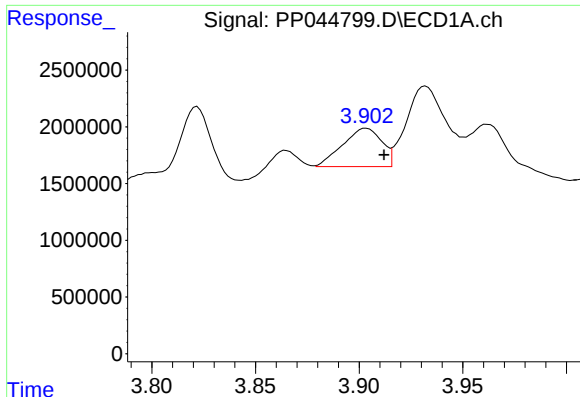

#1 Tetrachloro-m-xylene


R.T.: 3.902 min
Delta R.T.: -0.010 min
Response: 4510544
Conc: 2.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
WIPE-NWB-1755A

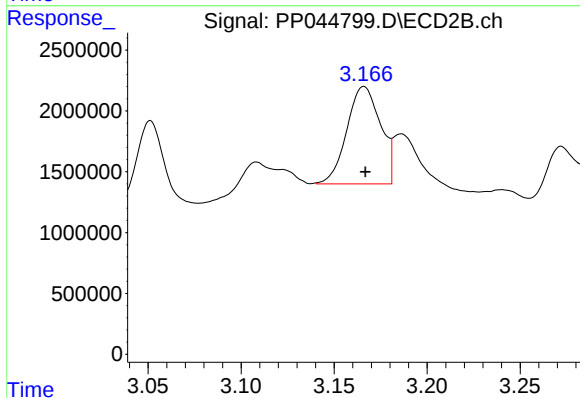


#1 Tetrachloro-m-xylene

R.T.: 3.166 min
Delta R.T.: -0.001 min
Response: 10182025
Conc: 5.82 ng/ml m

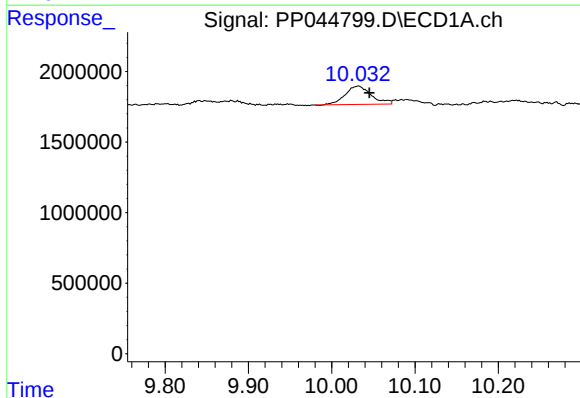

#2 Decachlorobiphenyl

R.T.: 10.032 min
Delta R.T.: -0.013 min
Response: 2844247
Conc: 2.07 ng/ml

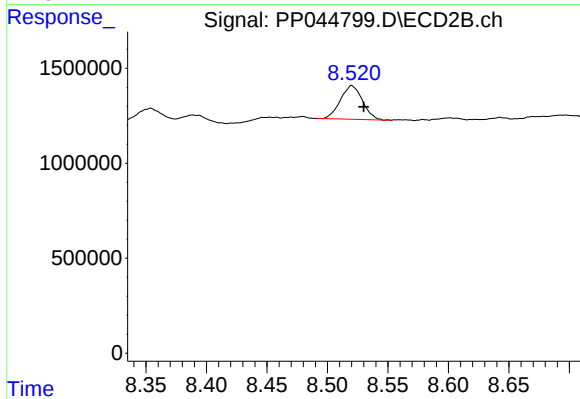

#2 Decachlorobiphenyl

R.T.: 8.520 min
Delta R.T.: -0.010 min
Response: 2247088
Conc: 1.46 ng/ml